




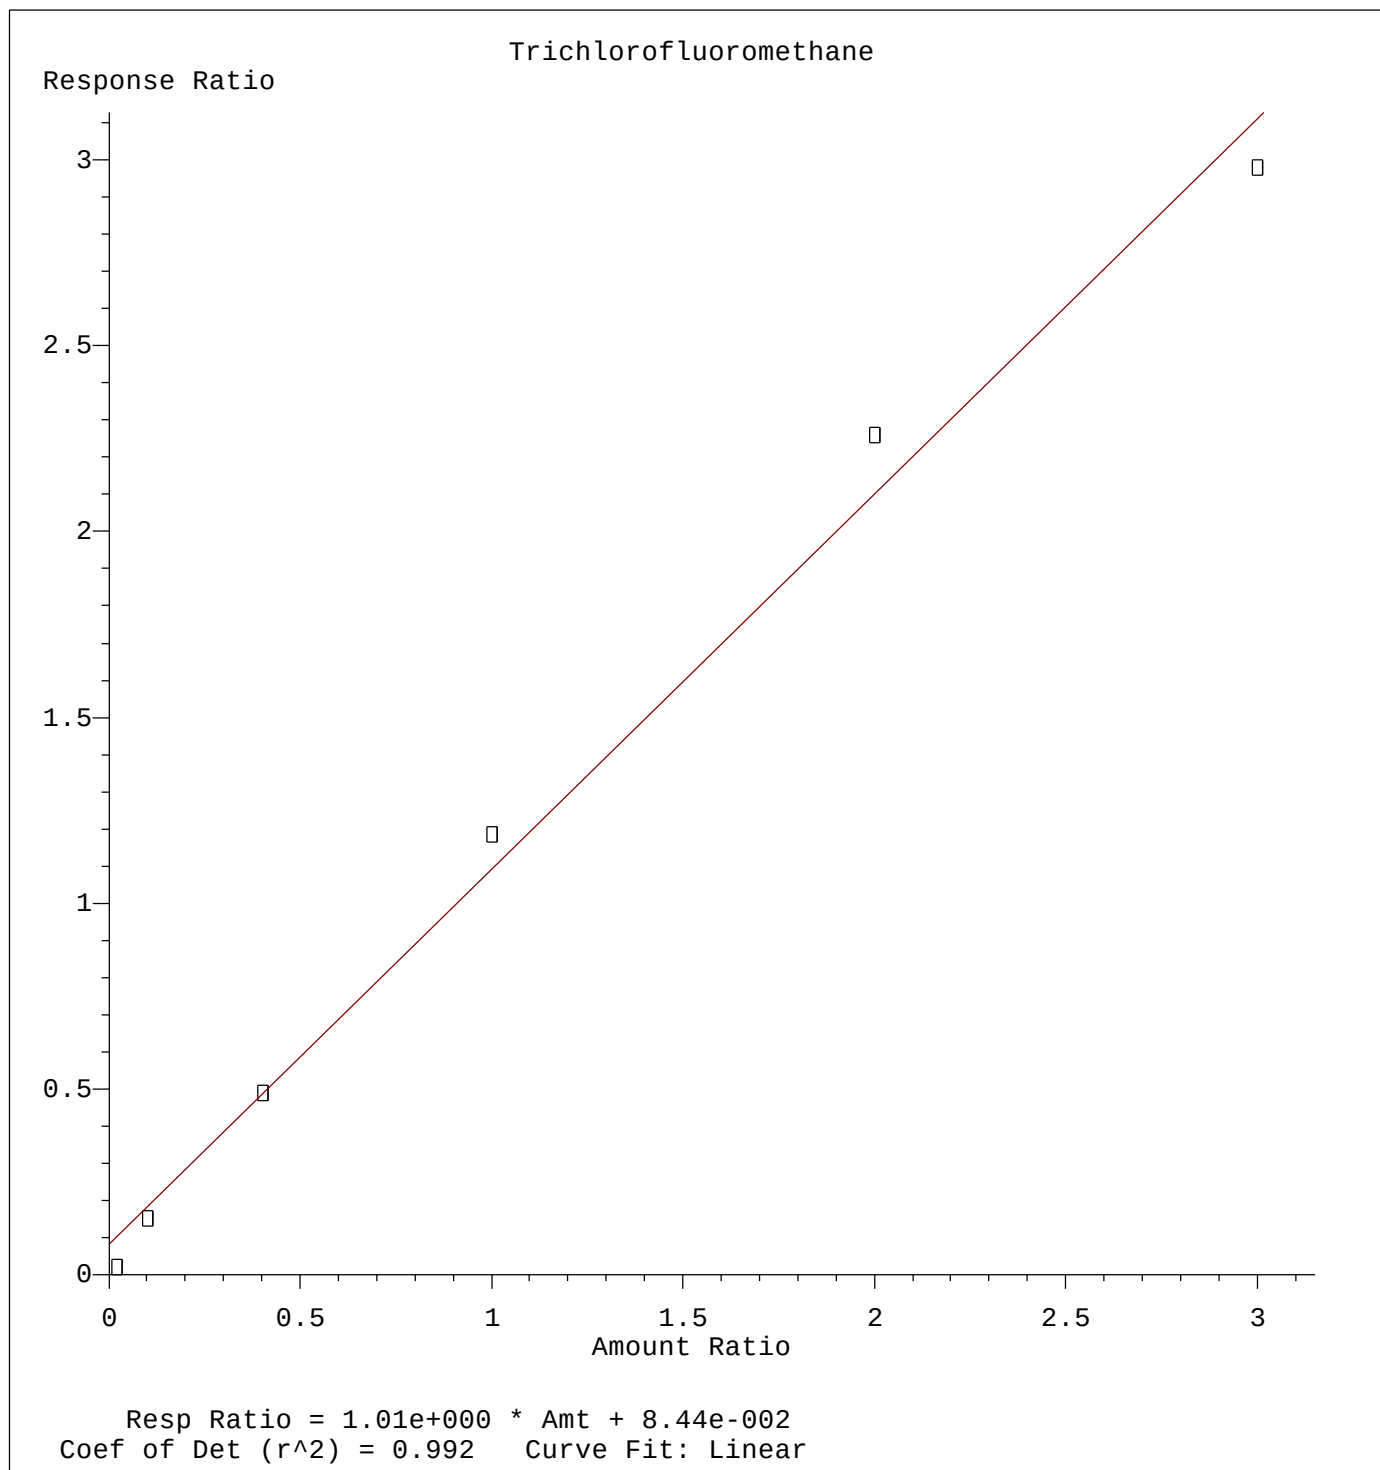

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N083120W.M
Calibration Table Last Updated: Tue Sep 01 04:19:36 2020

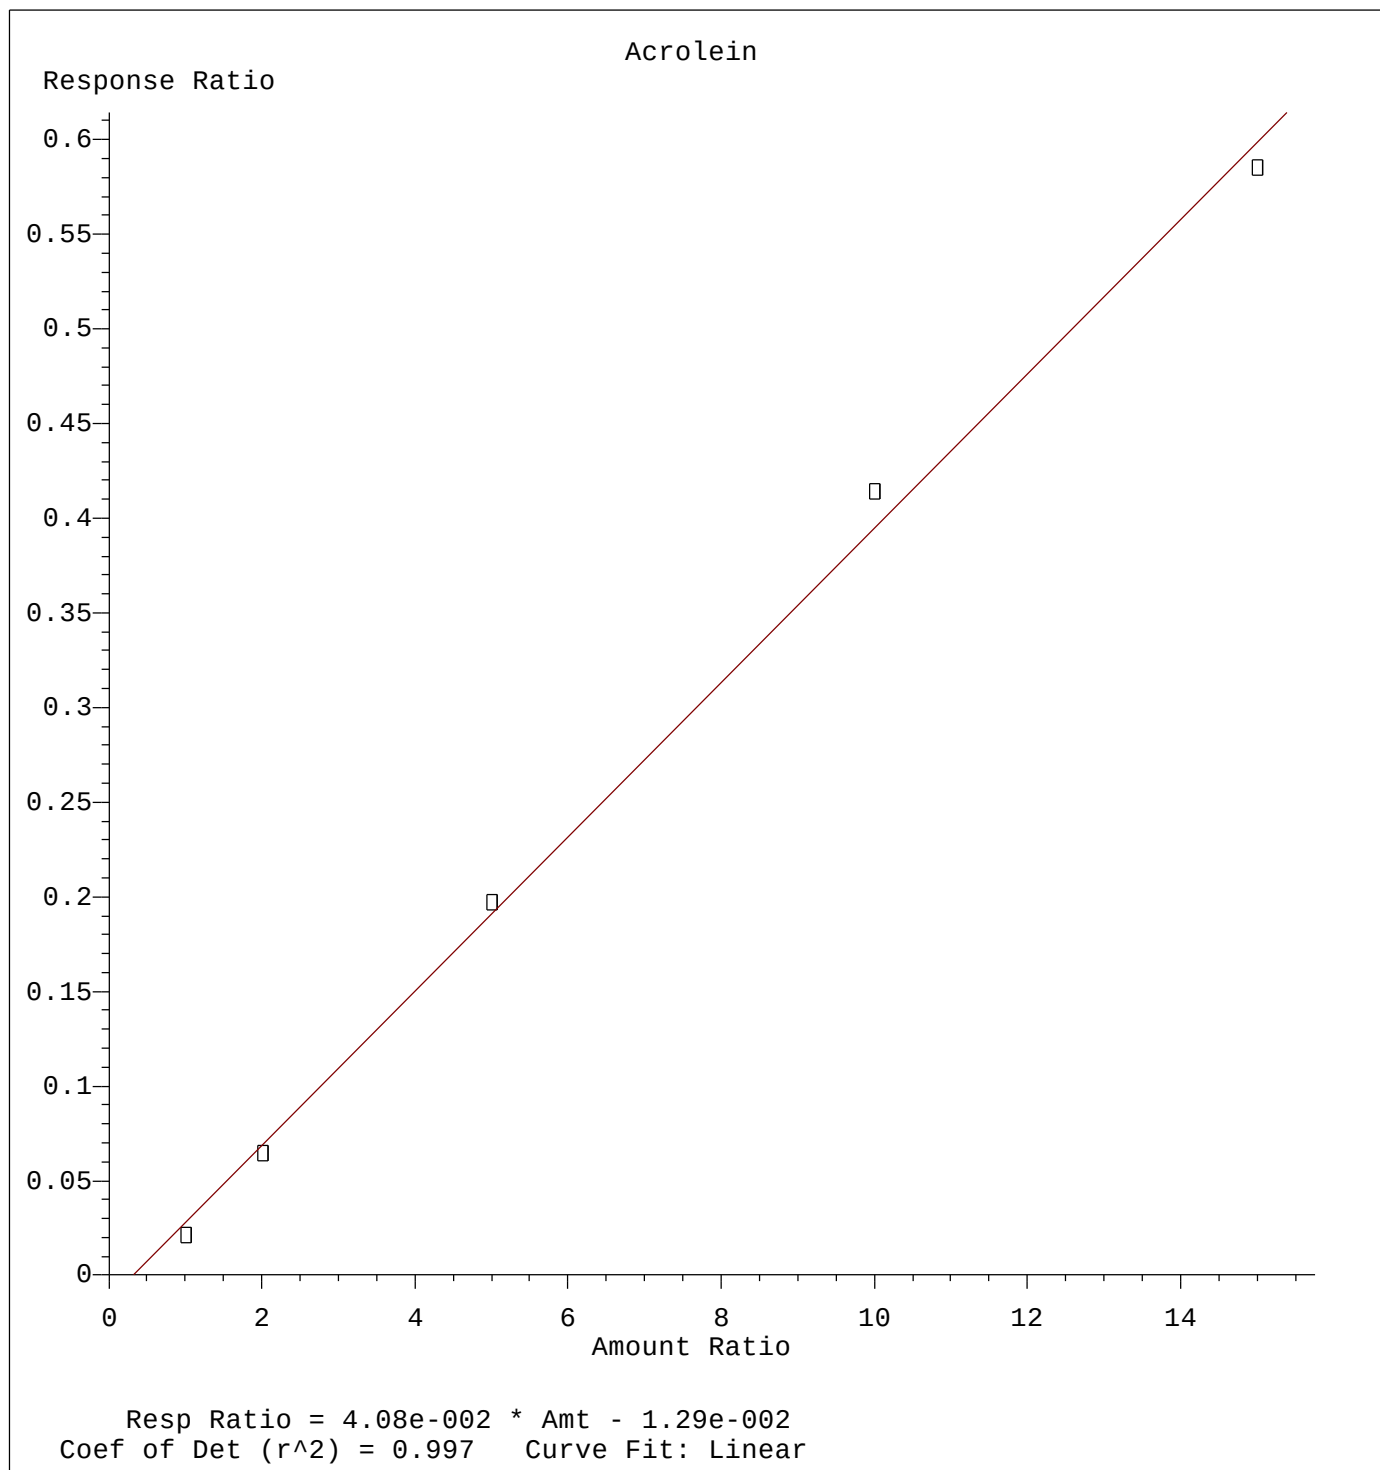


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N083120W.M
Calibration Table Last Updated: Tue Sep 01 04:19:58 2020

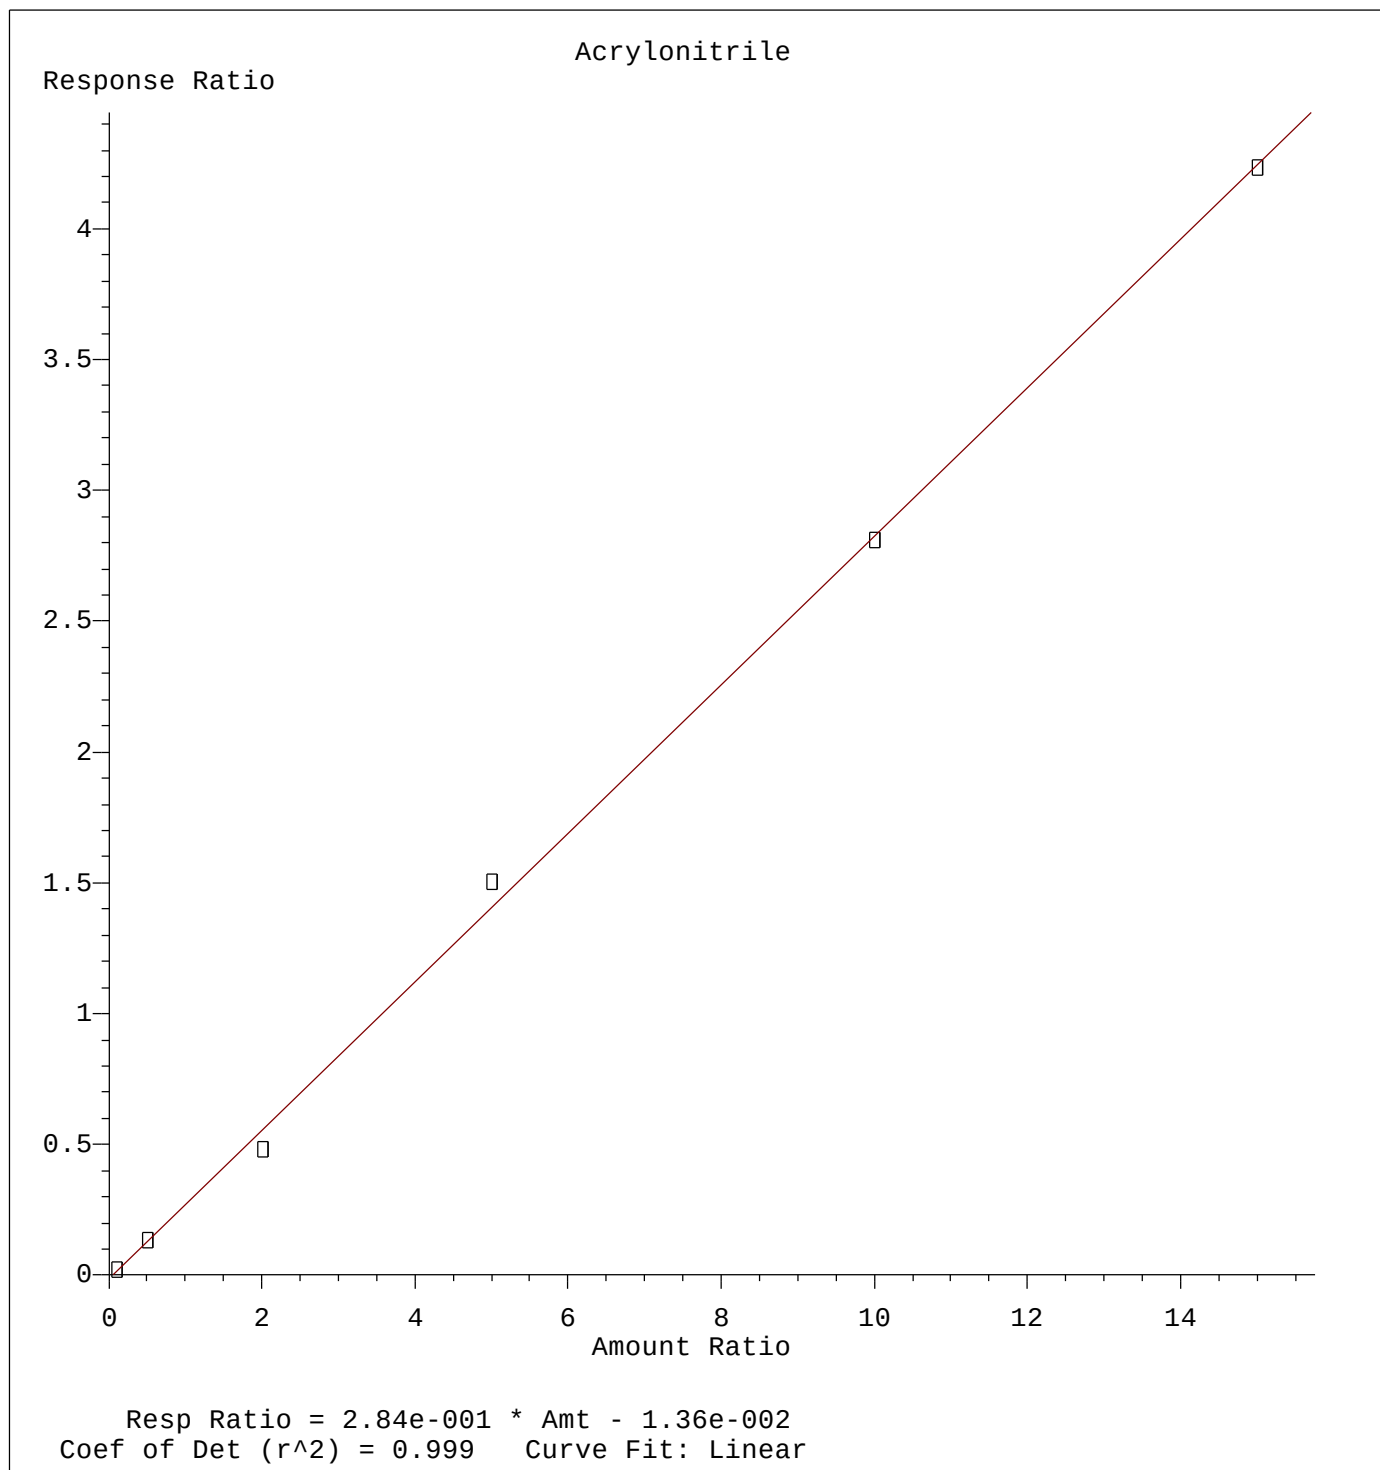

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N083120W.M
Calibration Table Last Updated: Tue Sep 01 04:20:21 2020


Methylene Chloride

Response Ratio

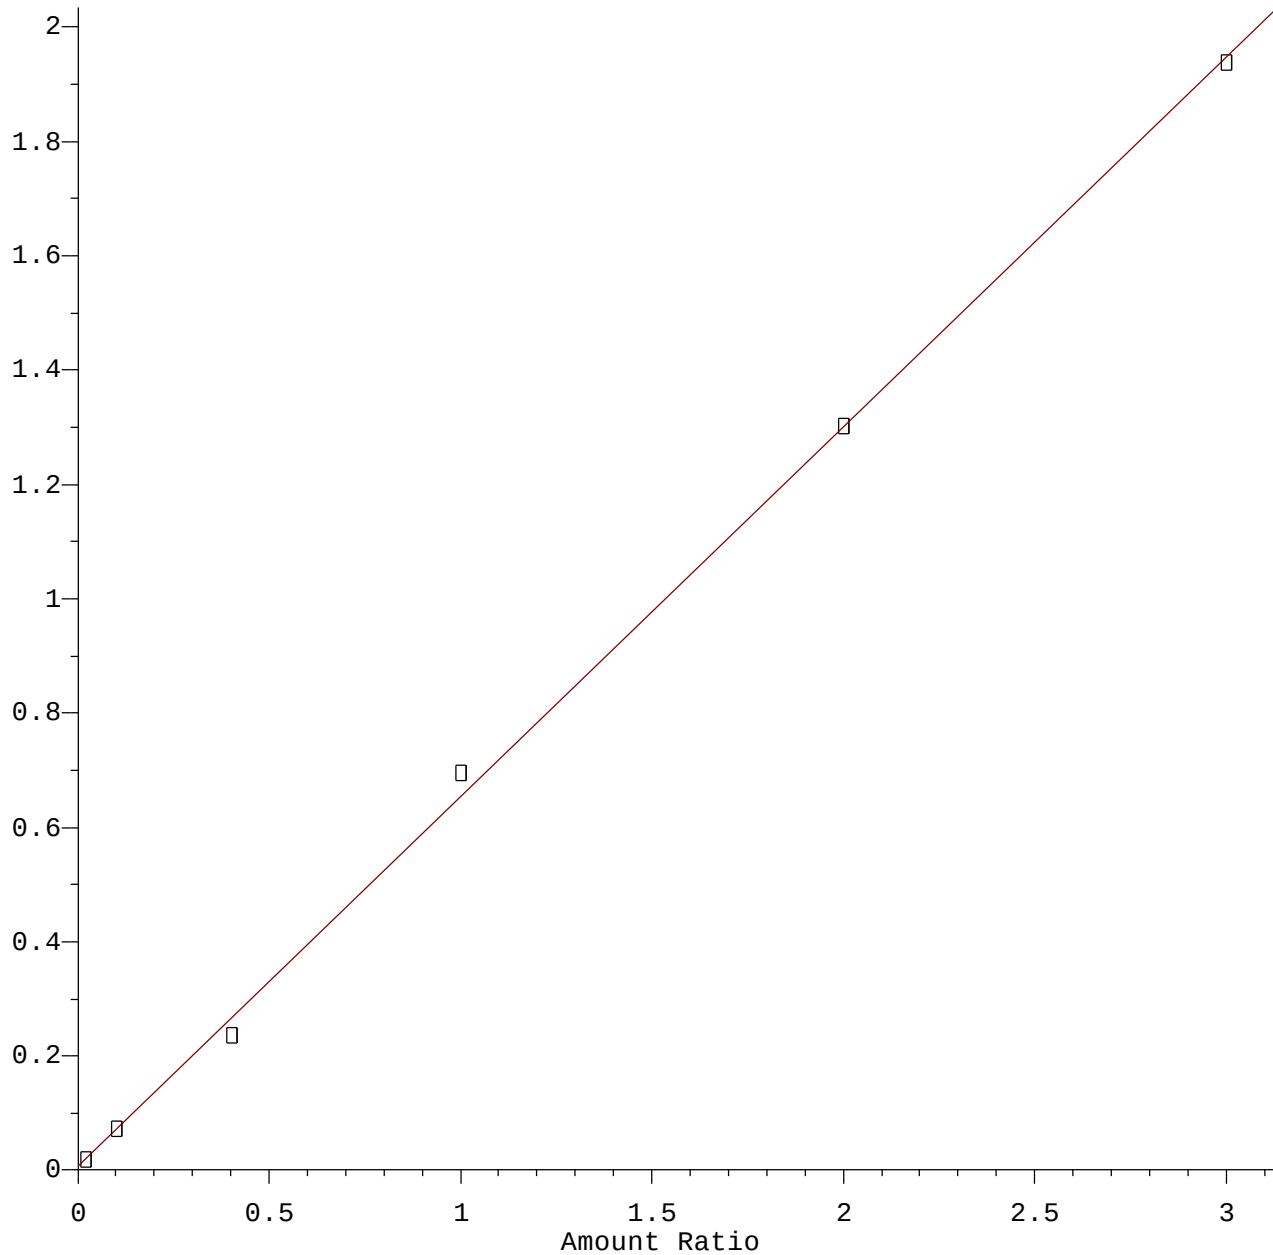


Resp Ratio = $6.47 \times 10^{-1} \times \text{Amt} + 6.43 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N083120W.M
Calibration Table Last Updated: Tue Sep 01 04:20:45 2020

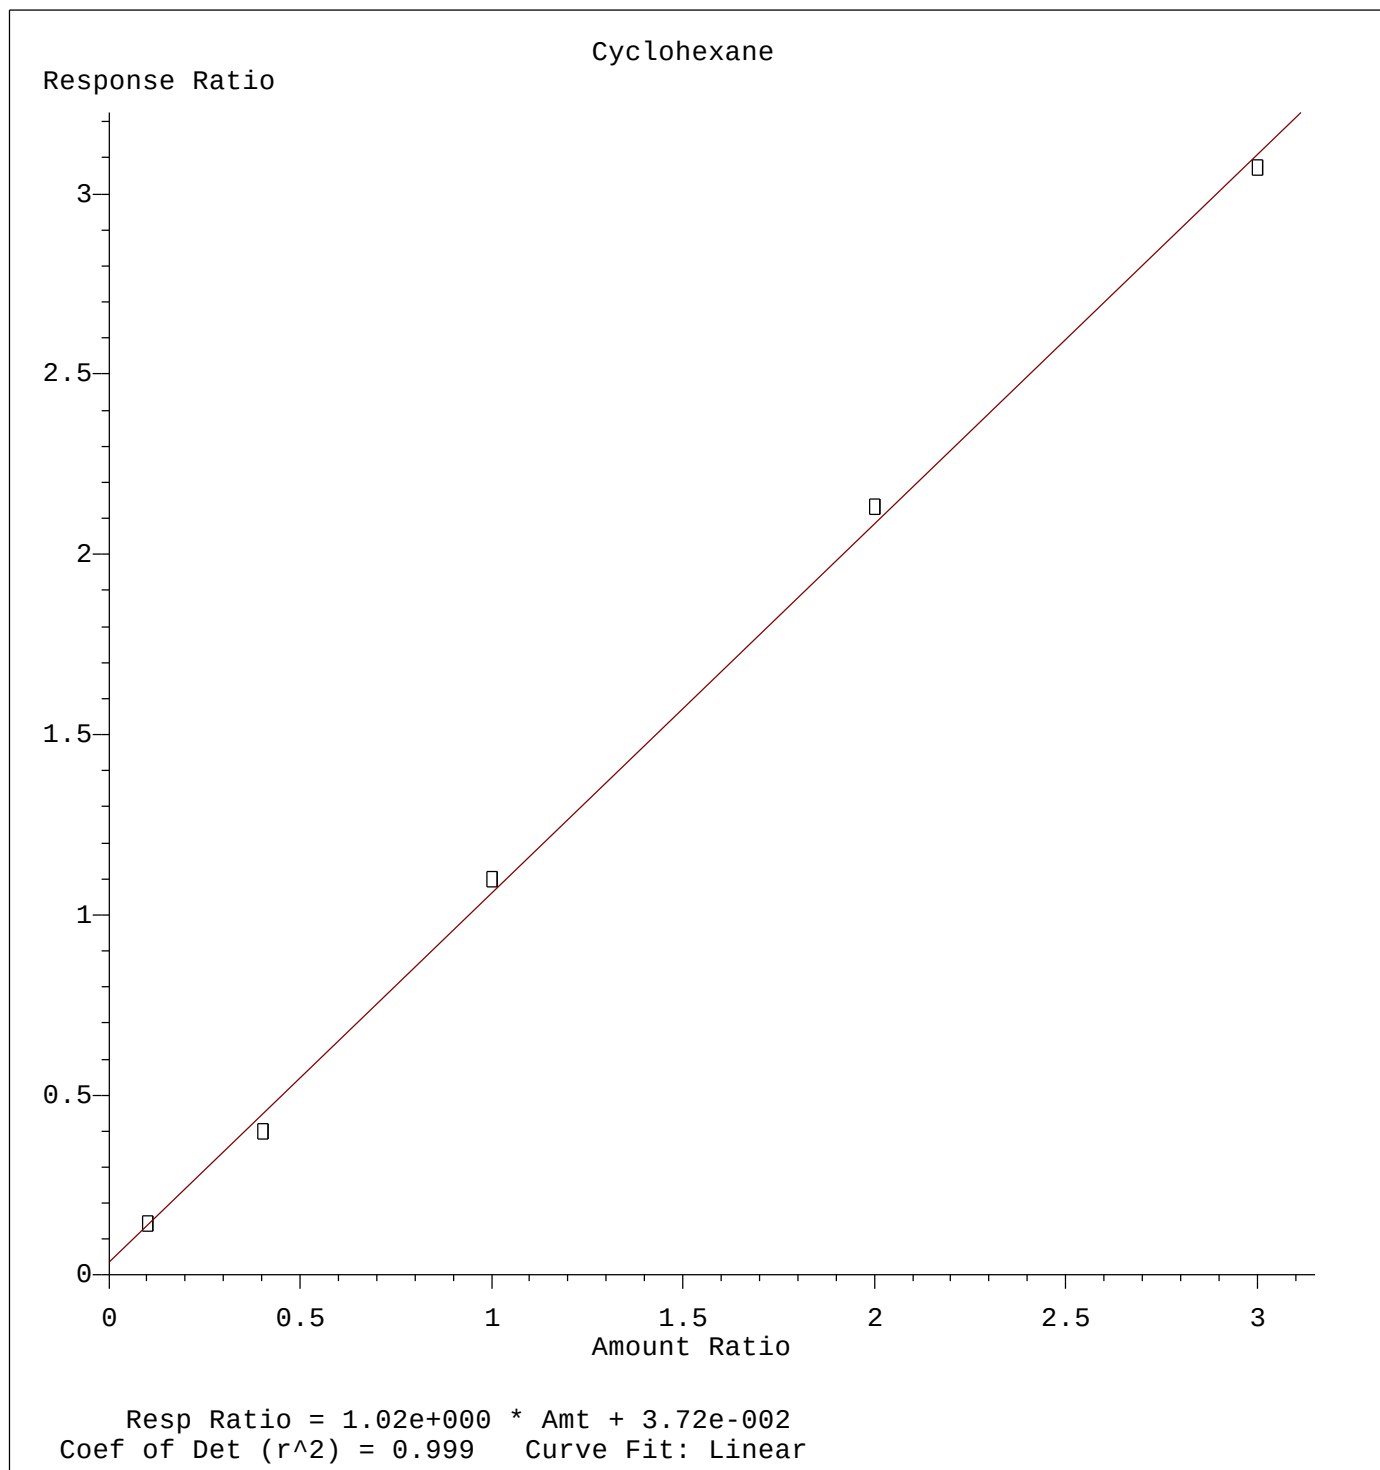

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N083120W.M
Calibration Table Last Updated: Tue Sep 01 04:21:09 2020

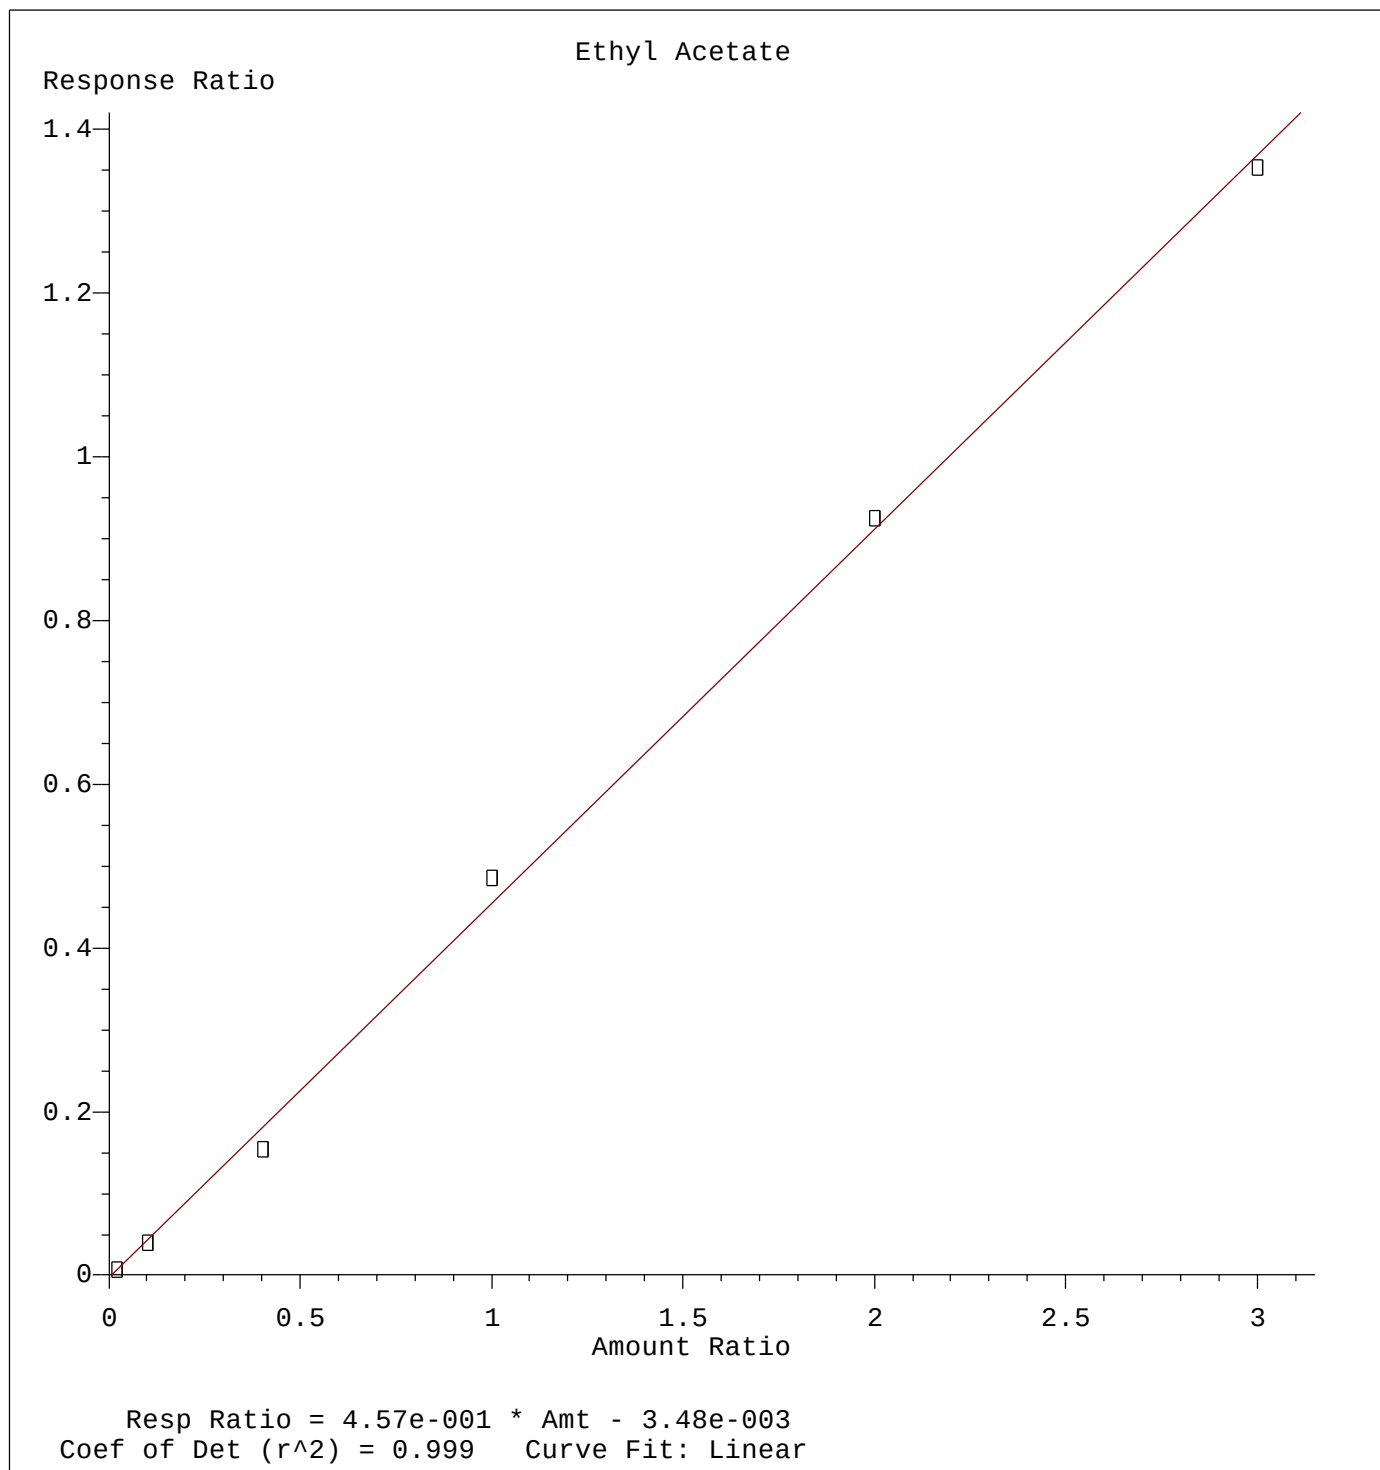

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N083120W.M
Calibration Table Last Updated: Tue Sep 01 04:21:28 2020