


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN083120\
 Data File : VN063146.D
 Acq On : 31 Aug 2020 9:01
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N083120W.M
 Title : SW846 8260
 Last Update : Tue Sep 01 04:21:28 2020

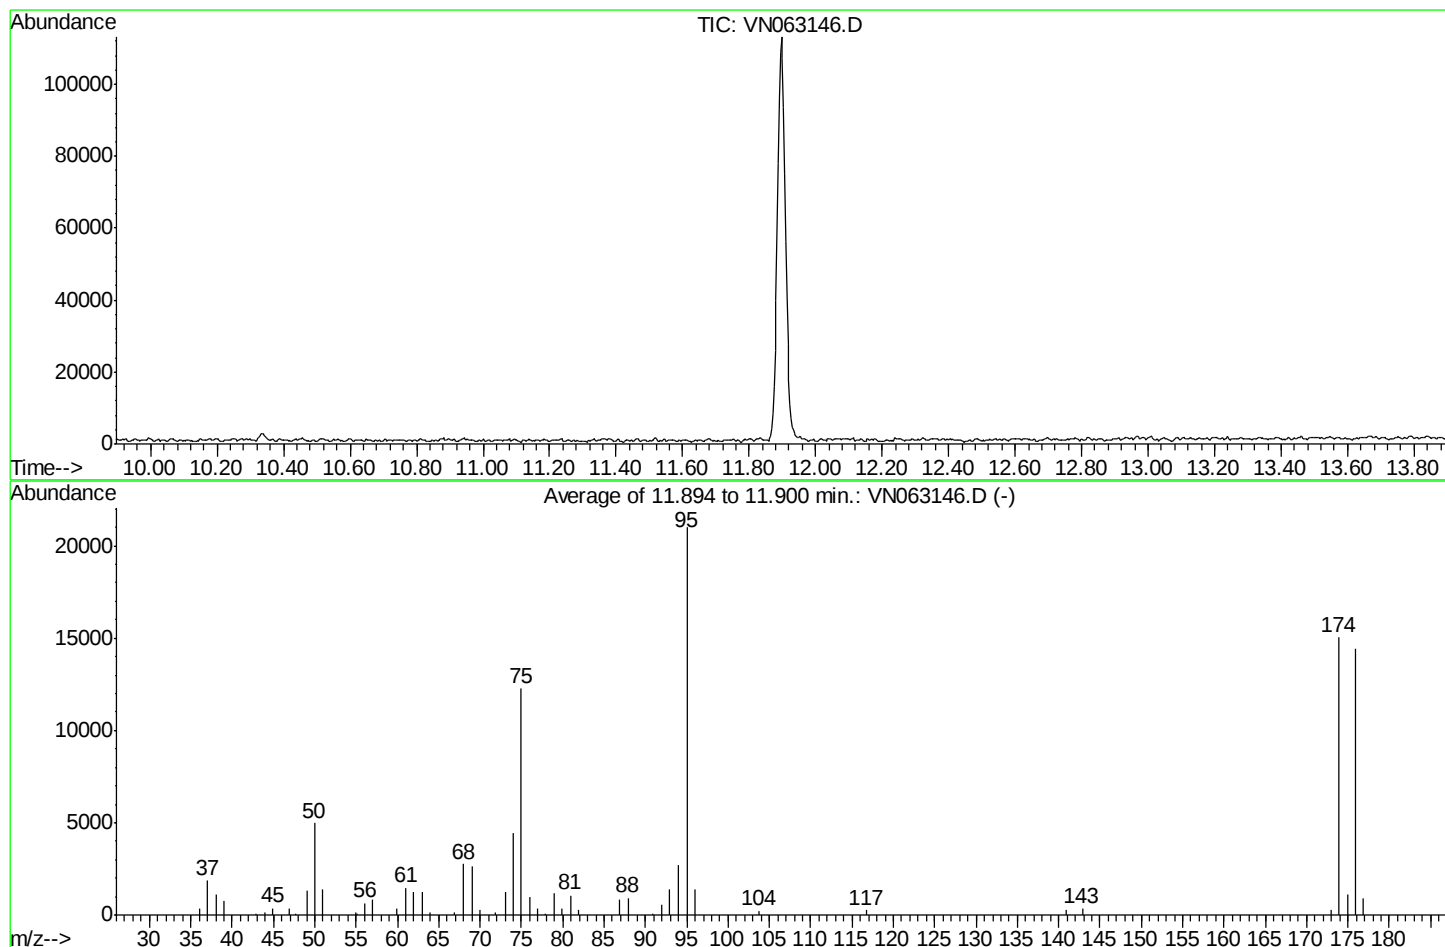

AutoFind: Scans 3158, 3159, 3160; Background Corrected with Scan 3145

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	4986	PASS
75	95	30	60	58.3	12246	PASS
95	95	100	100	100.0	21005	PASS
96	95	5	9	6.5	1358	PASS
173	174	0.00	2	1.8	273	PASS
174	95	50	100	71.6	15049	PASS
175	174	5	9	7.2	1083	PASS
176	174	95	101	96.1	14459	PASS
177	176	5	9	6.0	874	PASS