

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083122\
 Data File : VN074204.D
 Acq On : 31 Aug 2022 10:10
 Operator : JC\MD
 Sample : VN0831MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0831MBL01

Quant Time: Sep 01 00:20:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083022W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 31 07:02:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	180655	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.898	114	334409	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	309173	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	133694	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.363	65	135591	48.384	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	96.760%
35) Dibromofluoromethane	7.951	113	113620	52.213	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	104.420%
50) Toluene-d8	10.380	98	364489	42.533	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	85.060%#
62) 4-Bromofluorobenzene	12.669	95	137147	52.626	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	105.260%


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083122\
Data File : VN074204.D
Acq On : 31 Aug 2022 10:10
Operator : JC\MD
Sample : VN0831MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0831MBL01

Quant Time: Sep 01 00:20:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083022W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 31 07:02:40 2022
Response via : Initial Calibration




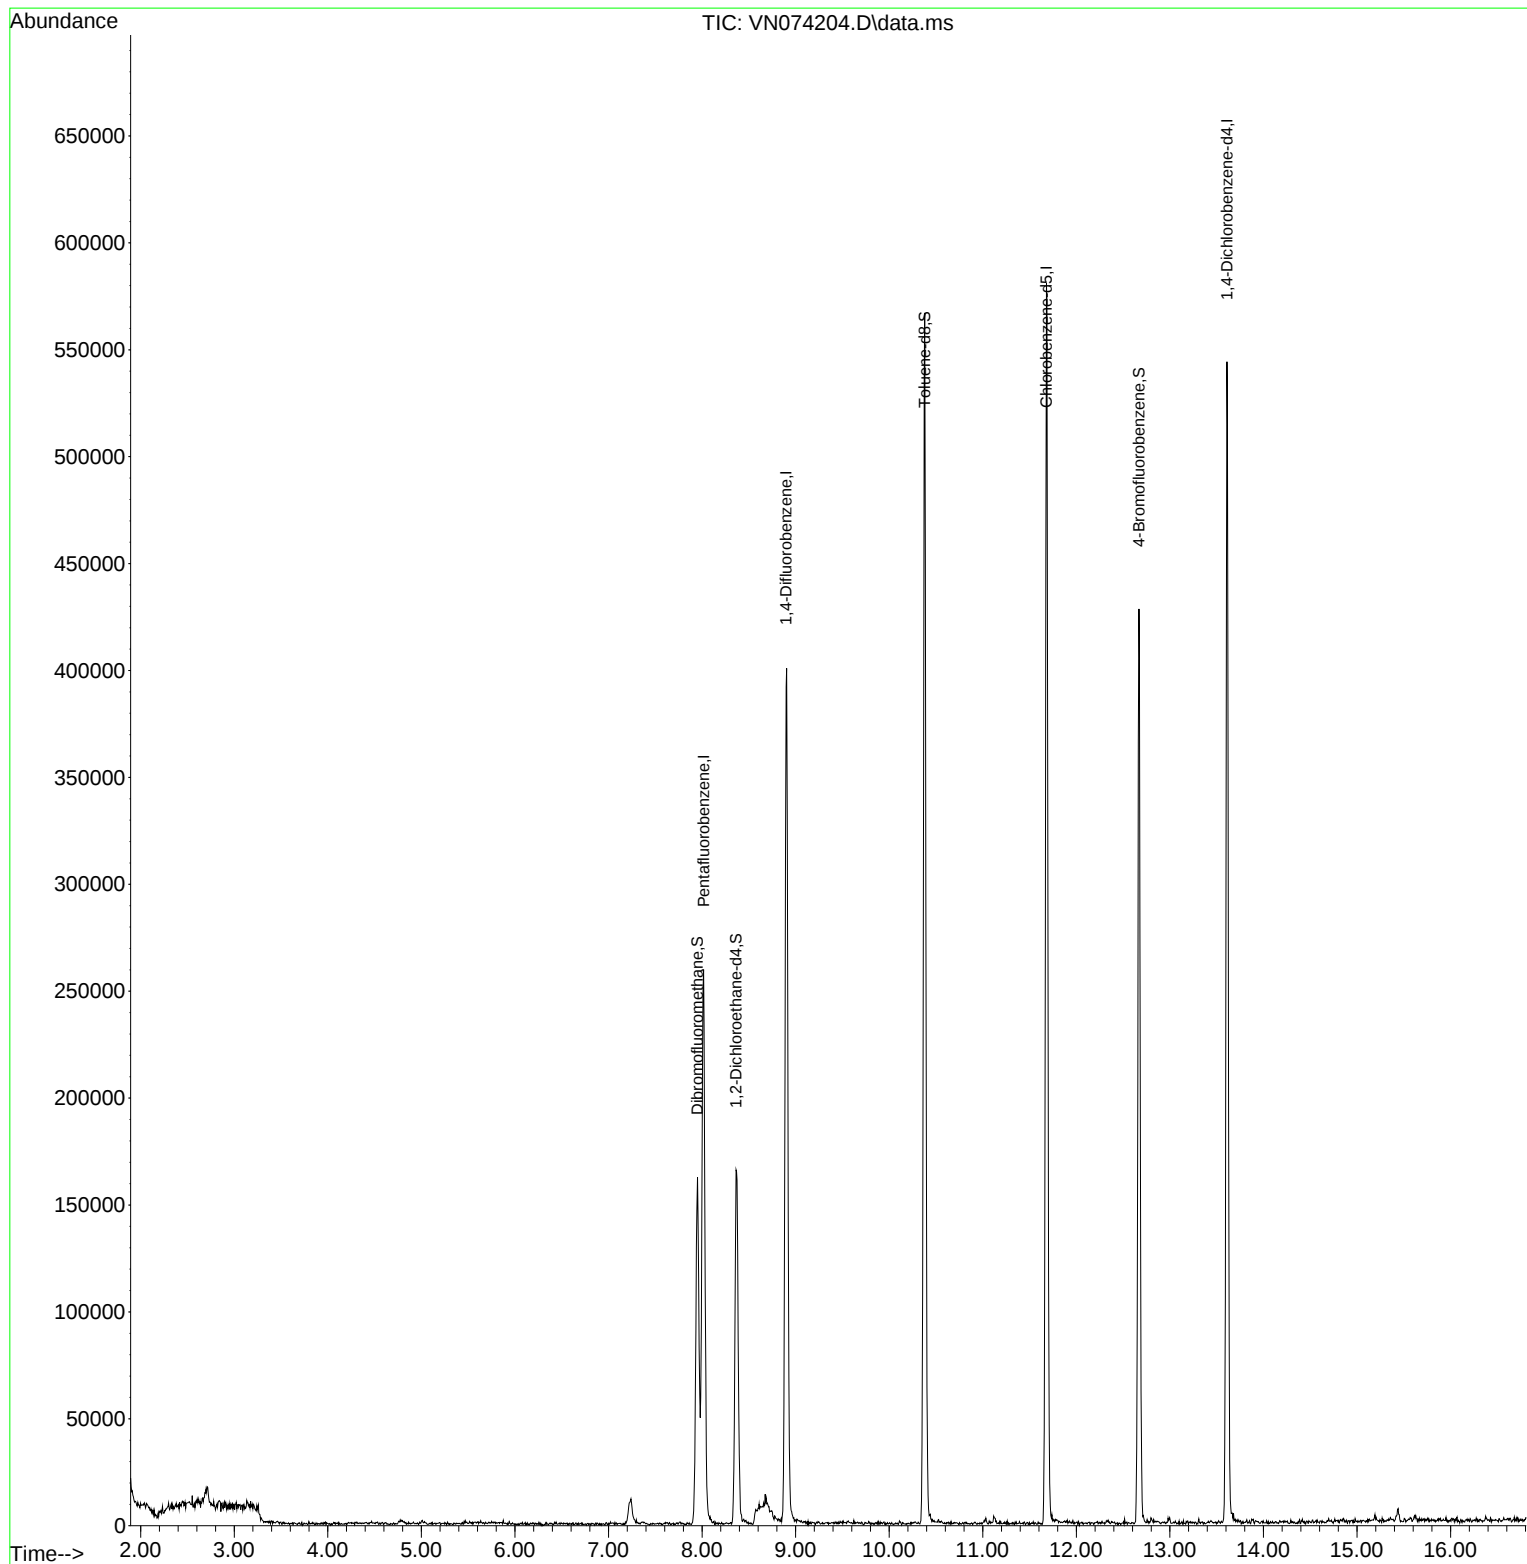


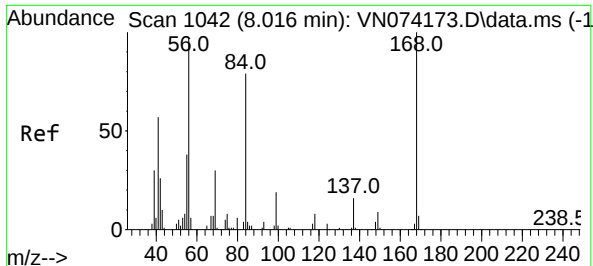

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1101
Delta R.T. -0.000 min
Lab File: VN074204.D
Acq: 31 Aug 2022 10:10




Instrument :
MSVOA_N
ClientSampleId :
VN0831MBL01


Tgt Ion:168 Resp: 180655
Ion Ratio Lower Upper
168 100
99 58.2 42.3 63.5

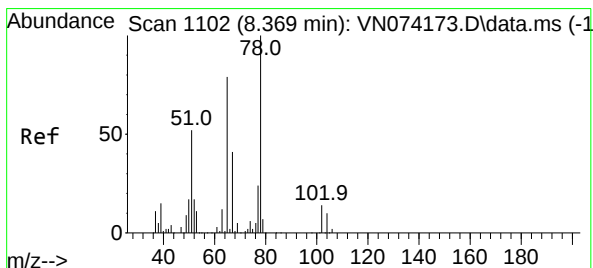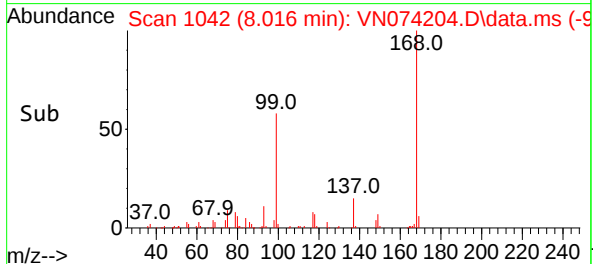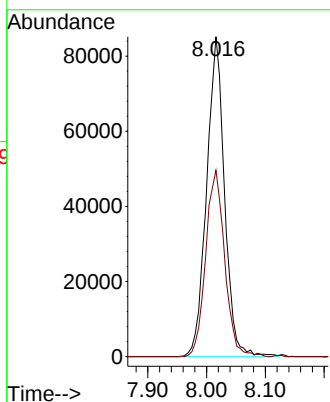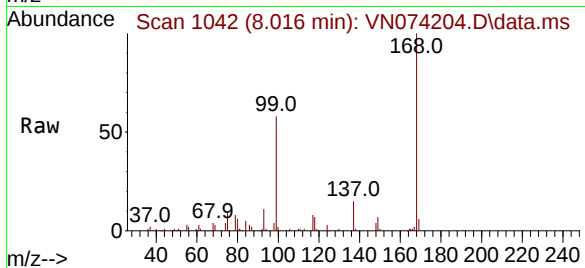

#33
1,2-Dichloroethane-d4
Concen: 48.384 ug/l
RT: 8.363 min Scan# 1101
Delta R.T. -0.006 min
Lab File: VN074204.D
Acq: 31 Aug 2022 10:10

Tgt Ion: 65 Resp: 135591
Ion Ratio Lower Upper
65 100
67 52.7 0.0 104.8

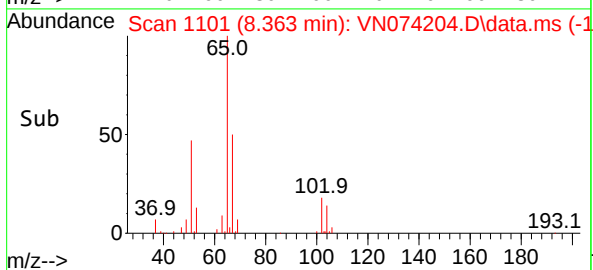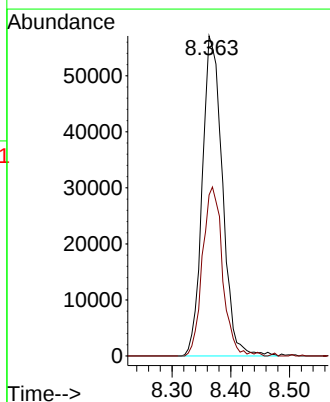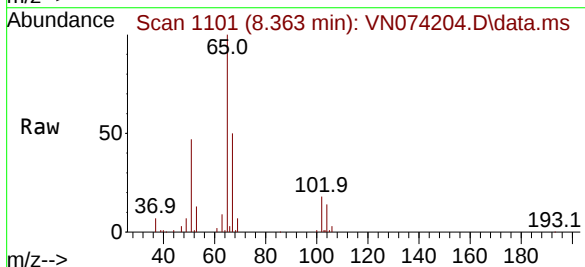

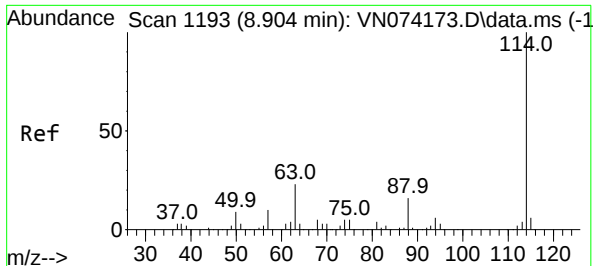

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.898 min Scan# 1193

Delta R.T. -0.006 min

Lab File: VN074204.D

Acq: 31 Aug 2022 10:10

Instrument :

MSVOA_N

ClientSampleId :

VN0831MBL01





Tgt Ion:114 Resp: 334409

Ion Ratio Lower Upper

114 100

63 23.3 0.0 40.0

88 13.4 0.0 32.6

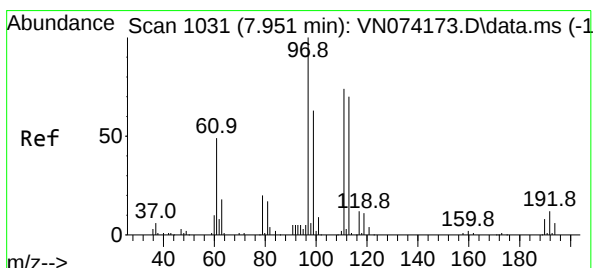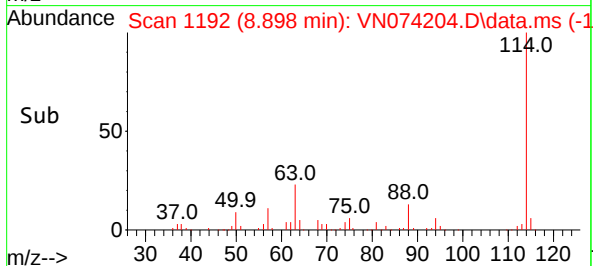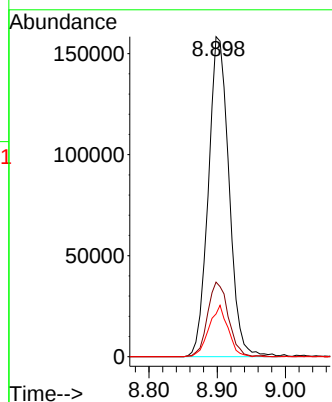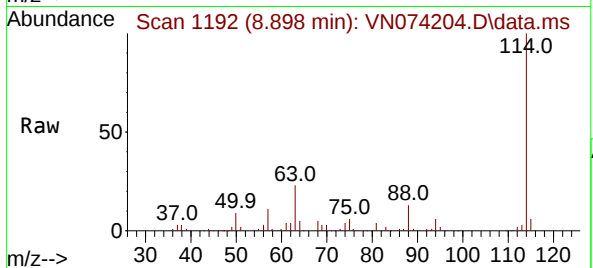

#35

Dibromofluoromethane

Concen: 52.213 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN074204.D

Acq: 31 Aug 2022 10:10




Tgt Ion:113 Resp: 113620


Ion Ratio Lower Upper

113 100

111 101.7 81.4 122.0

192 17.2 17.0 25.6


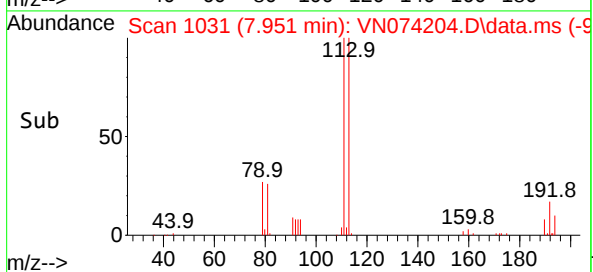
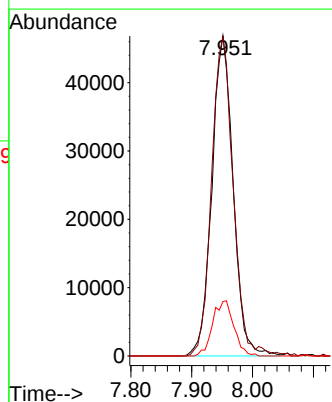
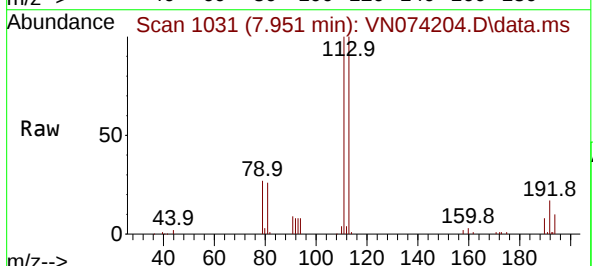


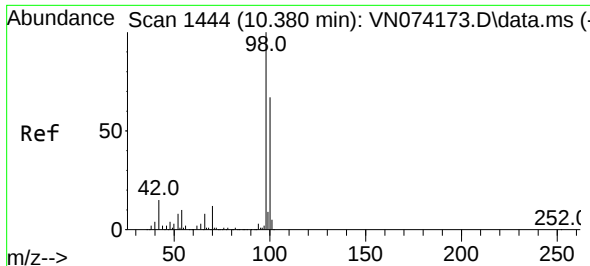

#50
Toluene-d8
Concen: 42.533 ug/l
RT: 10.380 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN074204.D
Acq: 31 Aug 2022 10:10




Instrument :
MSVOA_N
ClientSampleId :
VN0831MBL01


Tgt Ion: 98 Resp: 364489
Ion Ratio Lower Upper
98 100
100 65.3 52.6 78.8

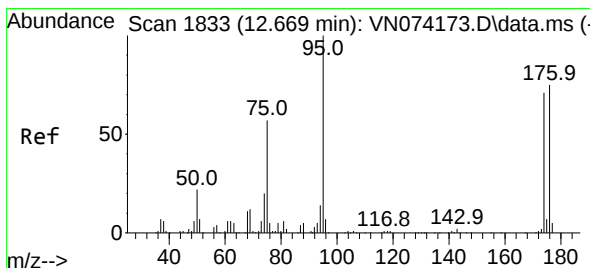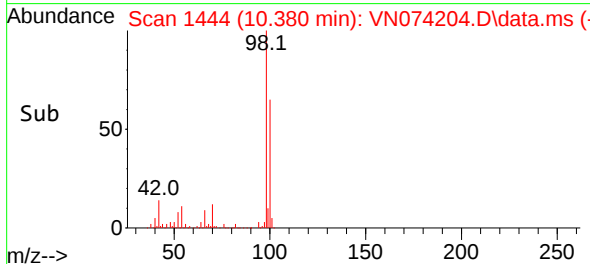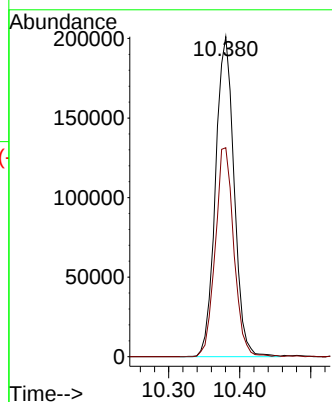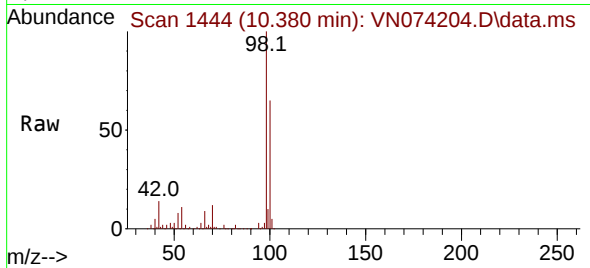

#62
4-Bromofluorobenzene
Concen: 52.626 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. 0.000 min
Lab File: VN074204.D
Acq: 31 Aug 2022 10:10

Tgt Ion: 95 Resp: 137147
Ion Ratio Lower Upper
95 100
174 75.2 0.0 167.6
176 69.5 0.0 163.4


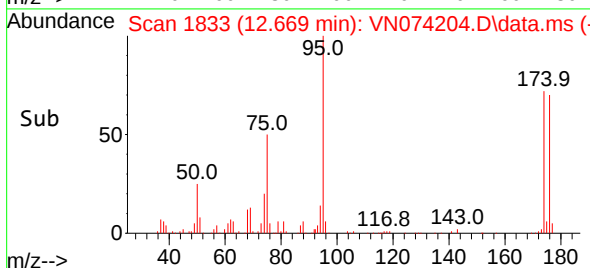
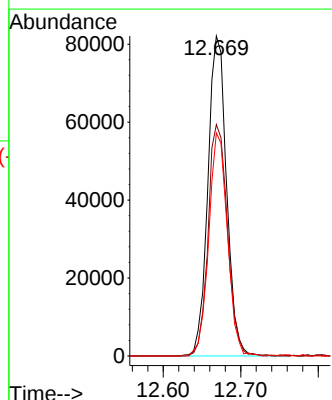
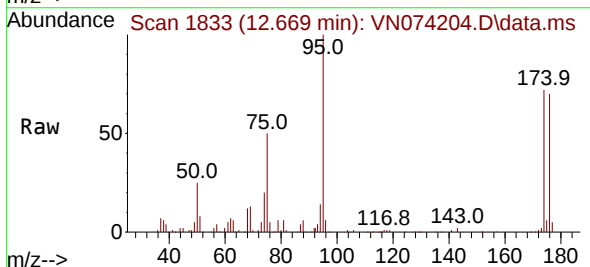


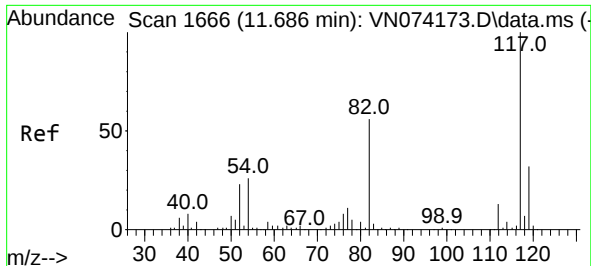

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.680 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN074204.D
Acq: 31 Aug 2022 10:10

Instrument :
MSVOA_N
ClientSampleId :
VN0831MBL01

Tgt Ion:117 Resp: 309173
Ion Ratio Lower Upper
117 100
82 61.3 44.2 66.2
119 30.9 25.4 38.0

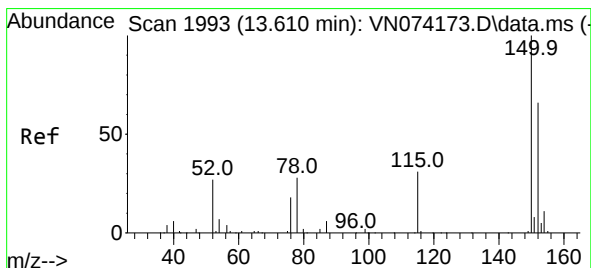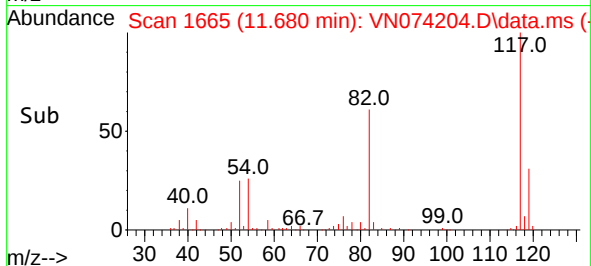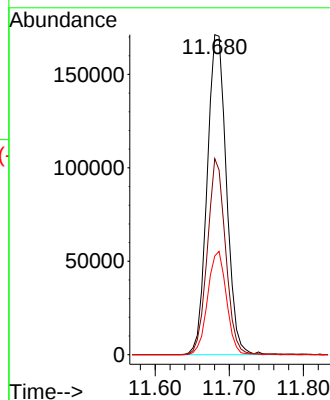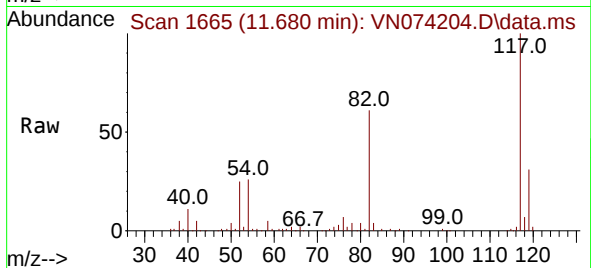

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.610 min Scan# 1993
Delta R.T. -0.000 min
Lab File: VN074204.D
Acq: 31 Aug 2022 10:10

Tgt Ion:152 Resp: 133694
Ion Ratio Lower Upper
152 100
115 58.9 28.9 86.7
150 156.1 0.0 356.2

