

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083122\
 Data File : VN074213.D
 Acq On : 31 Aug 2022 14:45
 Operator : JC\MD
 Sample : N4350-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 COMMUNITY-CENTER-KITCHEN-SINK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083022W.M
 Title : SW846 8260

Signal : TIC: VN074213.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.705	136	139	147	rVB7	9892	19368	1.47%	0.247%
2	7.616	964	974	986	rBV2	97212	263034	20.01%	3.352%
3	7.739	988	995	996	rBV3	13128	17142	1.30%	0.218%
4	7.951	1022	1031	1036	rBV	201622	454619	34.59%	5.794%
5	8.016	1036	1042	1057	rVB	298726	700159	53.28%	8.923%
6	8.369	1093	1102	1114	rBV	216223	498726	37.95%	6.356%
7	8.904	1183	1193	1206	rBV	481633	977931	74.41%	12.463%
8	9.704	1321	1329	1335	rBV3	17078	35190	2.68%	0.448%
9	10.380	1434	1444	1457	rBV	707216	1314231	100.00%	16.748%
10	11.092	1561	1565	1574	rVV2	13038	24201	1.84%	0.308%
11	11.180	1574	1580	1586	rVB3	21716	38778	2.95%	0.494%
12	11.686	1658	1666	1677	rBV	716625	1268194	96.50%	16.162%
13	12.398	1781	1787	1797	rVB3	10770	23781	1.81%	0.303%
14	12.669	1826	1833	1845	rVB	576119	981766	74.70%	12.512%
15	13.610	1983	1993	2004	rBV	686752	1189933	90.54%	15.164%
16	15.398	2290	2297	2308	rVB10	12872	39854	3.03%	0.508%


Sum of corrected areas: 7846907

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083122\
Data File : VN074213.D
Acq On : 31 Aug 2022 14:45
Operator : JC\MD
Sample : N4350-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
COMMUNITY-CENTER-KITCHEN-SINK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

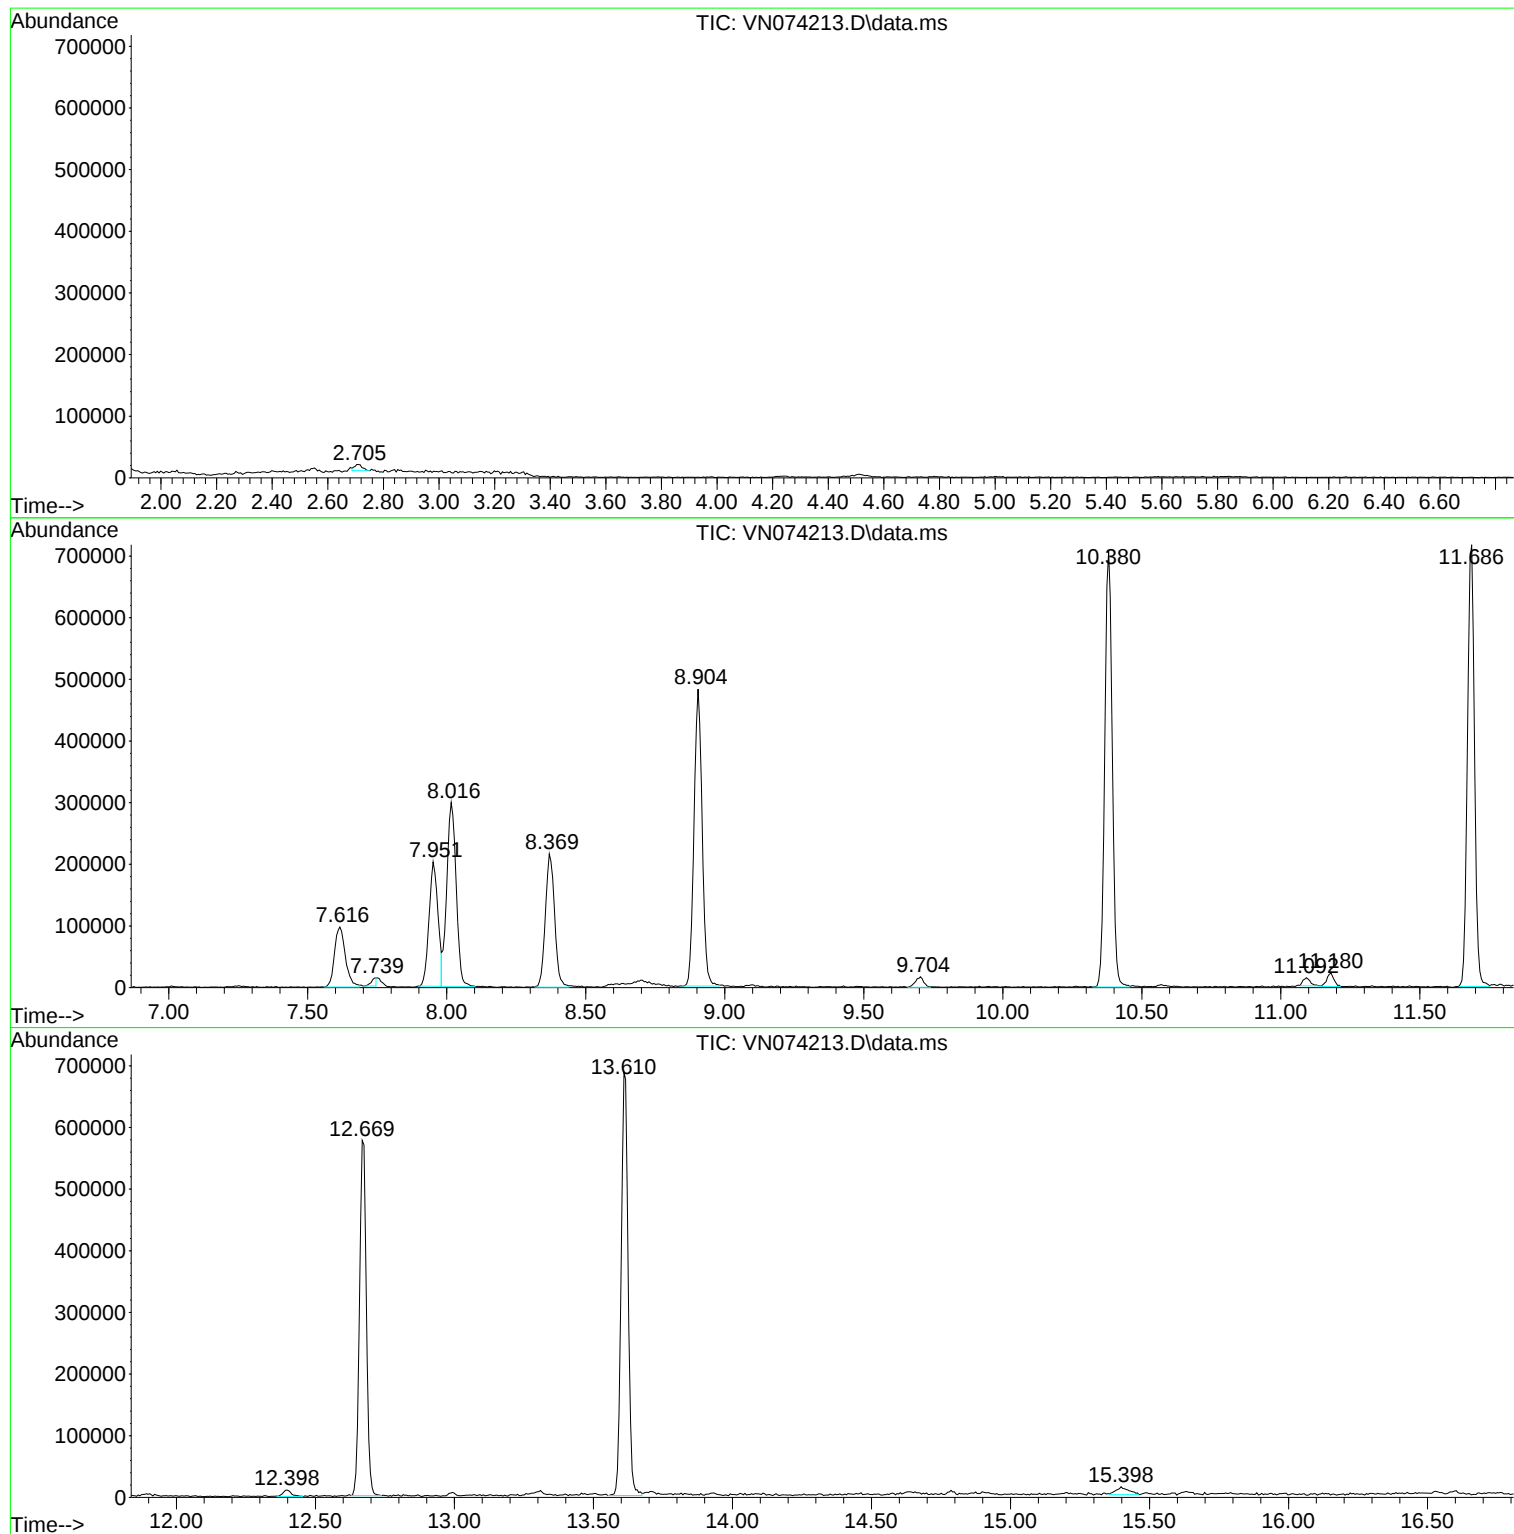

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083122\
Data File : VN074213.D
Acq On : 31 Aug 2022 14:45
Operator : JC\MD
Sample : N4350-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
COMMUNITY-CENTER-KITCHEN-SINK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083122\
Data File : VN074213.D
Acq On : 31 Aug 2022 14:45
Operator : JC\MD
Sample : N4350-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
COMMUNITY-CENTER-KITCHEN-SINK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc