
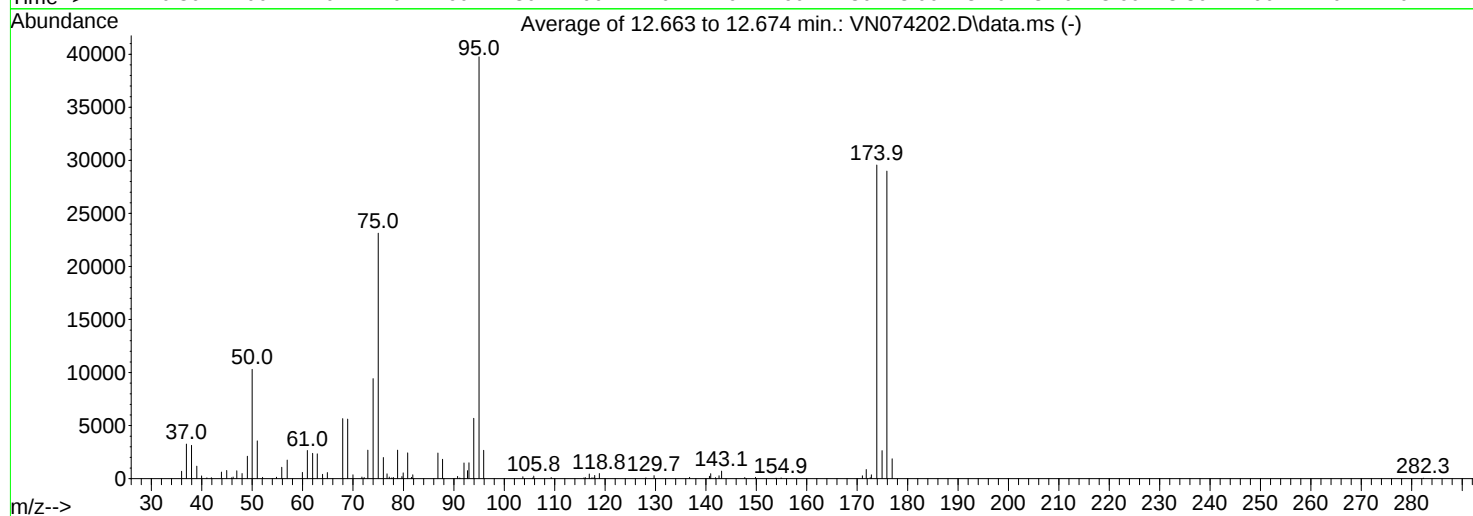


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083122\
 Data File : VN074202.D
 Acq On : 31 Aug 2022 08:53
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083022W.M
 Title : SW846 8260
 Last Update : Wed Aug 31 07:02:40 2022

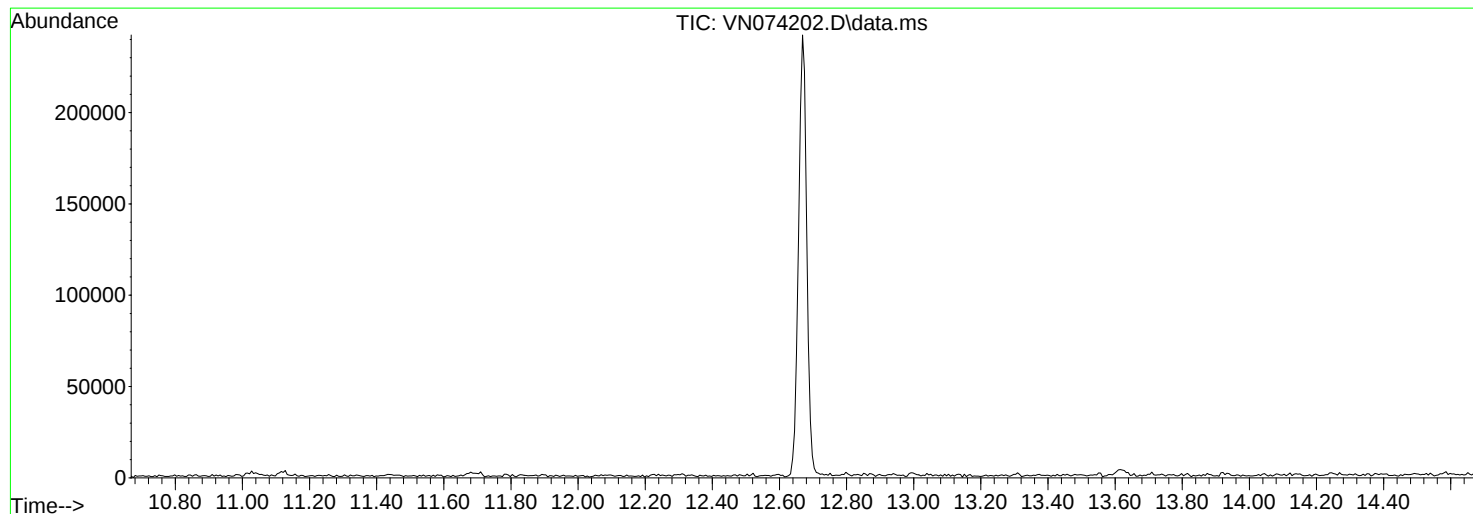

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.9	10307	PASS
75	95	30	60	58.2	23128	PASS
95	95	100	100	100.0	39755	PASS
96	95	5	9	6.7	2671	PASS
173	174	0.00	2	1.2	369	PASS
174	95	50	100	74.4	29565	PASS
175	174	5	9	8.9	2639	PASS
176	174	95	101	98.0	28984	PASS
177	176	5	9	6.5	1876	PASS