


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN090119\
Data File : VN057610.D
Acq On : 31 Aug 2019 12:38
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N090119W.M
Title : SW846 8260
Last Update : Mon Sep 02 06:48:16 2019

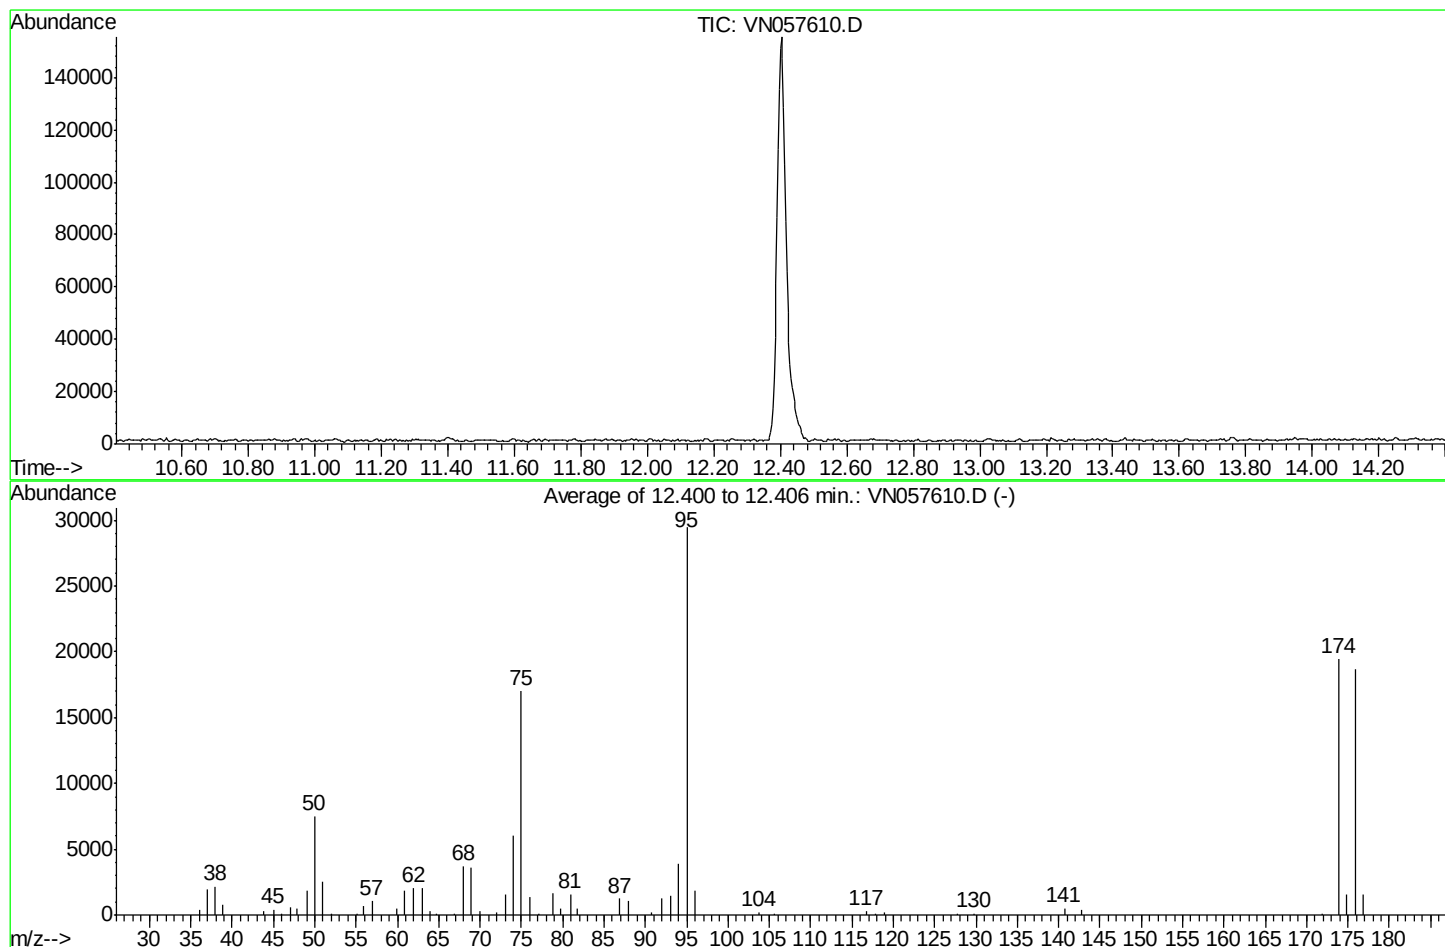

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.5	7527	PASS
75	95	30	60	57.9	17055	PASS
95	95	100	100	100.0	29464	PASS
96	95	5	9	6.4	1882	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	66.1	19482	PASS
175	174	5	9	7.8	1517	PASS
176	174	95	101	96.0	18693	PASS
177	176	5	9	8.1	1519	PASS