


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN090120\
Data File : VN063154.D
Acq On : 1 Sep 2020 13:49
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N083120W.M
Title : SW846 8260
Last Update : Tue Sep 01 04:21:28 2020

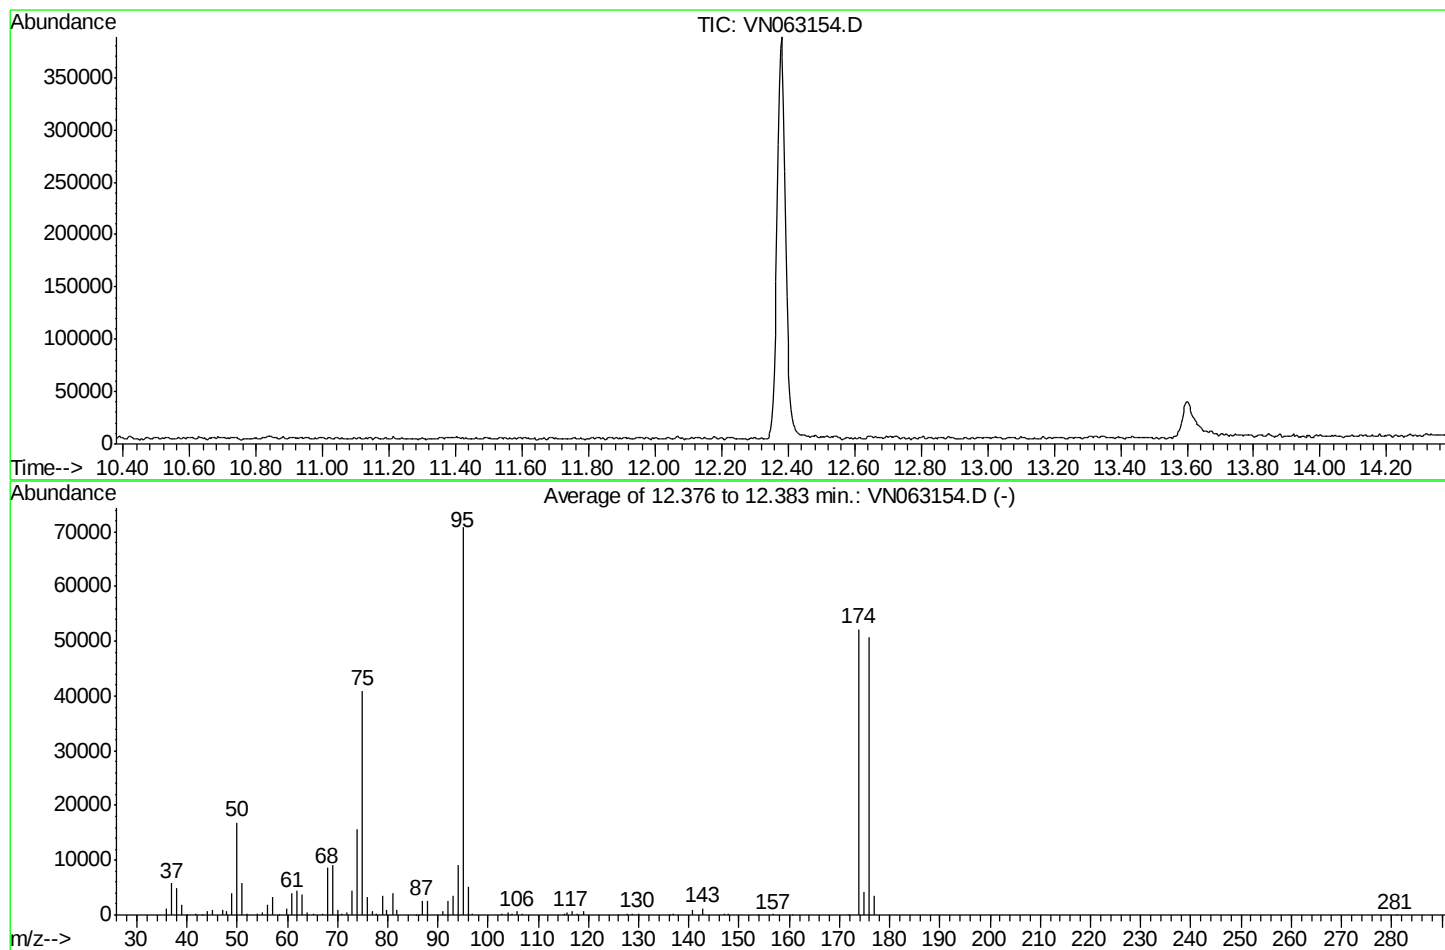

AutoFind: Scans 3308, 3309, 3310; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.9	16957	PASS
75	95	30	60	58.0	41040	PASS
95	95	100	100	100.0	70813	PASS
96	95	5	9	7.4	5257	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.7	52221	PASS
175	174	5	9	8.3	4315	PASS
176	174	95	101	97.1	50693	PASS
177	176	5	9	6.8	3448	PASS