

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090122\
 Data File : VN074265.D
 Acq On : 02 Sep 2022 01:17
 Operator : JC\MD
 Sample : N4376-05
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-45

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083022W.M

Title : SW846 8260

Signal : TIC: VN074265.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.704	132	139	144	rBV10	11350	26400	1.81%	0.329%
2	7.951	1021	1031	1037	rBV	211394	512617	35.18%	6.396%
3	8.016	1037	1042	1060	rVB	325913	733019	50.31%	9.146%
4	8.369	1092	1102	1116	rBV	231284	542742	37.25%	6.772%
5	8.681	1152	1155	1163	rVB4	5953	14856	1.02%	0.185%
6	8.904	1184	1193	1205	rBV	512805	1081365	74.21%	13.492%
7	10.380	1435	1444	1462	rBV	786812	1457074	100.00%	18.179%
8	11.686	1657	1666	1678	rBV	758415	1354402	92.95%	16.898%
9	12.669	1825	1833	1843	rBV	611729	1023695	70.26%	12.772%
10	13.610	1986	1993	2007	rVB	724872	1231472	84.52%	15.365%
11	15.433	2297	2303	2310	rBV2	10699	21789	1.50%	0.272%
12	16.527	2482	2489	2492	rBV5	9432	15597	1.07%	0.195%


Sum of corrected areas: 8015028

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090122\
Data File : VN074265.D
Acq On : 02 Sep 2022 01:17
Operator : JC\MD
Sample : N4376-05
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

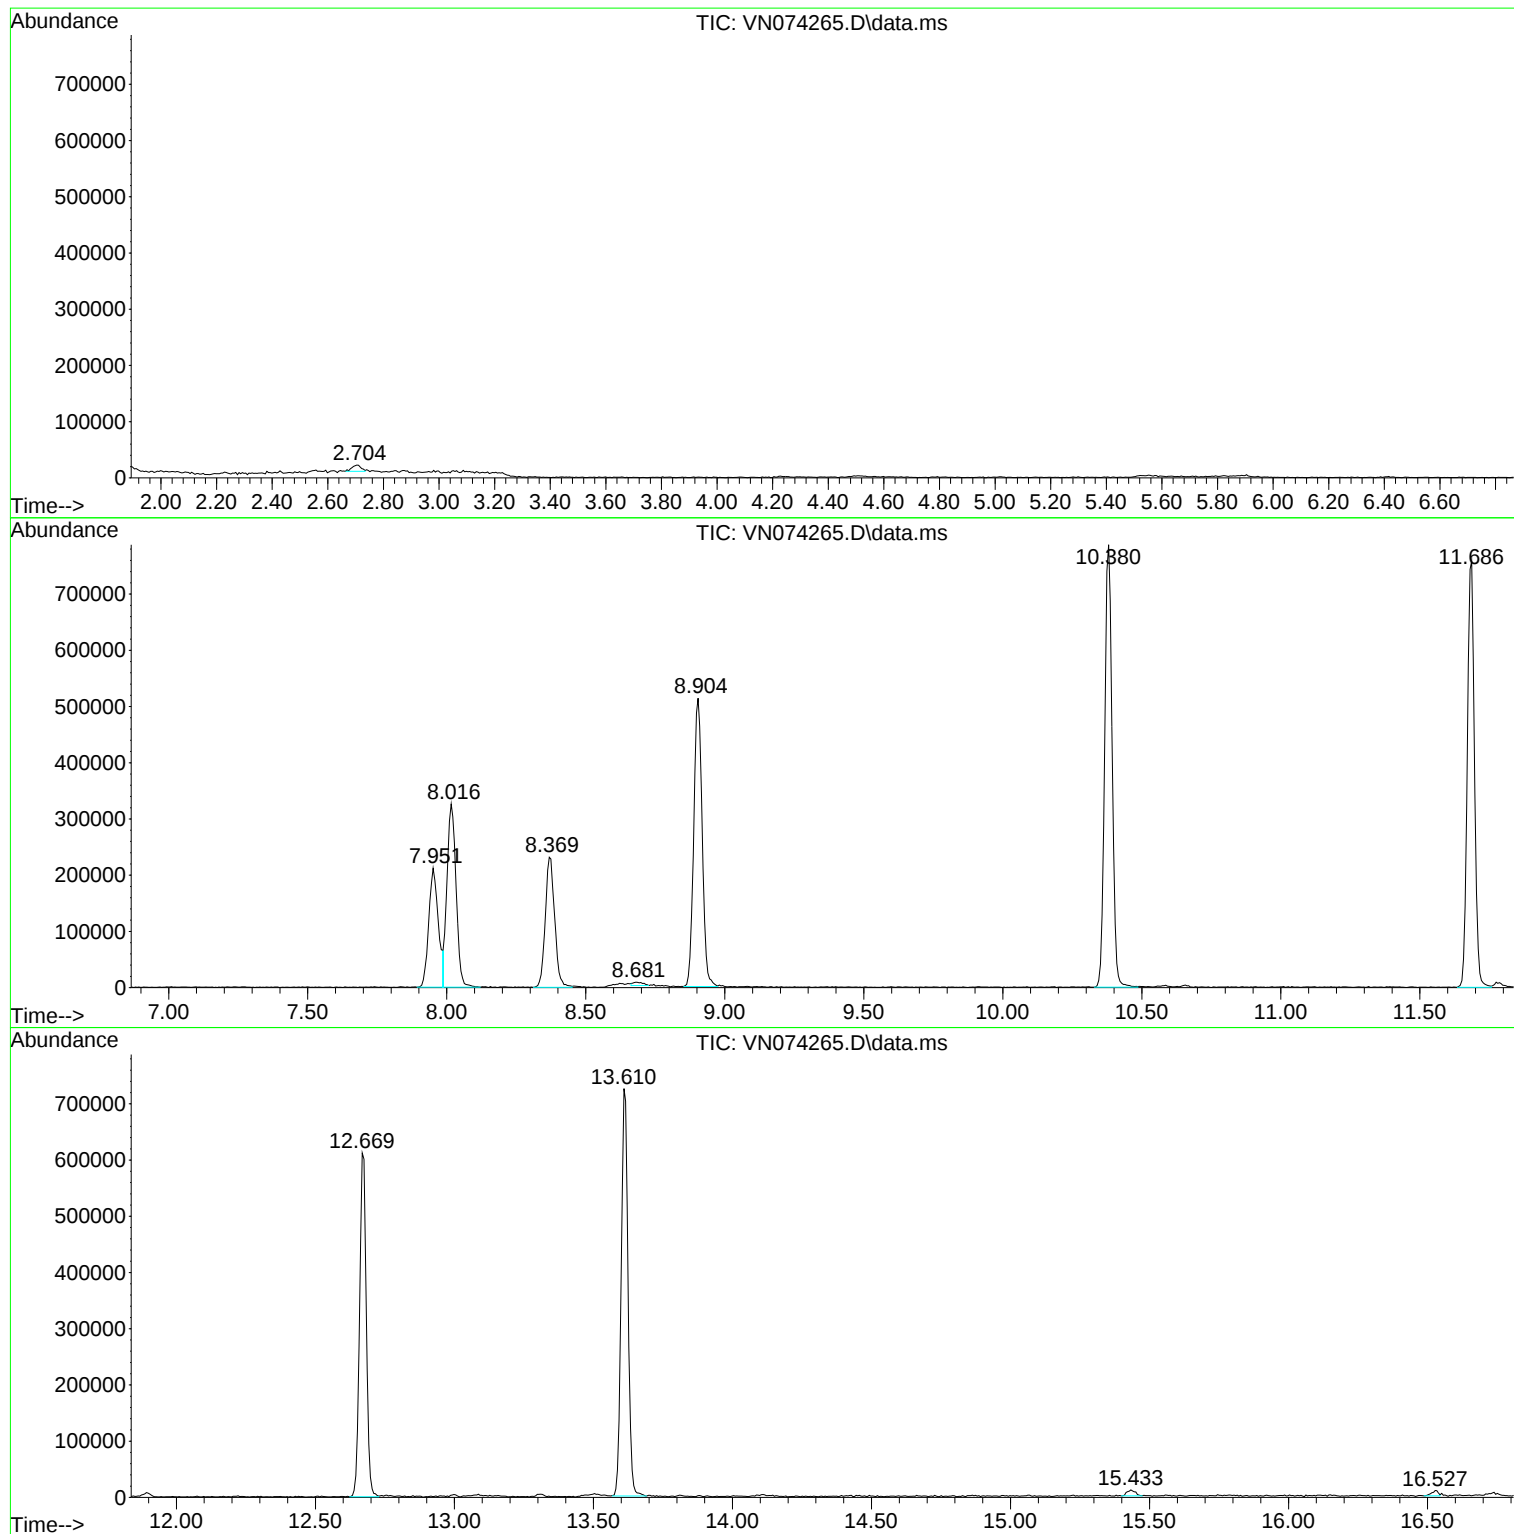

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090122\
Data File : VN074265.D
Acq On : 02 Sep 2022 01:17
Operator : JC\MD
Sample : N4376-05
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090122\
Data File : VN074265.D
Acq On : 02 Sep 2022 01:17
Operator : JC\MD
Sample : N4376-05
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------