


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090122\
Data File : VN074256.D
Acq On : 01 Sep 2022 21:13
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083022W.M
Title : SW846 8260
Last Update : Wed Aug 31 07:02:40 2022

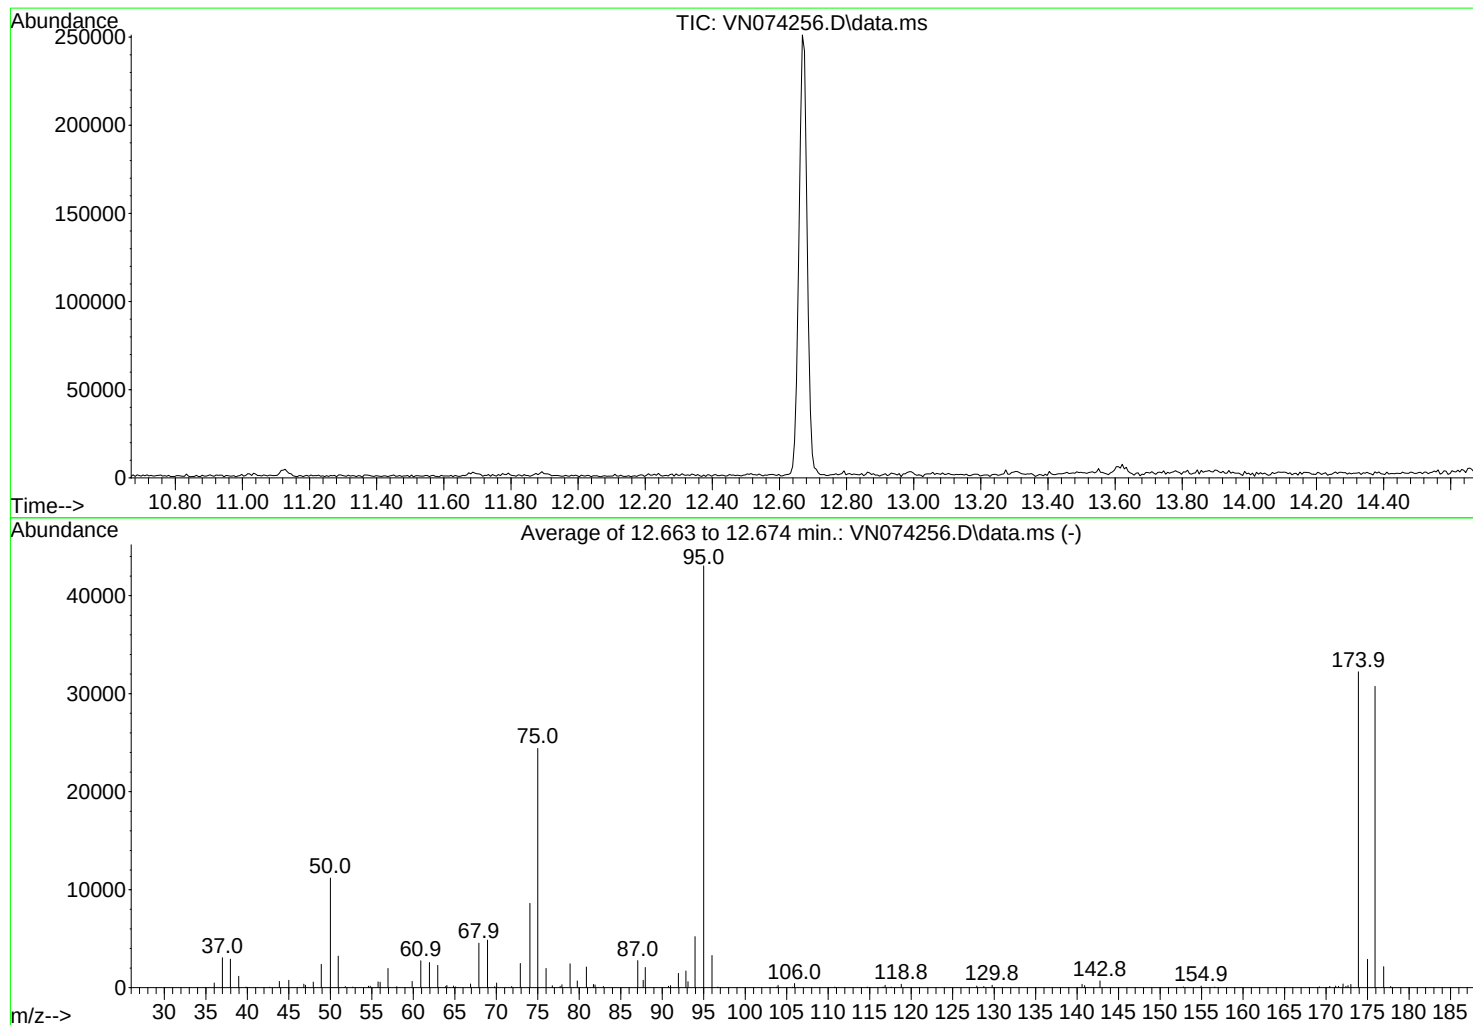

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.0	11190	PASS
75	95	30	60	56.7	24413	PASS
95	95	100	100	100.0	43045	PASS
96	95	5	9	7.6	3287	PASS
173	174	0.00	2	1.0	333	PASS
174	95	50	100	74.9	32240	PASS
175	174	5	9	9.0	2897	PASS
176	174	95	101	95.4	30752	PASS
177	176	5	9	7.0	2138	PASS