


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN090220\
 Data File : VN063181.D
 Acq On : 2 Sep 2020 8:53
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N083120W.M
 Title : SW846 8260
 Last Update : Tue Sep 01 04:21:28 2020

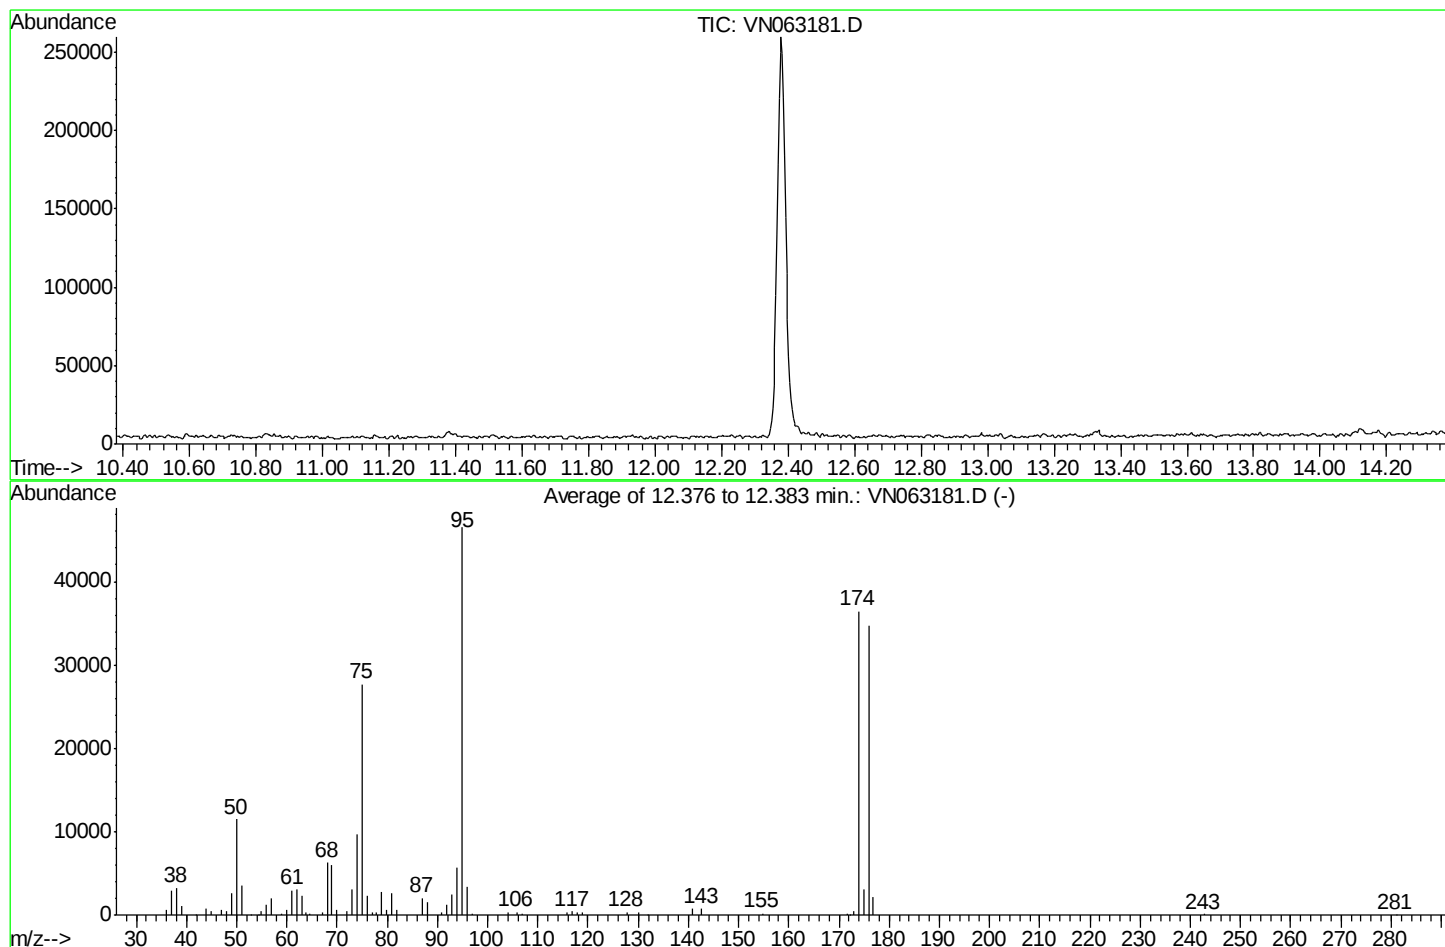

AutoFind: Scans 3308, 3309, 3310; Background Corrected with Scan 3295

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.7	11494	PASS
75	95	30	60	59.5	27672	PASS
95	95	100	100	100.0	46504	PASS
96	95	5	9	7.3	3416	PASS
173	174	0.00	2	1.1	396	PASS
174	95	50	100	78.3	36392	PASS
175	174	5	9	8.4	3072	PASS
176	174	95	101	95.4	34722	PASS
177	176	5	9	6.2	2169	PASS