
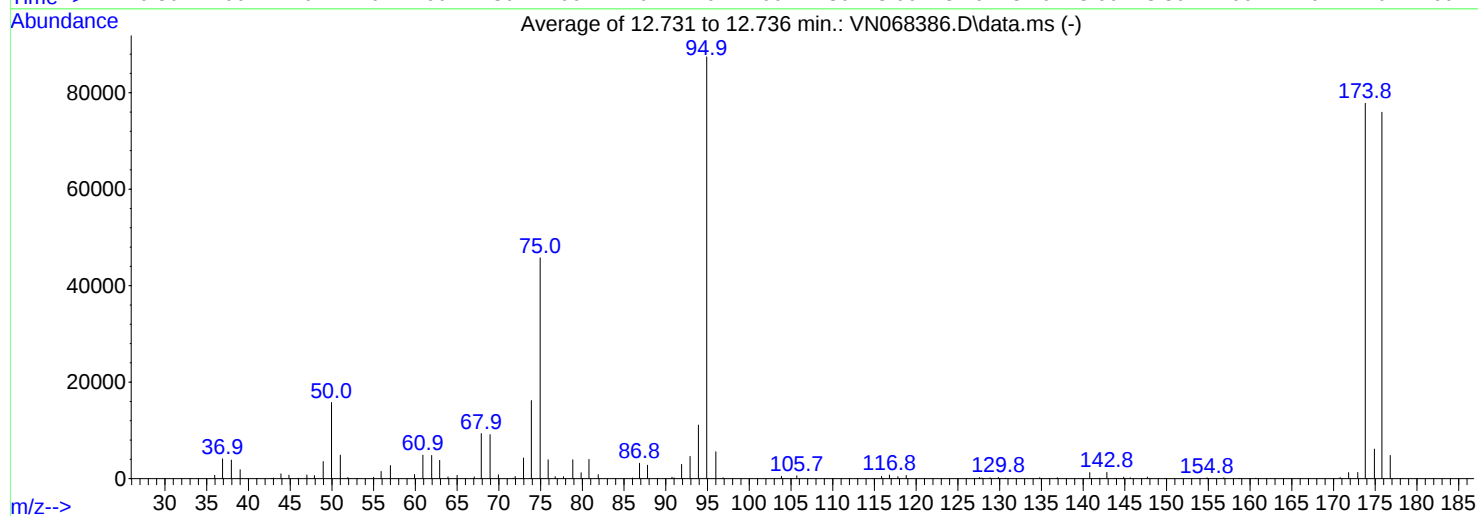


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN090221\  
 Data File : VN068386.D  
 Acq On : 2 Sep 2021 11:55  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N083021W.M  
 Title : SW846 8260  
 Last Update : Thu Sep 02 14:59:33 2021

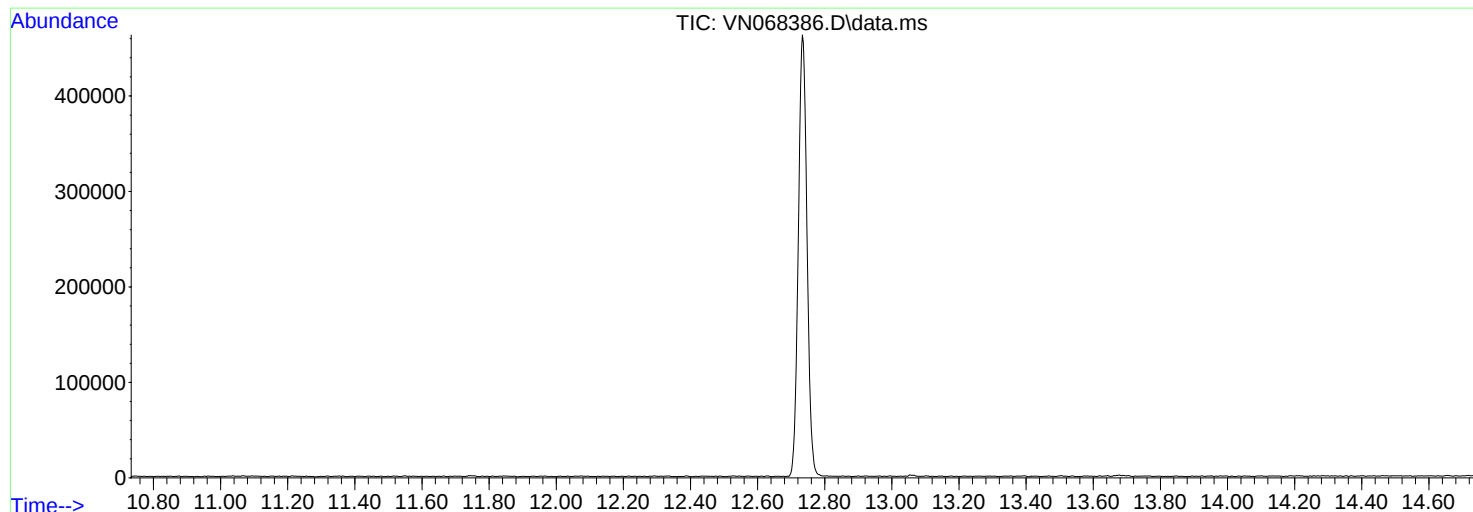

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3989

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 18.0         | 15773      | PASS                |
| 75             | 95              | 30              | 60              | 52.3         | 45765      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 87432      | PASS                |
| 96             | 95              | 5               | 9               | 6.4          | 5588       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.7          | 1294       | PASS                |
| 174            | 95              | 50              | 100             | 89.0         | 77800      | PASS                |
| 175            | 174             | 5               | 9               | 7.9          | 6137       | PASS                |
| 176            | 174             | 95              | 101             | 97.6         | 75939      | PASS                |
| 177            | 176             | 5               | 9               | 6.4          | 4825       | PASS                |