

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090222\
 Data File : VN074302.D
 Acq On : 02 Sep 2022 22:12
 Operator : JC\MD
 Sample : N4354-01DL 10X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-25DL

Quant Time: Sep 03 04:42:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090222W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 03 04:35:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.022	168	232231	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	414461	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	399023	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	189296	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	155747	43.023	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	86.040%
35) Dibromofluoromethane	7.957	113	139441	50.772	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.540%
50) Toluene-d8	10.380	98	481781	44.487	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	88.980%
62) 4-Bromofluorobenzene	12.668	95	182019	46.163	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	92.320%


Target Compounds				Qvalue		
6) Chloroethane	2.693	64	79460	17.089	ug/l #	49
11) Tert butyl alcohol	5.281	59	7745	11.793	ug/l #	93
16) Acetone	4.234	43	1730	1.143	ug/l	92
19) Methyl tert-butyl Ether	5.534	73	95944	10.589	ug/l	100
20) Methylene Chloride	5.010	84	807	Below Cal	#	71
25) 2-Butanone	7.251	43	634	0.248	ug/l #	45
26) 2,2-Dichloropropane	7.239	77	866	0.205	ug/l #	53
31) Cyclohexane	8.016	56	7993	1.653	ug/l #	33
36) 1,1-Dichloropropene	8.010	75	19927	5.112	ug/l #	41
38) Carbon Tetrachloride	8.022	117	23464	5.959	ug/l #	15
40) Benzene	8.392	78	211785	17.223	ug/l	100
42) 1,2-Dichloroethane	8.386	62	2193	0.479	ug/l	82
52) Toluene	10.445	92	159373	20.973	ug/l	99
53) t-1,3-Dichloropropene	10.439	75	2015	0.463	ug/l #	1
67) Ethyl Benzene	11.786	91	300390	18.681	ug/l	96
68) m/p-Xylenes	11.892	106	114573	19.088	ug/l	97
69) o-Xylene	12.216	106	120792	20.163	ug/l	95
70) Styrene	12.216	104	6901	0.719	ug/l #	1
73) Isopropylbenzene	12.521	105	11970	0.722	ug/l	99
76) 1,2,3-Trichloropropane	12.668	75	111208	20.743	ug/l #	1
78) n-propylbenzene	12.857	91	30442	1.607	ug/l	97
79) 2-Chlorotoluene	12.963	91	3039	0.261	ug/l #	40
80) 1,3,5-Trimethylbenzene	12.998	105	23672	1.781	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.668	75	111208	67.337	ug/l #	10
82) 4-Chlorotoluene	12.986	91	3320	0.304	ug/l #	40
83) tert-Butylbenzene	13.304	119	27277	2.261	ug/l #	57
84) 1,2,4-Trimethylbenzene	13.304	105	220032	16.344	ug/l	97
85) sec-Butylbenzene	13.304	105	220032	13.065	ug/l #	56
88) 1,4-Dichlorobenzene	13.627	146	337	0.215	ug/l #	1
90) Hexachloroethane	14.157	117	3150	1.234	ug/l #	9
95) Naphthalene	15.433	128	245624	18.418	ug/l	99
96) 1,2,3-Trichlorobenzene	15.621	180	59	0.429	ug/l #	15


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090222\
Data File : VN074302.D
Acq On : 02 Sep 2022 22:12
Operator : JC\MD
Sample : N4354-01DL 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-25DL

Quant Time: Sep 03 04:42:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090222W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 03 04:35:33 2022
Response via : Initial Calibration




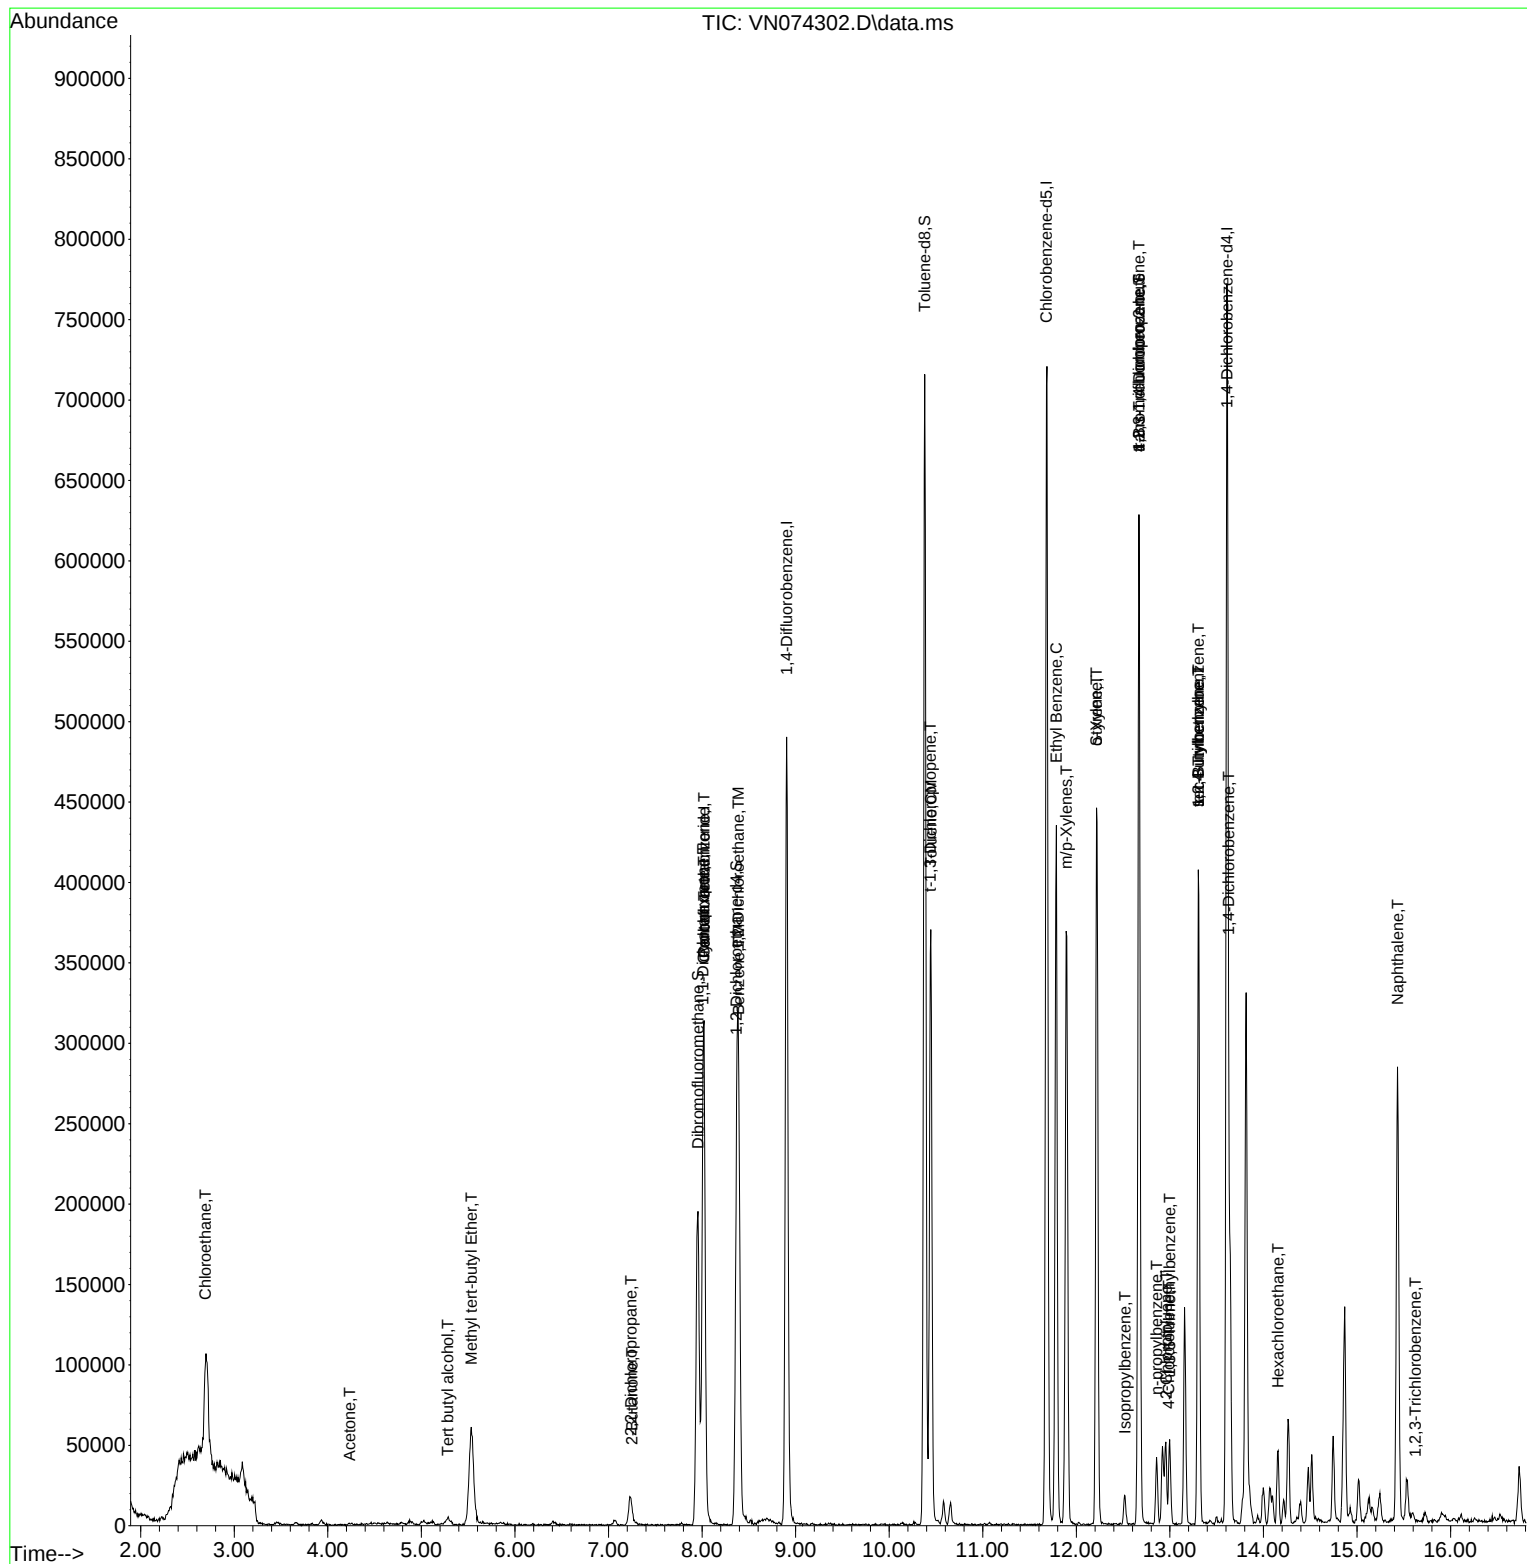




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.022 min Scan# 1043
Delta R.T. 0.006 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12




Instrument :
MSVOA_N
ClientSampleId :
MW-25DL


Tgt Ion:168 Resp: 232231
Ion Ratio Lower Upper
168 100
99 52.9 42.3 63.5

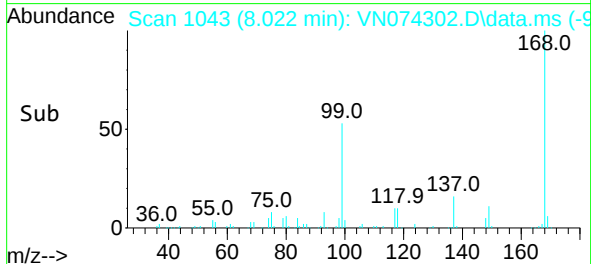

#6
Chloroethane
Concen: 17.089 ug/l
RT: 2.693 min Scan# 137
Delta R.T. -0.258 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12

Tgt Ion: 64 Resp: 79460
Ion Ratio Lower Upper
64 100
66 4.3 26.2 39.4#

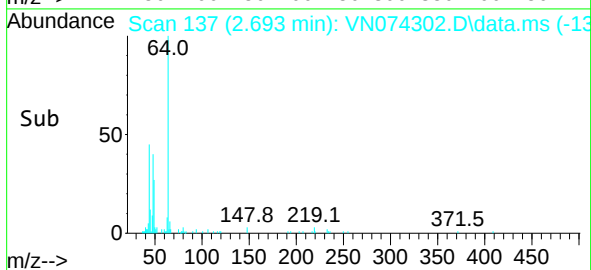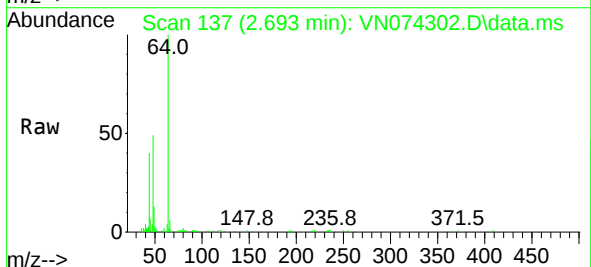



#11

Tert butyl alcohol

Concen: 11.793 ug/l

RT: 5.281 min Scan# 51

Delta R.T. -0.006 min

Lab File: VN074302.D

Acq: 02 Sep 2022 22:12

Instrument :

MSVOA_N

ClientSampleId :





MW-25DL

Tgt Ion: 59 Resp: 7745

Ion Ratio Lower Upper

59 100

57 7.7 8.3 12.5#

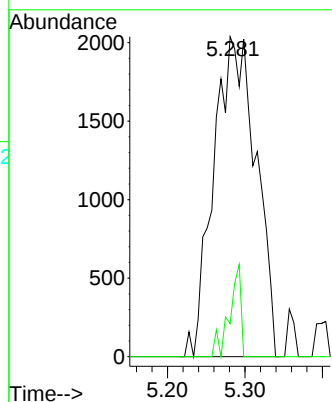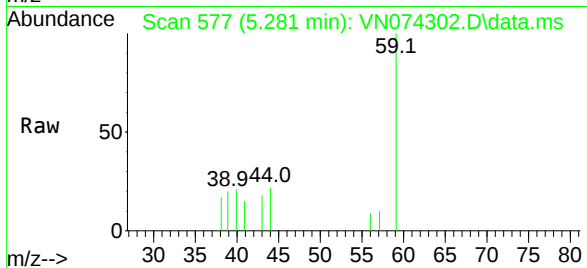

#16

Acetone

Concen: 1.143 ug/l

RT: 4.234 min Scan# 399

Delta R.T. 0.012 min

Lab File: VN074302.D




Acq: 02 Sep 2022 22:12


Tgt Ion: 43 Resp: 1730

Ion Ratio Lower Upper

43 100

58 36.9 26.0 39.0

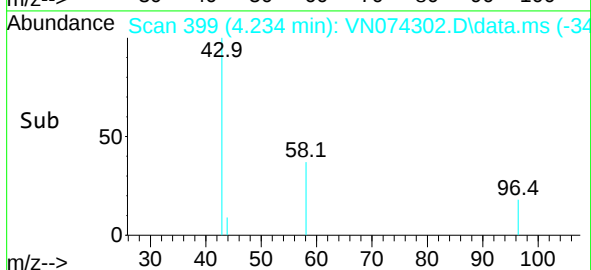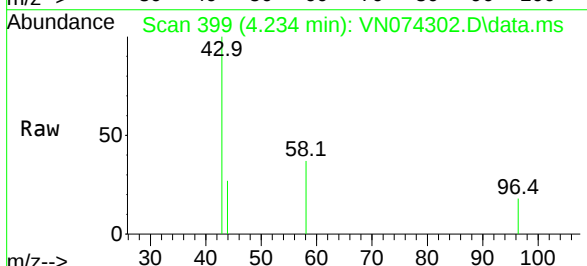



#19

Methyl tert-butyl Ether

Concen: 10.589 ug/l

RT: 5.534 min Scan# 61

Delta R.T. -0.000 min

Lab File: VN074302.D

Acq: 02 Sep 2022 22:12

Instrument :

MSVOA_N

ClientSampleId :





MW-25DL

Tgt Ion: 73 Resp: 95944

Ion Ratio Lower Upper

73 100

57 21.9 17.6 26.4

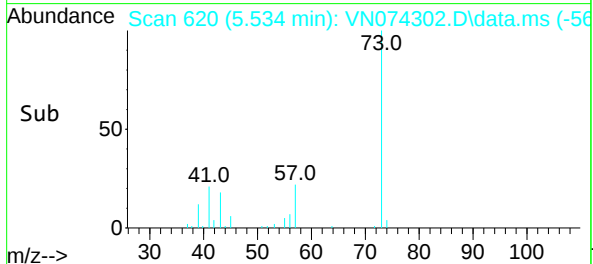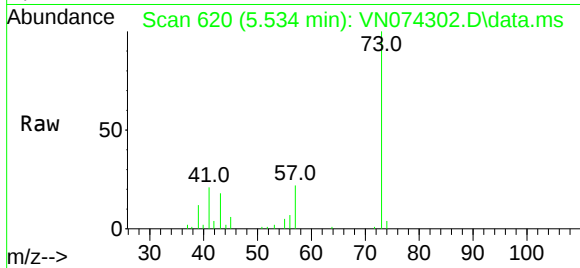

#20

Methylene Chloride

Concen: Below Cal

RT: 5.010 min Scan# 531

Delta R.T. 0.000 min

Lab File: VN074302.D

Acq: 02 Sep 2022 22:12

Tgt Ion: 84 Resp: 807




Ion Ratio Lower Upper


84 100

49 84.3 88.3 132.5#

51 0.0 28.2 42.2#

86 78.9 50.6 76.0#


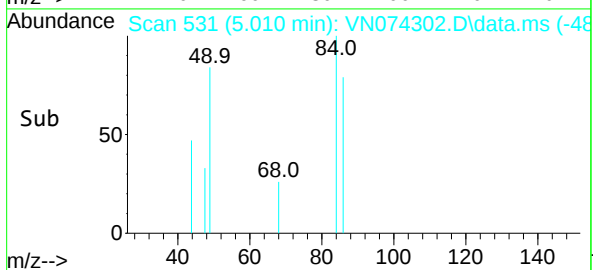

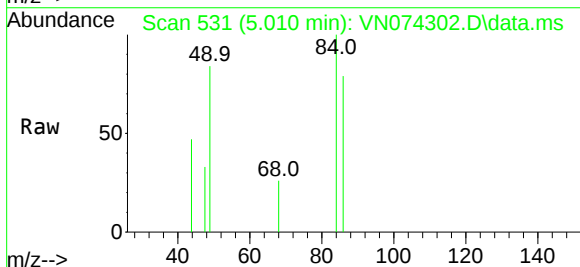




#25
2-Butanone
Concen: 0.248 ug/l
RT: 7.251 min Scan# 910
Delta R.T. -0.006 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12




Instrument :
MSVOA_N
ClientSampleId :
MW-25DL


Tgt Ion: 43 Resp: 634
Ion Ratio Lower Upper
43 100
72 0.0 23.7 35.5#

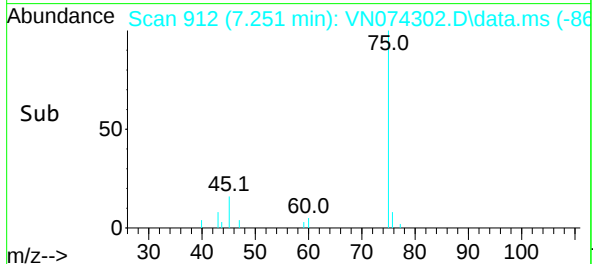

#26
2,2-Dichloropropane
Concen: 0.205 ug/l
RT: 7.239 min Scan# 910
Delta R.T. -0.006 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12

Tgt Ion: 77 Resp: 866
Ion Ratio Lower Upper
77 100
97 0.0 11.4 34.2#

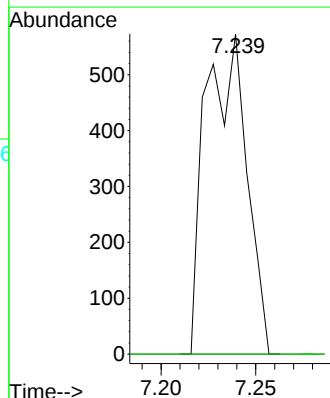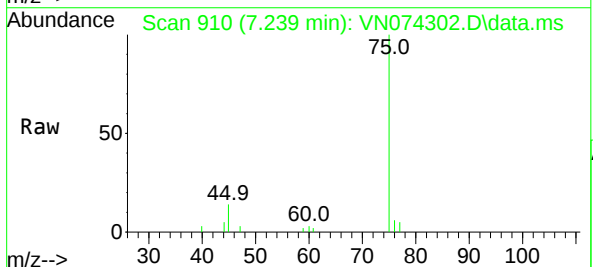

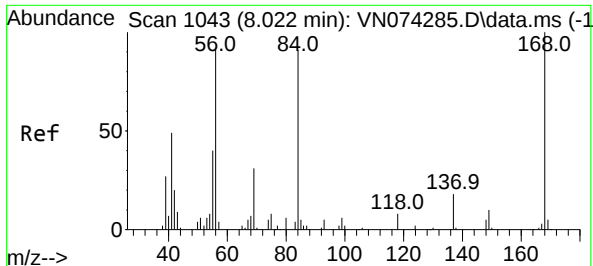

#31

Cyclohexane

Concen: 1.653 ug/l

RT: 8.016 min Scan# 1042

Delta R.T. -0.006 min

Lab File: VN074302.D

Acq: 02 Sep 2022 22:12

Instrument :

MSVOA_N

ClientSampleId :

MW-25DL





Tgt Ion: 56 Resp: 7993

Ion Ratio Lower Upper

56 100

69 153.0 27.8 41.8#

84 113.3 76.9 115.3

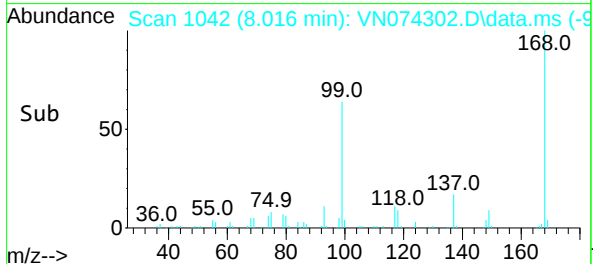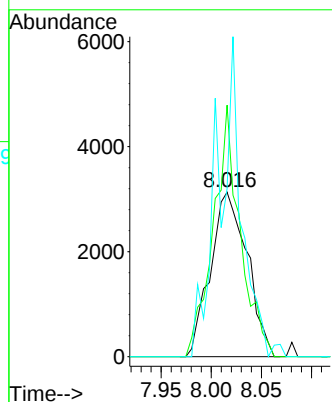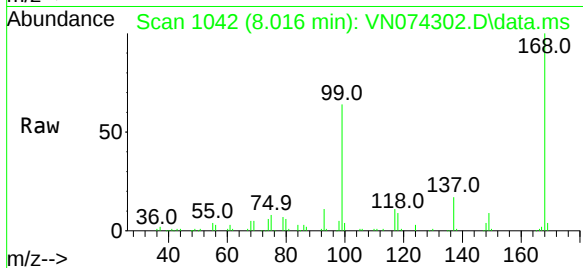

#33

1,2-Dichloroethane-d4

Concen: 43.023 ug/l

RT: 8.369 min Scan# 1102

Delta R.T. -0.000 min

Lab File: VN074302.D




Acq: 02 Sep 2022 22:12


Tgt Ion: 65 Resp: 155747

Ion Ratio Lower Upper

65 100

67 52.9 0.0 104.8

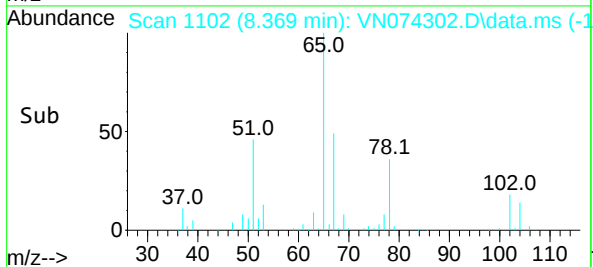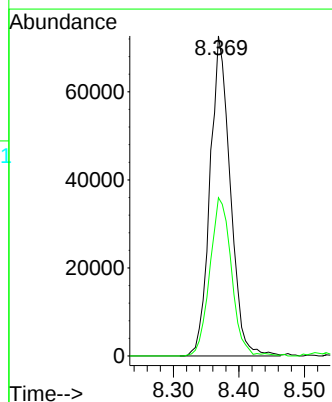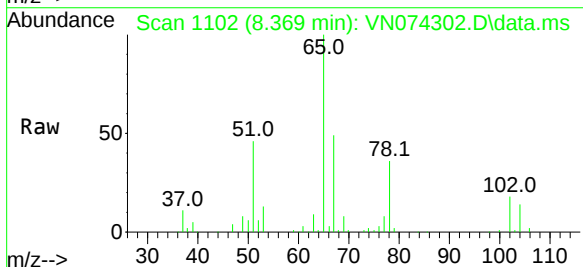

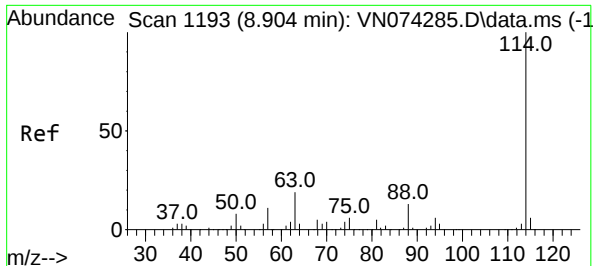

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. -0.000 min

Lab File: VN074302.D

Acq: 02 Sep 2022 22:12

Instrument :

MSVOA_N

ClientSampleId :

MW-25DL





Tgt Ion:114 Resp: 414461

Ion Ratio Lower Upper

114 100

63 19.2 0.0 40.0

88 13.0 0.0 32.6

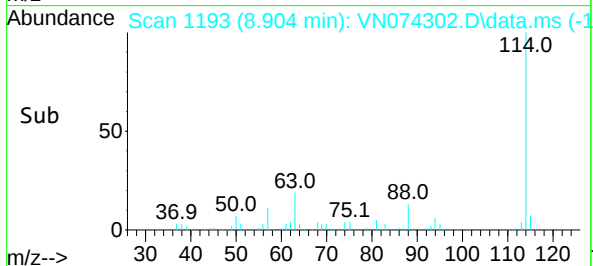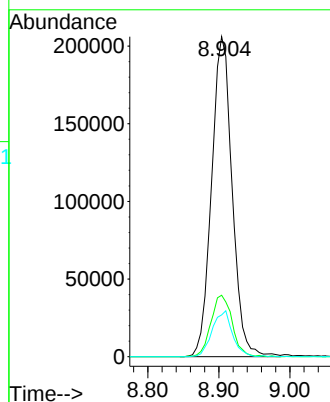

#35

Dibromofluoromethane

Concen: 50.772 ug/l

RT: 7.957 min Scan# 1032

Delta R.T. 0.006 min

Lab File: VN074302.D

Acq: 02 Sep 2022 22:12




Tgt Ion:113 Resp: 139441


Ion Ratio Lower Upper

113 100

111 103.6 81.4 122.0

192 17.5 17.0 25.6

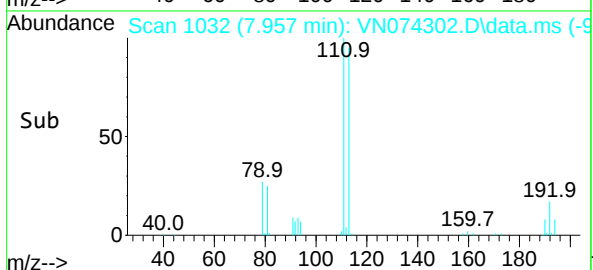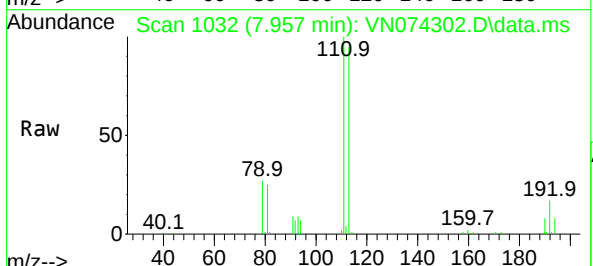

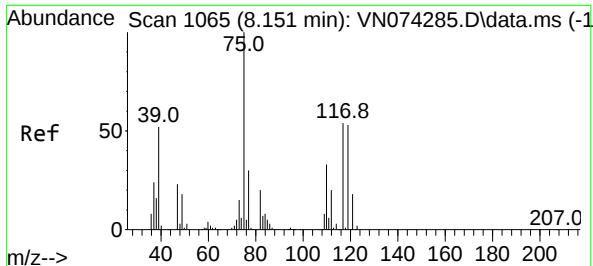

#36

1,1-Dichloropropene

Concen: 5.112 ug/l

RT: 8.010 min Scan# 1041

Delta R.T. -0.147 min

Lab File: VN074302.D

Acq: 02 Sep 2022 22:12

Instrument :

MSVOA_N

ClientSampleId :

MW-25DL





Tgt Ion: 75 Resp: 19927

Ion Ratio Lower Upper

75 100

110 0.0 18.3 54.8#

77 0.0 25.1 37.7#

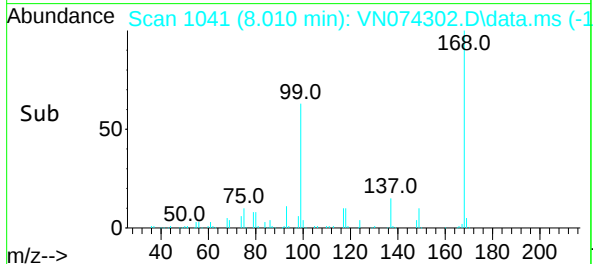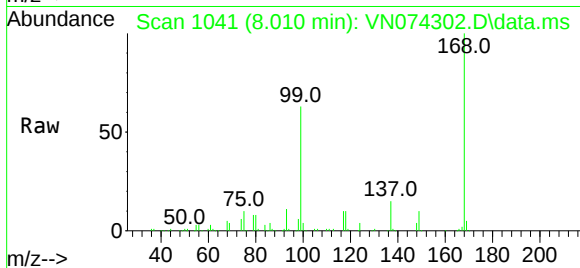

#38

Carbon Tetrachloride

Concen: 5.959 ug/l

RT: 8.022 min Scan# 1043

Delta R.T. -0.111 min

Lab File: VN074302.D

Acq: 02 Sep 2022 22:12




Tgt Ion: 117 Resp: 23464


Ion Ratio Lower Upper

117 100

119 2.8 75.8 113.8#

121 0.0 24.6 37.0#

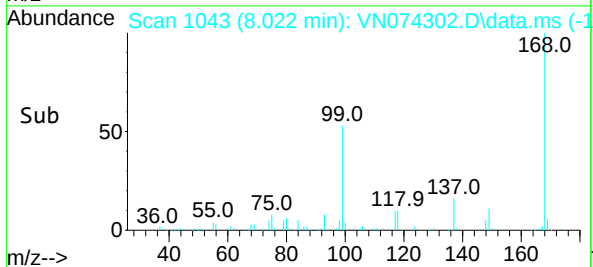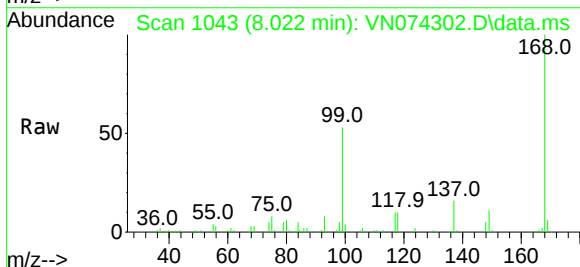



#40

Benzene

Concen: 17.223 ug/l

RT: 8.392 min Scan# 1106

Delta R.T. 0.000 min

Lab File: VN074302.D

Acq: 02 Sep 2022 22:12

Instrument :

MSVOA_N

ClientSampleId :





MW-25DL

Tgt Ion: 78 Resp: 211785

Ion Ratio Lower Upper

78 100

77 24.0 19.4 29.0

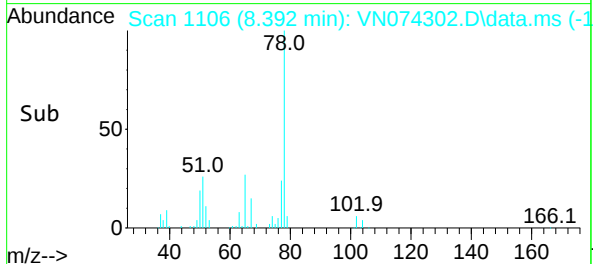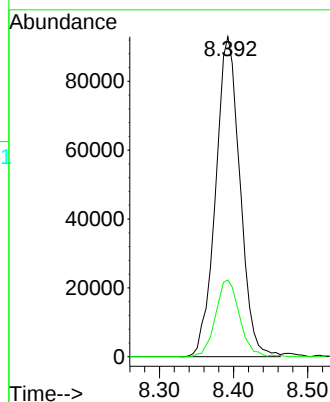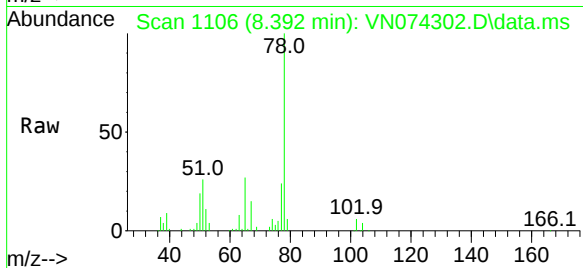

#42

1,2-Dichloroethane

Concen: 0.479 ug/l

RT: 8.386 min Scan# 1105

Delta R.T. -0.077 min

Lab File: VN074302.D




Acq: 02 Sep 2022 22:12


Tgt Ion: 62 Resp: 2193

Ion Ratio Lower Upper

62 100

98 16.3 0.0 19.4


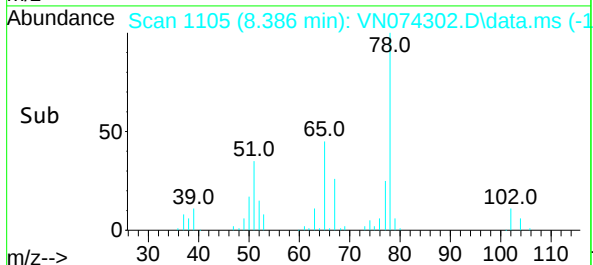

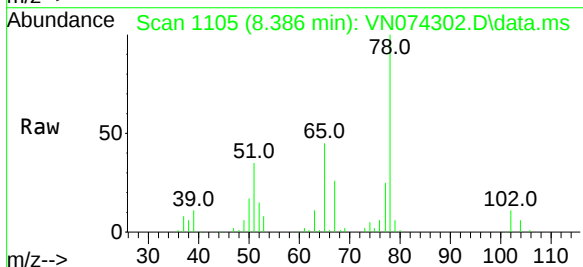




#50
Toluene-d8
Concen: 44.487 ug/l
RT: 10.380 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12




Instrument :
MSVOA_N
ClientSampleId :
MW-25DL


Tgt Ion: 98 Resp: 481781
Ion Ratio Lower Upper
98 100
100 64.4 52.6 78.8

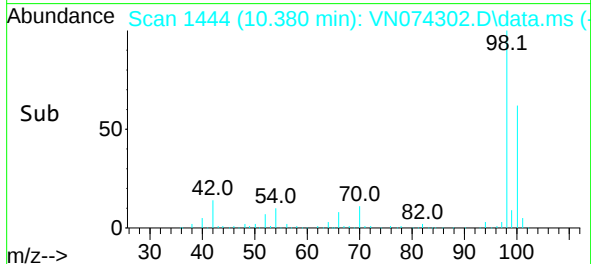

#52
Toluene
Concen: 20.973 ug/l
RT: 10.445 min Scan# 1455
Delta R.T. 0.000 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12

Tgt Ion: 92 Resp: 159373
Ion Ratio Lower Upper
92 100
91 171.8 138.6 207.8


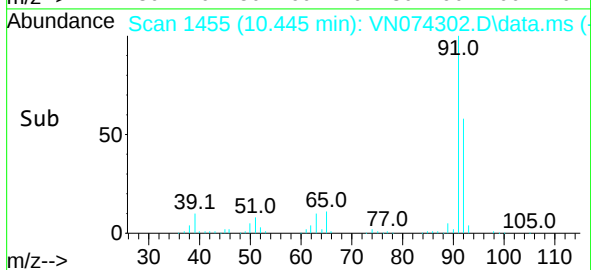

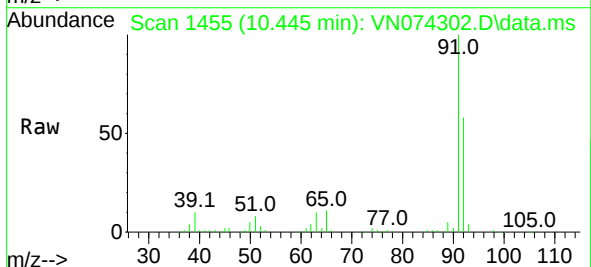




#53
t-1,3-Dichloropropene
Concen: 0.463 ug/l
RT: 10.439 min Scan# 1454
Delta R.T. -0.224 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12




Instrument :
MSVOA_N
ClientSampleId :
MW-25DL


Tgt Ion: 75 Resp: 2015
Ion Ratio Lower Upper
75 100
77 168.8 25.6 38.4#

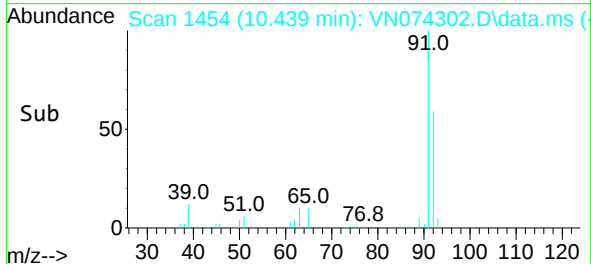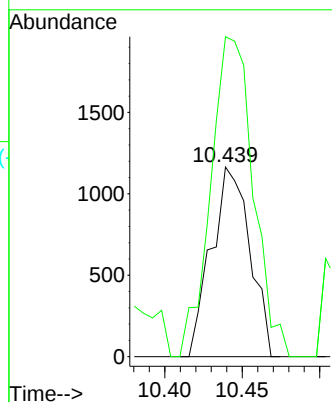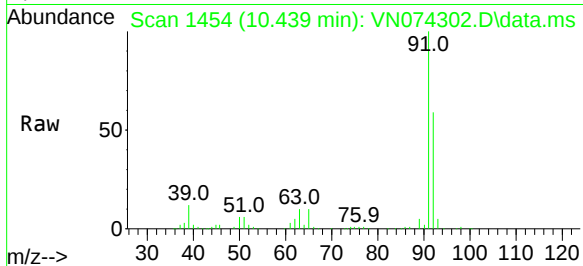

#62
4-Bromofluorobenzene
Concen: 46.163 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. -0.001 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12

Tgt Ion: 95 Resp: 182019
Ion Ratio Lower Upper
95 100
174 83.6 0.0 167.6
176 78.6 0.0 163.4


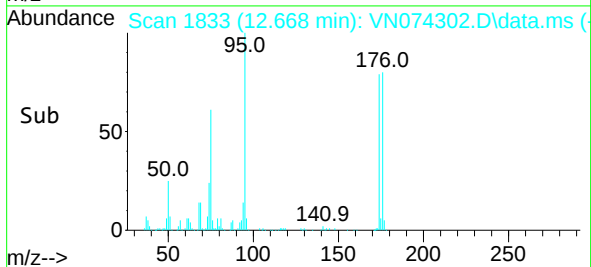

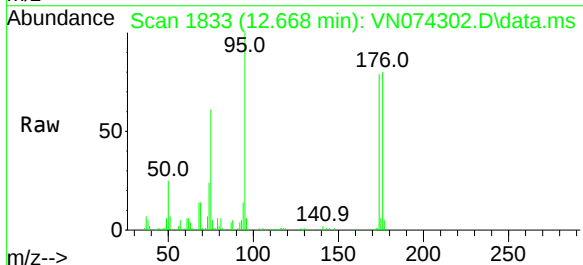




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.680 min Scan# 1
Delta R.T. -0.006 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12




Instrument :
MSVOA_N
ClientSampleId :
MW-25DL


Tgt Ion:117 Resp: 399023
Ion Ratio Lower Upper
117 100
82 55.4 44.2 66.2
119 29.8 25.4 38.0

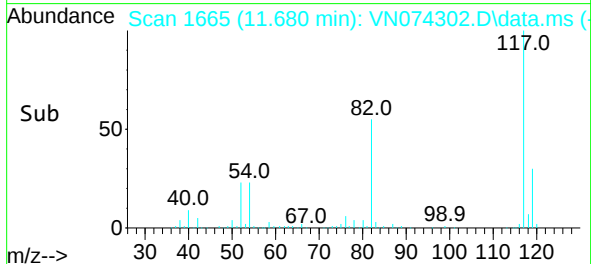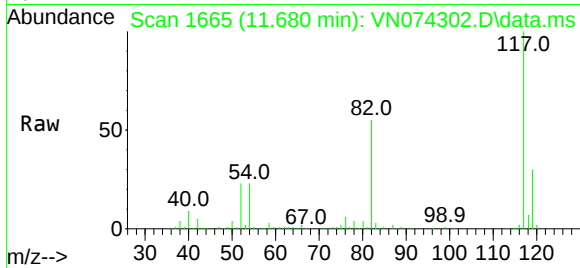

#67
Ethyl Benzene
Concen: 18.681 ug/l
RT: 11.786 min Scan# 1683
Delta R.T. 0.000 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12

Tgt Ion: 91 Resp: 300390
Ion Ratio Lower Upper
91 100
106 29.0 24.9 37.3


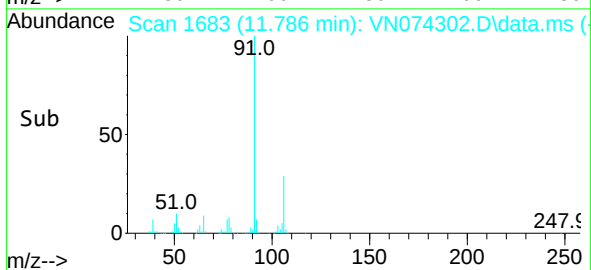

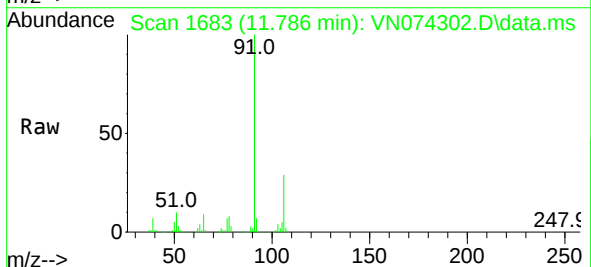




#68
m/p-Xylenes
Concen: 19.088 ug/l
RT: 11.892 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12




Instrument :
MSVOA_N
ClientSampleId :
MW-25DL


Tgt Ion:106 Resp: 114573
Ion Ratio Lower Upper
106 100
91 203.5 158.9 238.3

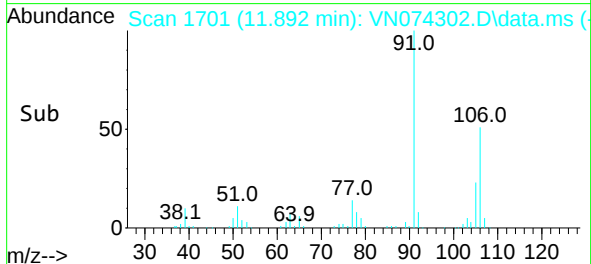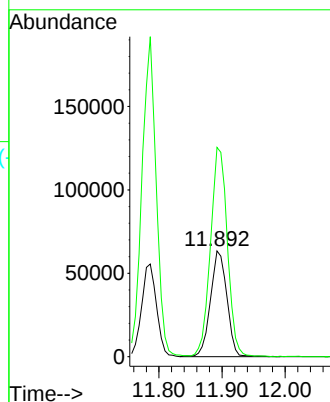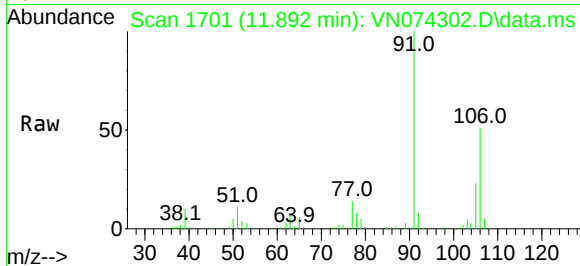

#69
o-Xylene
Concen: 20.163 ug/l
RT: 12.216 min Scan# 1756
Delta R.T. -0.005 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12

Tgt Ion:106 Resp: 120792
Ion Ratio Lower Upper
106 100
91 219.2 106.0 318.0

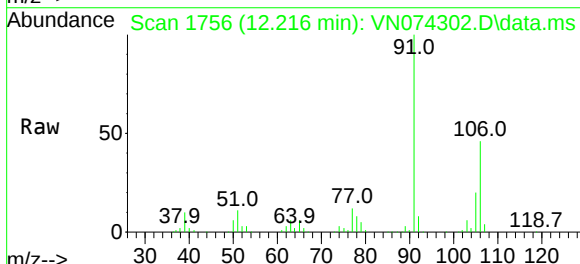



#70

Styrene

Concen: 0.719 ug/l

RT: 12.216 min Scan# 1

Delta R.T. -0.018 min

Lab File: VN074302.D

Acq: 02 Sep 2022 22:12

Instrument :

MSVOA_N

ClientSampleId :

MW-25DL





Tgt Ion:104 Resp: 6901

Ion Ratio Lower Upper

104 100

78 285.1 39.5 59.3#

103 243.1 44.0 66.0#

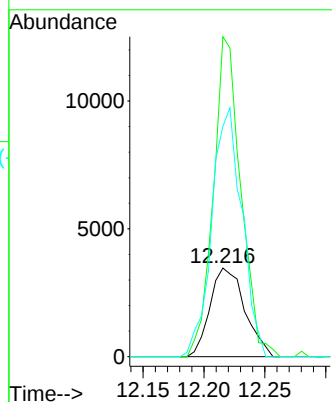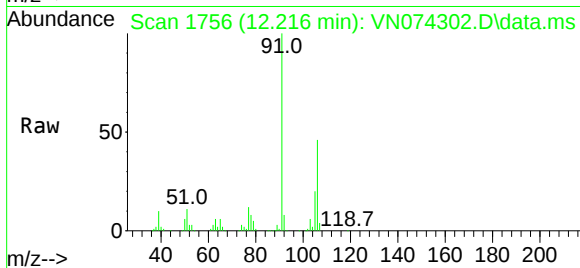

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.610 min Scan# 1993

Delta R.T. -0.000 min

Lab File: VN074302.D

Acq: 02 Sep 2022 22:12




Tgt Ion:152 Resp: 189296


Ion Ratio Lower Upper

152 100

115 60.3 28.9 86.7

150 158.3 0.0 356.2


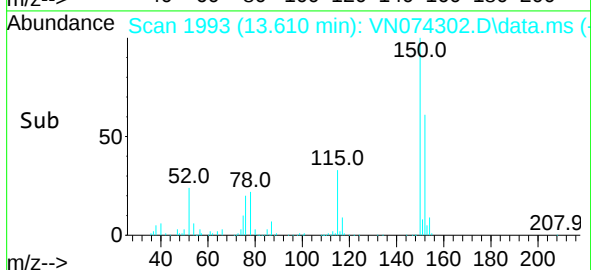

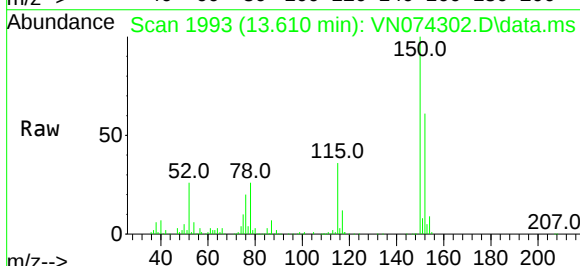




#73
Isopropylbenzene
Concen: 0.722 ug/l
RT: 12.521 min Scan# 1808
Delta R.T. 0.005 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12




Instrument :
MSVOA_N
ClientSampleId :
MW-25DL


Tgt Ion:105 Resp: 11970
Ion Ratio Lower Upper
105 100
120 26.4 13.5 40.4

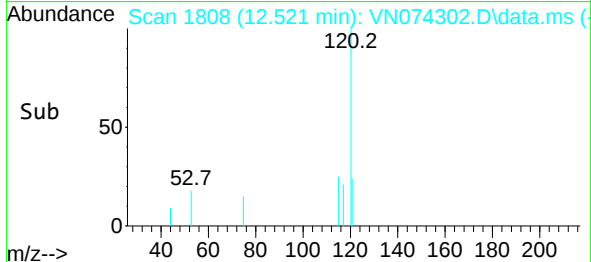

#76
1,2,3-Trichloropropane
Concen: 20.743 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. -0.153 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12

Tgt Ion: 75 Resp: 111208
Ion Ratio Lower Upper
75 100
77 1.7 98.5 295.5#


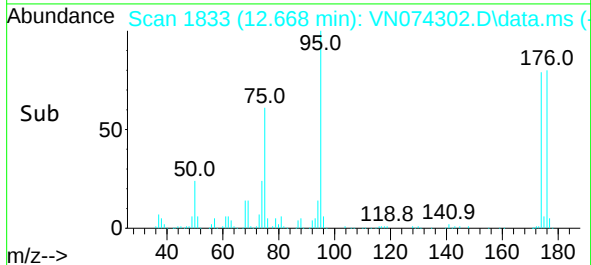

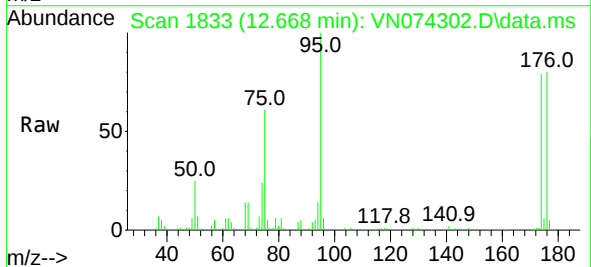




#78
n-propylbenzene
Concen: 1.607 ug/l
RT: 12.857 min Scan# 1865
Delta R.T. -0.006 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12




Instrument :
MSVOA_N
ClientSampleId :
MW-25DL


Tgt Ion: 91 Resp: 30442
Ion Ratio Lower Upper
91 100
120 22.2 11.9 35.5

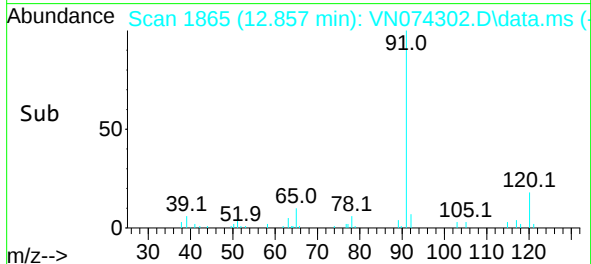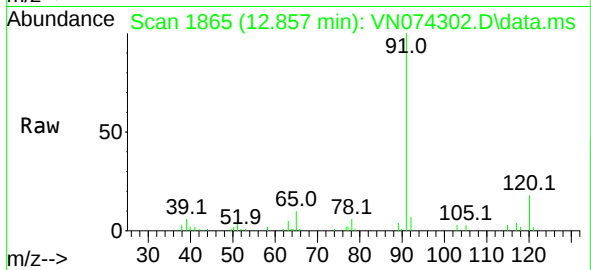

#79
2-Chlorotoluene
Concen: 0.261 ug/l
RT: 12.963 min Scan# 1883
Delta R.T. 0.018 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12

Tgt Ion: 91 Resp: 3039
Ion Ratio Lower Upper
91 100
126 0.0 17.3 51.9#

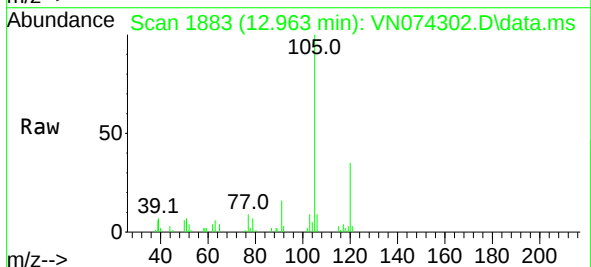

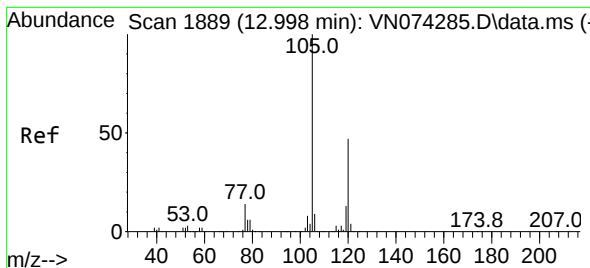

#80

1,3,5-Trimethylbenzene

Concen: 1.781 ug/l

RT: 12.998 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN074302.D

Acq: 02 Sep 2022 22:12

Instrument :

MSVOA_N

ClientSampleId :





MW-25DL

Tgt Ion:105 Resp: 23672

Ion Ratio Lower Upper

105 100

120 51.7 24.9 74.7

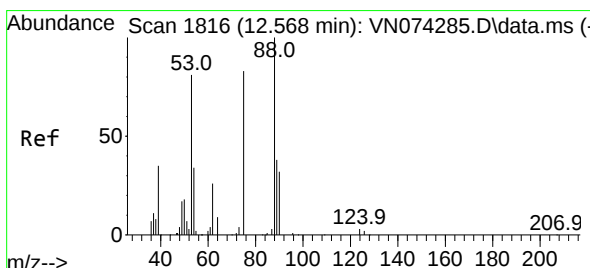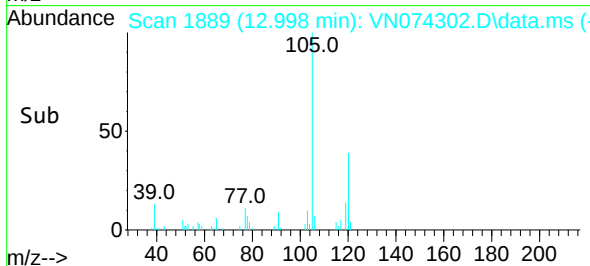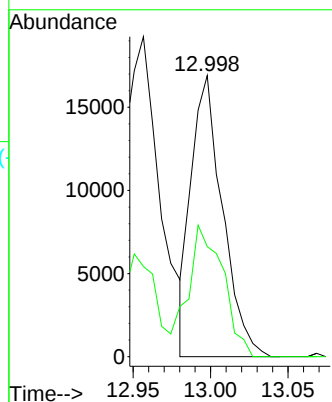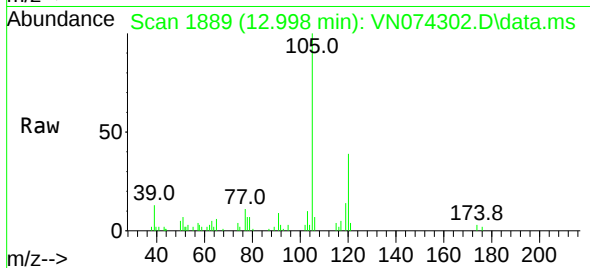

#81

trans-1,4-Dichloro-2-butene

Concen: 67.337 ug/l

RT: 12.668 min Scan# 1833

Delta R.T. 0.105 min

Lab File: VN074302.D

Acq: 02 Sep 2022 22:12




Tgt Ion: 75 Resp: 111208


Ion Ratio Lower Upper

75 100

53 0.0 78.0 117.0#

89 0.1 37.2 55.8#


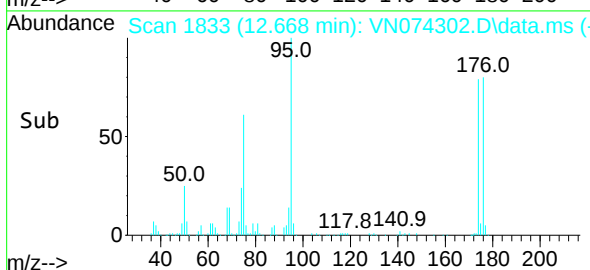

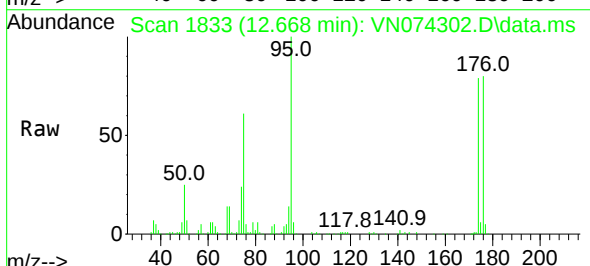


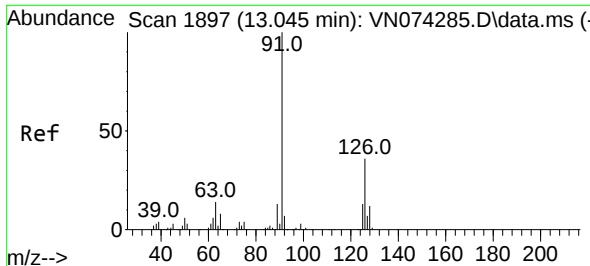

#82
4-Chlorotoluene
Concen: 0.304 ug/l
RT: 12.986 min Scan# 11
Delta R.T. -0.059 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12




Instrument :
MSVOA_N
ClientSampleId :
MW-25DL


Tgt Ion: 91 Resp: 3320
Ion Ratio Lower Upper
91 100
126 0.0 17.2 51.6#

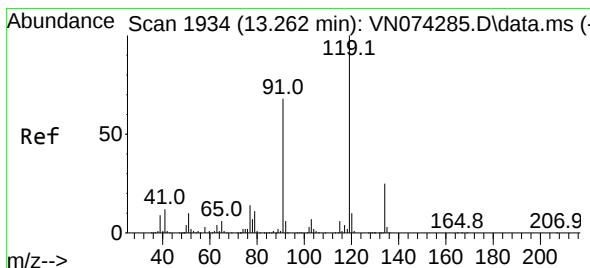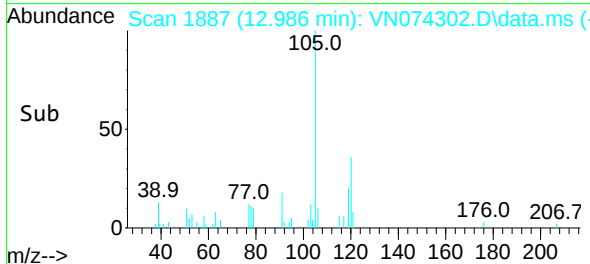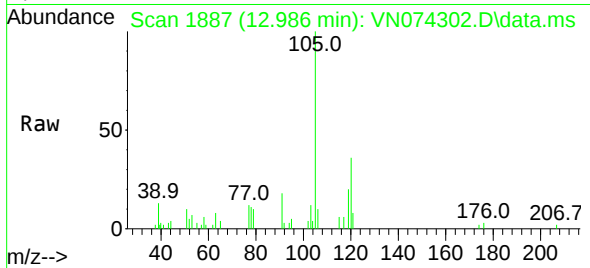

#83
tert-Butylbenzene
Concen: 2.261 ug/l
RT: 13.304 min Scan# 1941
Delta R.T. 0.041 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12

Tgt Ion: 119 Resp: 27277
Ion Ratio Lower Upper
119 100
91 93.2 31.6 94.8
134 0.3 13.7 41.1#


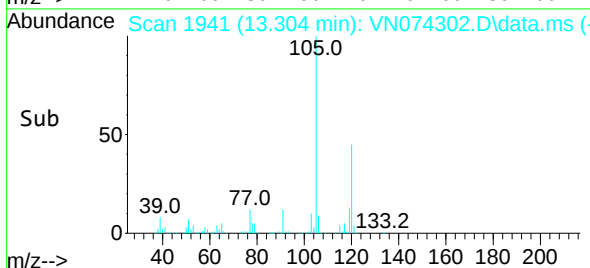
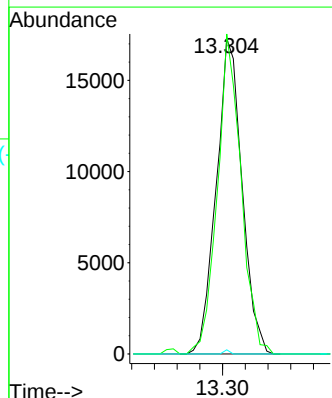
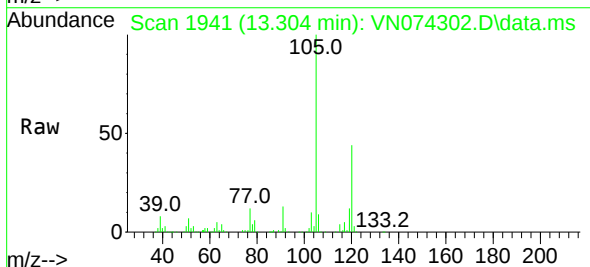




#84
1,2,4-Trimethylbenzene
Concen: 16.344 ug/l
RT: 13.304 min Scan# 1941
Delta R.T. -0.006 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12




Instrument :
MSVOA_N
ClientSampleId :
MW-25DL


Tgt Ion:105 Resp: 220032
Ion Ratio Lower Upper
105 100
120 44.5 23.3 69.8

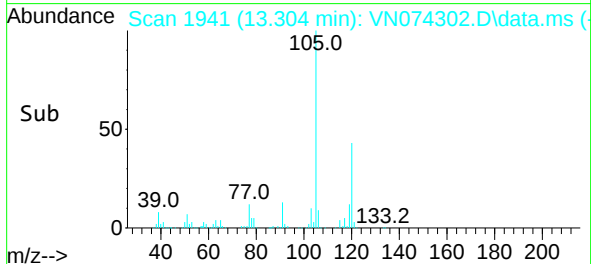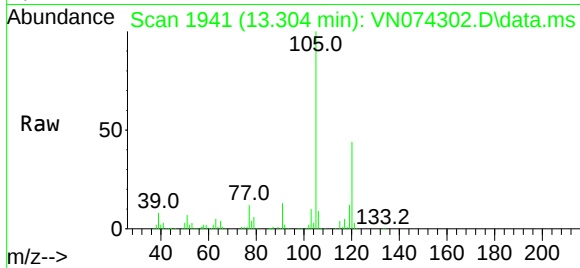

#85
sec-Butylbenzene
Concen: 13.065 ug/l
RT: 13.304 min Scan# 1941
Delta R.T. -0.135 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12

Tgt Ion:105 Resp: 220032
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#




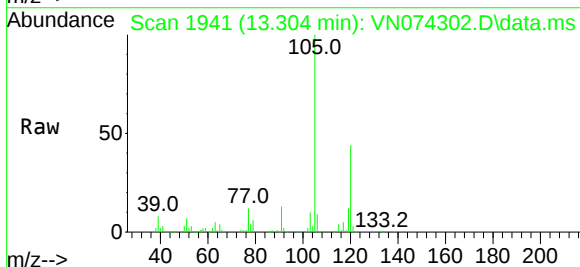




#88
1,4-Dichlorobenzene
Concen: 0.215 ug/l
RT: 13.627 min Scan# 1996
Delta R.T. -0.006 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12




Instrument :
MSVOA_N
ClientSampleId :
MW-25DL


Tgt Ion:146 Resp: 337
Ion Ratio Lower Upper
146 100
111 874.2 19.1 57.1#
148 384.6 31.4 94.3#

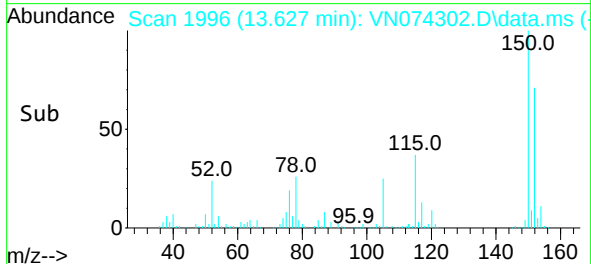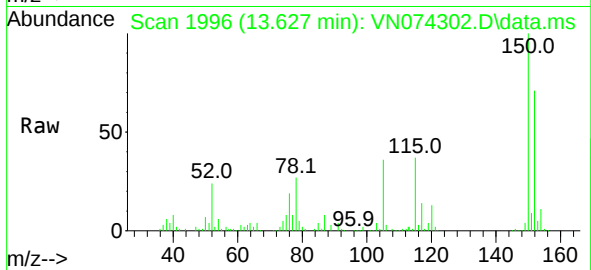

#90
Hexachloroethane
Concen: 1.234 ug/l
RT: 14.157 min Scan# 2086
Delta R.T. 0.006 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12

Tgt Ion:117 Resp: 3150
Ion Ratio Lower Upper
117 100
201 0.0 40.6 122.0#




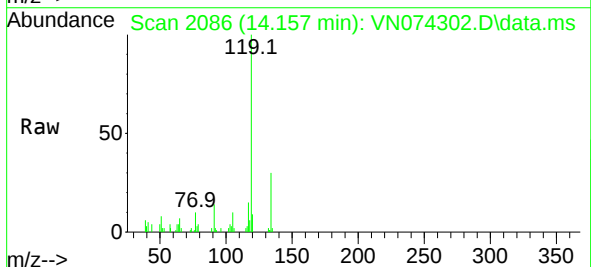




#95
Naphthalene
Concen: 18.418 ug/l
RT: 15.433 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12

Instrument :
MSVOA_N
ClientSampleId :
MW-25DL

Tgt Ion:128 Resp: 245624
Ion Ratio Lower Upper
128 100
127 13.3 10.3 15.5
129 10.2 8.6 13.0

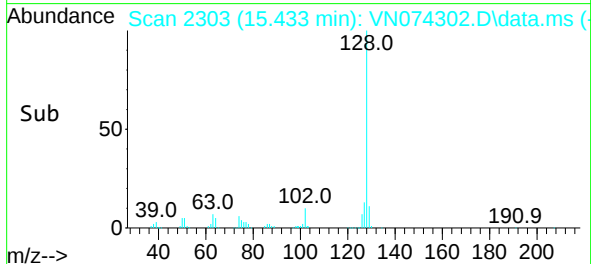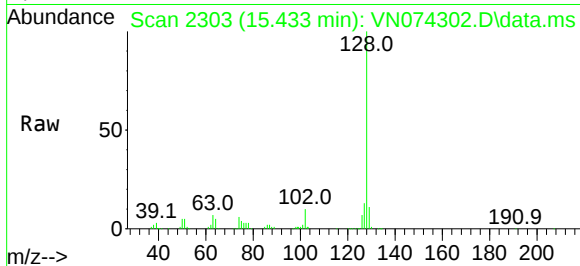

#96
1,2,3-Trichlorobenzene
Concen: 0.429 ug/l
RT: 15.621 min Scan# 2335
Delta R.T. -0.006 min
Lab File: VN074302.D
Acq: 02 Sep 2022 22:12

Tgt Ion:180 Resp: 59
Ion Ratio Lower Upper
180 100
182 135.6 47.8 143.3
145 152.5 15.5 46.5#

