

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090222\
 Data File : VN074313.D
 Acq On : 03 Sep 2022 02:40
 Operator : JC\MD
 Sample : N4355-09
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-35

Quant Time: Sep 03 07:09:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090222W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 03 04:35:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	327393	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	599605	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	564137	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	261043	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	231348	45.331	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	90.660%		
35) Dibromofluoromethane	7.951	113	194690	49.000	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	98.000%		
50) Toluene-d8	10.380	98	678420	43.301	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	86.600%		
62) 4-Bromofluorobenzene	12.668	95	256092	44.973	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	89.940%		
Target Compounds						Qvalue
3) Chloromethane	2.275	50	2422	0.541	ug/l #	74
6) Chloroethane	2.693	64	76159	11.618	ug/l #	51
10) Methyl Iodide	4.345	142	58	5.063	ug/l #	44
11) Tert butyl alcohol	5.281	59	98558	106.447	ug/l	99
15) Acrylonitrile	5.522	53	676	0.265	ug/l #	27
16) Acetone	4.234	43	6925	3.247	ug/l #	77
18) Methyl Acetate	4.781	43	1819	0.283	ug/l #	59
19) Methyl tert-butyl Ether	5.534	73	98376	7.702	ug/l	100
20) Methylene Chloride	5.004	84	111	Below Cal	#	38
22) Diisopropyl ether	6.416	45	17302	1.422	ug/l #	84
23) Vinyl Acetate	6.416	43	11231	1.062	ug/l #	68
25) 2-Butanone	7.257	43	1434	0.398	ug/l #	78
31) Cyclohexane	8.022	56	18683	2.741	ug/l #	76
36) 1,1-Dichloropropene	8.016	75	29567	5.243	ug/l #	49
38) Carbon Tetrachloride	8.016	117	33577	5.894	ug/l #	15
39) Methylcyclohexane	9.398	83	2773	0.408	ug/l #	78
40) Benzene	8.392	78	1196628	67.265	ug/l	100
42) 1,2-Dichloroethane	8.386	62	11094	1.676	ug/l	82
43) Isopropyl Acetate	8.463	43	3255	0.304	ug/l #	53
52) Toluene	10.439	92	5638	0.513	ug/l	95
59) 2-Hexanone	11.074	43	2389	0.421	ug/l	82
67) Ethyl Benzene	11.780	91	70789	3.114	ug/l	95
68) m/p-Xylenes	11.886	106	16506	1.945	ug/l	96
69) o-Xylene	12.227	106	2461	0.291	ug/l	88
73) Isopropylbenzene	12.515	105	20497	0.897	ug/l	99
76) 1,2,3-Trichloropropane	12.668	75	149732	20.252	ug/l #	1
78) n-propylbenzene	12.862	91	21504	0.823	ug/l	98
80) 1,3,5-Trimethylbenzene	12.992	105	3866	0.211	ug/l	93
81) trans-1,4-Dichloro-2-b...	12.668	75	149732	65.745	ug/l #	11
84) 1,2,4-Trimethylbenzene	13.310	105	18291	0.985	ug/l	94
90) Hexachloroethane	14.215	117	3661	1.040	ug/l #	9
93) 1,2,4-Trichlorobenzene	15.204	180	71	0.869	ug/l #	1
95) Naphthalene	15.433	128	44106	3.062	ug/l #	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

MSVOA_N


ClientSampleId :


MW-35

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090222\
Data File : VN074313.D
Acq On : 03 Sep 2022 02:40
Operator : JC\MD
Sample : N4355-09
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-35

Quant Time: Sep 03 07:09:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090222W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 03 04:35:33 2022
Response via : Initial Calibration




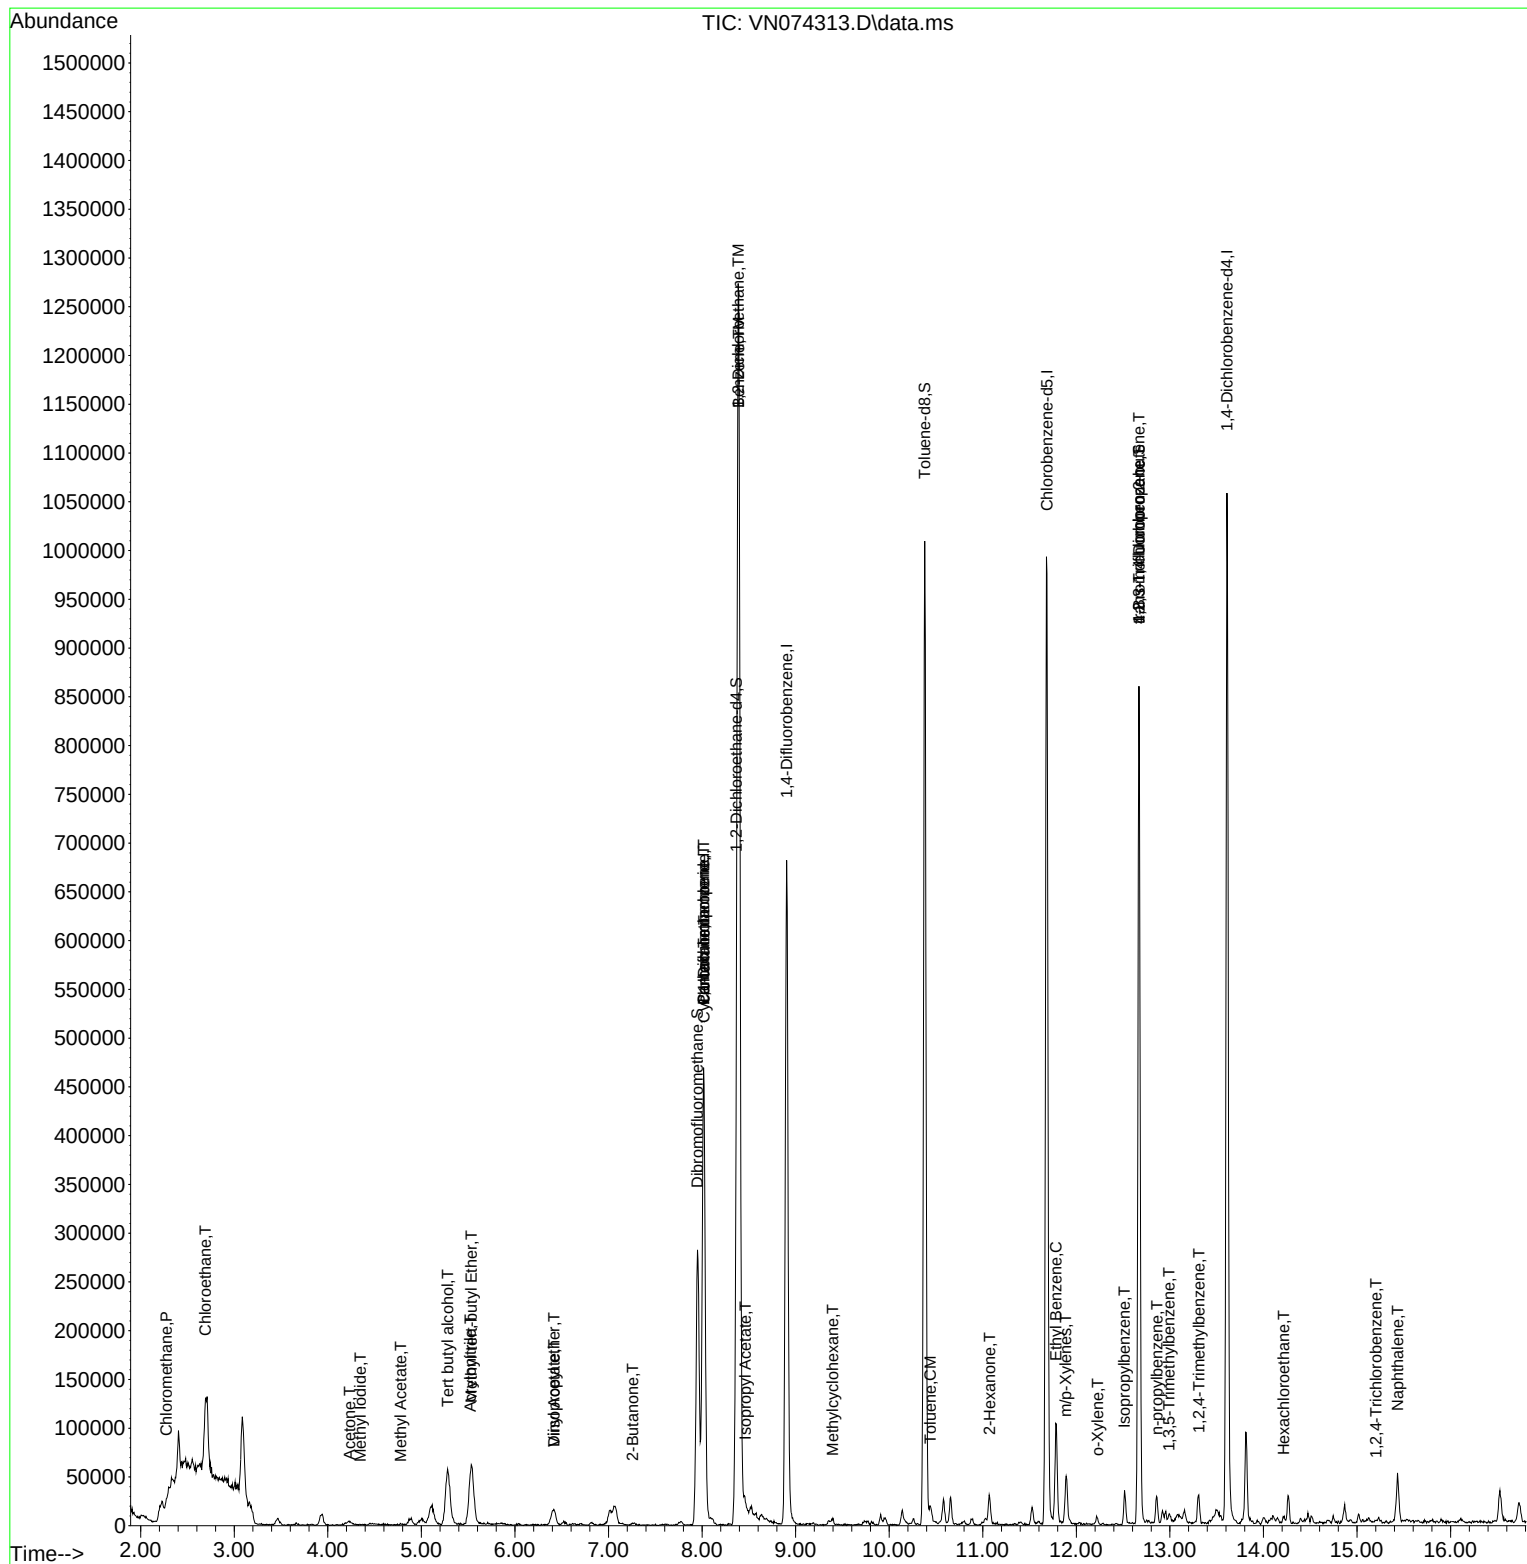




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40




Instrument :
MSVOA_N
ClientSampleId :
MW-35


Tgt Ion:168 Resp: 327393
Ion Ratio Lower Upper
168 100
99 60.7 42.3 63.5

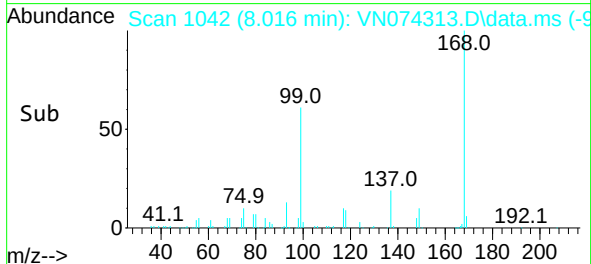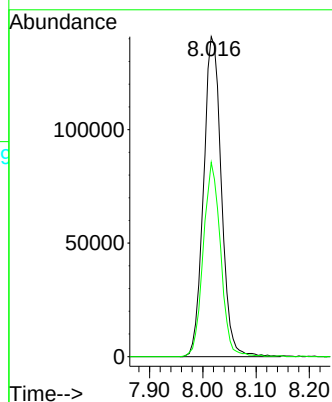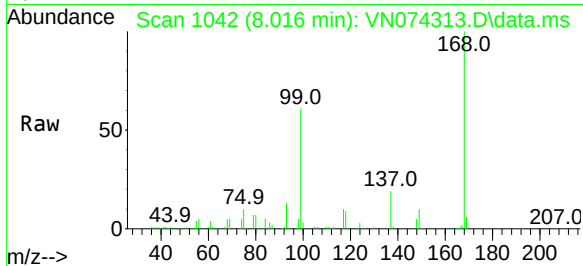

#3
Chloromethane
Concen: 0.541 ug/l
RT: 2.275 min Scan# 66
Delta R.T. 0.006 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40

Tgt Ion: 50 Resp: 2422
Ion Ratio Lower Upper
50 100
52 17.5 25.7 38.5#



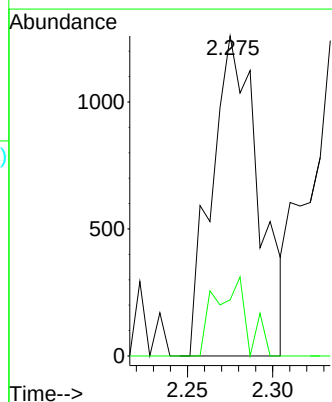
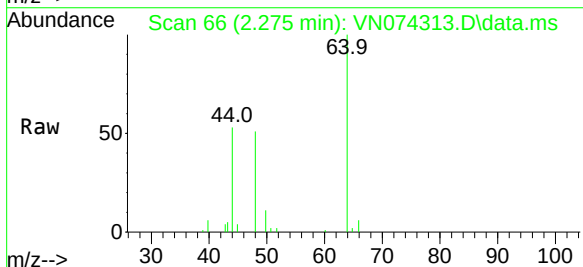




#6
Chloroethane
Concen: 11.618 ug/l
RT: 2.693 min Scan# 11
Delta R.T. -0.258 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40




Instrument :
MSVOA_N
ClientSampleId :
MW-35


Tgt Ion: 64 Resp: 76159
Ion Ratio Lower Upper
64 100
66 5.4 26.2 39.4#

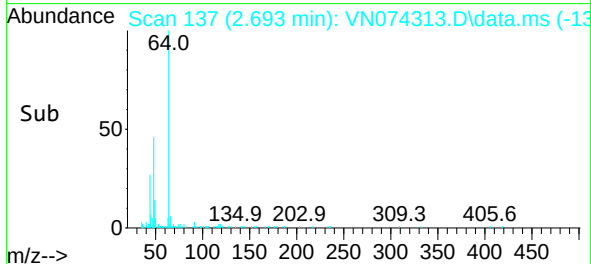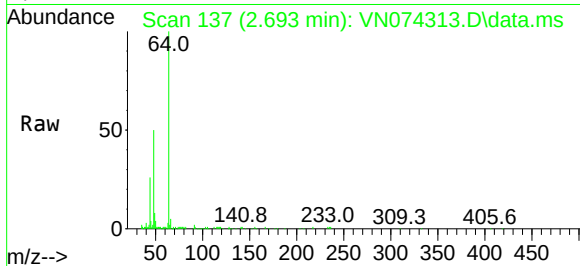

#10
Methyl Iodide
Concen: 5.063 ug/l
RT: 4.345 min Scan# 418
Delta R.T. -0.001 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40

Tgt Ion: 142 Resp: 58
Ion Ratio Lower Upper
142 100
127 0.0 31.3 46.9#
141 0.0 11.2 16.8#

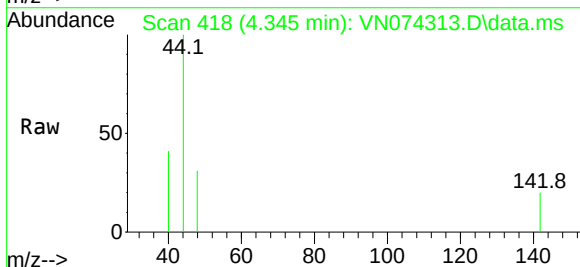



#11

Tert butyl alcohol

Concen: 106.447 ug/l

RT: 5.281 min Scan# 5

Delta R.T. -0.006 min

Lab File: VN074313.D

Acq: 03 Sep 2022 02:40

Instrument :

MSVOA_N

ClientSampleId :





MW-35

Tgt Ion: 59 Resp: 98558

Ion Ratio Lower Upper

59 100

57 10.9 8.3 12.5

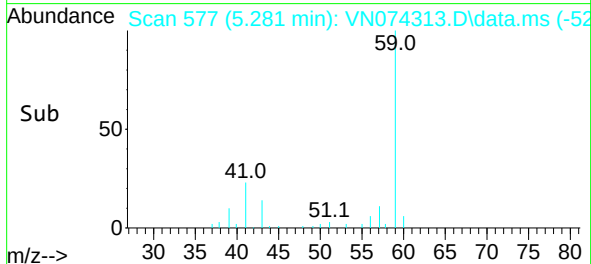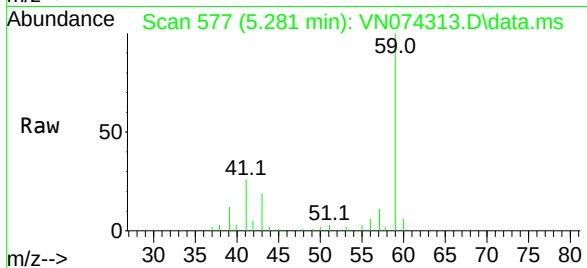

#15

Acrylonitrile

Concen: 0.265 ug/l

RT: 5.522 min Scan# 618

Delta R.T. 0.053 min

Lab File: VN074313.D

Acq: 03 Sep 2022 02:40




Tgt Ion: 53 Resp: 676


Ion Ratio Lower Upper

53 100

52 0.0 66.4 99.6#

51 51.9 28.5 42.7#

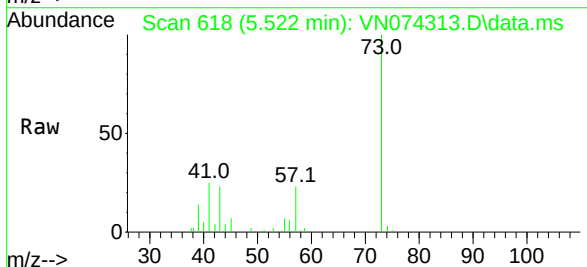



#16

Acetone

Concen: 3.247 ug/l

RT: 4.234 min Scan# 399

Delta R.T. 0.012 min

Lab File: VN074313.D

Acq: 03 Sep 2022 02:40

Instrument :

MSVOA_N

ClientSampleId :





MW-35

Tgt Ion: 43 Resp: 6925

Ion Ratio Lower Upper

43 100

58 19.4 26.0 39.0#

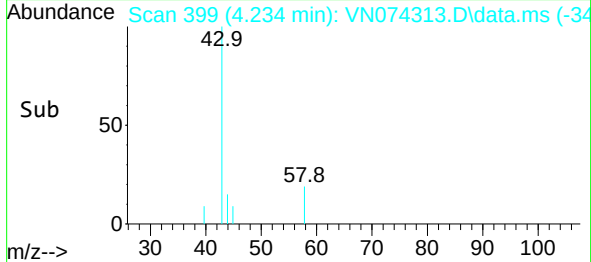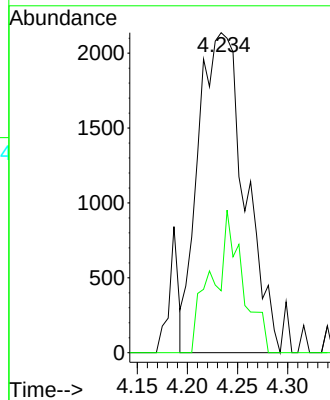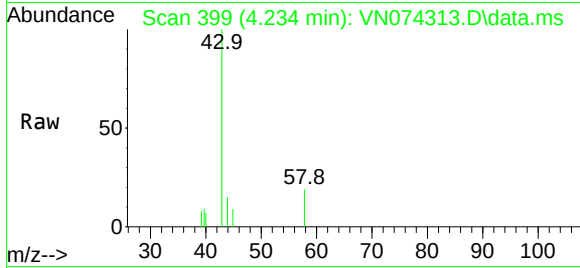

#18

Methyl Acetate

Concen: 0.283 ug/l

RT: 4.781 min Scan# 492

Delta R.T. 0.006 min

Lab File: VN074313.D




Acq: 03 Sep 2022 02:40


Tgt Ion: 43 Resp: 1819

Ion Ratio Lower Upper

43 100

74 5.6 21.6 32.4#

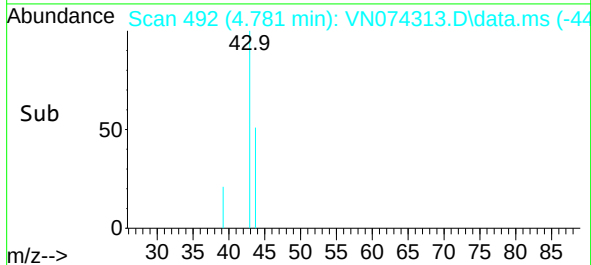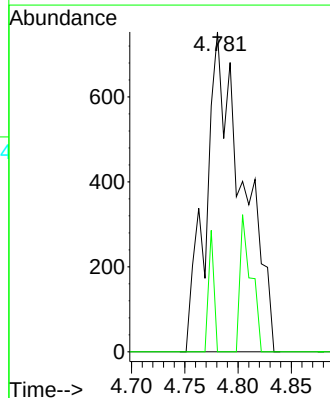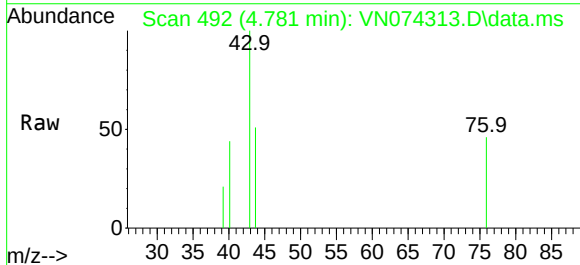



#19

Methyl tert-butyl Ether

Concen: 7.702 ug/l

RT: 5.534 min Scan# 61

Delta R.T. -0.000 min

Lab File: VN074313.D

Acq: 03 Sep 2022 02:40

Instrument :

MSVOA_N

ClientSampleId :





MW-35

Tgt Ion: 73 Resp: 98376

Ion Ratio Lower Upper

73 100

57 21.8 17.6 26.4

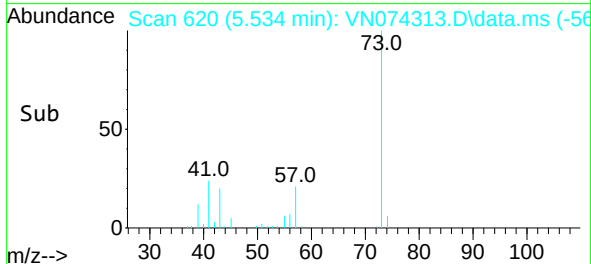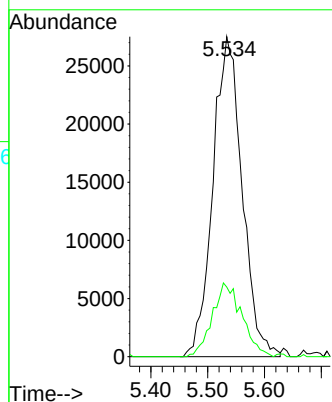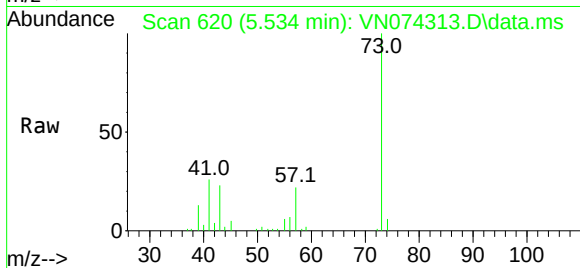

#20

Methylene Chloride

Concen: Below Cal

RT: 5.004 min Scan# 530

Delta R.T. -0.006 min

Lab File: VN074313.D

Acq: 03 Sep 2022 02:40

Tgt Ion: 84 Resp: 111




Ion Ratio Lower Upper


84 100

49 70.2 88.3 132.5#

51 0.0 28.2 42.2#

86 145.7 50.6 76.0#




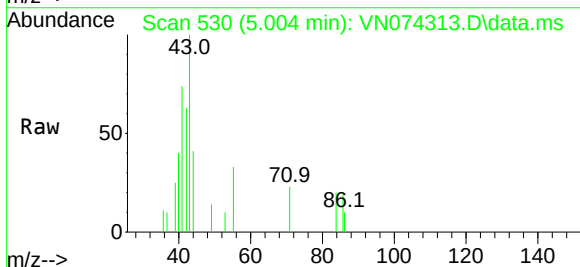




#22
Diisopropyl ether
Concen: 1.422 ug/l
RT: 6.416 min Scan# 770
Delta R.T. -0.000 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40




Instrument :
MSVOA_N
ClientSampleId :
MW-35


Tgt Ion: 45 Resp: 17302
Ion Ratio Lower Upper
45 100
43 74.0 46.6 70.0#
87 32.6 24.3 36.5
59 20.2 9.6 14.4#

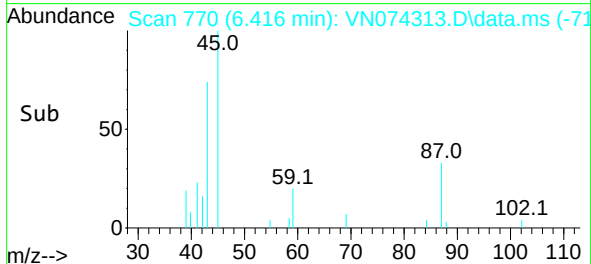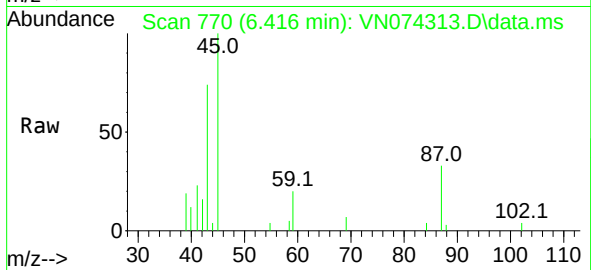

#23
Vinyl Acetate
Concen: 1.062 ug/l
RT: 6.416 min Scan# 770
Delta R.T. 0.065 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40

Tgt Ion: 43 Resp: 11231
Ion Ratio Lower Upper
43 100
86 0.0 10.0 15.0#





#25

2-Butanone

Concen: 0.398 ug/l

RT: 7.257 min Scan# 913

Delta R.T. -0.000 min

Lab File: VN074313.D

Acq: 03 Sep 2022 02:40

Instrument :

MSVOA_N

ClientSampleId :





MW-35

Tgt Ion: 43 Resp: 1434

Ion Ratio Lower Upper

43 100

72 17.5 23.7 35.5#

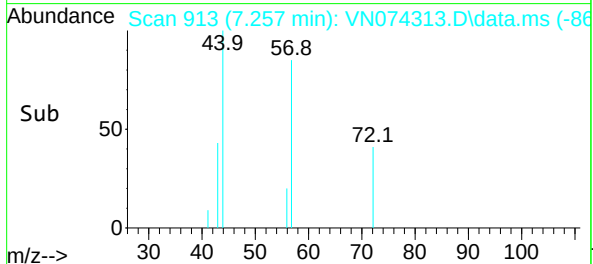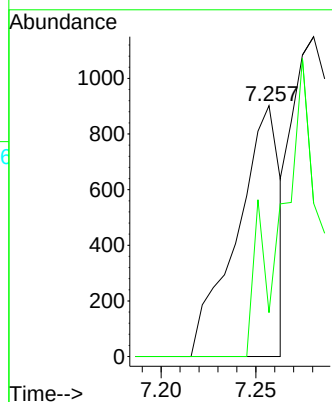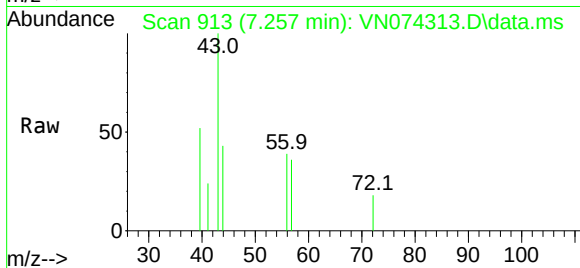

#31

Cyclohexane

Concen: 2.741 ug/l

RT: 8.022 min Scan# 1043

Delta R.T. -0.000 min

Lab File: VN074313.D

Acq: 03 Sep 2022 02:40




Tgt Ion: 56 Resp: 18683


Ion Ratio Lower Upper

56 100

69 86.8 27.8 41.8#

84 96.1 76.9 115.3

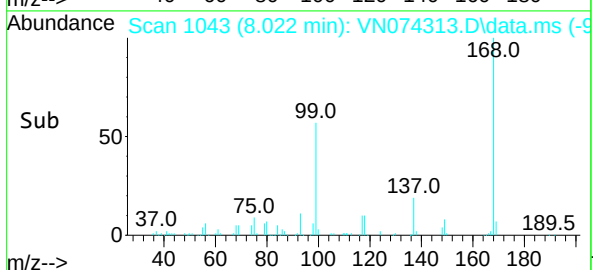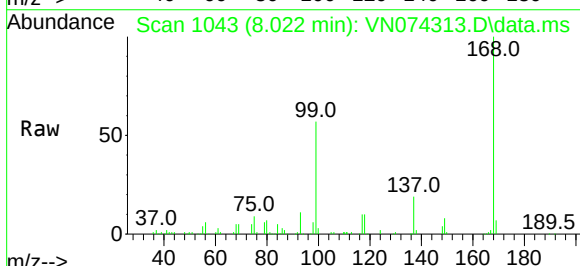

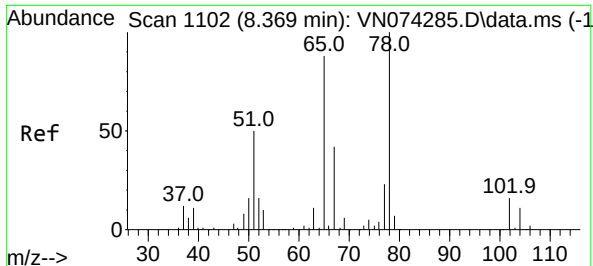

#33

1,2-Dichloroethane-d4

Concen: 45.331 ug/l

RT: 8.369 min Scan# 1102

Delta R.T. -0.000 min

Lab File: VN074313.D

Acq: 03 Sep 2022 02:40

Instrument :

MSVOA_N

ClientSampleId :





MW-35

Tgt Ion: 65 Resp: 231348

Ion Ratio Lower Upper

65 100

67 49.6 0.0 104.8

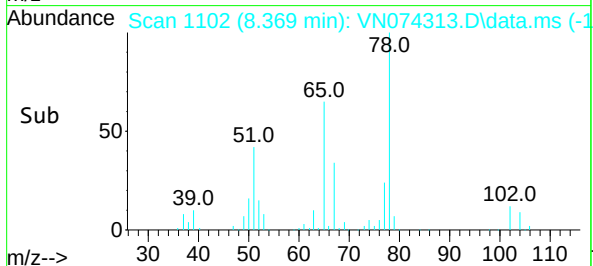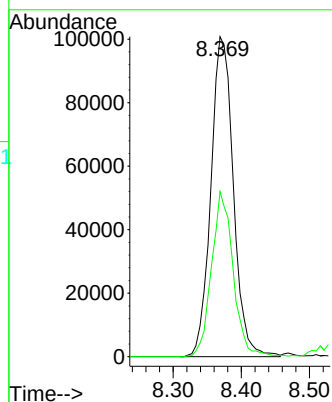

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. -0.000 min

Lab File: VN074313.D

Acq: 03 Sep 2022 02:40




Tgt Ion: 114 Resp: 599605


Ion Ratio Lower Upper

114 100

63 19.7 0.0 40.0

88 13.7 0.0 32.6


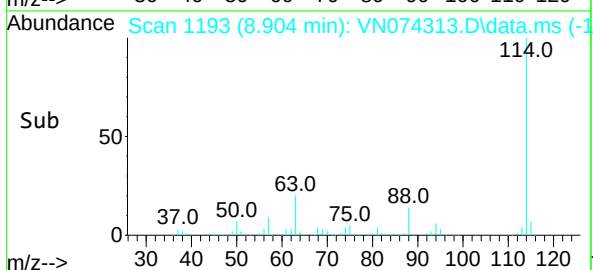

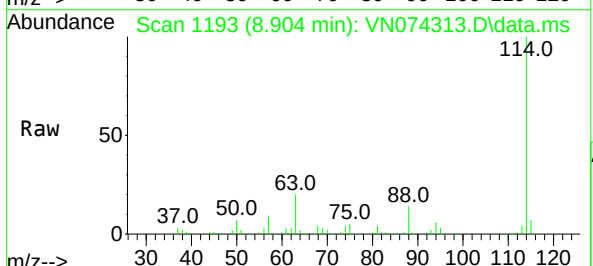


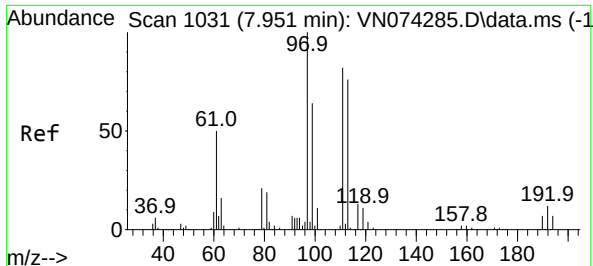

#35
Dibromofluoromethane
Concen: 49.000 ug/l
RT: 7.951 min Scan# 1042
Delta R.T. 0.000 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40




Instrument :
MSVOA_N
ClientSampleId :
MW-35


Tgt Ion:113 Resp: 194690
Ion Ratio Lower Upper
113 100
111 103.1 81.4 122.0
192 18.6 17.0 25.6

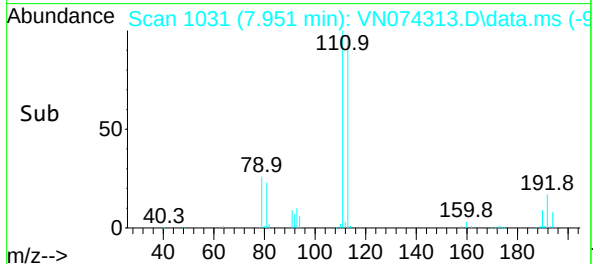

#36
1,1-Dichloropropene
Concen: 5.243 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.141 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40


Tgt Ion: 75 Resp: 29567
Ion Ratio Lower Upper
75 100
110 9.4 18.3 54.8#
77 0.0 25.1 37.7#

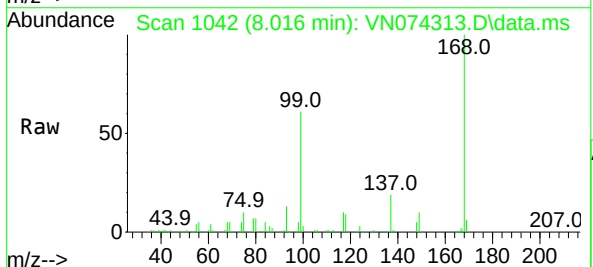



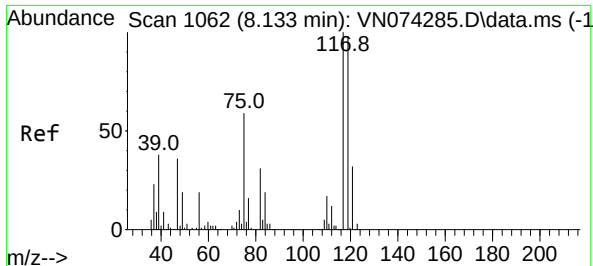


#38
Carbon Tetrachloride
Concen: 5.894 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.117 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40

Instrument :
MSVOA_N
ClientSampleId :
MW-35



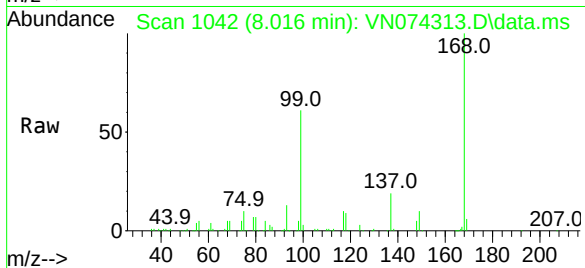



Tgt Ion:117 Resp: 33577
Ion Ratio Lower Upper
117 100
119 2.8 75.8 113.8#
121 0.0 24.6 37.0#

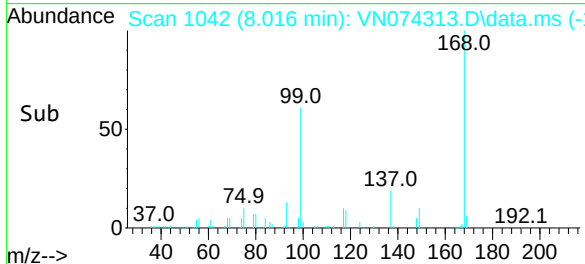

#39
Methylcyclohexane
Concen: 0.408 ug/l
RT: 9.398 min Scan# 1277
Delta R.T. 0.006 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40

Tgt Ion: 83 Resp: 2773
Ion Ratio Lower Upper
83 100
55 47.5 57.8 86.8#
98 42.1 39.4 59.2

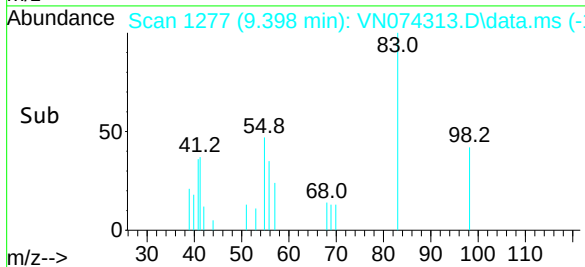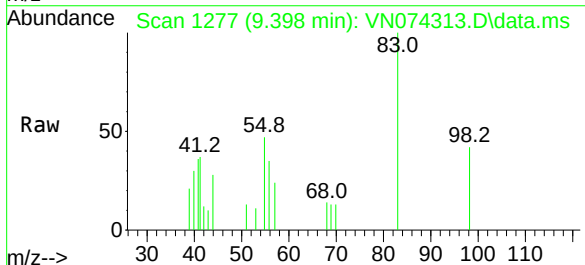



#40

Benzene

Concen: 67.265 ug/l

RT: 8.392 min Scan# 1106

Delta R.T. 0.000 min

Lab File: VN074313.D

Acq: 03 Sep 2022 02:40

Instrument :

MSVOA_N

ClientSampleId :





MW-35

Tgt Ion: 78 Resp: 1196628

Ion Ratio Lower Upper

78 100

77 24.1 19.4 29.0

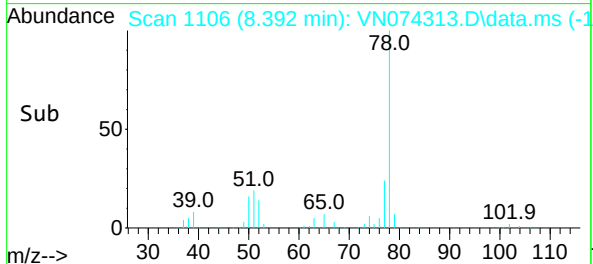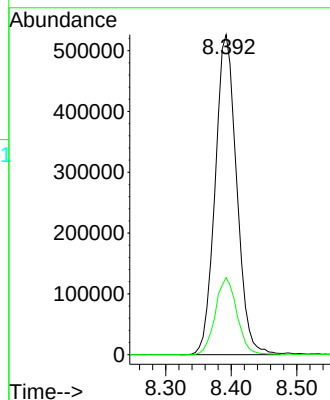

#42

1,2-Dichloroethane

Concen: 1.676 ug/l

RT: 8.386 min Scan# 1105

Delta R.T. -0.077 min

Lab File: VN074313.D




Acq: 03 Sep 2022 02:40


Tgt Ion: 62 Resp: 11094

Ion Ratio Lower Upper

62 100

98 3.1 0.0 19.4

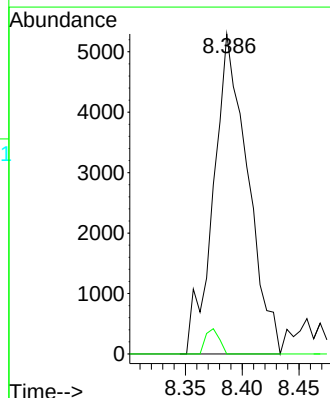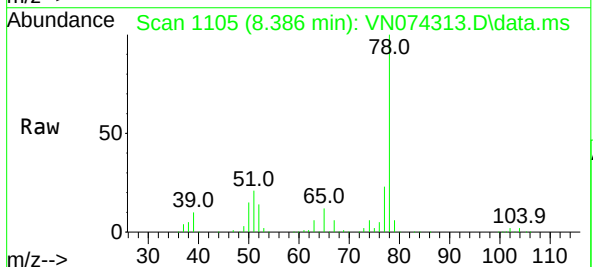

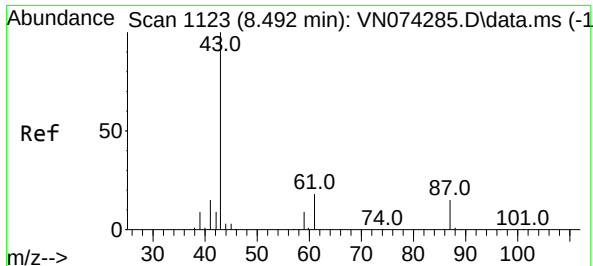

#43

Isopropyl Acetate

Concen: 0.304 ug/l

RT: 8.463 min Scan# 1118

Delta R.T. -0.029 min

Lab File: VN074313.D

Acq: 03 Sep 2022 02:40

Instrument :

MSVOA_N

ClientSampleId :

MW-35





Tgt Ion: 43 Resp: 3255

Ion Ratio Lower Upper

43 100

61 0.0 21.9 32.9#

87 0.0 12.0 18.0#

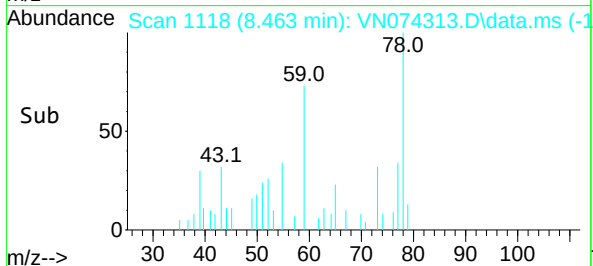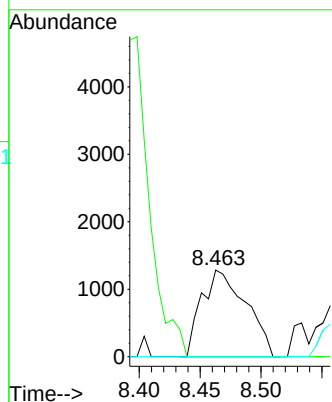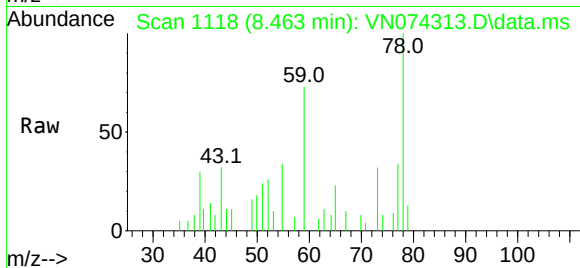

#50

Toluene-d8

Concen: 43.301 ug/l

RT: 10.380 min Scan# 1444

Delta R.T. 0.000 min

Lab File: VN074313.D




Acq: 03 Sep 2022 02:40


Tgt Ion: 98 Resp: 678420

Ion Ratio Lower Upper

98 100

100 65.3 52.6 78.8


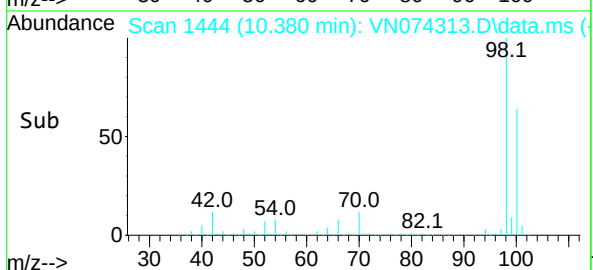

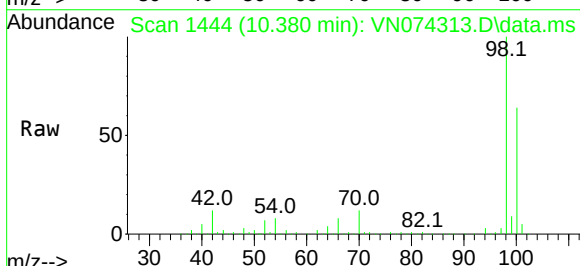




#52
Toluene
Concen: 0.513 ug/l
RT: 10.439 min Scan# 1454
Delta R.T. -0.006 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40




Instrument :
MSVOA_N
ClientSampleId :
MW-35


Tgt Ion: 92 Resp: 5638
Ion Ratio Lower Upper
92 100
91 180.2 138.6 207.8

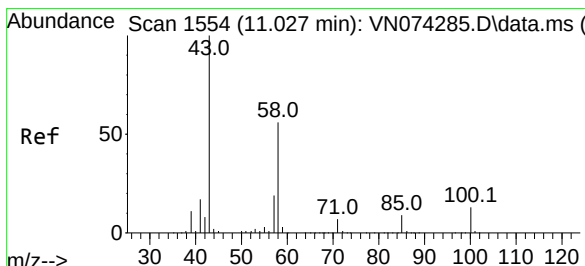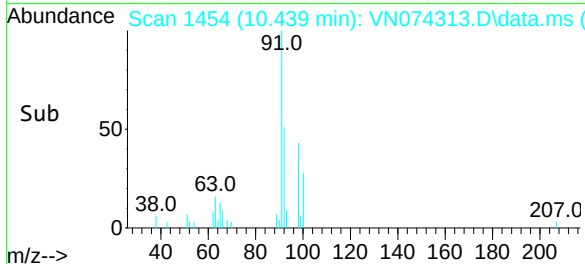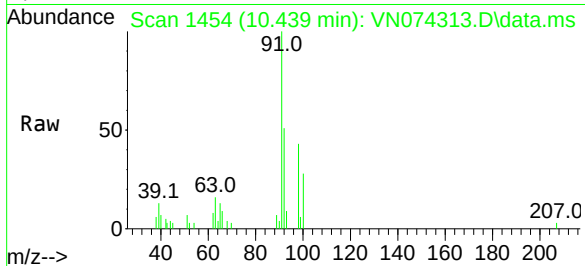

#59
2-Hexanone
Concen: 0.421 ug/l
RT: 11.074 min Scan# 1562
Delta R.T. 0.047 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40

Tgt Ion: 43 Resp: 2389
Ion Ratio Lower Upper
43 100
58 45.8 29.7 89.1


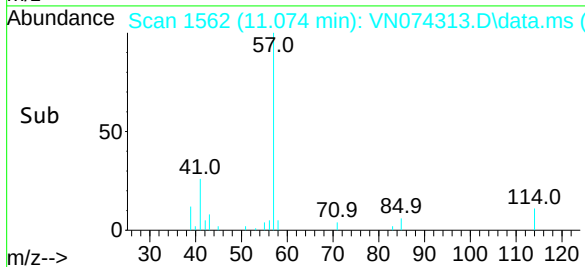

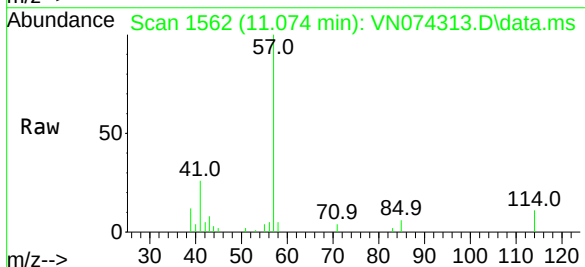


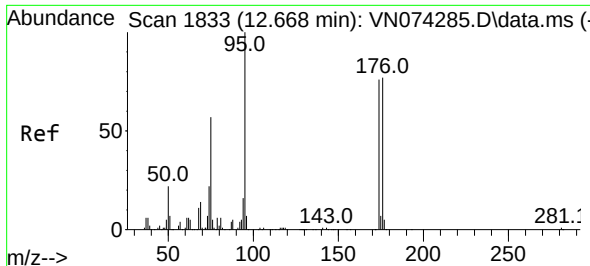

#62
4-Bromofluorobenzene
Concen: 44.973 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. -0.001 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40




Instrument :
MSVOA_N
ClientSampleId :
MW-35


Tgt Ion: 95 Resp: 256092
Ion Ratio Lower Upper
95 100
174 79.8 0.0 167.6
176 78.4 0.0 163.4

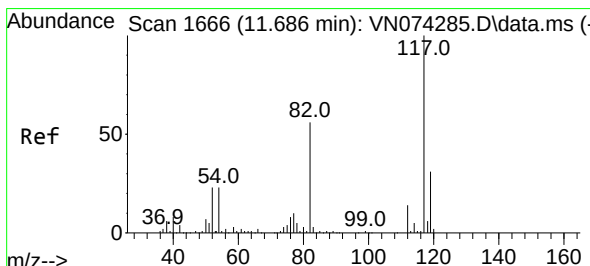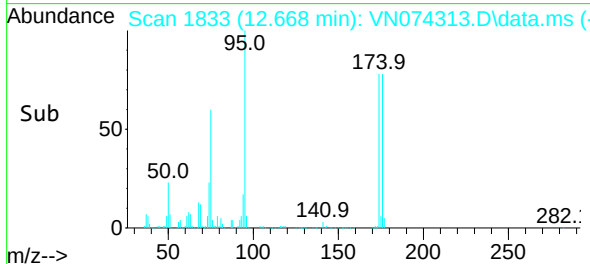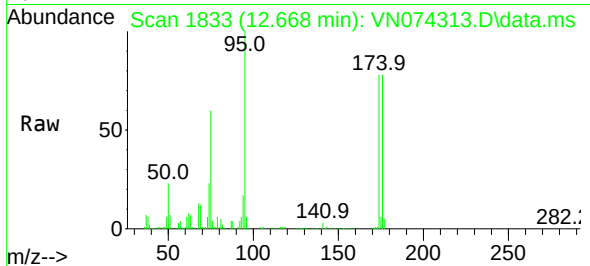

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1666
Delta R.T. 0.000 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40

Tgt Ion: 117 Resp: 564137
Ion Ratio Lower Upper
117 100
82 53.1 44.2 66.2
119 31.3 25.4 38.0


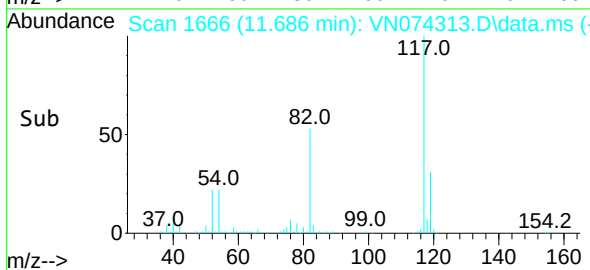

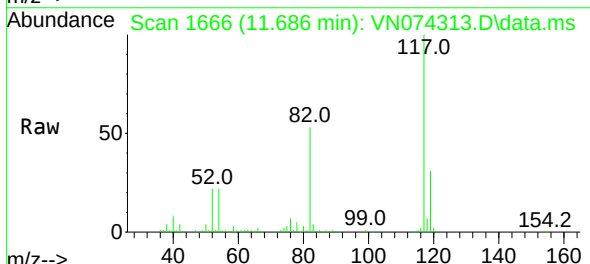




#67
Ethyl Benzene
Concen: 3.114 ug/l
RT: 11.780 min Scan# 1682
Delta R.T. -0.006 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40




Instrument :
MSVOA_N
ClientSampleId :
MW-35


Tgt Ion: 91 Resp: 70789
Ion Ratio Lower Upper
91 100
106 28.5 24.9 37.3

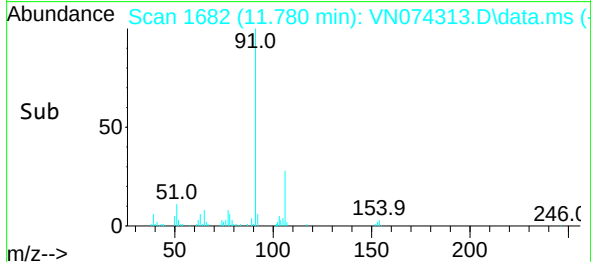

#68
m/p-Xylenes
Concen: 1.945 ug/l
RT: 11.886 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40

Tgt Ion: 106 Resp: 16506
Ion Ratio Lower Upper
106 100
91 192.2 158.9 238.3




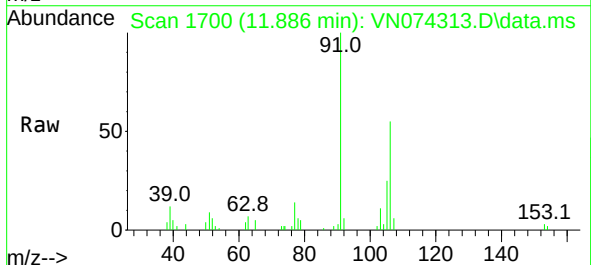




#69
o-Xylene
Concen: 0.291 ug/l
RT: 12.227 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40




Instrument :
MSVOA_N
ClientSampleId :
MW-35


Tgt Ion:106 Resp: 2461
Ion Ratio Lower Upper
106 100
91 193.6 106.0 318.0

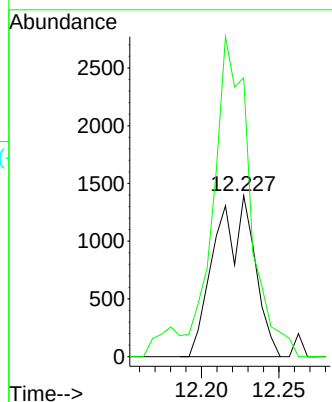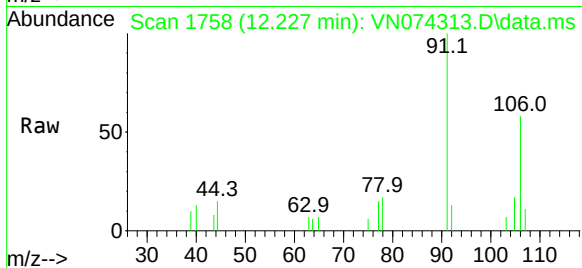

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.610 min Scan# 1993
Delta R.T. -0.000 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40

Tgt Ion:152 Resp: 261043
Ion Ratio Lower Upper
152 100
115 60.1 28.9 86.7
150 158.2 0.0 356.2

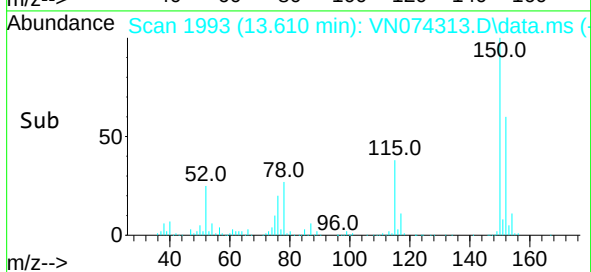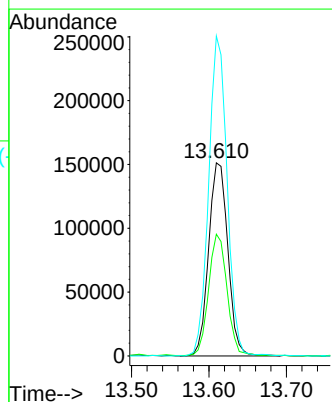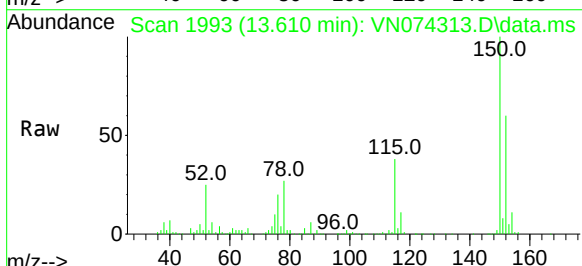



#73

Isopropylbenzene

Concen: 0.897 ug/l

RT: 12.515 min Scan# 1807

Delta R.T. -0.001 min

Lab File: VN074313.D

Acq: 03 Sep 2022 02:40

Instrument :

MSVOA_N

ClientSampleId :





MW-35

Tgt Ion:105 Resp: 20497

Ion Ratio Lower Upper

105 100

120 27.4 13.5 40.4



#76

1,2,3-Trichloropropane

Concen: 20.252 ug/l

RT: 12.668 min Scan# 1833

Delta R.T. -0.153 min

Lab File: VN074313.D




Acq: 03 Sep 2022 02:40


Tgt Ion: 75 Resp: 149732

Ion Ratio Lower Upper

75 100

77 1.4 98.5 295.5#


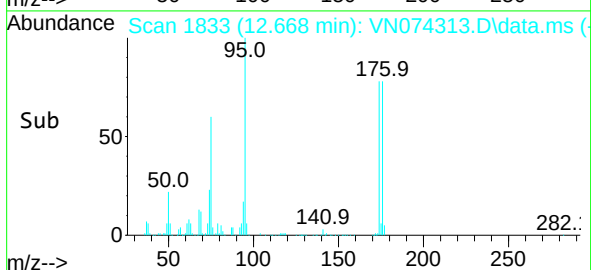






#78
n-propylbenzene
Concen: 0.823 ug/l
RT: 12.862 min Scan# 1866
Delta R.T. -0.001 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40




Instrument :
MSVOA_N
ClientSampleId :
MW-35


Tgt Ion: 91 Resp: 21504
Ion Ratio Lower Upper
91 100
120 24.9 11.9 35.5

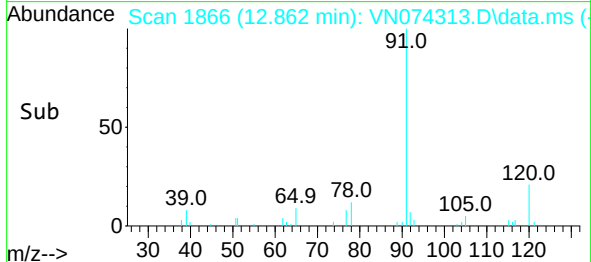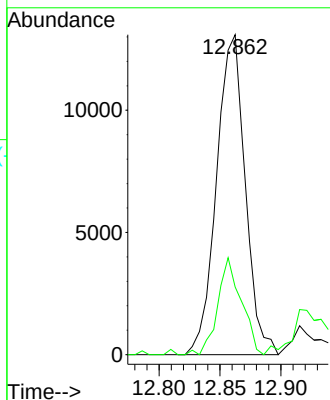

#80
1,3,5-Trimethylbenzene
Concen: 0.211 ug/l
RT: 12.992 min Scan# 1888
Delta R.T. -0.006 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40

Tgt Ion: 105 Resp: 3866
Ion Ratio Lower Upper
105 100
120 44.9 24.9 74.7



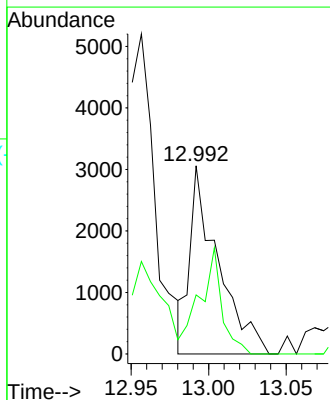
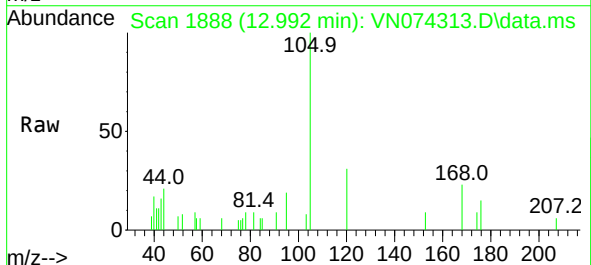


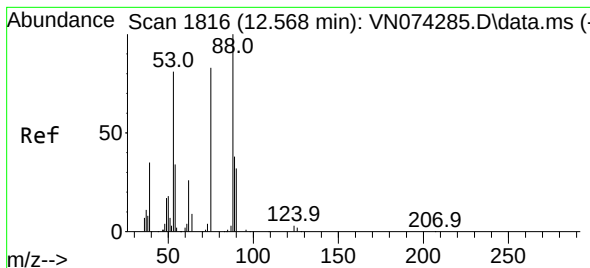

#81
 trans-1,4-Dichloro-2-butene
 Concen: 65.745 ug/l
 RT: 12.668 min Scan# 1816
 Delta R.T. 0.105 min
 Lab File: VN074313.D
 Acq: 03 Sep 2022 02:40




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-35


Tgt Ion: 75 Resp: 149732
 Ion Ratio Lower Upper
 75 100
 53 0.0 78.0 117.0#
 89 0.3 37.2 55.8#

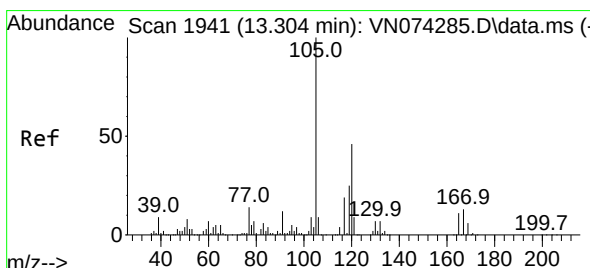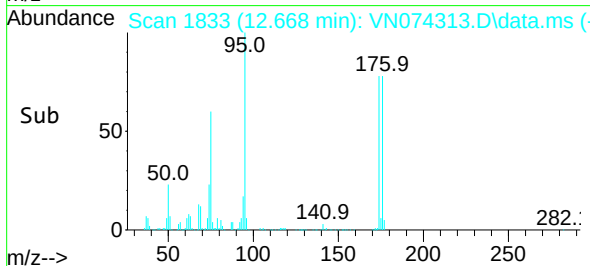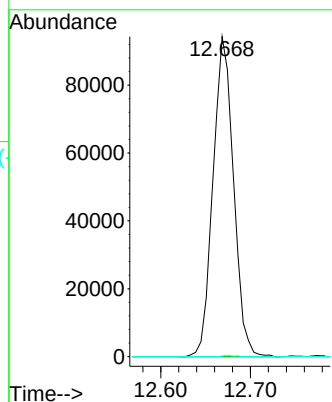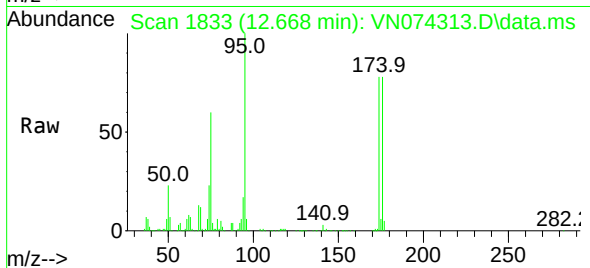

#84
 1,2,4-Trimethylbenzene
 Concen: 0.985 ug/l
 RT: 13.310 min Scan# 1942
 Delta R.T. -0.000 min
 Lab File: VN074313.D
 Acq: 03 Sep 2022 02:40

Tgt Ion: 105 Resp: 18291
 Ion Ratio Lower Upper
 105 100
 120 42.2 23.3 69.8


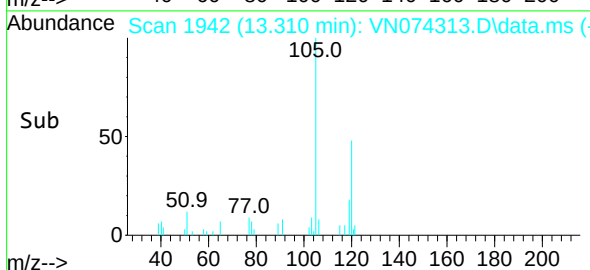

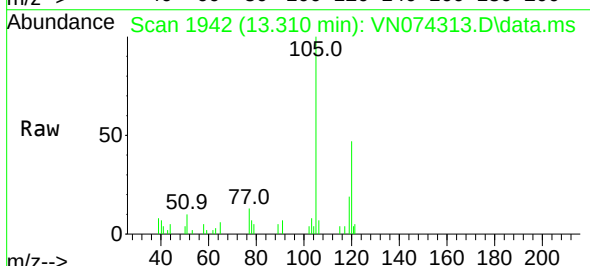




#90
Hexachloroethane
Concen: 1.040 ug/l
RT: 14.215 min Scan# 2084
Delta R.T. 0.064 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40




Instrument :
MSVOA_N
ClientSampleId :
MW-35


Tgt Ion:117 Resp: 3661
Ion Ratio Lower Upper
117 100
201 0.0 40.6 122.0#

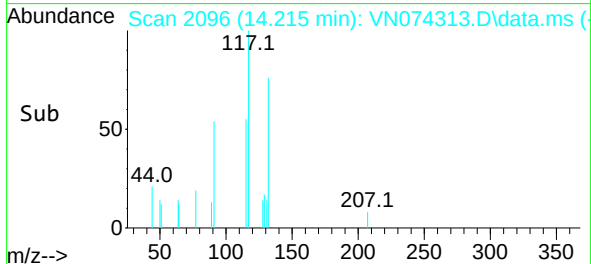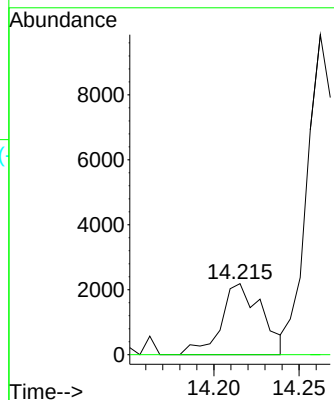

#93
1,2,4-Trichlorobenzene
Concen: 0.869 ug/l
RT: 15.204 min Scan# 2264
Delta R.T. 0.006 min
Lab File: VN074313.D
Acq: 03 Sep 2022 02:40

Tgt Ion:180 Resp: 71
Ion Ratio Lower Upper
180 100
182 0.0 47.5 142.5#
145 111.3 14.5 43.5#

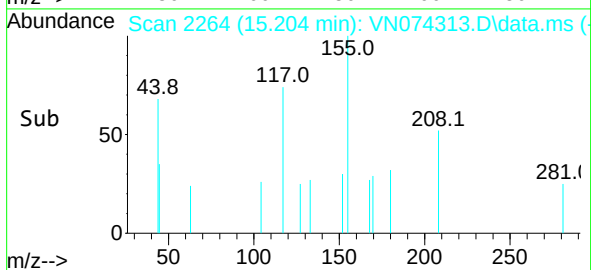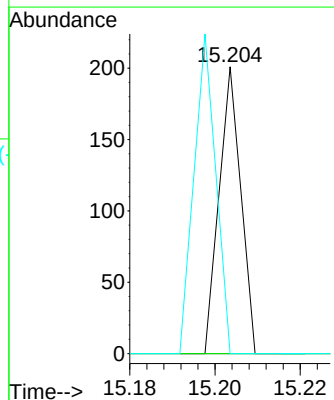

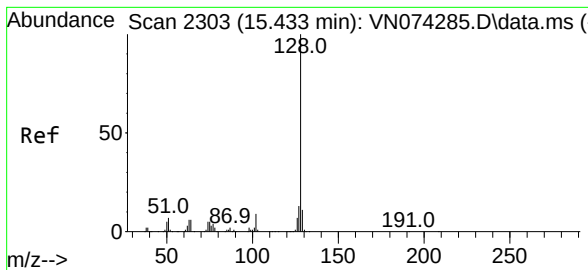

#95
 Naphthalene
 Concen: 3.062 ug/l
 RT: 15.433 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN074313.D
 Acq: 03 Sep 2022 02:40

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-35

Tgt Ion:	128	Resp:	44106
Ion	Ratio	Lower	Upper
128	100		
127	15.0	10.3	15.5
129	13.6	8.6	13.0#

