



Methyl Iodide

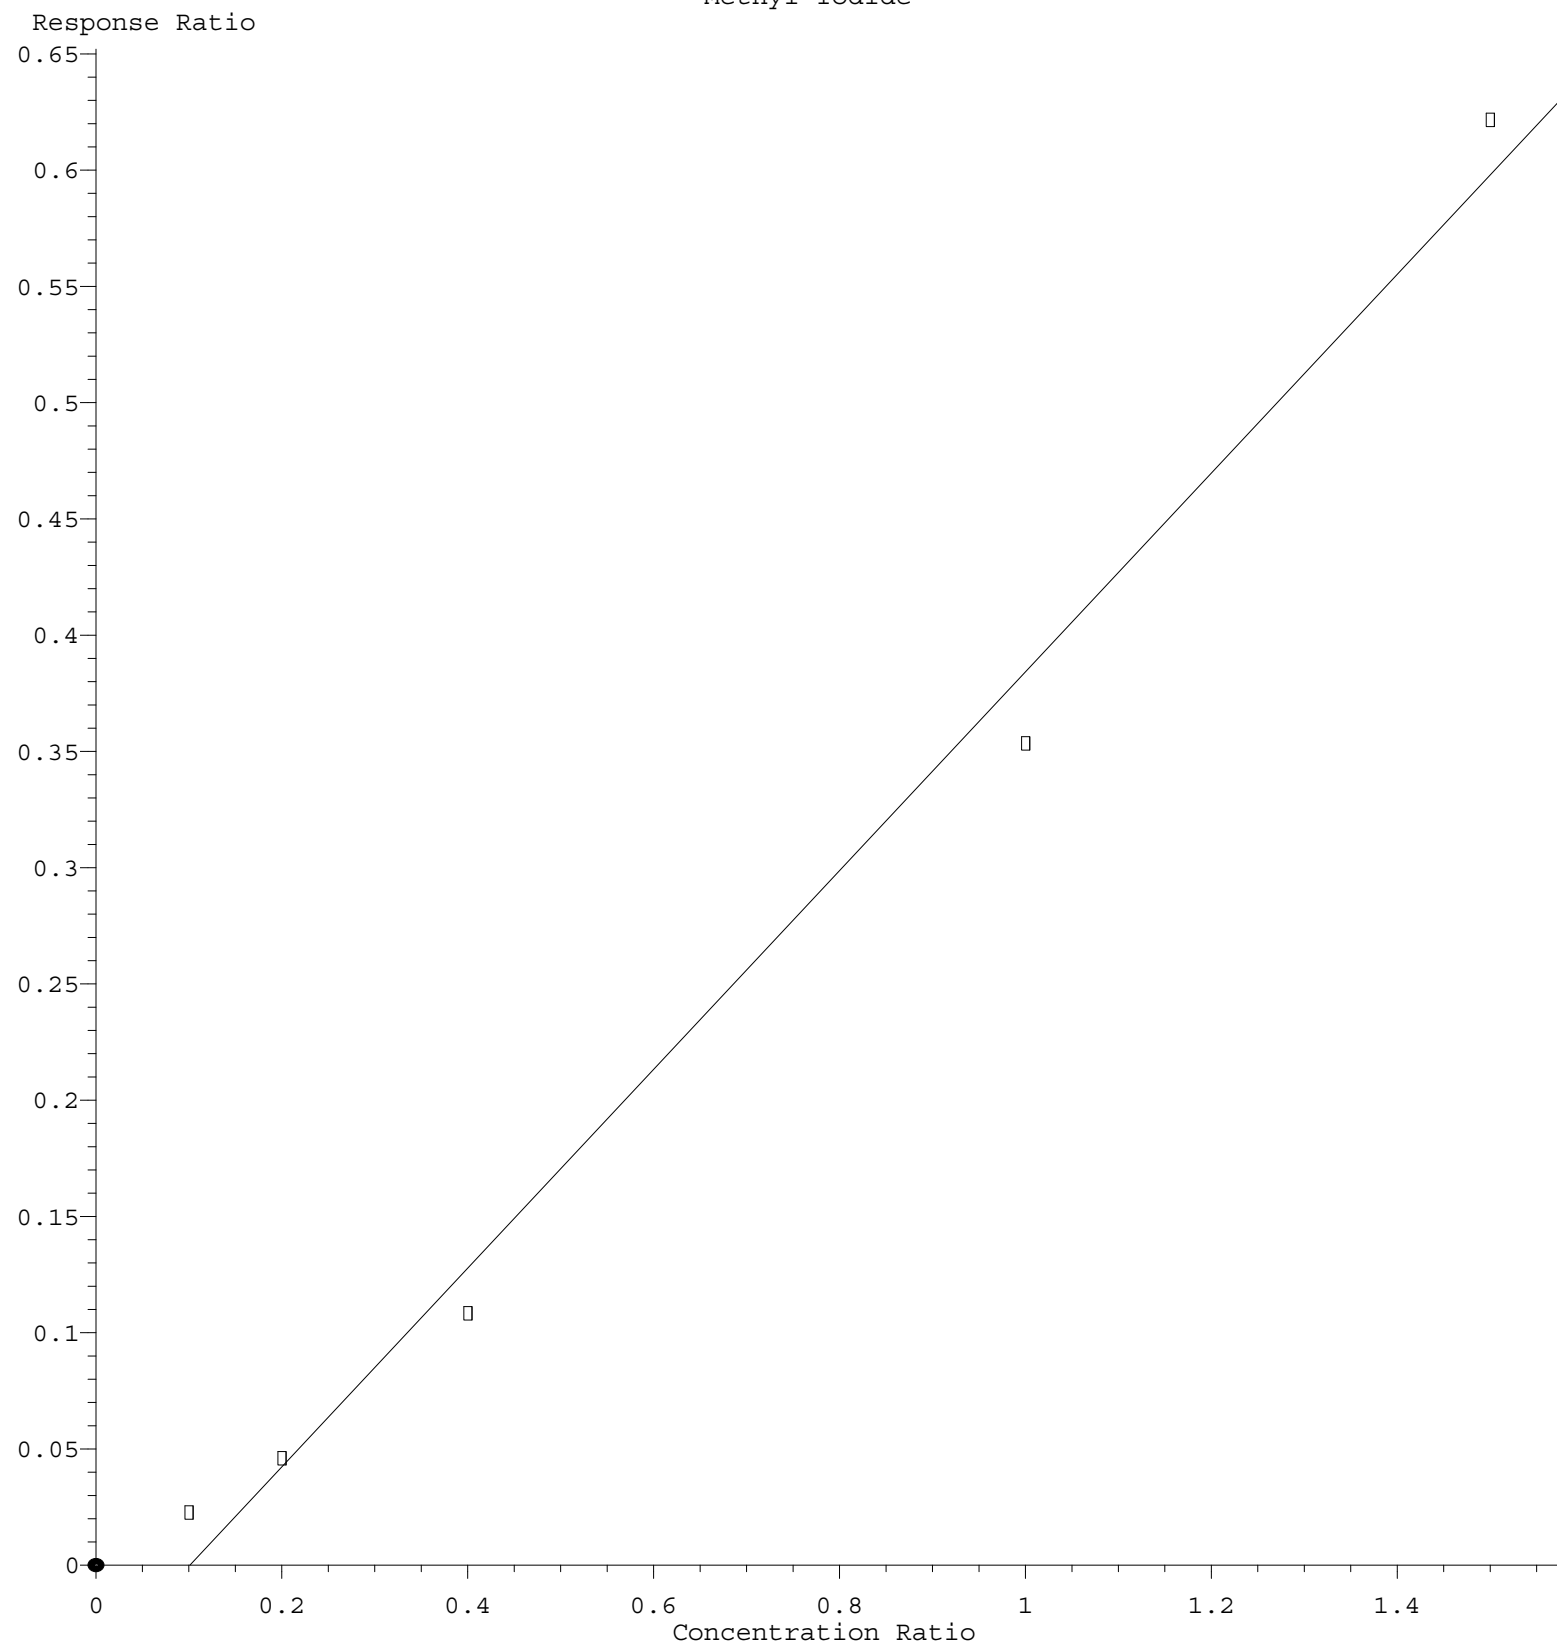

Response = $4.273\text{e-}001 * \text{Amt} - 4.309\text{e-}002$
Coef of Det (r^2) = 0.990656 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090222W.M
Calibration Table Last Updated: Sat Sep 03 04:35:33 2022

Methylene Chloride

Response Ratio

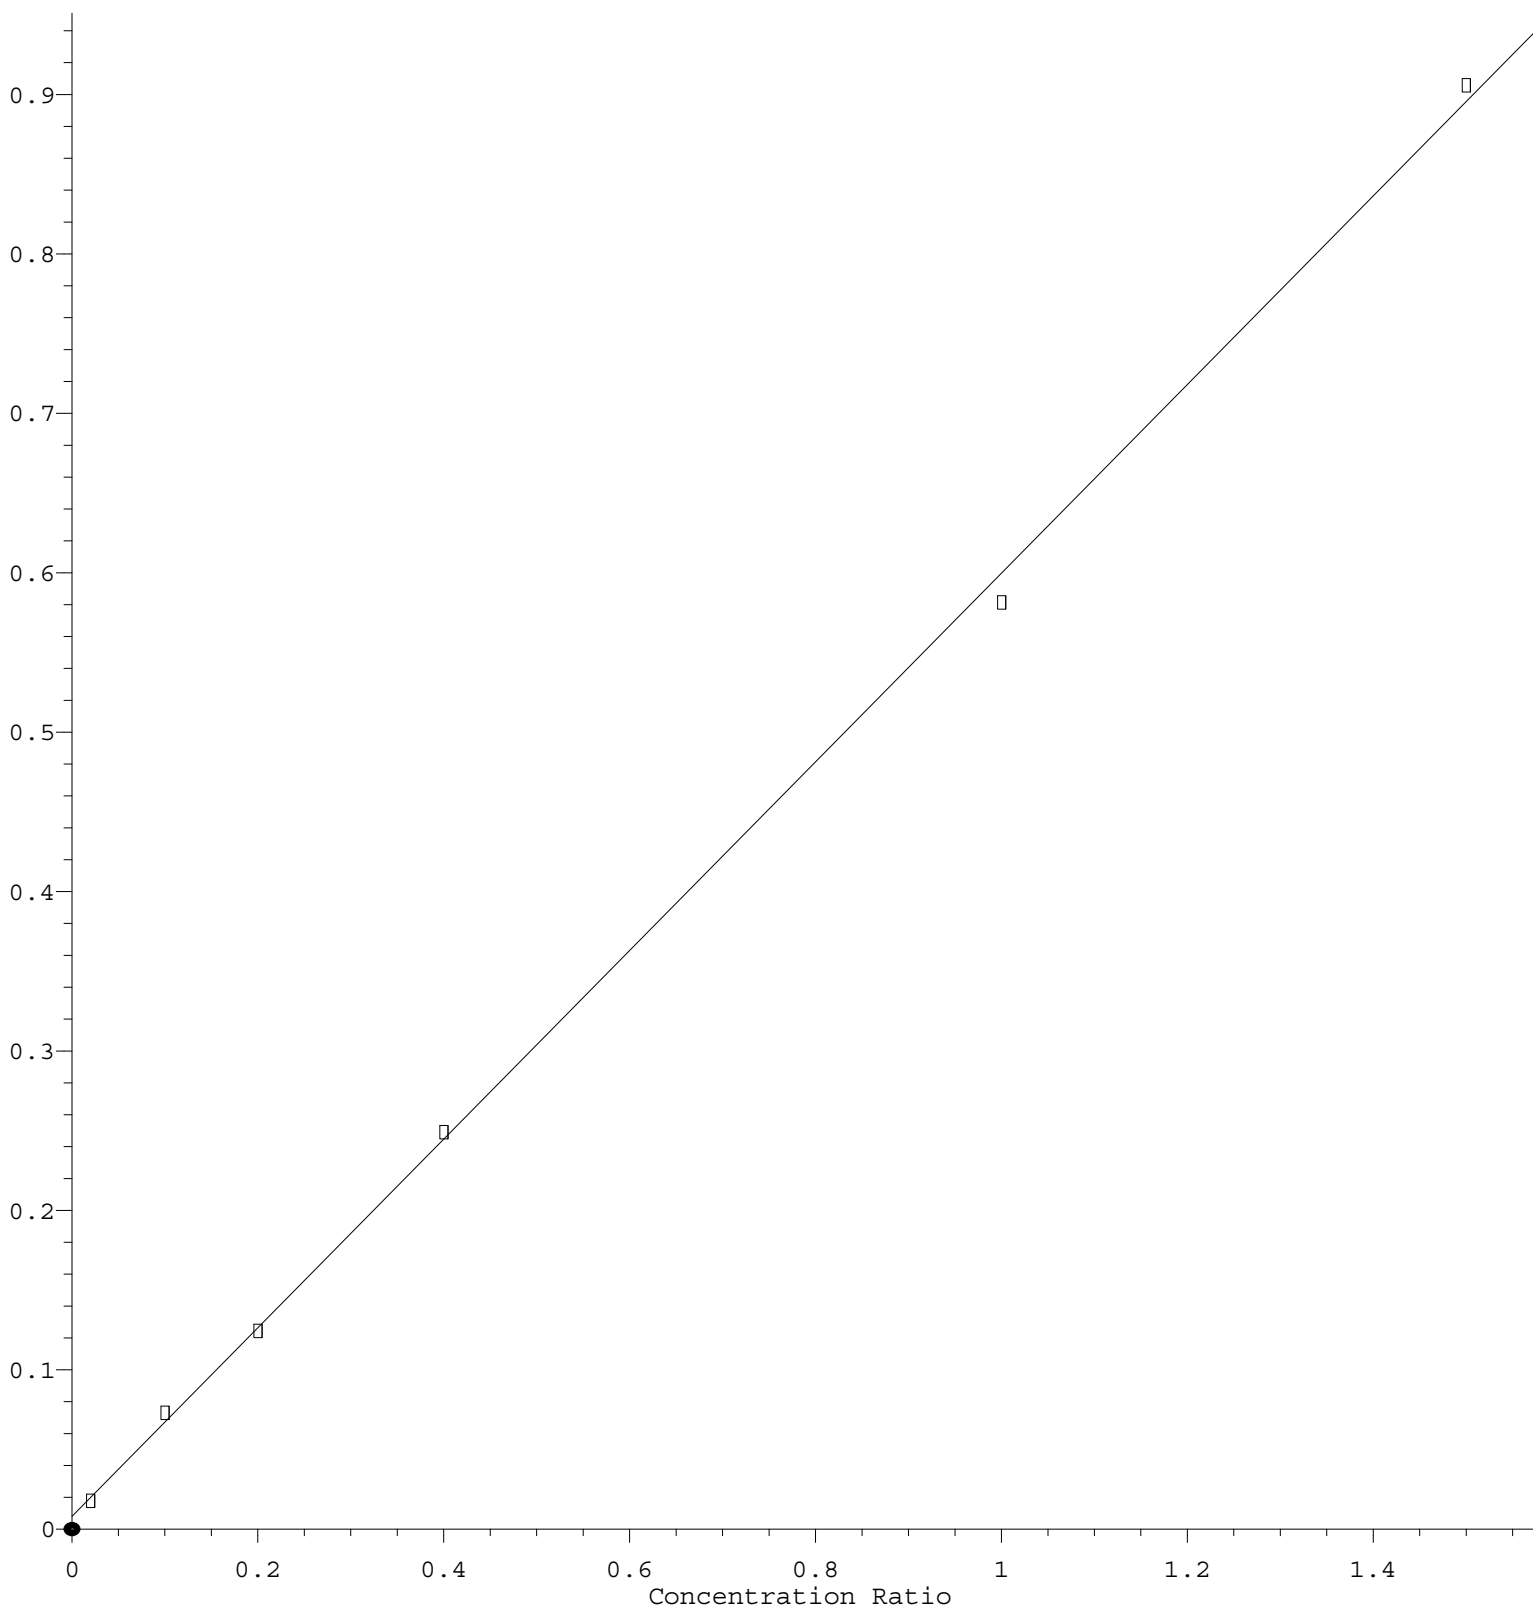


$$\text{Response} = 5.916\text{e-}001 * \text{Amt} + 7.686\text{e-}003$$

Coef of Det (r^2) = 0.999172 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090222W.M


Calibration Table Last Updated: Sat Sep 03 04:35:33 2022

Bromochloromethane

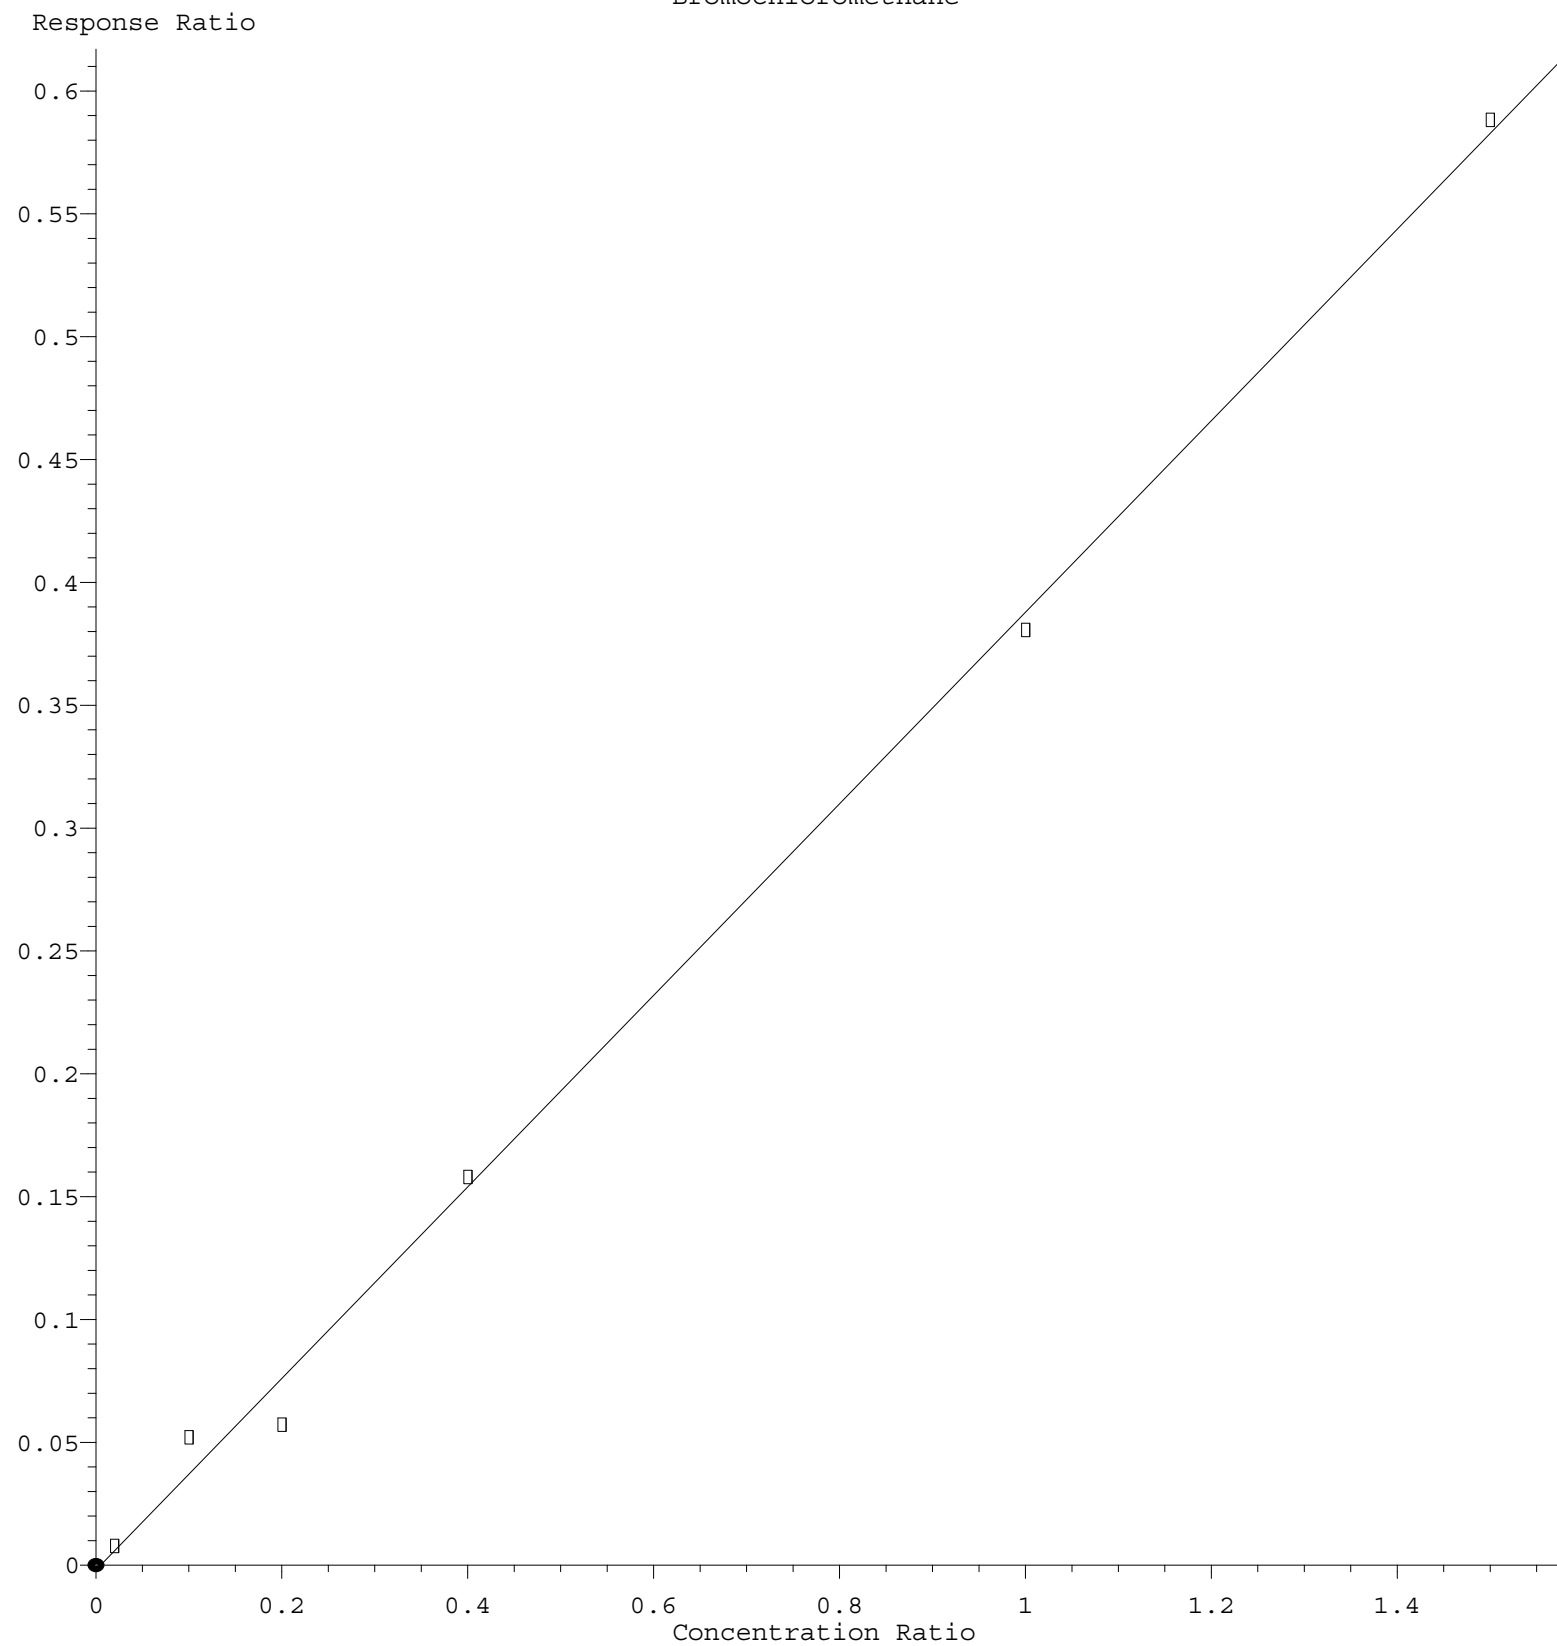

Response = 3.899e-001 * Amt - 1.940e-003
 Coef of Det (r^2) = 0.997415 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090222W.M
 Calibration Table Last Updated: Sat Sep 03 04:35:33 2022


4-Bromofluorobenzene

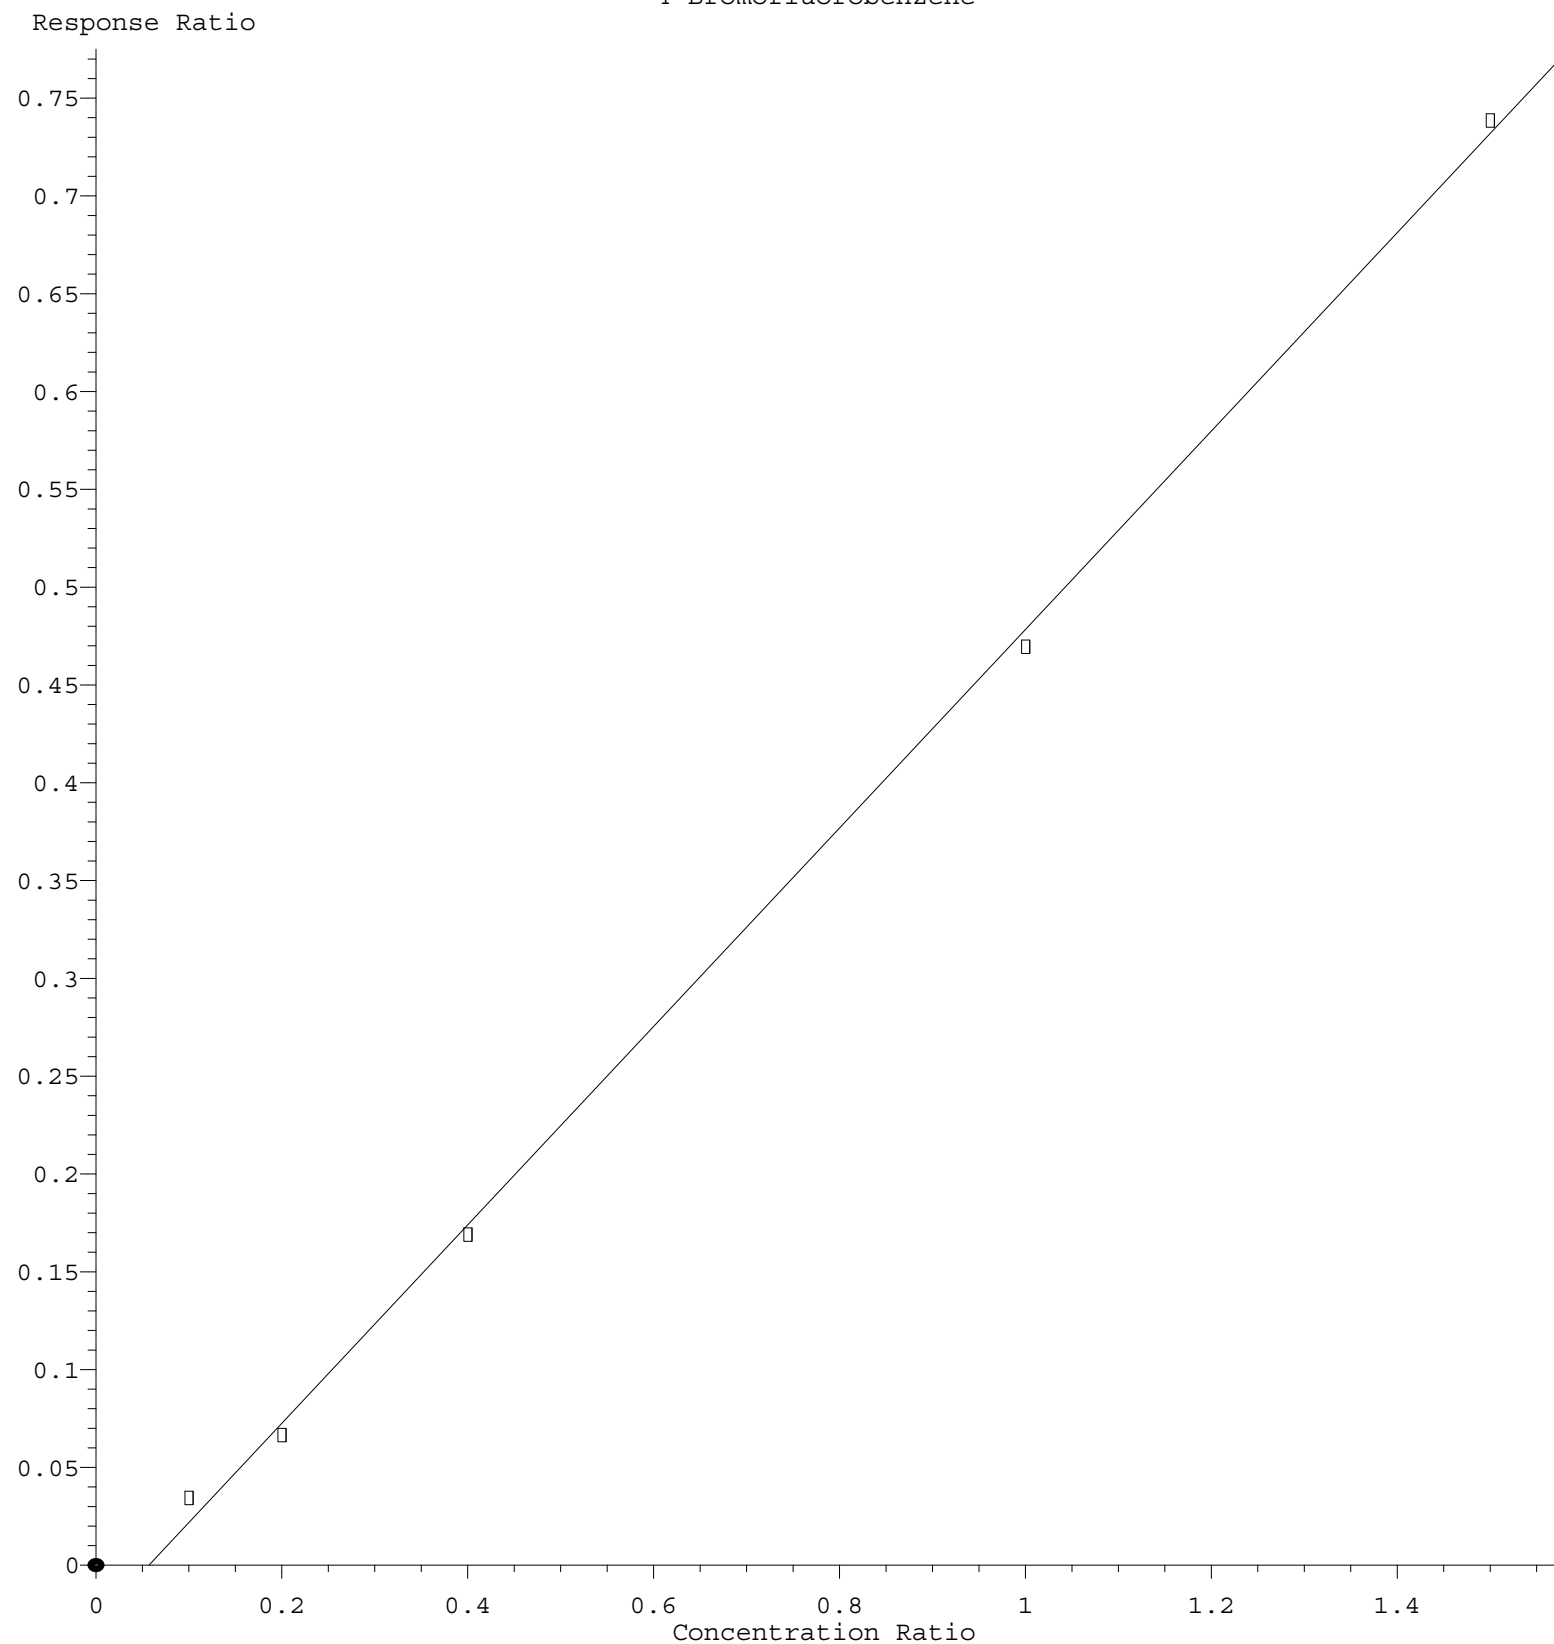

Response = $5.069 \times 10^{-1} \times \text{Amt} - 2.884 \times 10^{-2}$
Coef of Det (r^2) = 0.999061 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090222W.M
Calibration Table Last Updated: Sat Sep 03 04:35:33 2022

1,4-Dichlorobenzene

Response Ratio

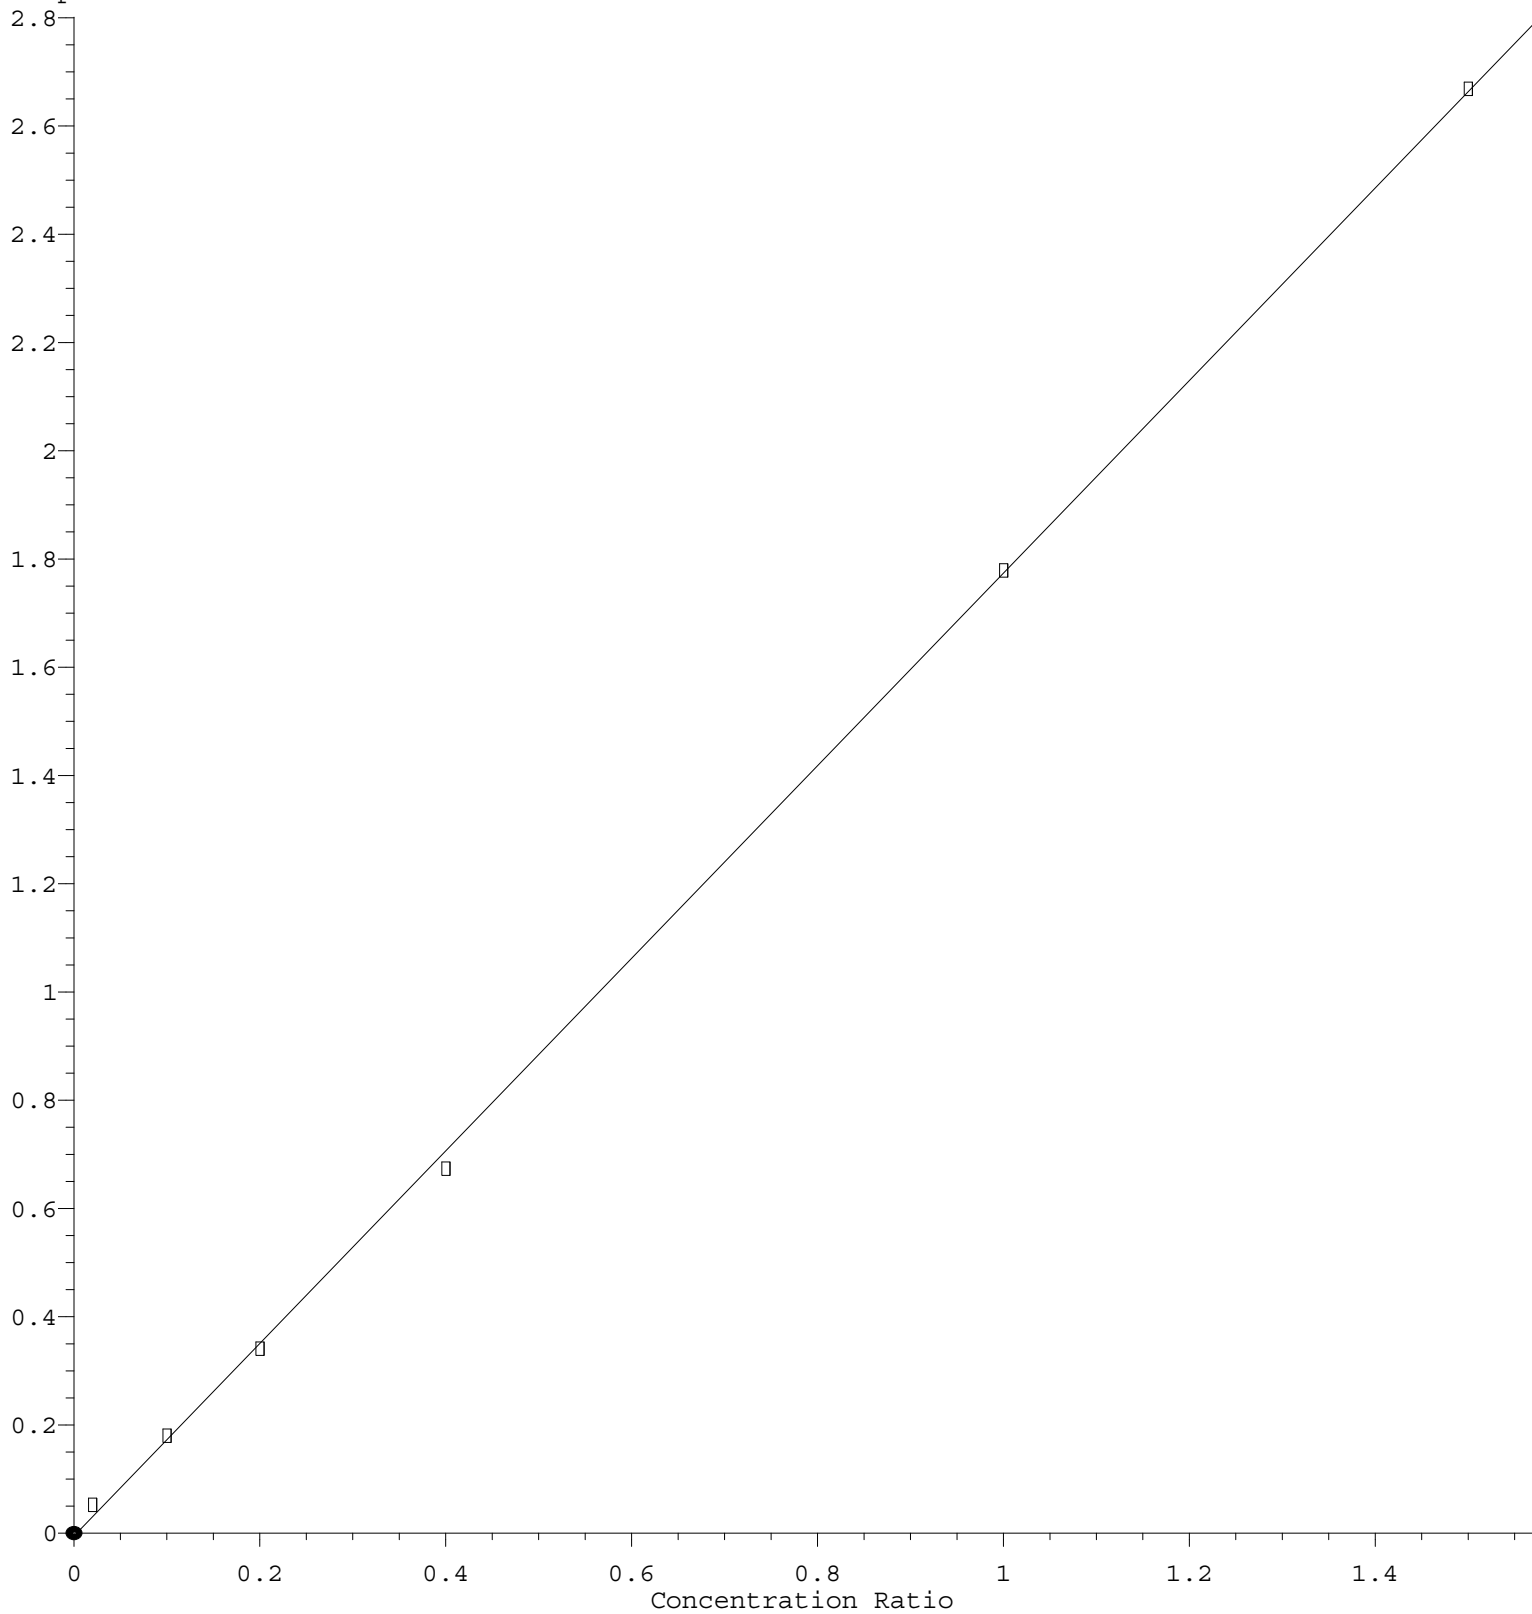

$$\text{Response} = 1.779\text{e}+000 * \text{Amt} - 5.888\text{e}-003$$


Coef of Det (r^2) = 0.999676 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090222W.M

Calibration Table Last Updated: Sat Sep 03 04:35:33 2022


1,2,4-Trichlorobenzene

Response Ratio

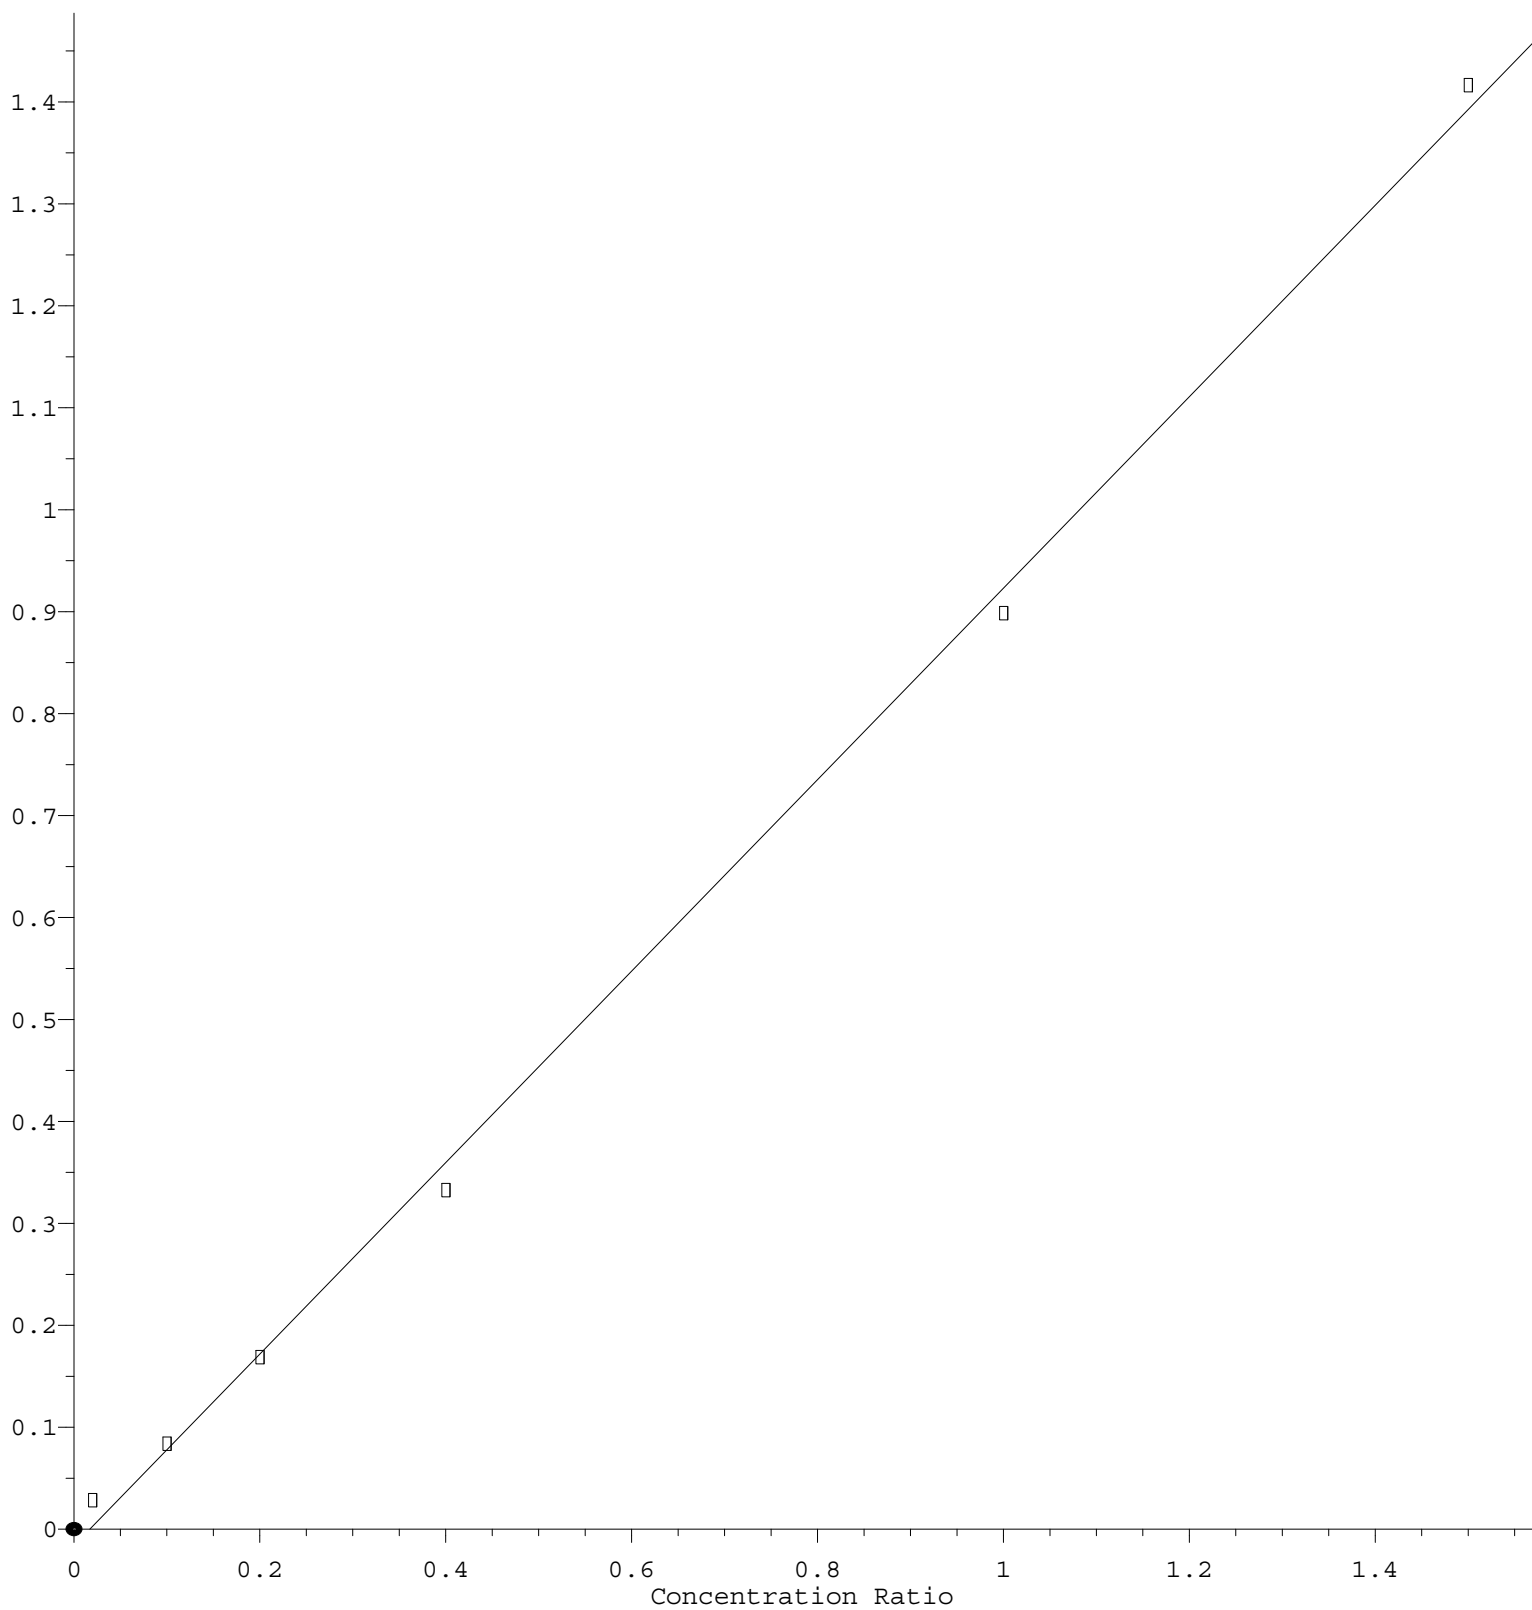

Response = $9.394 \times 10^{-1} \times \text{Amt} - 1.605 \times 10^{-2}$
Coef of Det (r^2) = 0.998303 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090222W.M
Calibration Table Last Updated: Sat Sep 03 04:35:33 2022


Hexachlorobutadiene

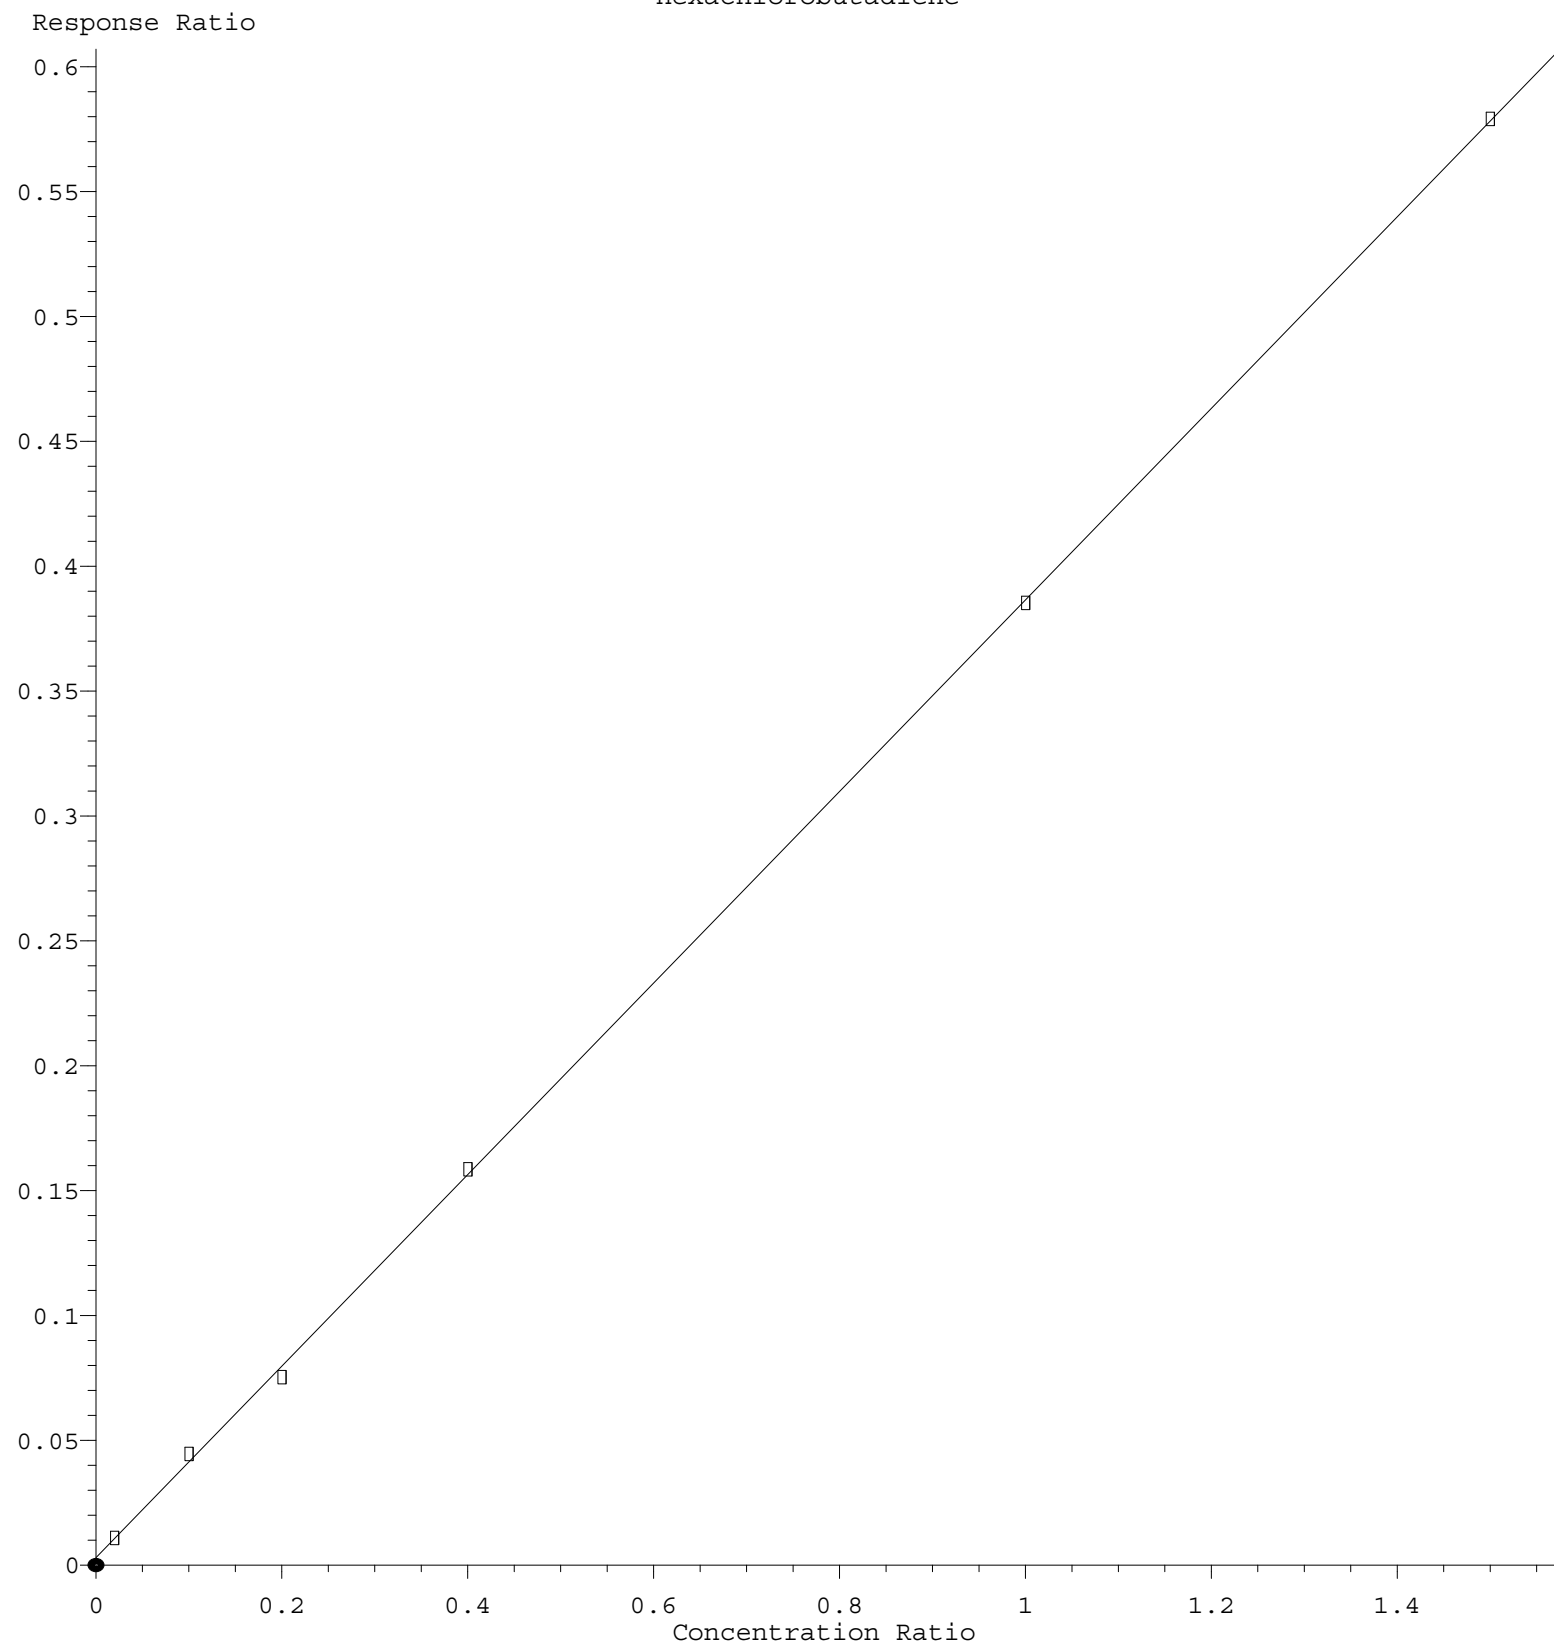

Response = $3.834 \times 10^{-1} \times \text{Amt} + 3.130 \times 10^{-3}$
Coef of Det (r^2) = 0.999859 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090222W.M
Calibration Table Last Updated: Sat Sep 03 04:35:33 2022

Naphthalene

Response Ratio

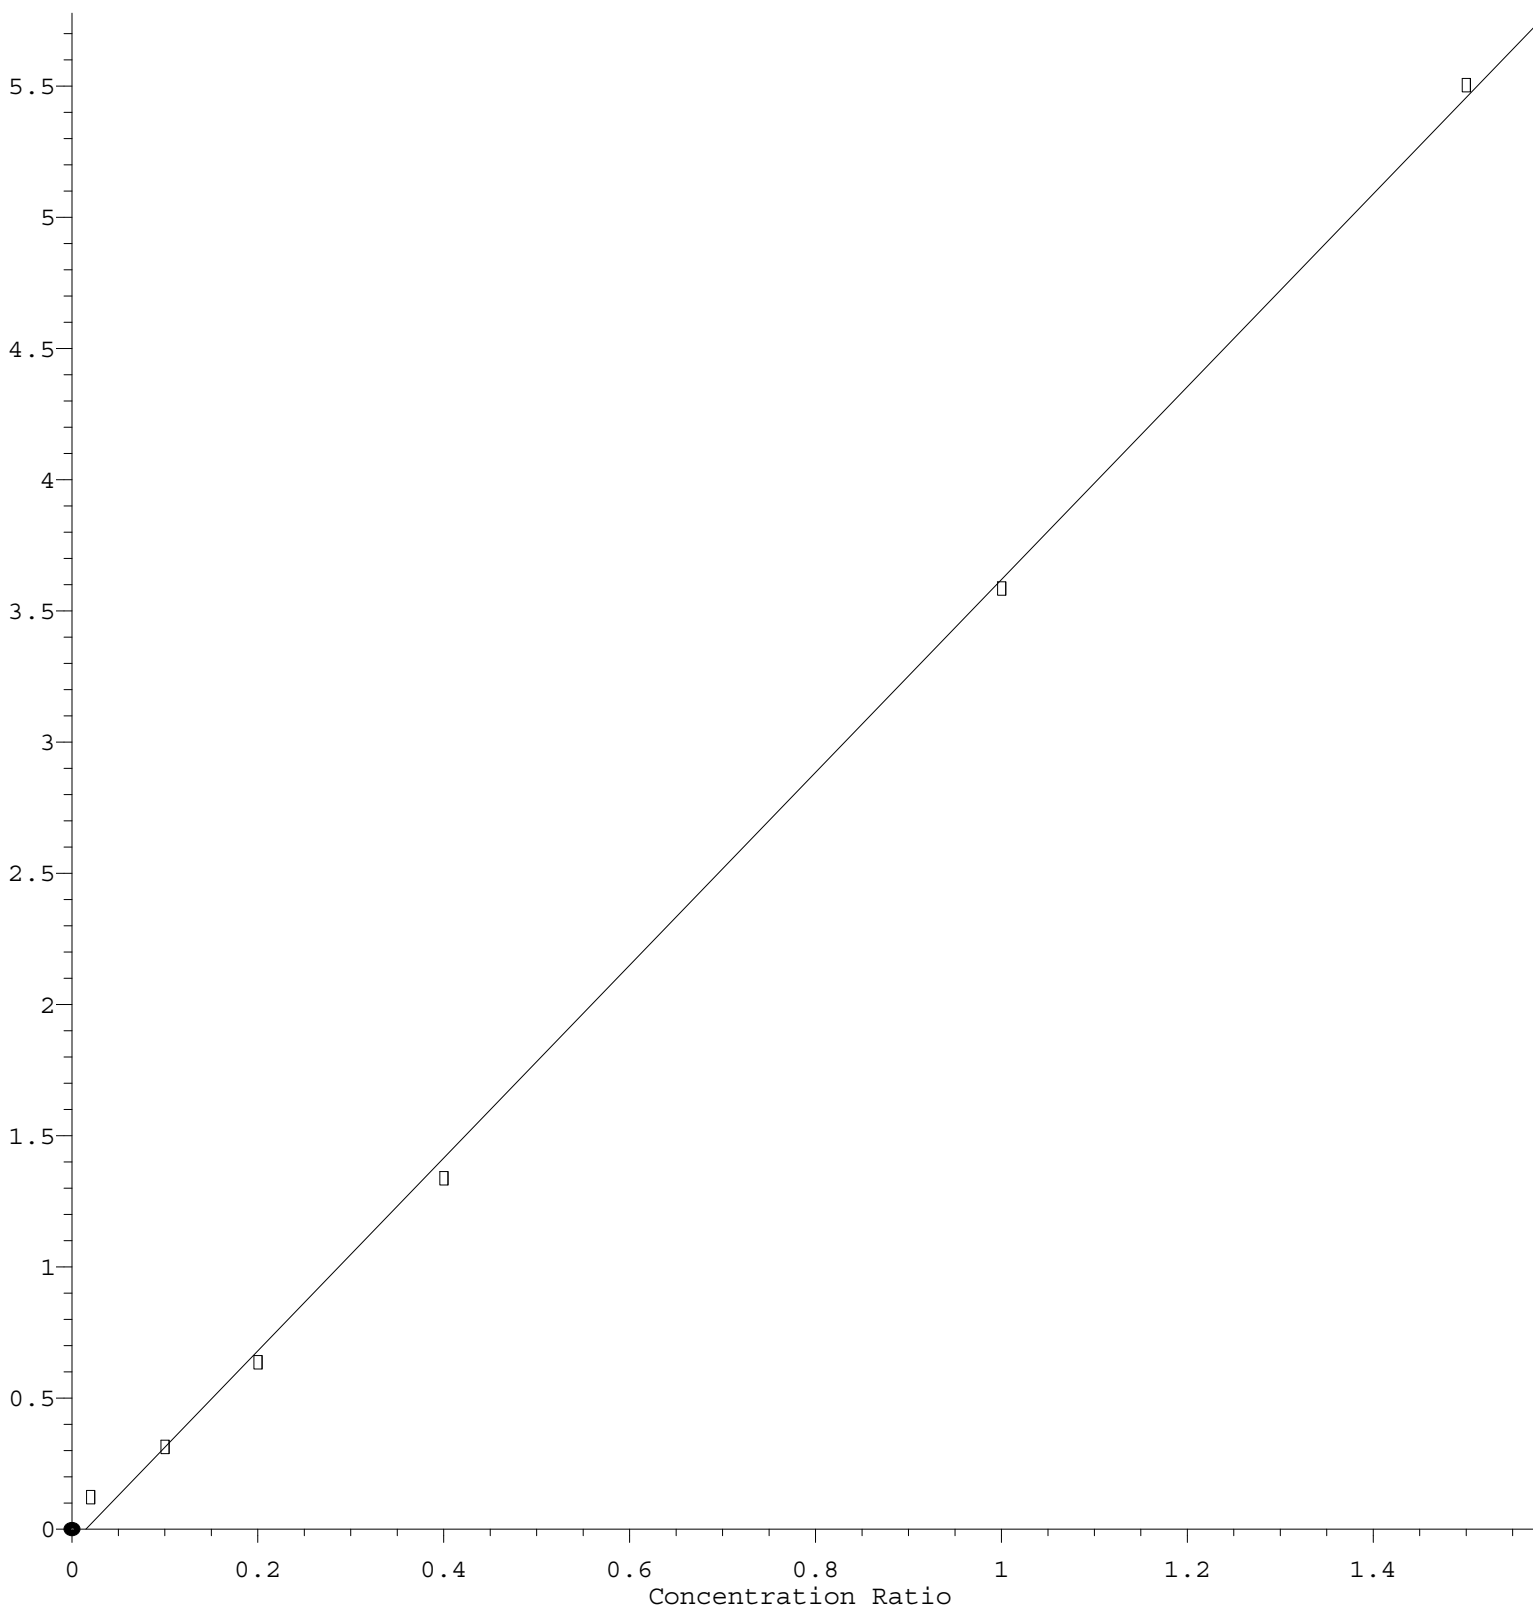

$$\text{Response} = 3.675\text{e}+000 * \text{Amt} - 5.611\text{e}-002$$


Coef of Det (r^2) = 0.999062 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090222W.M

Calibration Table Last Updated: Sat Sep 03 04:35:33 2022

1,2,3-Trichlorobenzene

Response Ratio

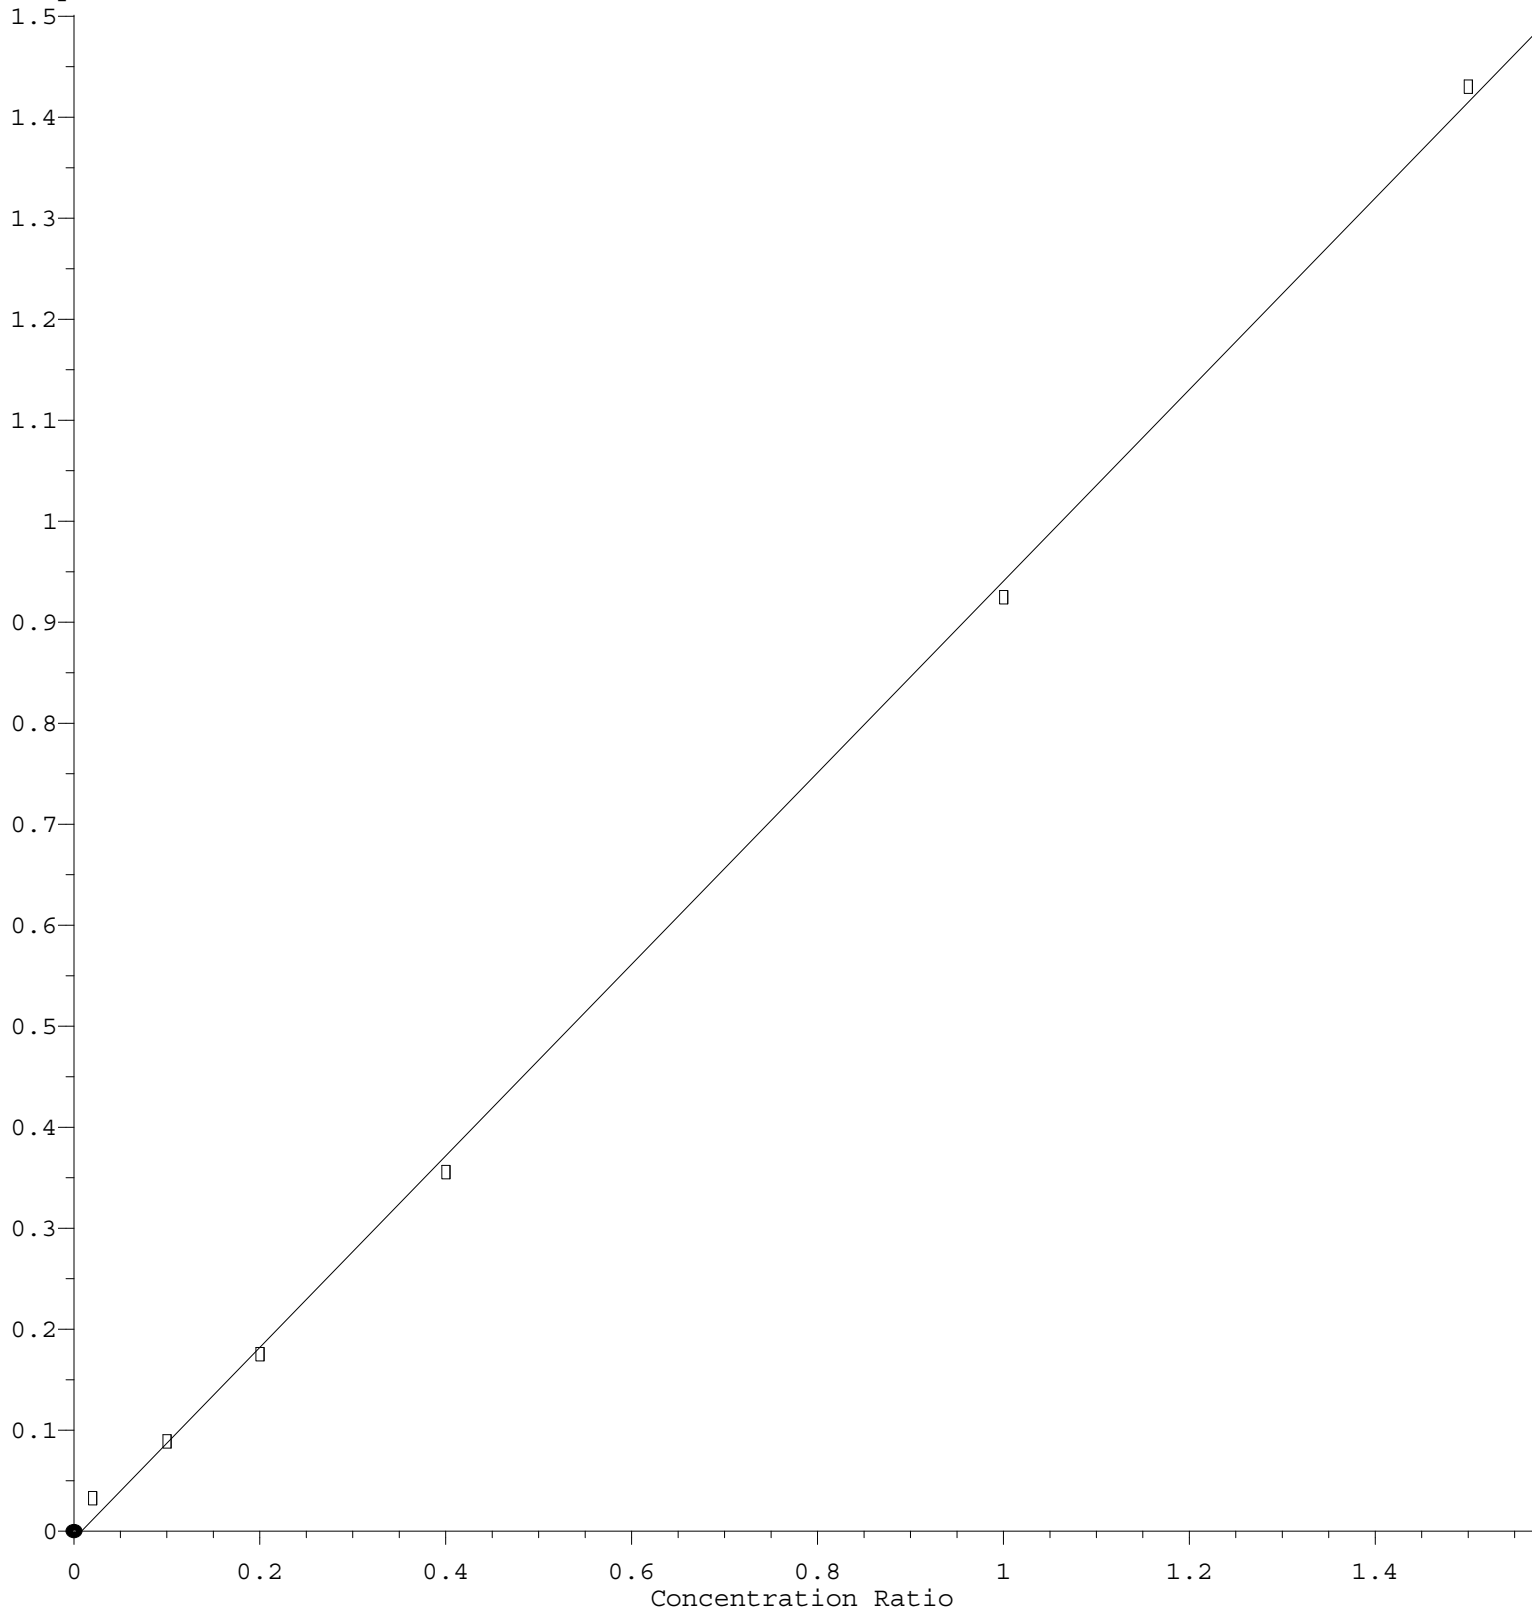

$$\text{Response} = 9.484\text{e-}001 * \text{Amt} - 7.825\text{e-}003$$

Coef of Det (r^2) = 0.999194 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090222W.M

Calibration Table Last Updated: Sat Sep 03 04:35:33 2022