

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090222\
 Data File : VN074308.D
 Acq On : 03 Sep 2022 00:38
 Operator : JC\MD
 Sample : N4355-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-42

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090222W.M

Title : SW846 8260

Signal : TIC: VN074308.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.299	62	70	72	rBV4	7266	16762	1.19%	0.204%
2	2.351	72	79	80	rBV3	10043	18220	1.30%	0.222%
3	2.704	132	139	149	rVB4	67607	186014	13.23%	2.263%
4	7.951	1020	1031	1036	rBV	217185	509105	36.20%	6.194%
5	8.016	1036	1042	1057	rVB	339135	779151	55.41%	9.479%
6	8.375	1091	1103	1118	rBV	228117	508477	36.16%	6.186%
7	8.904	1184	1193	1205	rBV2	524638	1057367	75.19%	12.864%
8	10.380	1435	1444	1457	rBV	772927	1406206	100.00%	17.108%
9	11.680	1657	1665	1681	rBV	780945	1368264	97.30%	16.646%
10	12.668	1826	1833	1843	rVB	660857	1060617	75.42%	12.904%
11	13.610	1986	1993	2001	rBV	812952	1309407	93.12%	15.930%




Sum of corrected areas: 8219590

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090222\
Data File : VN074308.D
Acq On : 03 Sep 2022 00:38
Operator : JC\MD
Sample : N4355-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

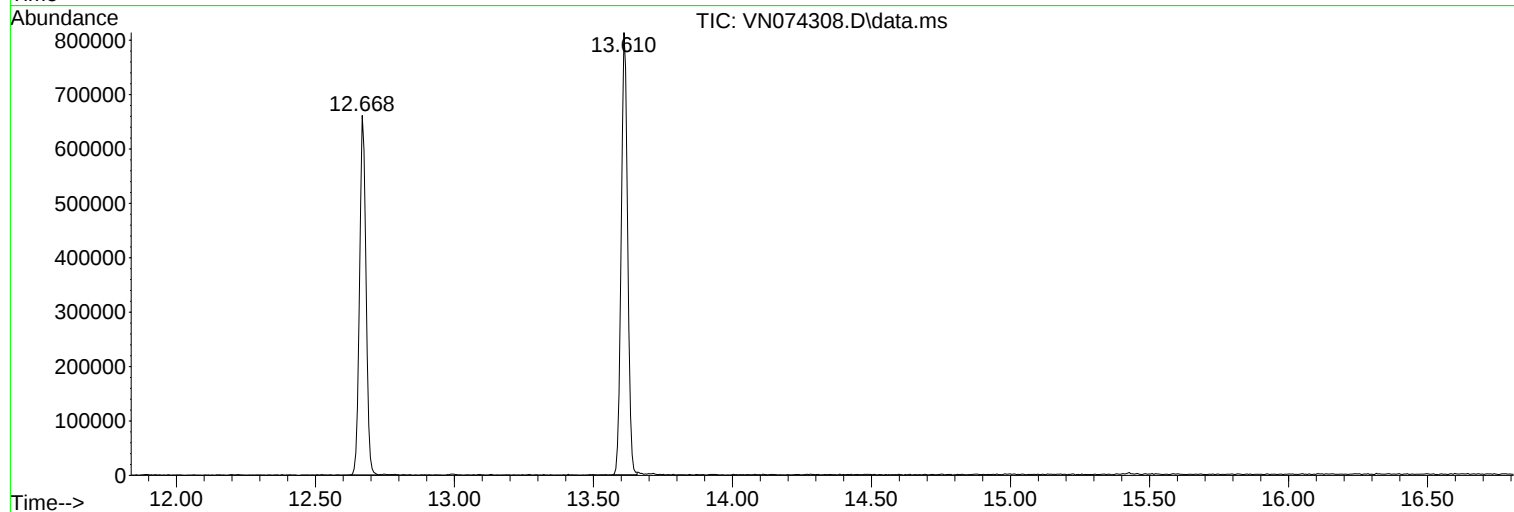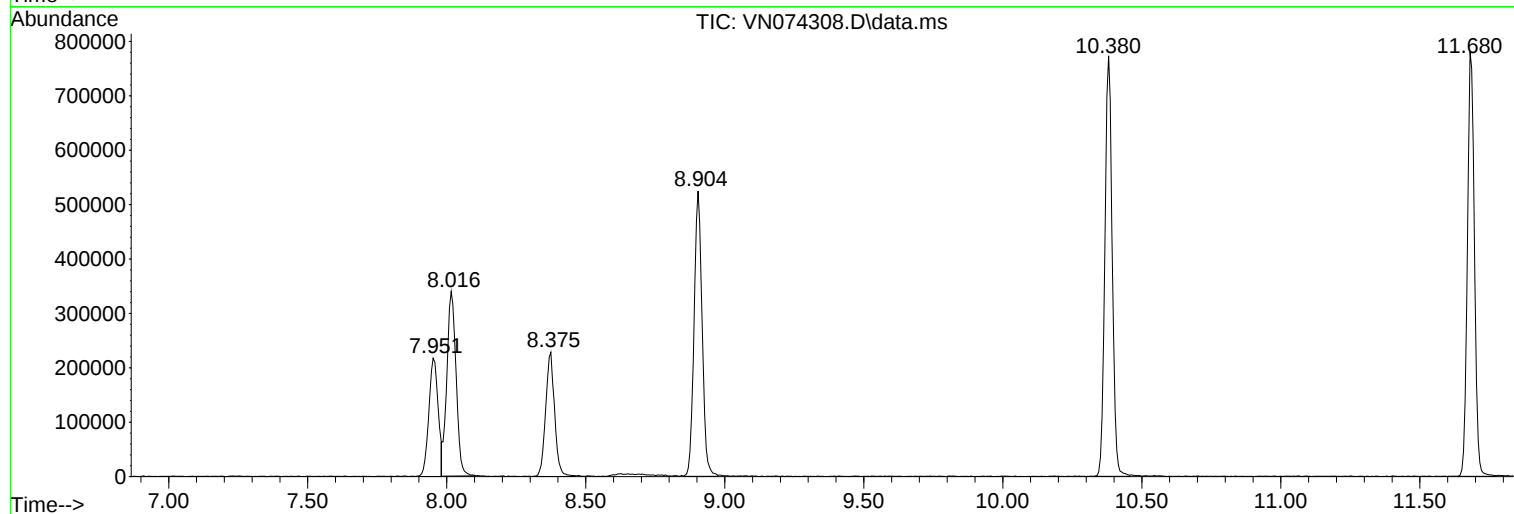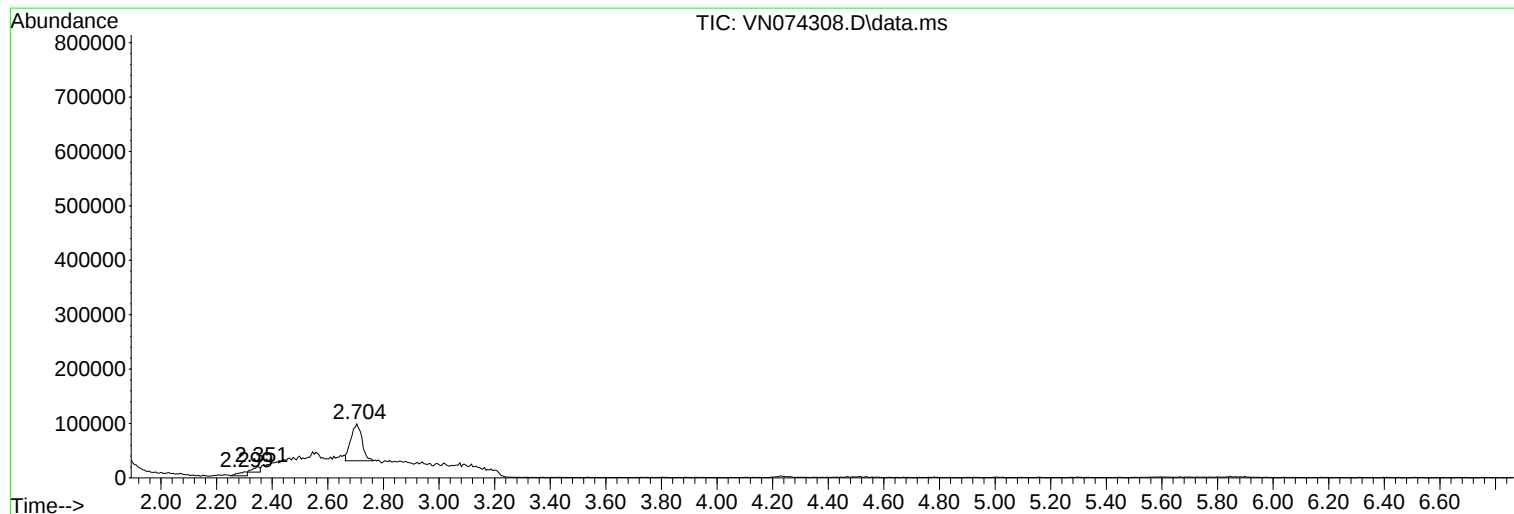

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090222\
Data File : VN074308.D
Acq On : 03 Sep 2022 00:38
Operator : JC\MD
Sample : N4355-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 31 Sample Multiplier: 1










Instrument :
MSVOA_N
ClientSampleId :
MW-42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 tert-Butyl isopropyl disulf... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
2.704	11.94 ug/l	186014	Pentafluorobenzene	8.016	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	tert-Butyl isopropyl disulfide, ...	452	C7F16S2	1000226-69-7	64
2	Ethyl Chloride	64	C2H5Cl	000075-00-3	45
3	Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	43
4	Methanesulfonamide, 1-chloro-	129	CH4ClNO2S	021335-43-3	38
5	Sulfur dioxide	64	O2S	007446-09-5	37

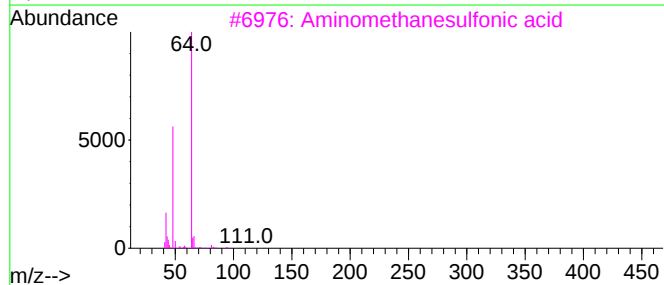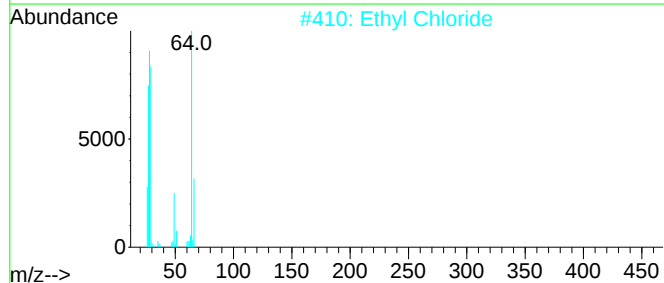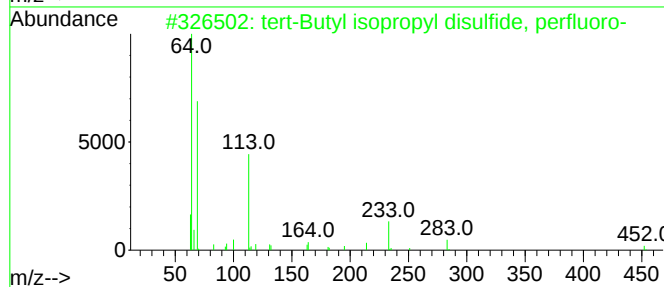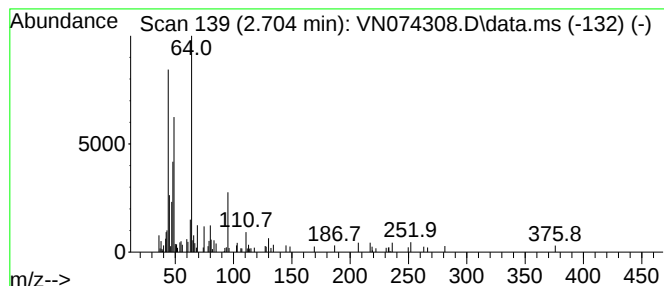

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090222\
Data File : VN074308.D
Acq On : 03 Sep 2022 00:38
Operator : JC\MD
Sample : N4355-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
tert-Butyl isop...	2.704	11.9	ug/l	186014	1	8.016	779151	50.0