


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090222\
 Data File : VN074289.D
 Acq On : 02 Sep 2022 16:17
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090222W.M
 Title : SW846 8260
 Last Update : Sat Sep 03 04:35:33 2022

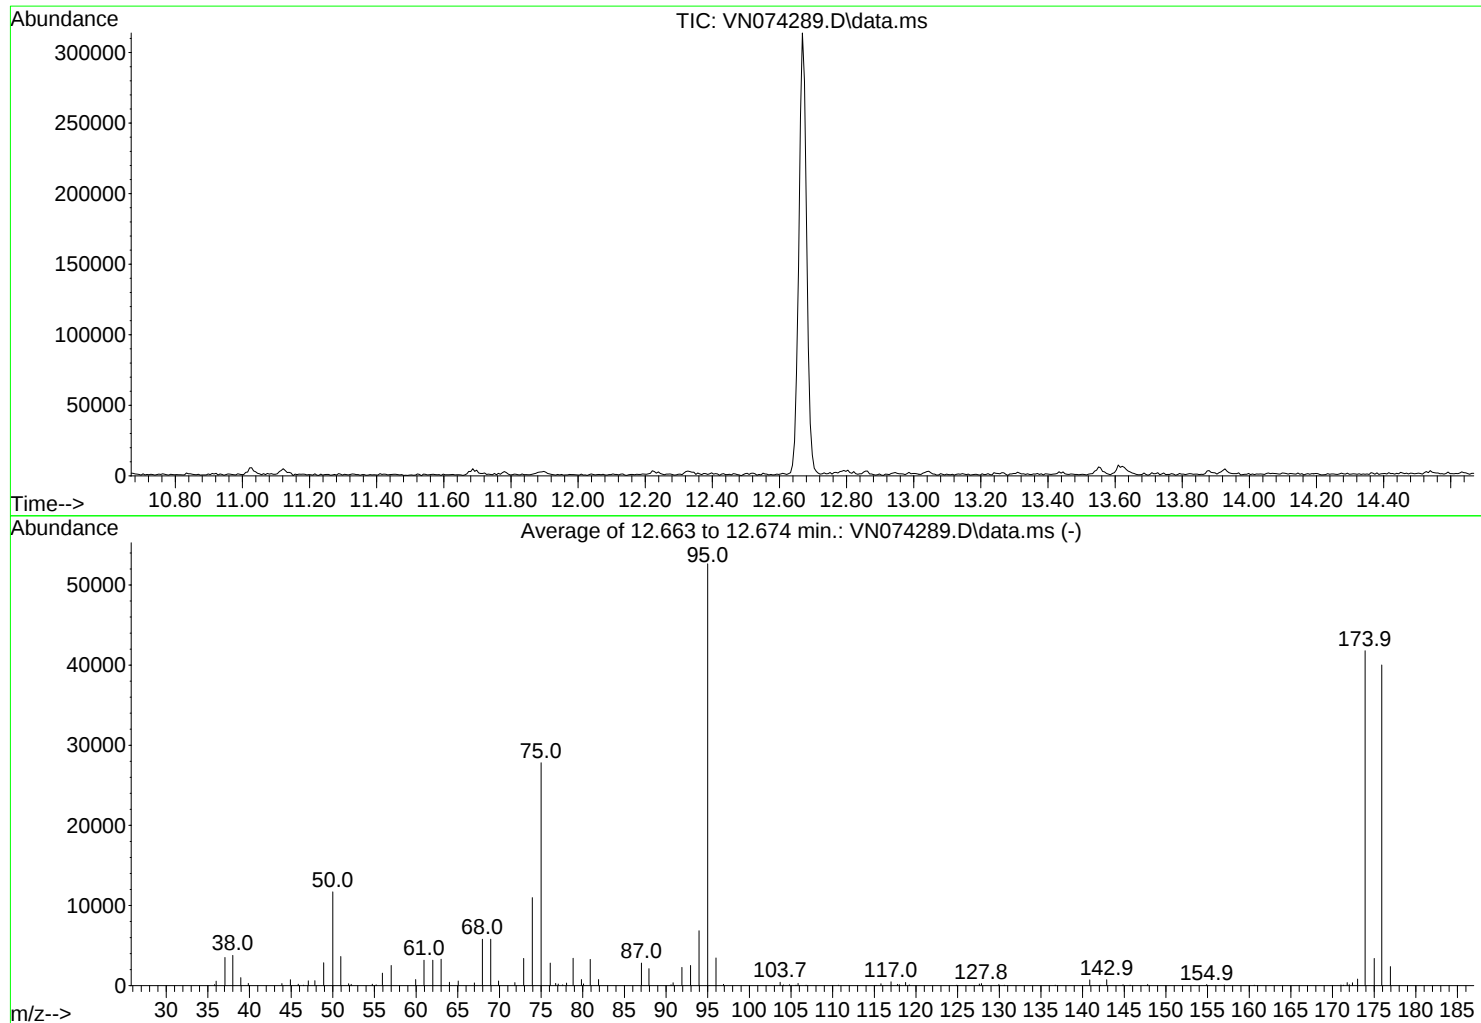

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	11702	PASS
75	95	30	60	52.8	27811	PASS
95	95	100	100	100.0	52640	PASS
96	95	5	9	6.6	3464	PASS
173	174	0.00	2	1.9	810	PASS
174	95	50	100	79.4	41787	PASS
175	174	5	9	8.1	3396	PASS
176	174	95	101	95.8	40019	PASS
177	176	5	9	5.9	2378	PASS