
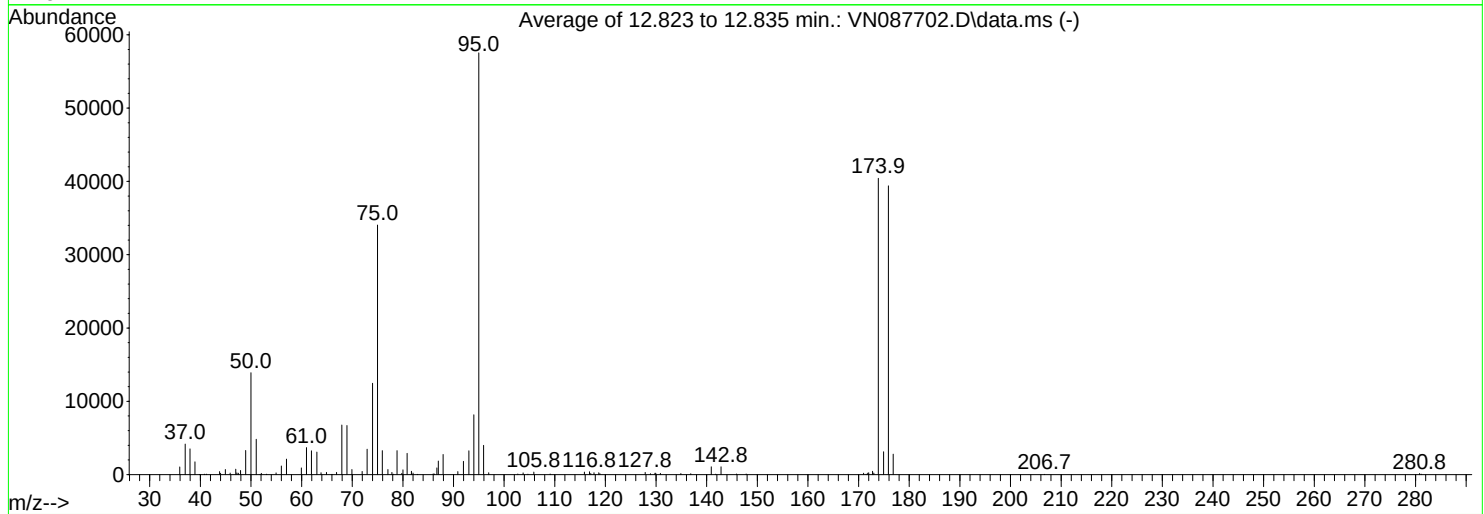


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN087702\
Data File : VN087702.D
Acq On : 02 Sep 2025 09:28
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
Title : SW846 8260
Last Update : Fri Aug 22 02:55:42 2025

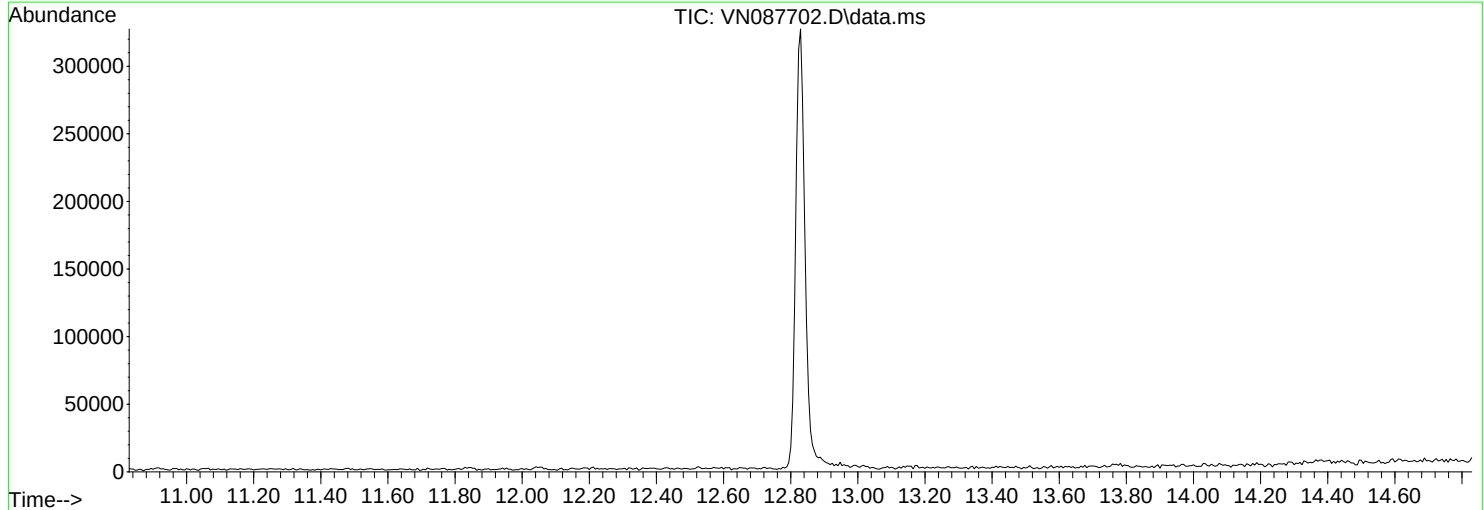

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.2	13915	PASS
75	95	30	60	59.2	34056	PASS
95	95	100	100	100.0	57536	PASS
96	95	5	9	6.9	3989	PASS
173	174	0.00	2	1.1	464	PASS
174	95	50	100	70.3	40427	PASS
175	174	5	9	7.7	3116	PASS
176	174	95	101	97.4	39395	PASS
177	176	5	9	7.1	2799	PASS

Average of 12.823 to 12.835 min.: VN087702.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	1049	47.00	748	56.00	1171	68.95	670
37.00	4172	47.20	241	57.00	2114	69.95	69
37.95	3507	47.50	200	59.95	916	71.95	43
38.95	1750	47.95	570	60.95	3684	72.95	346
39.85	31	48.95	3302	61.95	3256	74.00	12469
40.80	74	50.00	13915	63.00	3082	75.00	34056
41.20	75	51.05	4819	63.85	272	75.95	3264
43.80	427	51.80	52	64.90	305	77.05	705
44.00	183	52.05	178	66.00	51	77.85	298
44.95	703	53.10	58	66.90	296	78.10	70
45.90	210	54.95	249	67.95	6770	78.85	3268

Average of 12.823 to 12.835 min.: VN087702.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.80	173	90.85	416	109.10	85	130.85	175
80.00	651	91.95	1810	115.85	342	134.90	144
80.85	2912	93.05	3244	116.85	397	136.85	133
81.70	458	94.00	8165	117.10	153	140.90	1060
82.00	214	95.00	57536	117.75	259	141.80	71
82.90	50	95.95	3989	118.70	262	142.85	1071
86.00	111	96.95	254	118.90	125	145.90	97
86.20	85	102.70	81	127.85	315	147.80	89
86.70	913	103.75	245	128.90	140	171.00	208
87.00	1859	104.70	63	129.80	199	171.50	67
87.95	2744	105.85	354	129.95	198	171.80	208

Average of 12.823 to 12.835 min.: VN087702.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.00	272						
172.75	464						
173.00	221						
173.90	40427						
174.95	3116						
175.90	39395						
176.85	2799						
206.70	50						
280.80	147						
281.10	76						