

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN090319\
 Data File : VN057672.D
 Acq On : 3 Sep 2019 19:20
 Operator : JC/SP
 Sample : K4651-02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TT-006-IDW/GW-20190830

Quant Time: Sep 05 15:24:32 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA N\METHODS\624N090319W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Wed Sep 04 02:08:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	7.18	128	57649	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	8.58	114	347496	30.00	ug/l	0.00
57) Chlorobenzene-d5	11.41	117	263401	30.00	ug/l	0.00

System Monitoring Compounds

27) 1,2-Dichloroethane-d4	8.01	65	185118	30.21	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	100.70%
60) 4-Bromofluorobenzene	12.40	95	103345	22.97	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	76.57%
63) Toluene-d8	10.09	98	423772	33.41	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	111.37%


Target Compounds					Ovalue
37) Trichloroethene	8.83	130	34192	9.034 ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN090319\
Data File : VN057672.D
Acq On : 3 Sep 2019 19:20
Operator : JC/SP
Sample : K4651-02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TT-006-IDW/GW-20190830

Quant Time: Sep 05 15:24:32 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA N\METHODS\624N090319W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Wed Sep 04 02:08:50 2019
Response via : Initial Calibration

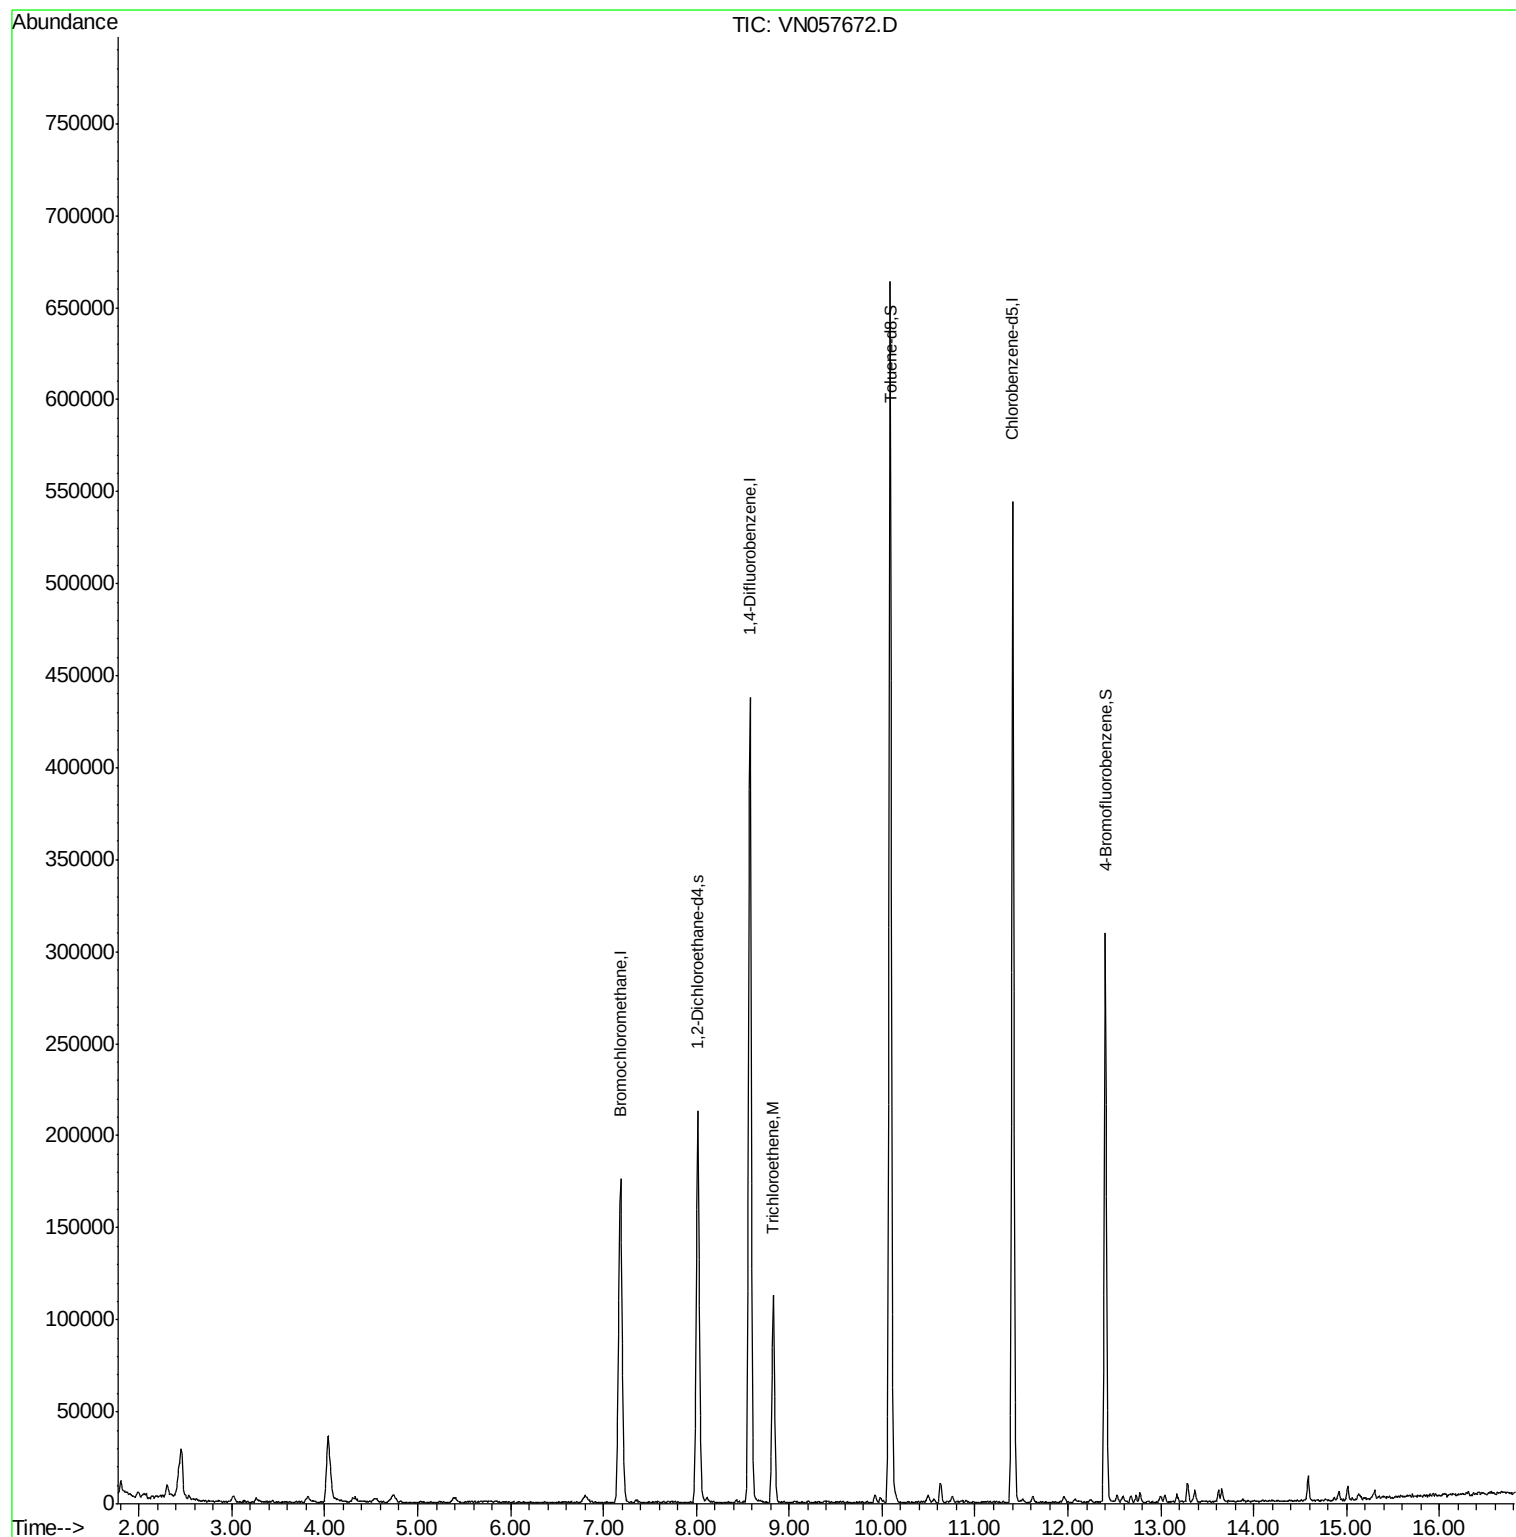

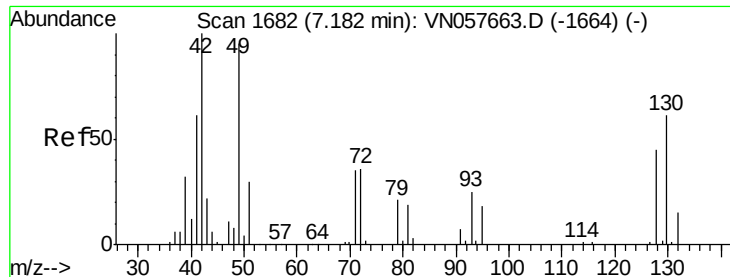

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 7.18 min Scan# 1683

Delta R.T. 0.00 min

Lab File: VN057672.D

Acq: 3 Sep 2019 19:20

Instrument :

MSVOA_N

ClientSampleId :

TT-006-IDW/GW-20190830


Tot Ion:128 Resp: 57649

Ion Ratio Lower Upper

128 100

49 207.3 0.0 544.5




130 131.8 0.0 324.7

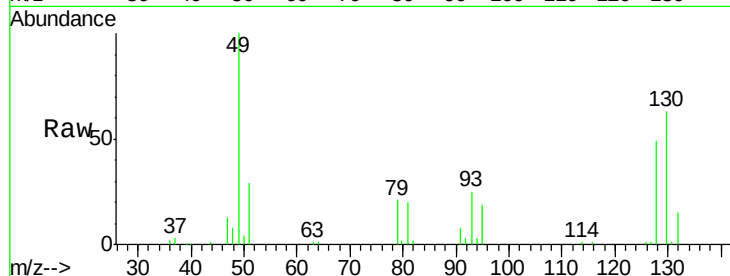

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VN0

Ion 130.00 (129.70 to 130.70): V

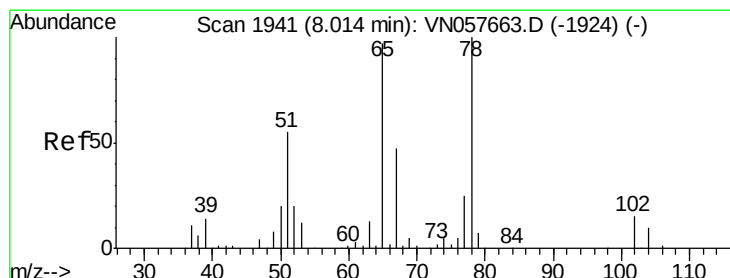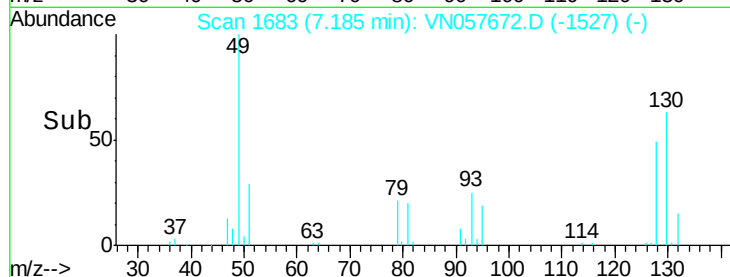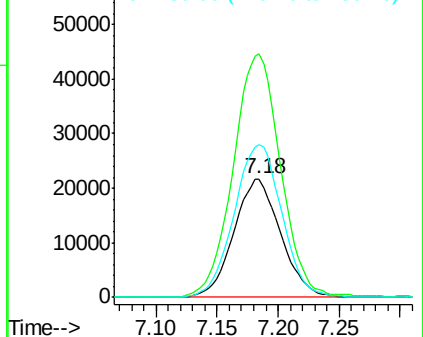

#27

1,2-Dichloroethane-d4

Concen: 30.207 ug/l

RT: 8.01 min Scan# 1941

Delta R.T. -0.00 min

Lab File: VN057672.D


Acq: 3 Sep 2019 19:20

Tgt Ion: 65 Resp: 185118

Ion Ratio Lower Upper



65 100


67 48.9 38.6 57.8

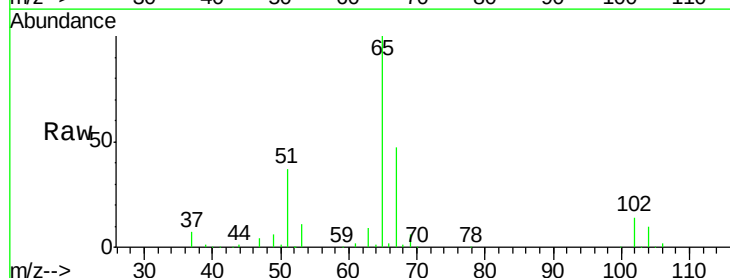

Abundance Ion 65.00 (64.70 to 65.70): VN0

Ion 67.00 (66.70 to 67.70): VN0



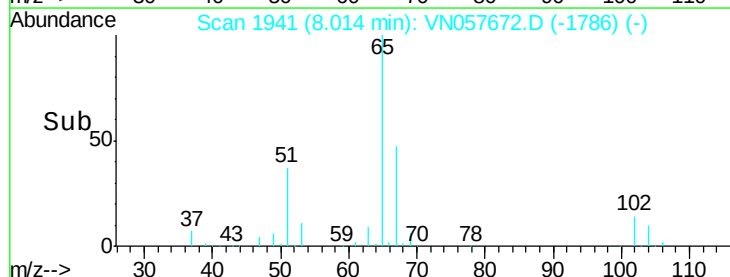
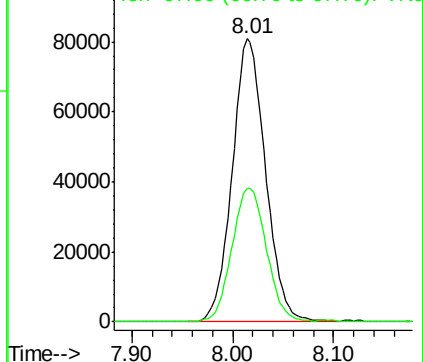


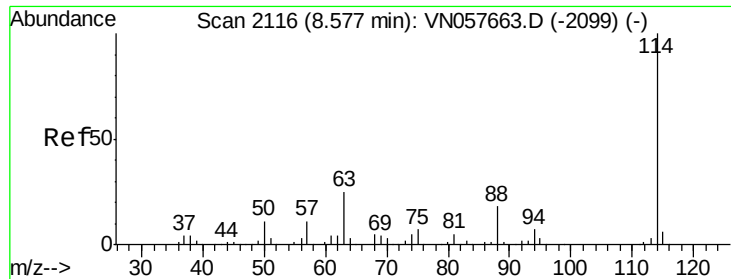

#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 8.58 min Scan# 2116
 Delta R.T. -0.00 min
 Lab File: VN057672.D
 Acq: 3 Sep 2019 19:20




Instrument :
 MSVOA_N
 ClientSampleId :
 TT-006-IDW/GW-20190830


Tot Ion:114 Resp: 347496
 Ion Ratio Lower Upper
 114 100
 63 25.5 20.6 30.8
 88 17.3 14.3 21.5

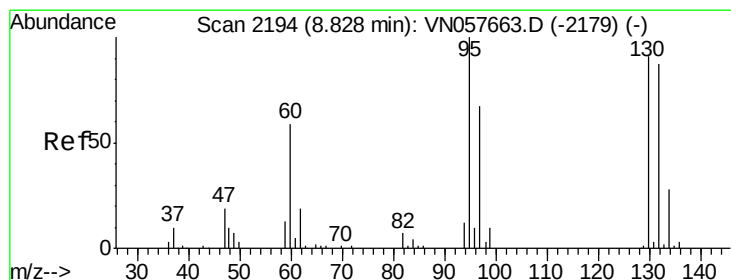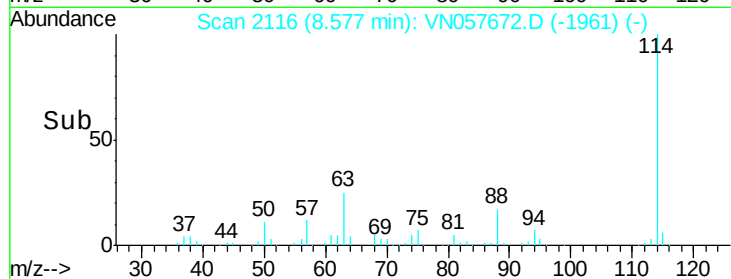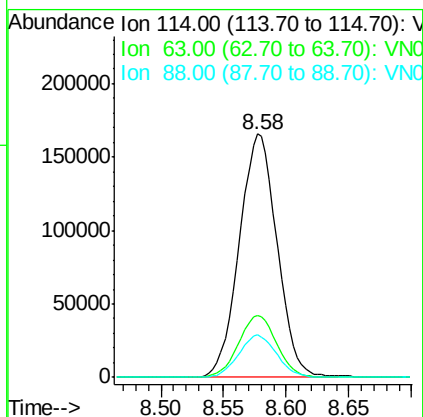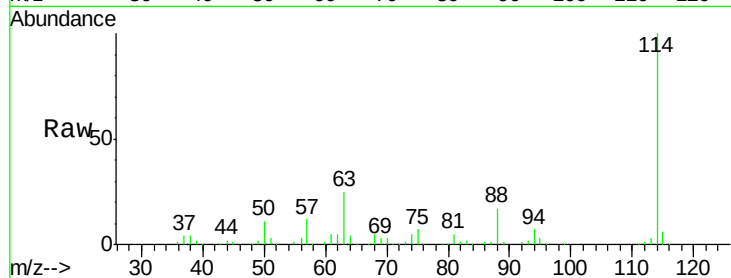

#37
 Trichloroethene
 Concen: 9.034 ug/l
 RT: 8.83 min Scan# 2195
 Delta R.T. 0.00 min
 Lab File: VN057672.D
 Acq: 3 Sep 2019 19:20

Tgt Ion:130 Resp: 34192
 Ion Ratio Lower Upper
 130 100
 95 105.5 87.5 131.3


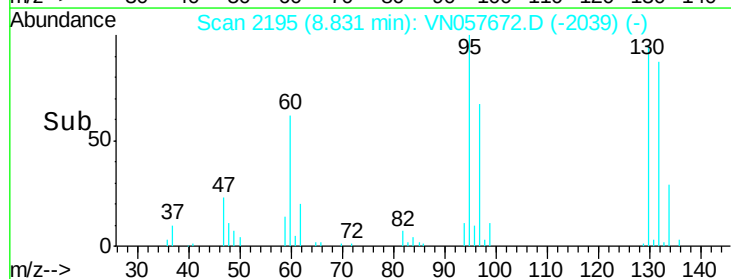
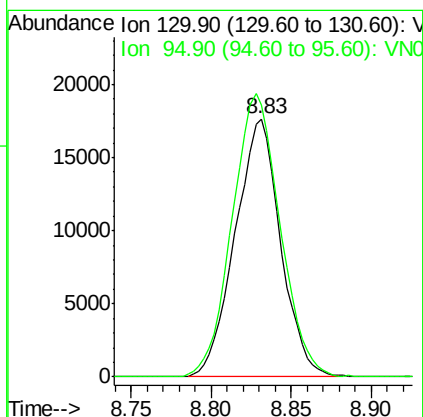
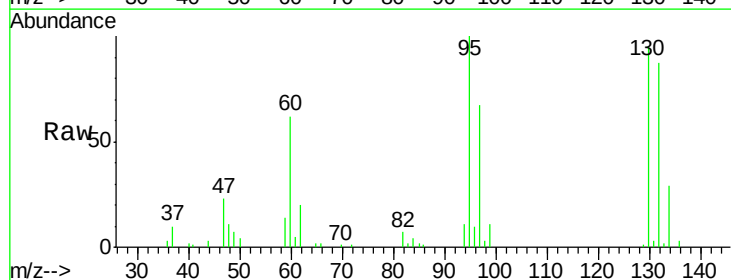


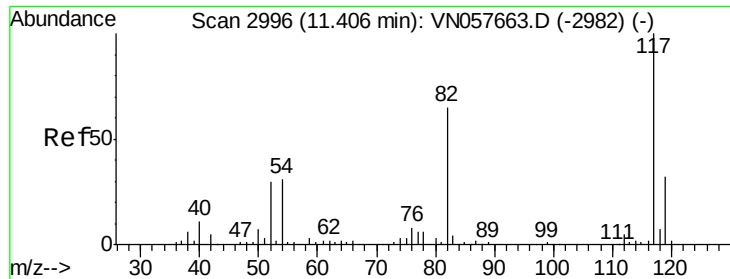

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. -0.00 min
Lab File: VN057672.D
Acq: 3 Sep 2019 19:20




Instrument :
MSVOA_N
ClientSampleId :
TT-006-IDW/GW-20190830


Tot Ion:117 Resp: 263401
Ion Ratio Lower Upper
117 100
82 64.3 51.2 76.8
119 31.5 25.8 38.6

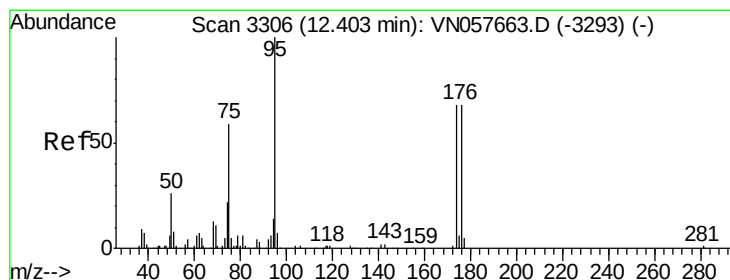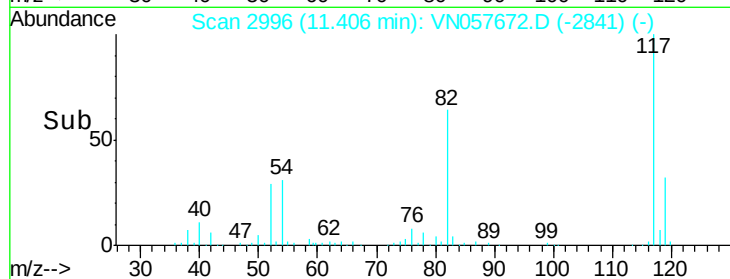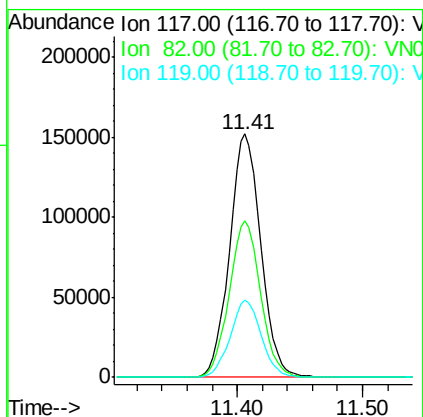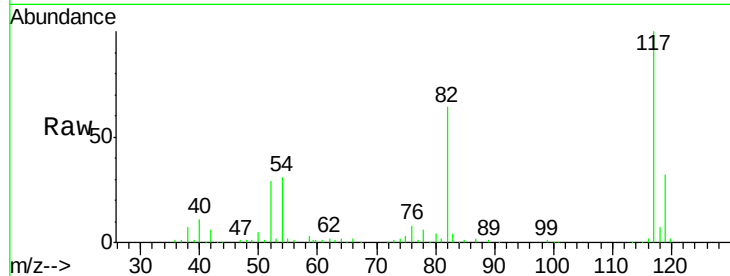

#60
4-Bromofluorobenzene
Concen: 22.965 ug/l
RT: 12.40 min Scan# 3306
Delta R.T. -0.00 min
Lab File: VN057672.D
Acq: 3 Sep 2019 19:20

Tgt Ion: 95 Resp: 103345
Ion Ratio Lower Upper
95 100
174 67.3 55.0 82.6
176 65.1 53.7 80.5

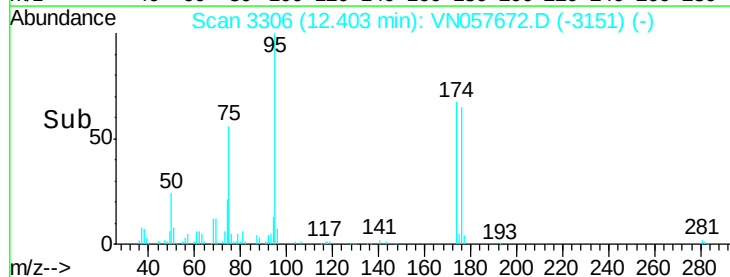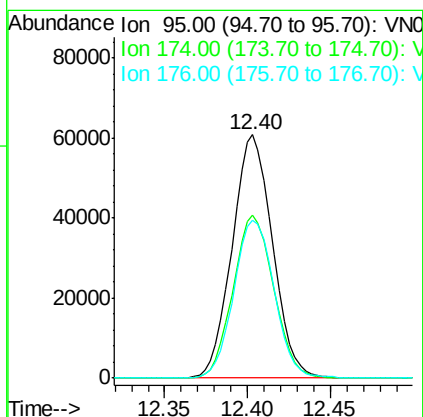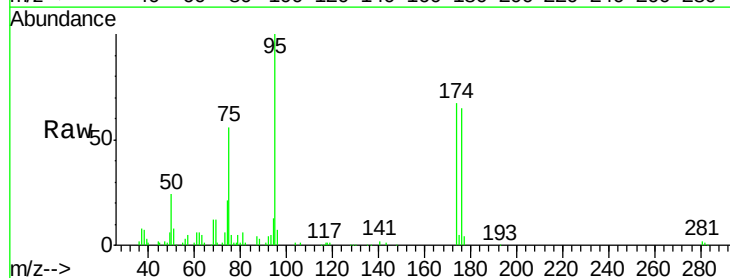

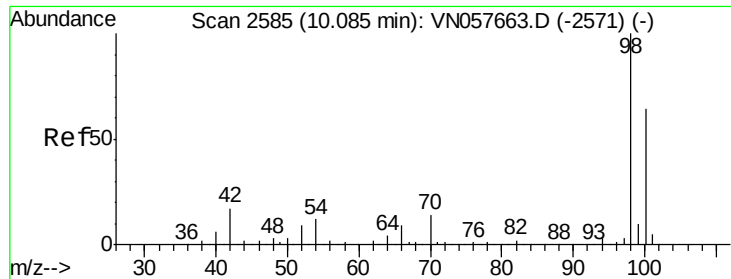

#63

Toluene-d8

Concen: 33.411 ug/l

RT: 10.09 min Scan# 2586

Delta R.T. 0.00 min

Lab File: VN057672.D

Acq: 3 Sep 2019 19:20

Instrument :

MSVOA_N

ClientSampleId :

TT-006-IDW/GW-20190830

Tot Ion: 98 Resp: 423772

Ion Ratio Lower Upper

98 100

100 63.3 51.0 76.6

