


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN090319\
Data File : VN057660.D
Acq On : 3 Sep 2019 10:40
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N090319W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Sep 04 02:08:50 2019

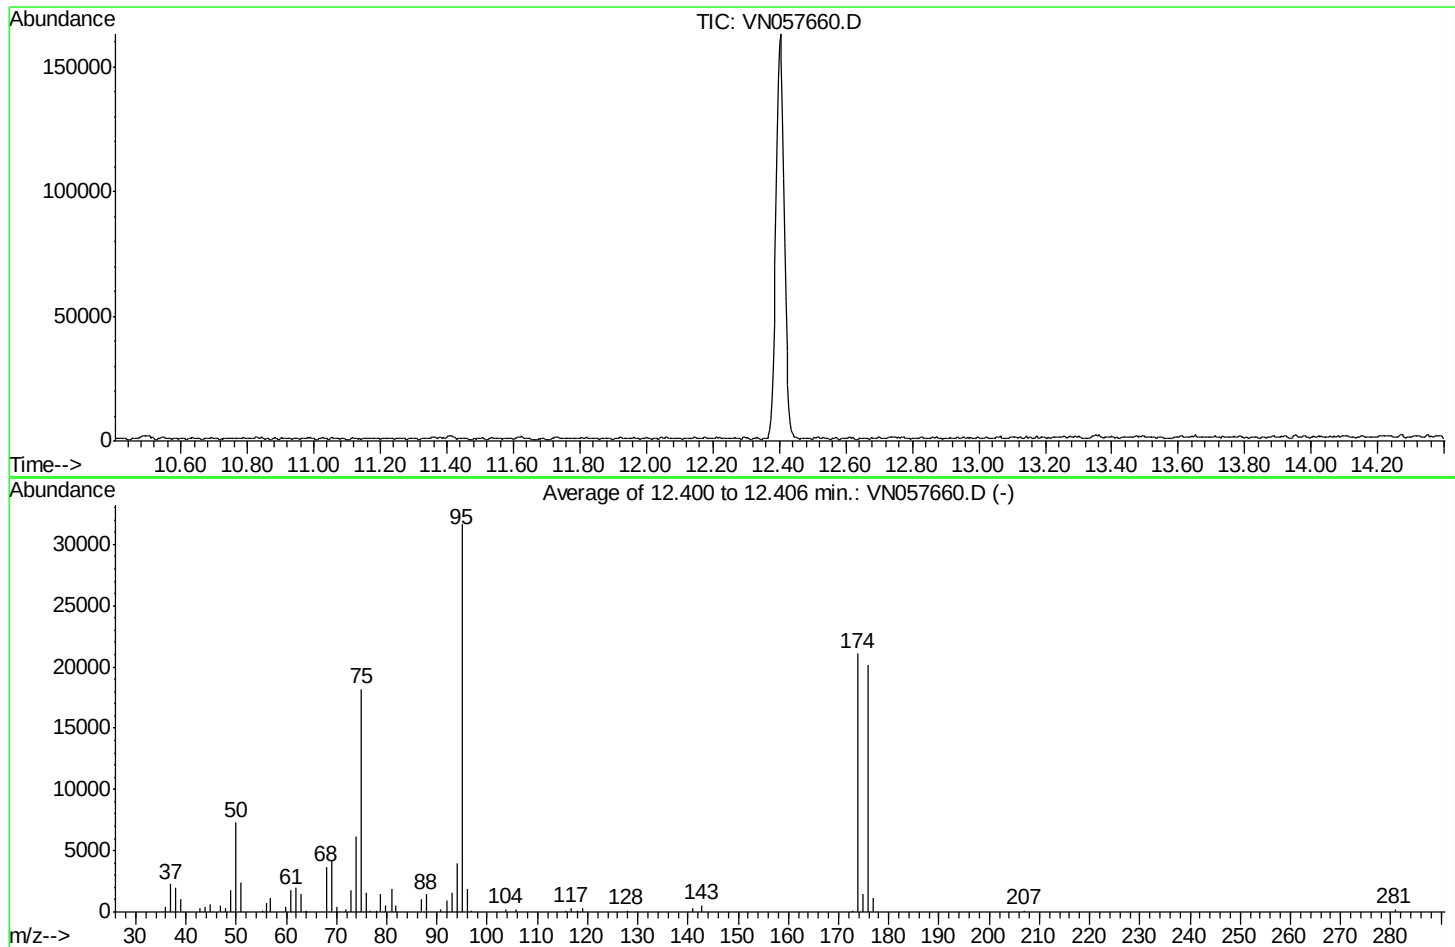

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	7295	PASS
75	95	30	60	57.5	18181	PASS
95	95	100	100	100.0	31632	PASS
96	95	5	9	6.0	1887	PASS
173	174	0.00	2	0.6	123	PASS
174	95	50	100	66.7	21090	PASS
175	174	5	9	7.0	1483	PASS
176	174	95	101	95.8	20210	PASS
177	176	5	9	5.9	1202	PASS