


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN090320\
Data File : VN063207.D
Acq On : 3 Sep 2020 8:54
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N083120W.M
Title : SW846 8260
Last Update : Tue Sep 01 04:21:28 2020

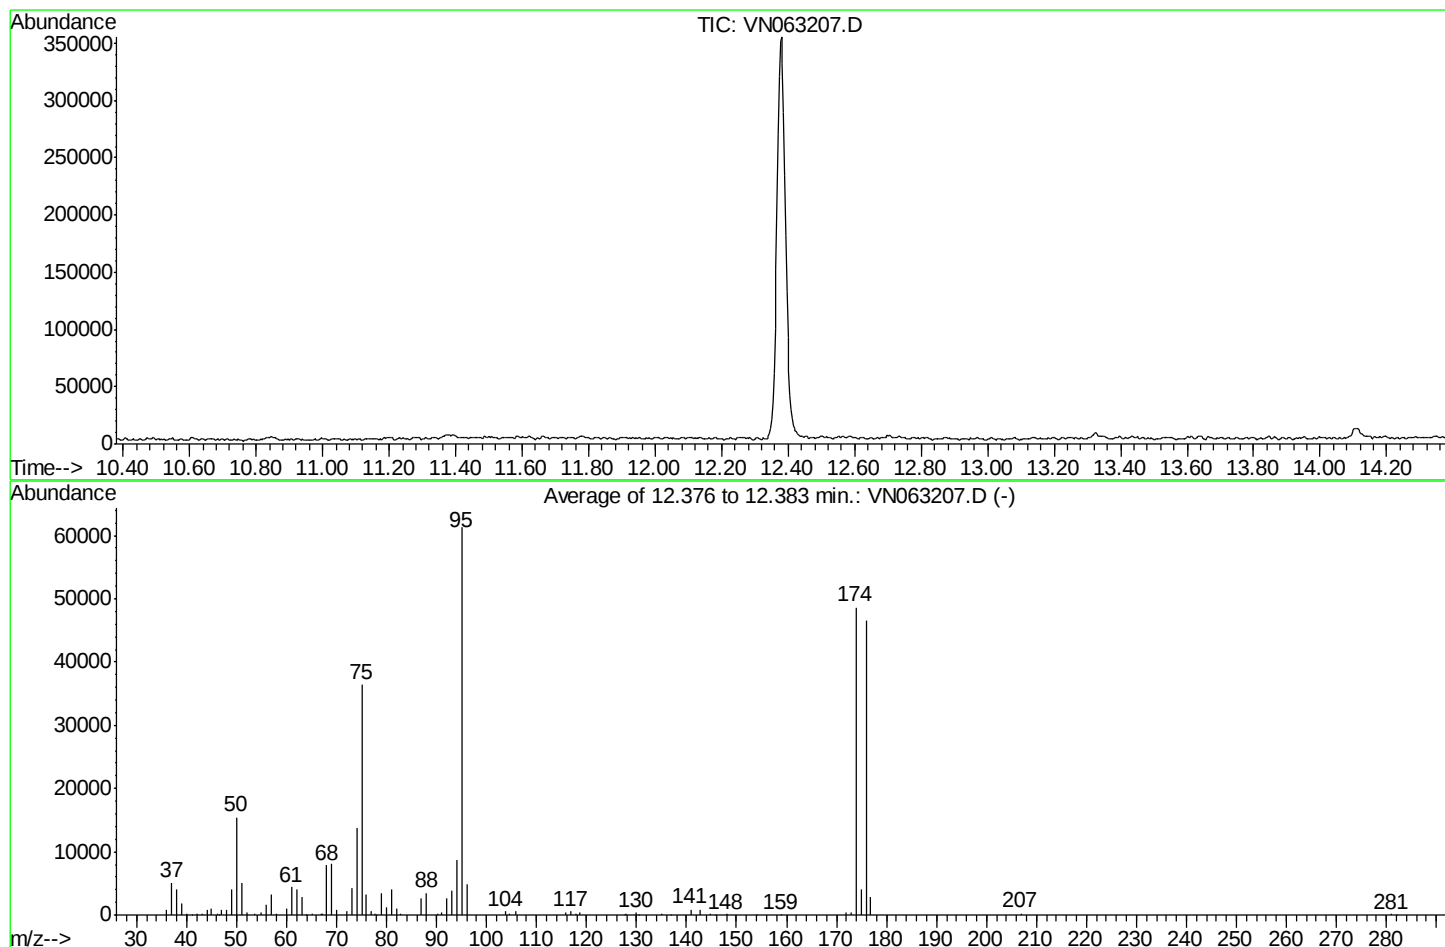

AutoFind: Scans 3308, 3309, 3310; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.2	15447	PASS
75	95	30	60	59.4	36410	PASS
95	95	100	100	100.0	61301	PASS
96	95	5	9	7.9	4867	PASS
173	174	0.00	2	0.7	325	PASS
174	95	50	100	79.3	48589	PASS
175	174	5	9	8.5	4123	PASS
176	174	95	101	96.0	46642	PASS
177	176	5	9	5.9	2774	PASS