
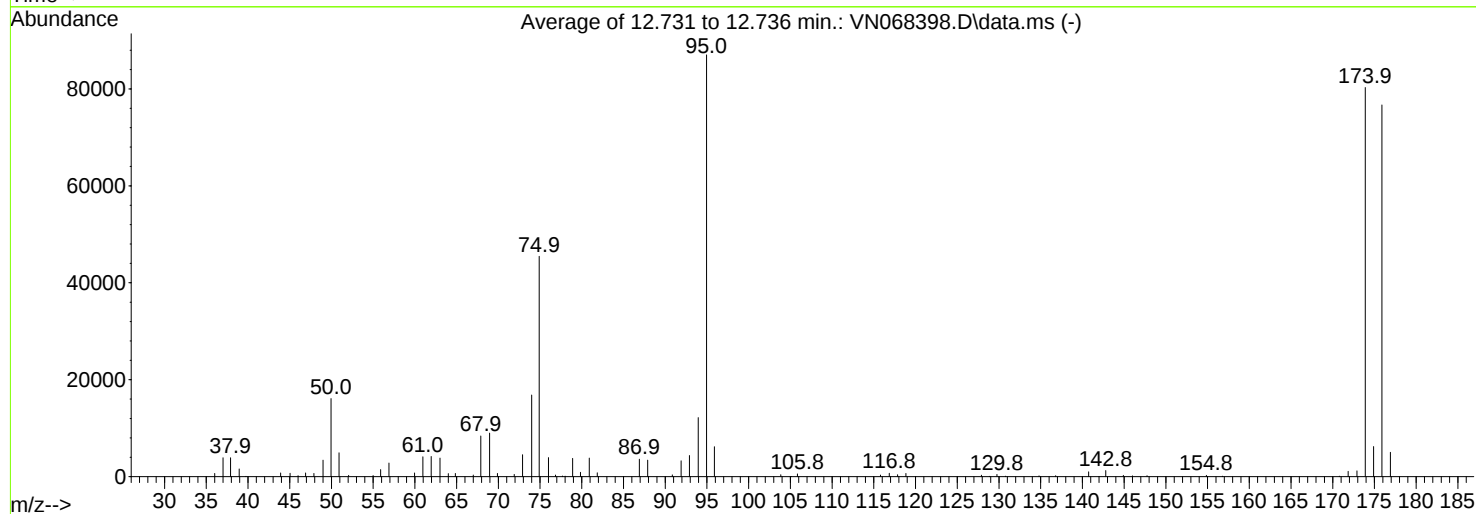


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090321\
 Data File : VN068398.D
 Acq On : 3 Sep 2021 9:13
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N090321W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Sep 03 13:24:01 2021

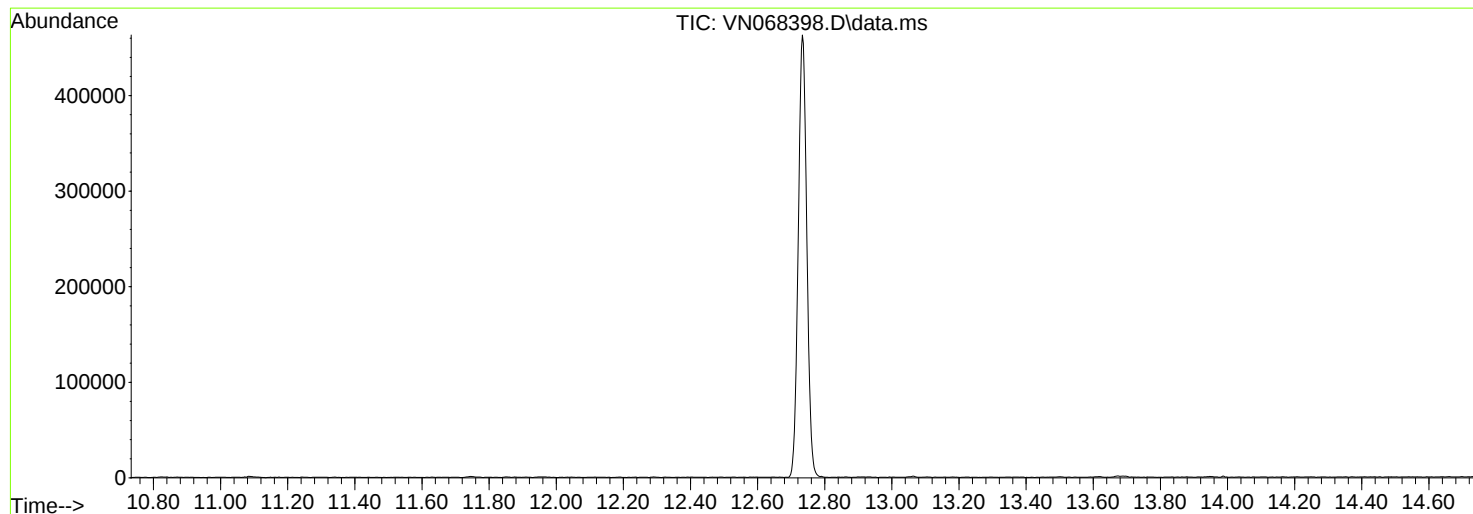

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	16105	PASS
75	95	30	60	52.2	45461	PASS
95	95	100	100	100.0	87035	PASS
96	95	5	9	7.1	6189	PASS
173	174	0.00	2	1.5	1176	PASS
174	95	50	100	92.3	80299	PASS
175	174	5	9	7.7	6200	PASS
176	174	95	101	95.5	76699	PASS
177	176	5	9	6.6	5024	PASS