

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090322\
 Data File : VN074323.D
 Acq On : 03 Sep 2022 17:44
 Operator : JC\MD
 Sample : N4355-08
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-16R

Quant Time: Sep 05 05:37:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090222W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 03 04:35:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.016	168	317105	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	584846	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	554857	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	258848	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	229046	46.336	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	92.680%		
35) Dibromofluoromethane	7.951	113	200037	51.616	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	103.240%		
50) Toluene-d8	10.381	98	685502	44.857	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	89.720%		
62) 4-Bromofluorobenzene	12.669	95	251097	45.194	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	90.380%		
Target Compounds						Qvalue
3) Chloromethane	2.275	50	10559	2.437	ug/l #	55
6) Chloroethane	2.693	64	162063	25.525	ug/l #	53
10) Methyl Iodide	4.346	142	91	5.075	ug/l #	44
11) Tert butyl alcohol	5.287	59	37653	41.986	ug/l	97
16) Acetone	4.228	43	31211	15.108	ug/l	96
17) Carbon Disulfide	4.457	76	4901	0.629	ug/l #	75
18) Methyl Acetate	4.793	43	1463	0.235	ug/l #	65
19) Methyl tert-butyl Ether	5.534	73	141835	11.464	ug/l	98
20) Methylene Chloride	5.022	84	1032	Below Cal	#	26
22) Diisopropyl ether	6.416	45	8825	0.749	ug/l #	91
23) Vinyl Acetate	6.404	43	4712	0.460	ug/l #	68
25) 2-Butanone	7.257	43	58941	16.896	ug/l	95
29) Tetrahydrofuran	7.628	42	556	0.250	ug/l #	70
31) Cyclohexane	8.022	56	9913	1.502	ug/l #	38
36) 1,1-Dichloropropene	8.022	75	28959	5.265	ug/l #	51
37) Ethyl Acetate	7.257	43	58941	8.193	ug/l #	67
38) Carbon Tetrachloride	8.022	117	34641	6.234	ug/l #	17
40) Benzene	8.392	78	207179	11.940	ug/l	94
51) 4-Methyl-2-Pentanone	10.375	43	4814	0.658	ug/l #	1
52) Toluene	10.445	92	11713	1.092	ug/l	89
55) 1,1,2-Trichloroethane	10.692	97	960	0.209	ug/l #	16
68) m/p-Xylenes	11.886	106	2893	0.347	ug/l #	66
71) Bromoform	12.663	173	3548	1.087	ug/l #	1
76) 1,2,3-Trichloropropane	12.669	75	150598	20.542	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.669	75	150598	66.686	ug/l #	10
84) 1,2,4-Trimethylbenzene	13.298	105	4609	0.250	ug/l	89
88) 1,4-Dichlorobenzene	13.633	146	466	0.216	ug/l #	26
93) 1,2,4-Trichlorobenzene	15.198	180	66	0.868	ug/l #	63
95) Naphthalene	15.433	128	8174	1.193	ug/l #	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090322\
Data File : VN074323.D
Acq On : 03 Sep 2022 17:44
Operator : JC\MD
Sample : N4355-08
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-16R

Quant Time: Sep 05 05:37:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090222W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 03 04:35:33 2022
Response via : Initial Calibration




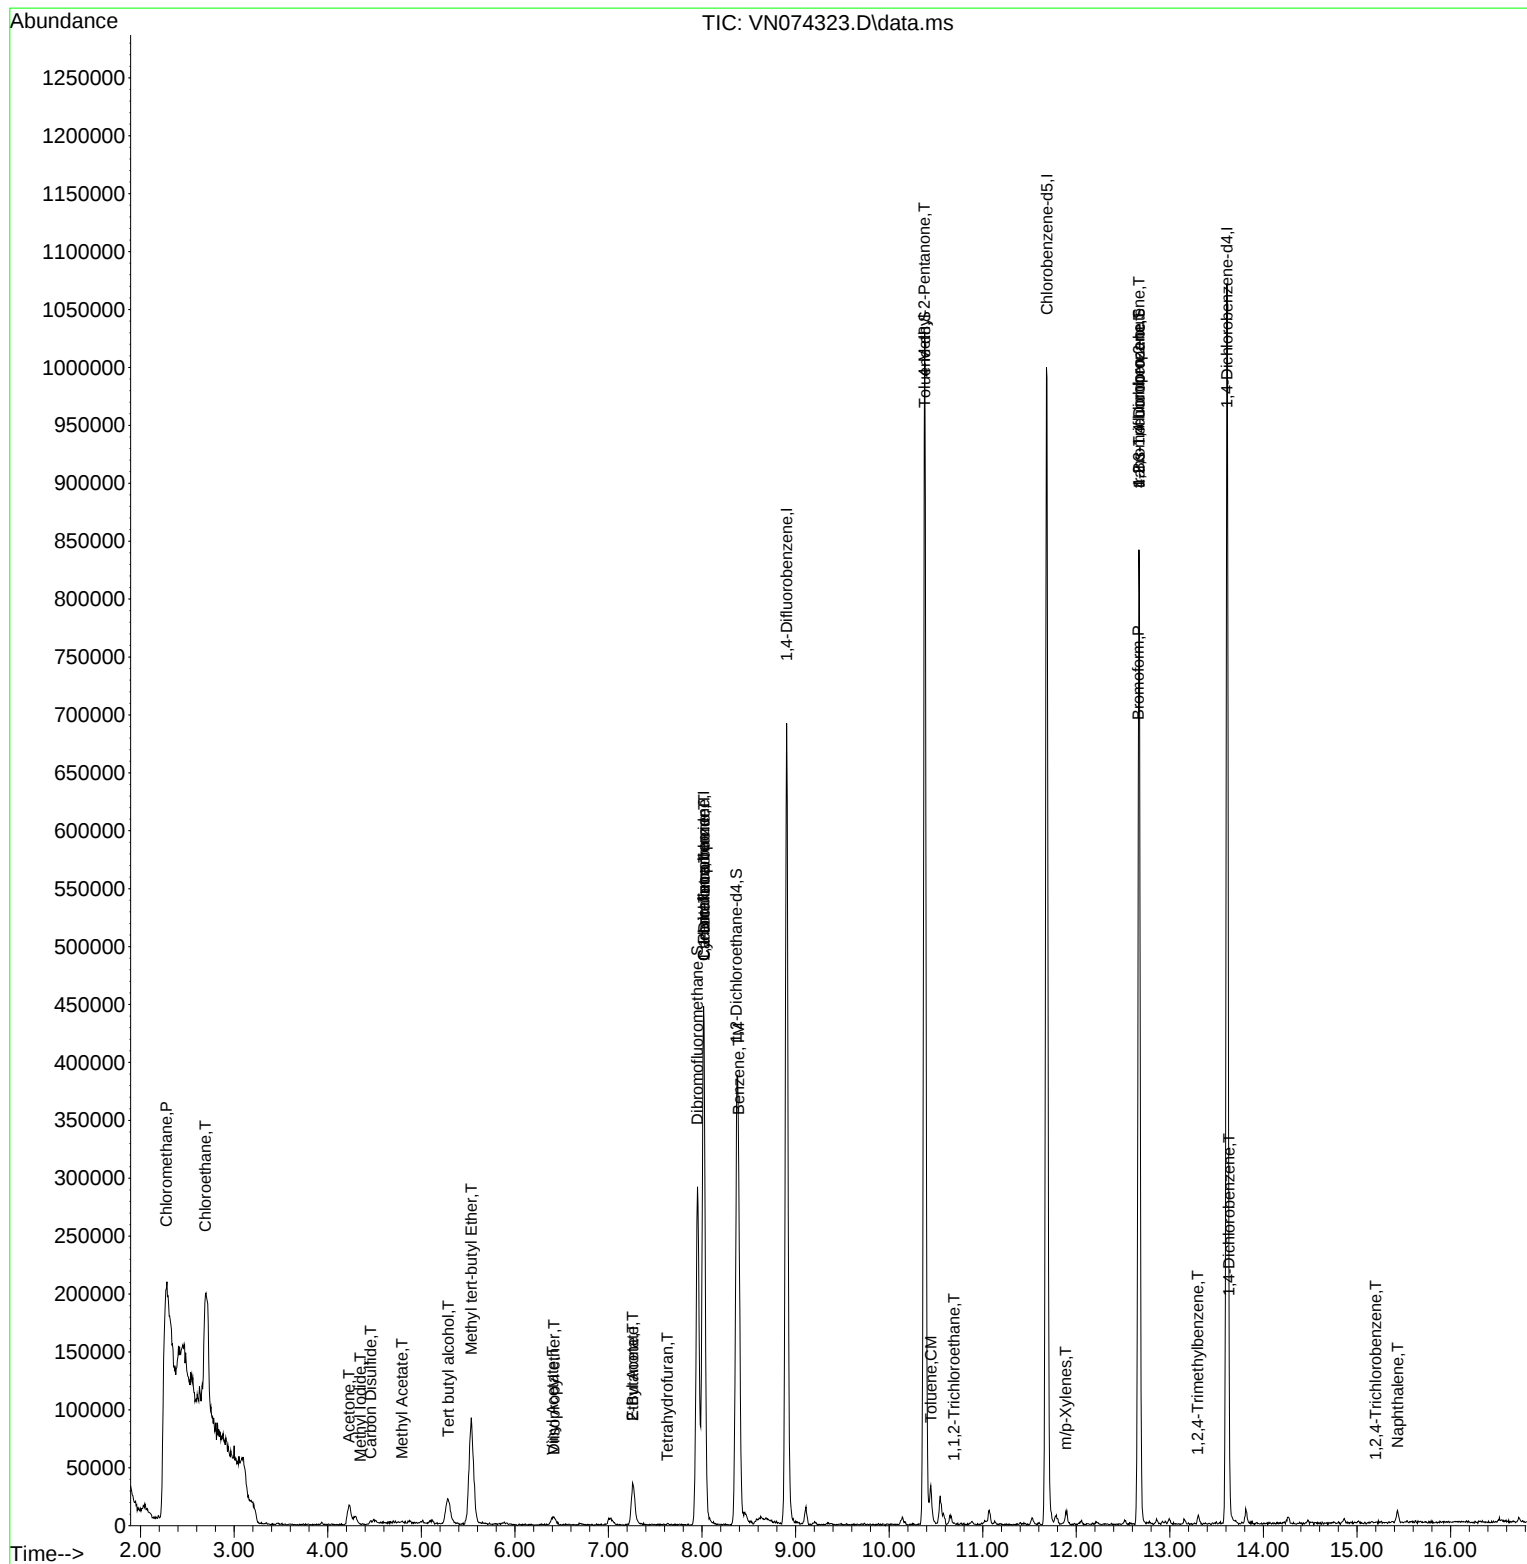




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44




Instrument :
MSVOA_N
ClientSampleId :
MW-16R


Tgt Ion:168 Resp: 317105
Ion Ratio Lower Upper
168 100
99 58.0 42.3 63.5

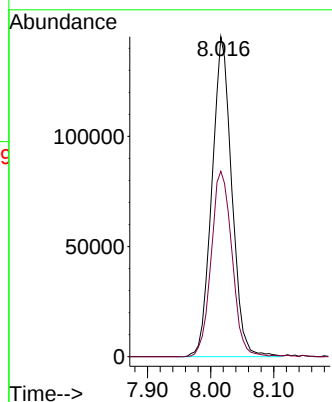

#3
Chloromethane
Concen: 2.437 ug/l
RT: 2.275 min Scan# 66
Delta R.T. 0.006 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44

Tgt Ion: 50 Resp: 10559
Ion Ratio Lower Upper
50 100
52 7.2 25.7 38.5#


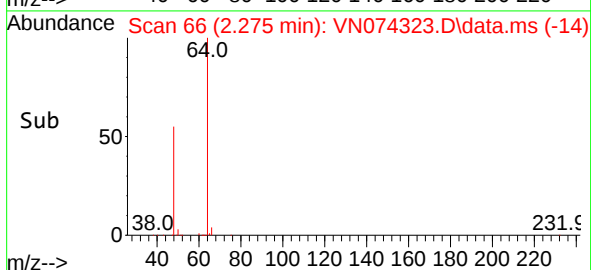






#6
Chloroethane
Concen: 25.525 ug/l
RT: 2.693 min Scan# 11
Delta R.T. -0.258 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44




Instrument :
MSVOA_N
ClientSampleId :
MW-16R


Tgt Ion: 64 Resp: 162063
Ion Ratio Lower Upper
64 100
66 6.3 26.2 39.4#

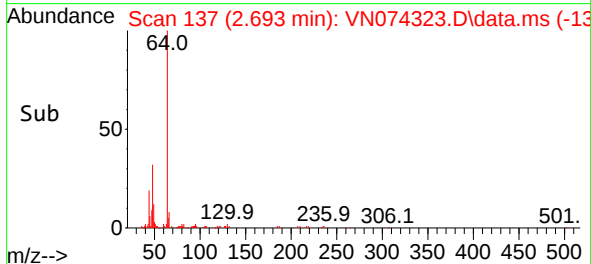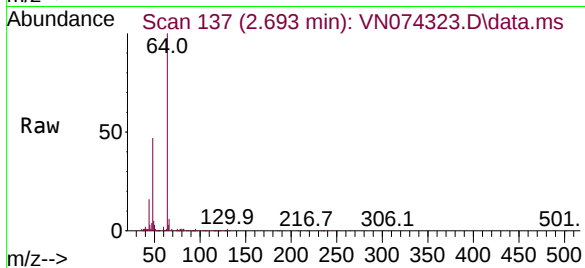

#10
Methyl Iodide
Concen: 5.075 ug/l
RT: 4.346 min Scan# 418
Delta R.T. -0.000 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44

Tgt Ion: 142 Resp: 91
Ion Ratio Lower Upper
142 100
127 0.0 31.3 46.9#
141 0.0 11.2 16.8#


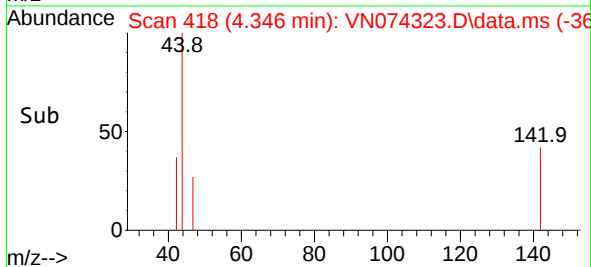

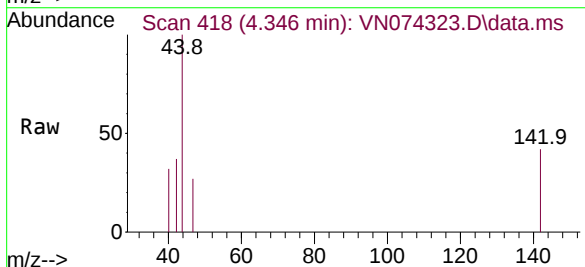




#11
Tert butyl alcohol
Concen: 41.986 ug/l
RT: 5.287 min Scan# 51
Delta R.T. -0.000 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44




Instrument :
MSVOA_N
ClientSampleId :
MW-16R


Tgt Ion: 59 Resp: 37653
Ion Ratio Lower Upper
59 100
57 11.5 8.3 12.5

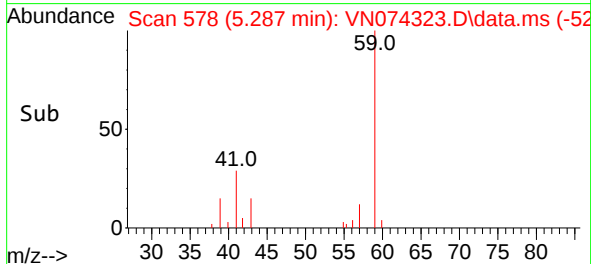

#16
Acetone
Concen: 15.108 ug/l
RT: 4.228 min Scan# 398
Delta R.T. 0.006 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44

Tgt Ion: 43 Resp: 31211
Ion Ratio Lower Upper
43 100
58 34.9 26.0 39.0


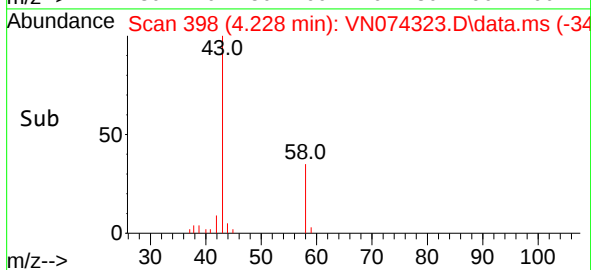

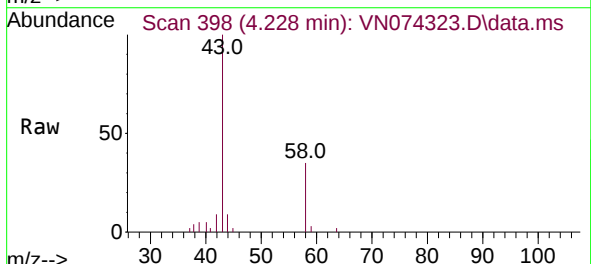


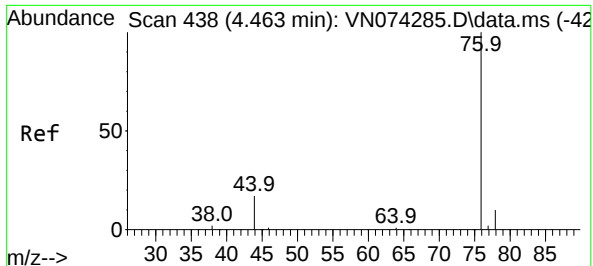

#17
Carbon Disulfide
Concen: 0.629 ug/l
RT: 4.457 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44




Instrument :
MSVOA_N
ClientSampleId :
MW-16R


Tgt Ion: 76 Resp: 4901
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

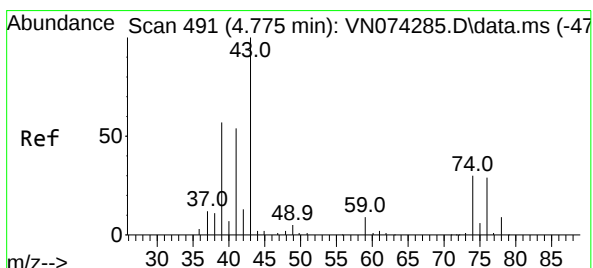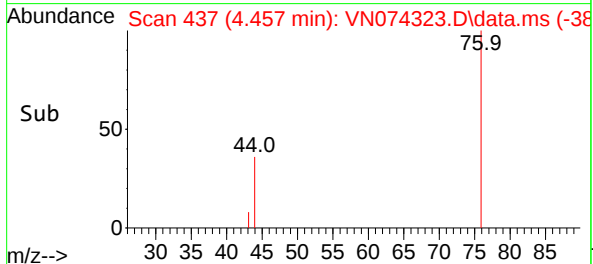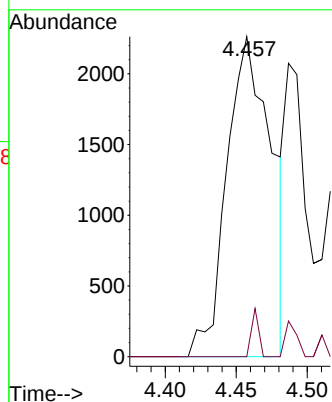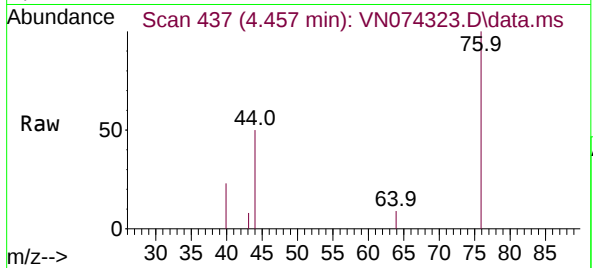

#18
Methyl Acetate
Concen: 0.235 ug/l
RT: 4.793 min Scan# 494
Delta R.T. 0.018 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44

Tgt Ion: 43 Resp: 1463
Ion Ratio Lower Upper
43 100
74 8.7 21.6 32.4#

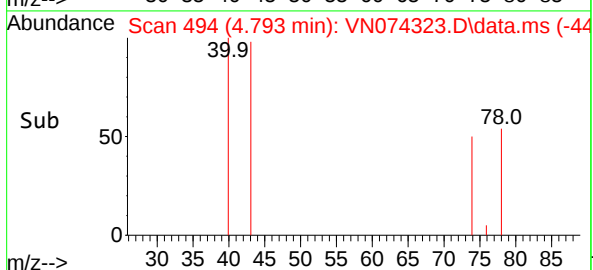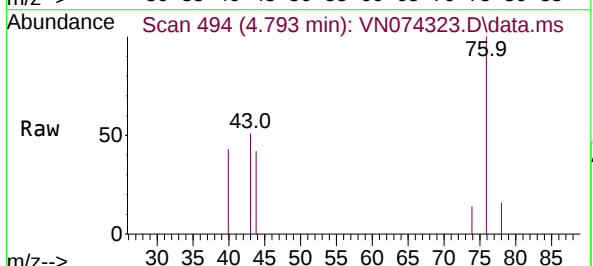



#19

Methyl tert-butyl Ether

Concen: 11.464 ug/l

RT: 5.534 min Scan# 61

Delta R.T. -0.000 min

Lab File: VN074323.D

Acq: 03 Sep 2022 17:44

Instrument :

MSVOA_N

ClientSampleId :





MW-16R

Tgt Ion: 73 Resp: 141835

Ion Ratio Lower Upper

73 100

57 20.8 17.6 26.4

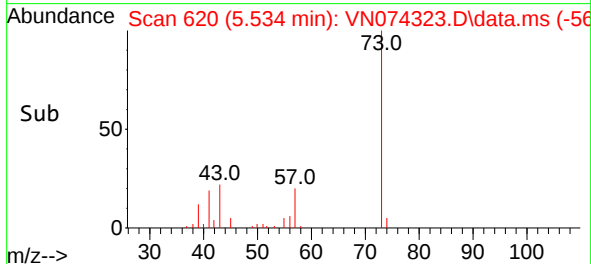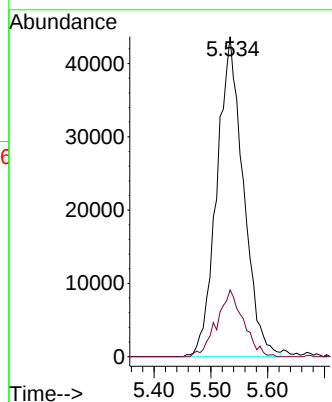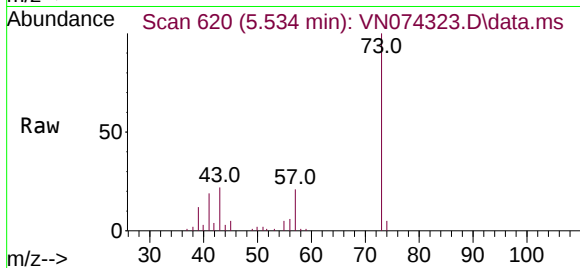

#20

Methylene Chloride

Concen: Below Cal

RT: 5.022 min Scan# 533

Delta R.T. 0.012 min

Lab File: VN074323.D

Acq: 03 Sep 2022 17:44

Tgt Ion: 84 Resp: 1032




Ion Ratio Lower Upper


84 100

49 31.6 88.3 132.5#

51 0.0 28.2 42.2#

86 0.0 50.6 76.0#


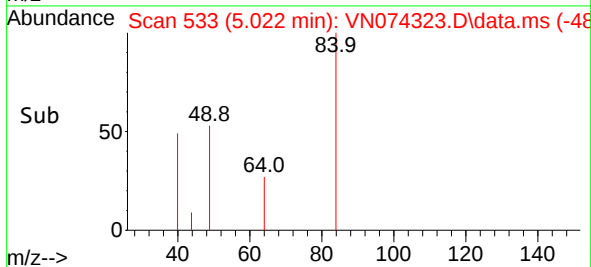

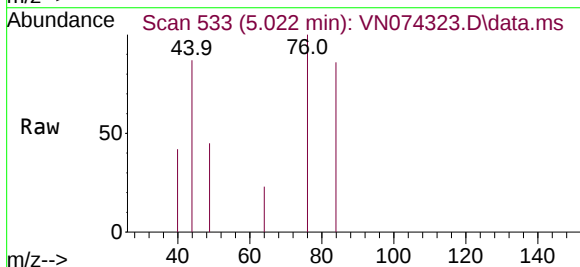




#22
Diisopropyl ether
Concen: 0.749 ug/l
RT: 6.416 min Scan# 71
Delta R.T. 0.000 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44




Instrument :
MSVOA_N
ClientSampleId :
MW-16R


Tgt Ion:	45	Resp:	8825
Ion	Ratio	Lower	Upper
45	100		
43	49.8	46.6	70.0
87	28.0	24.3	36.5
59	8.5	9.6	14.4

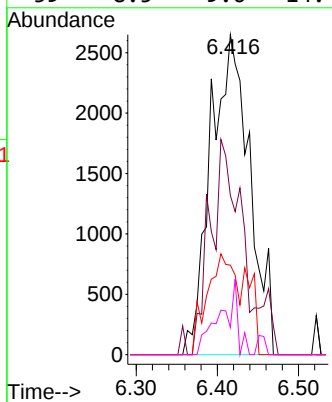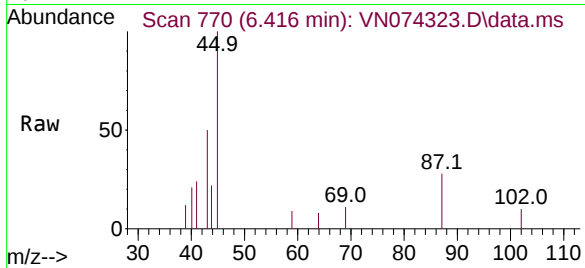

#23
Vinyl Acetate
Concen: 0.460 ug/l
RT: 6.404 min Scan# 768
Delta R.T. 0.053 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44

Tgt Ion:	43	Resp:	4712
Ion	Ratio	Lower	Upper
43	100		
86	0.0	10.0	15.0

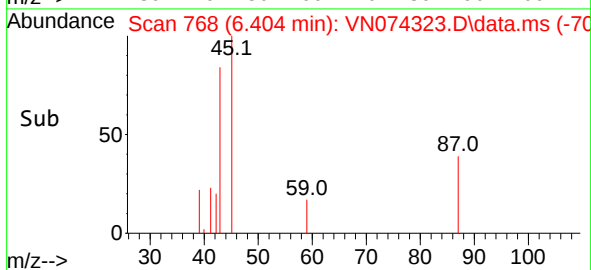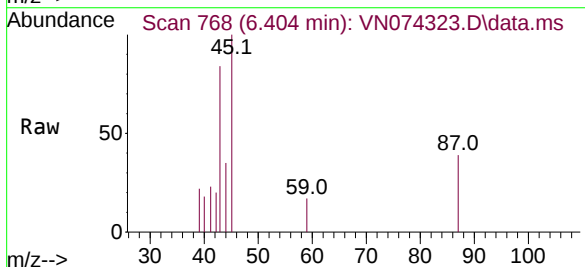

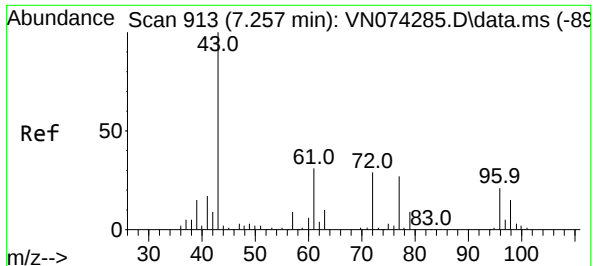

#25

2-Butanone

Concen: 16.896 ug/l

RT: 7.257 min Scan# 913

Delta R.T. 0.000 min

Lab File: VN074323.D

Acq: 03 Sep 2022 17:44

Instrument :

MSVOA_N

ClientSampleId :





MW-16R

Tgt Ion: 43 Resp: 58941

Ion Ratio Lower Upper

43 100

72 26.9 23.7 35.5

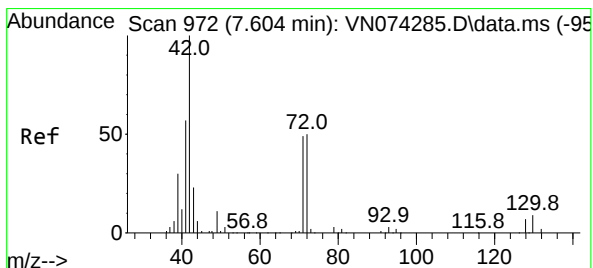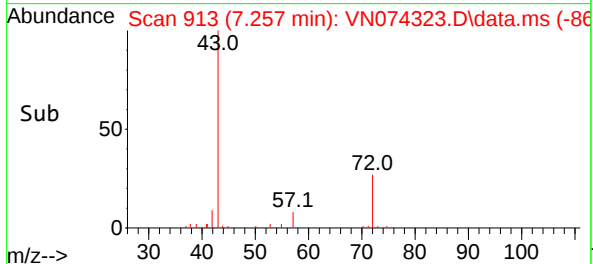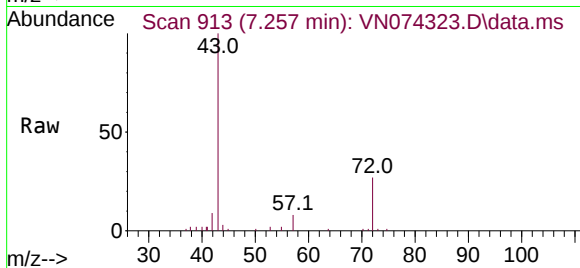

#29

Tetrahydrofuran

Concen: 0.250 ug/l

RT: 7.628 min Scan# 976

Delta R.T. 0.018 min

Lab File: VN074323.D

Acq: 03 Sep 2022 17:44




Tgt Ion: 42 Resp: 556


Ion Ratio Lower Upper

42 100

72 30.6 39.7 59.5#

71 24.1 36.6 55.0#


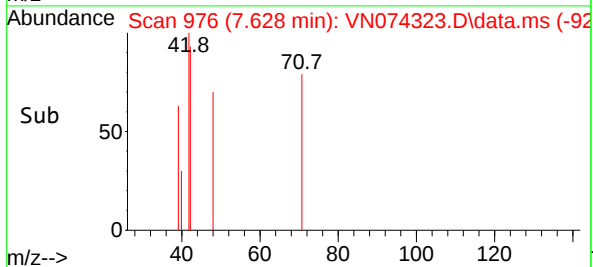

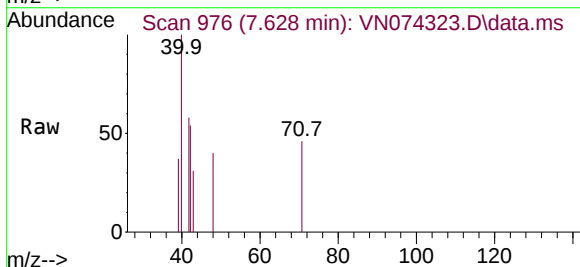


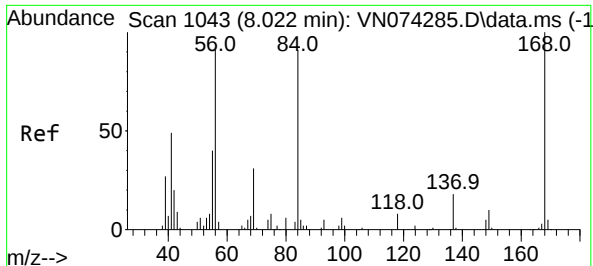

#31
Cyclohexane
Concen: 1.502 ug/l
RT: 8.022 min Scan# 1043
Delta R.T. -0.000 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44




Instrument :
MSVOA_N
ClientSampleId :
MW-16R


Tgt Ion: 56 Resp: 9913
Ion Ratio Lower Upper
56 100
69 106.6 27.8 41.8#
84 56.9 76.9 115.3#

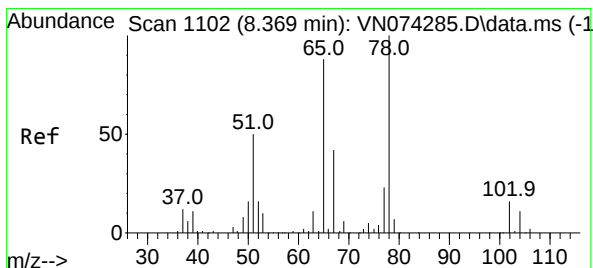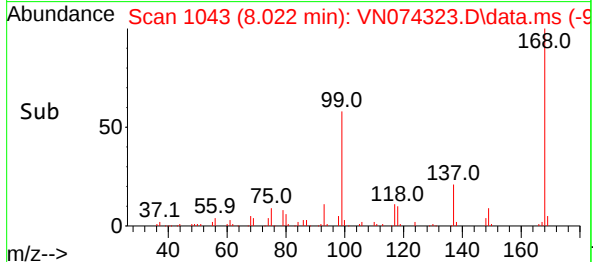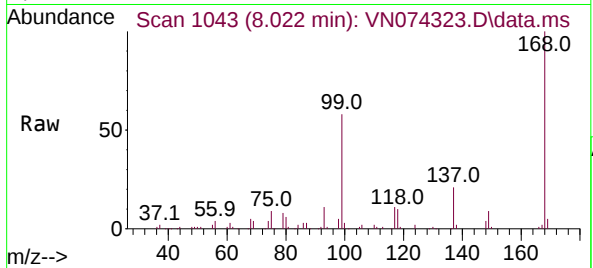

#33
1,2-Dichloroethane-d4
Concen: 46.336 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. -0.000 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44

Tgt Ion: 65 Resp: 229046
Ion Ratio Lower Upper
65 100
67 52.6 0.0 104.8

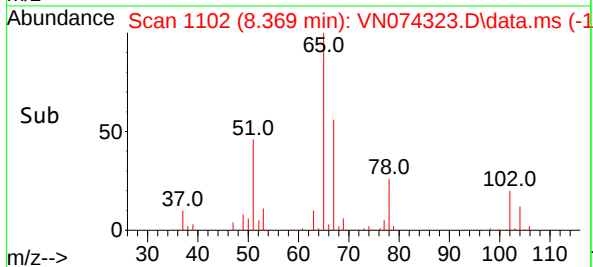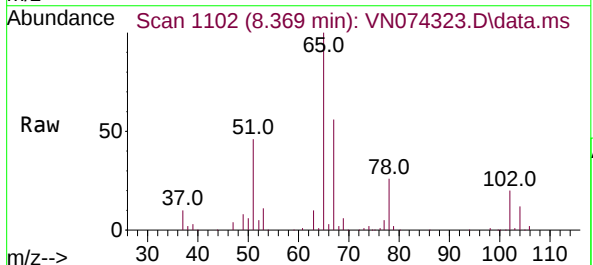

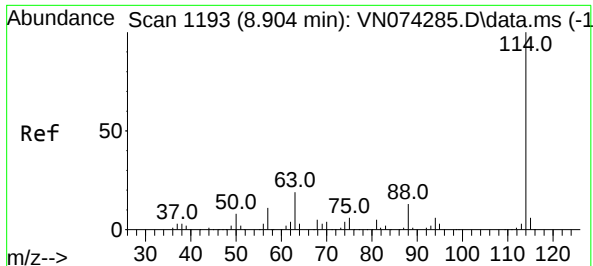

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.000 min

Lab File: VN074323.D

Acq: 03 Sep 2022 17:44

Instrument :

MSVOA_N

ClientSampleId :

MW-16R





Tgt Ion:114 Resp: 584846

Ion Ratio Lower Upper

114 100

63 20.0 0.0 40.0

88 13.4 0.0 32.6

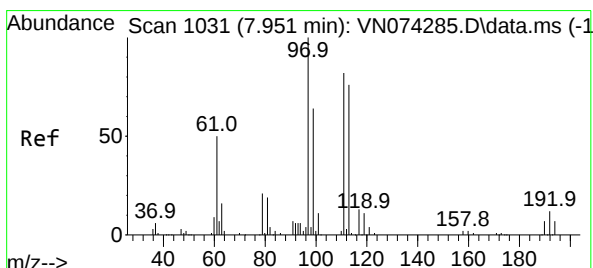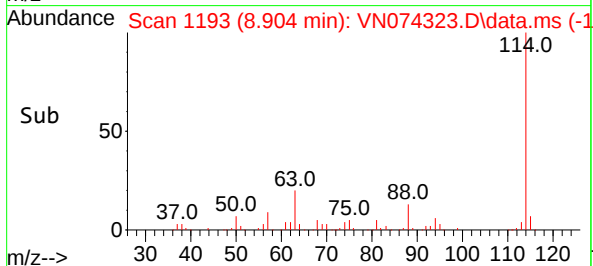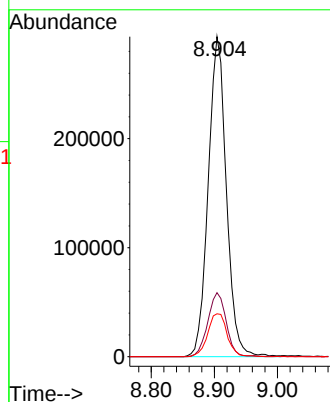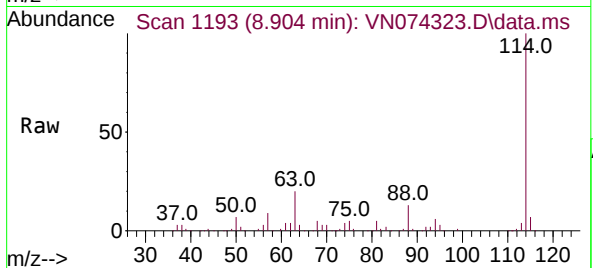

#35

Dibromofluoromethane

Concen: 51.616 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN074323.D

Acq: 03 Sep 2022 17:44




Tgt Ion:113 Resp: 200037


Ion Ratio Lower Upper

113 100

111 103.0 81.4 122.0

192 17.7 17.0 25.6

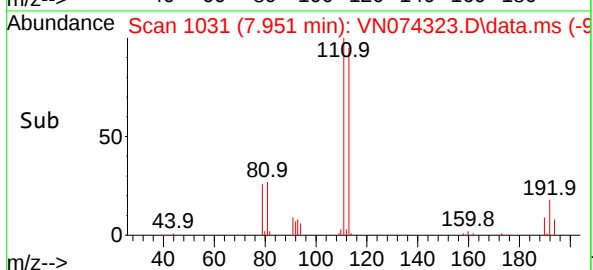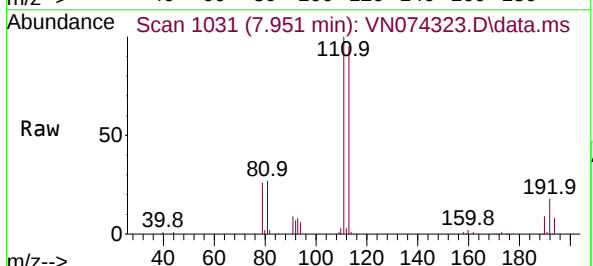



#36

1,1-Dichloropropene

Concen: 5.265 ug/l

RT: 8.022 min Scan# 1

Delta R.T. -0.135 min

Lab File: VN074323.D

Acq: 03 Sep 2022 17:44

Instrument :

MSVOA_N

ClientSampleId :

MW-16R





Tgt Ion: 75 Resp: 28959

Ion Ratio Lower Upper

75 100

110 11.5 18.3 54.8#

77 0.0 25.1 37.7#

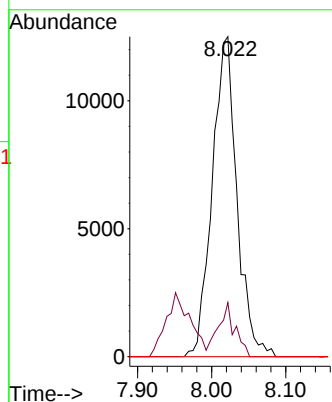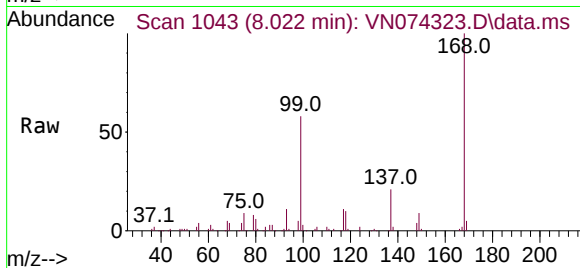

#37

Ethyl Acetate

Concen: 8.193 ug/l

RT: 7.257 min Scan# 913

Delta R.T. -0.077 min

Lab File: VN074323.D

Acq: 03 Sep 2022 17:44




Tgt Ion: 43 Resp: 58941


Ion Ratio Lower Upper

43 100

61 0.1 11.8 17.6#

70 0.1 9.3 13.9#


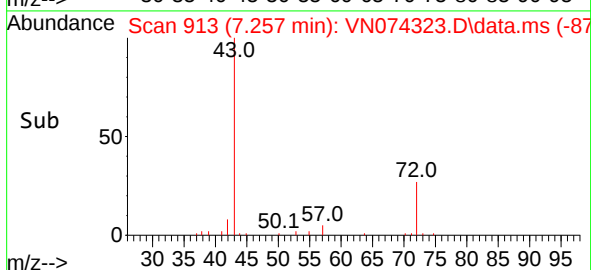

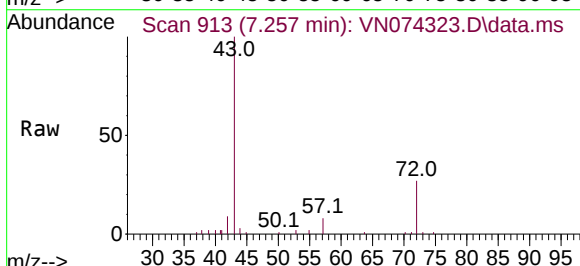


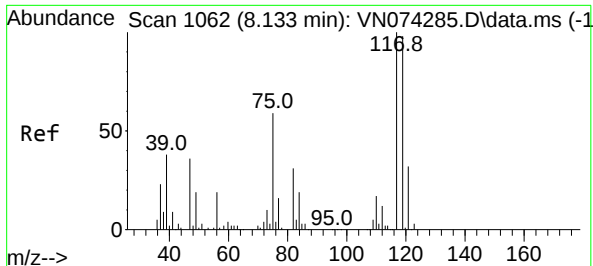

#38
Carbon Tetrachloride
Concen: 6.234 ug/l
RT: 8.022 min Scan# 1106
Delta R.T. -0.111 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44




Instrument :
MSVOA_N
ClientSampleId :
MW-16R


Tgt Ion:117 Resp: 34641
Ion Ratio Lower Upper
117 100
119 6.0 75.8 113.8#
121 0.0 24.6 37.0#

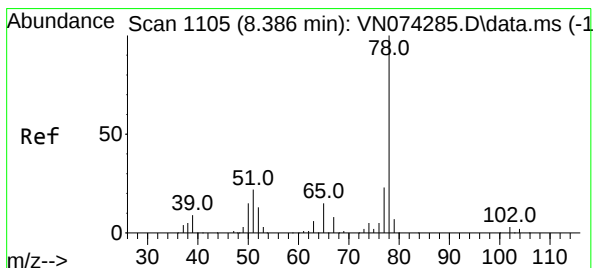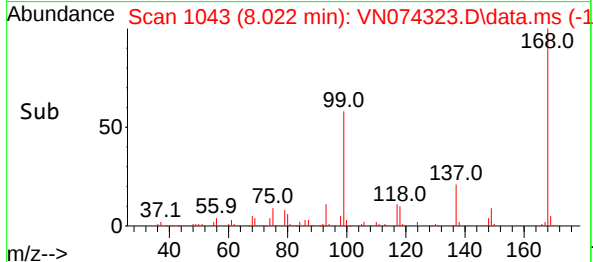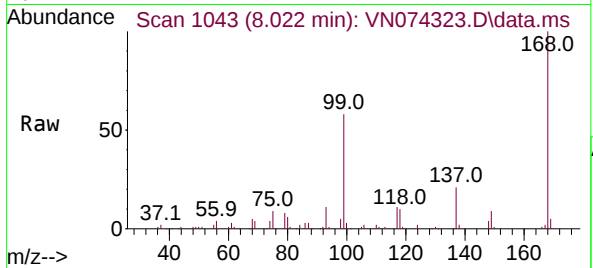

#40
Benzene
Concen: 11.940 ug/l
RT: 8.392 min Scan# 1106
Delta R.T. 0.000 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44

Tgt Ion: 78 Resp: 207179
Ion Ratio Lower Upper
78 100
77 21.4 19.4 29.0


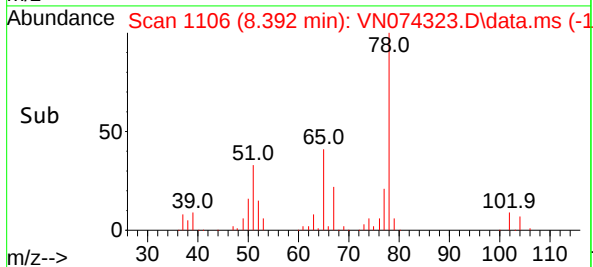

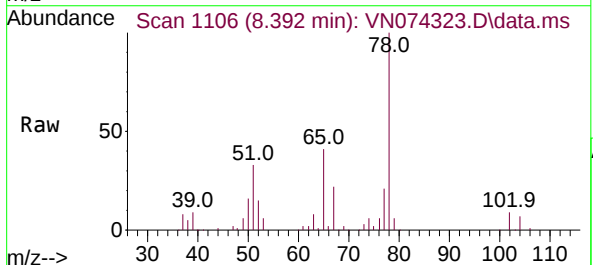




#50
Toluene-d8
Concen: 44.857 ug/l
RT: 10.381 min Scan# 1444
Delta R.T. 0.001 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44




Instrument :
MSVOA_N
ClientSampleId :
MW-16R


Tgt Ion: 98 Resp: 685502
Ion Ratio Lower Upper
98 100
100 63.9 52.6 78.8

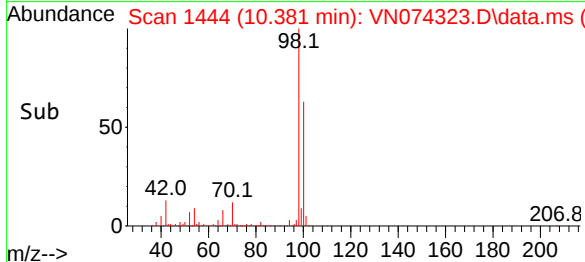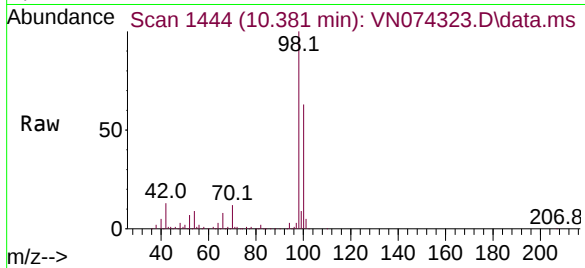

#51
4-Methyl-2-Pentanone
Concen: 0.658 ug/l
RT: 10.375 min Scan# 1443
Delta R.T. 0.100 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44

Tgt Ion: 43 Resp: 4814
Ion Ratio Lower Upper
43 100
58 130.1 34.1 51.1#


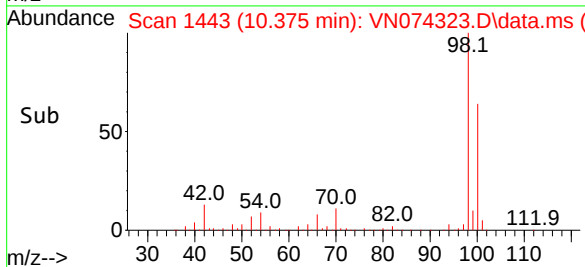

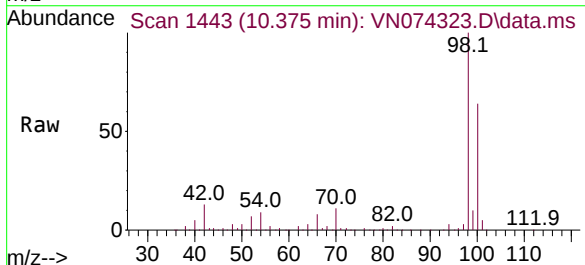




#52
Toluene
Concen: 1.092 ug/l
RT: 10.445 min Scan# 1455
Delta R.T. 0.000 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44




Instrument :
MSVOA_N
ClientSampleId :
MW-16R


Tgt Ion: 92 Resp: 11713
Ion Ratio Lower Upper
92 100
91 158.1 138.6 207.8

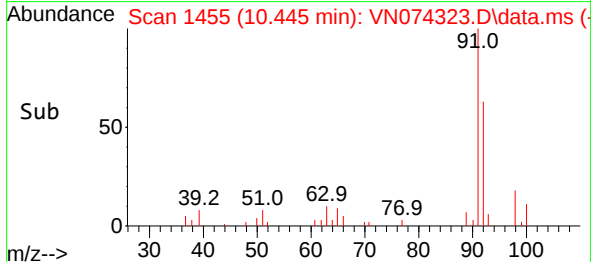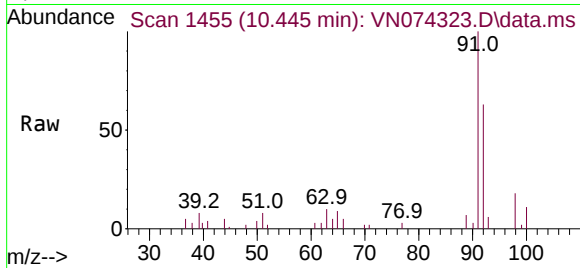

#55
1,1,2-Trichloroethane
Concen: 0.209 ug/l
RT: 10.692 min Scan# 1497
Delta R.T. -0.147 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44

Tgt Ion: 97 Resp: 960
Ion Ratio Lower Upper
97 100
83 0.0 66.2 99.4#
85 0.0 43.9 65.9#
99 0.0 50.6 76.0#


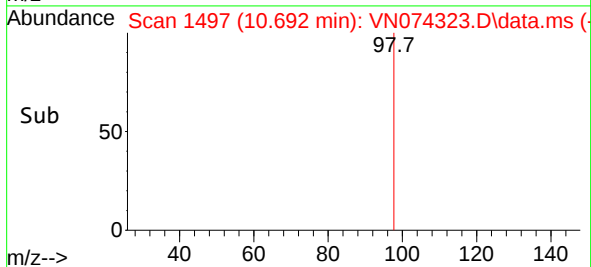

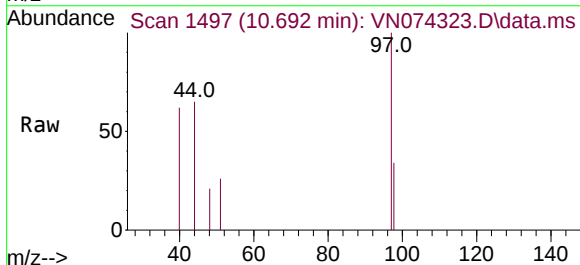


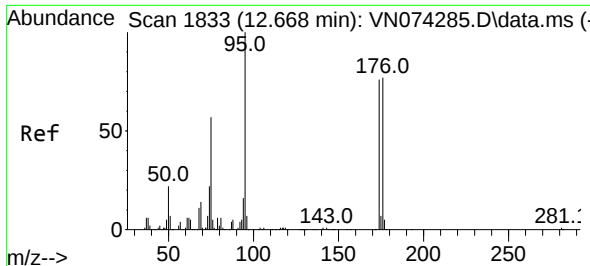

#62
4-Bromofluorobenzene
Concen: 45.194 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. -0.000 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44




Instrument :
MSVOA_N
ClientSampleId :
MW-16R


Tgt Ion: 95 Resp: 251097
Ion Ratio Lower Upper
95 100
174 79.0 0.0 167.6
176 77.7 0.0 163.4

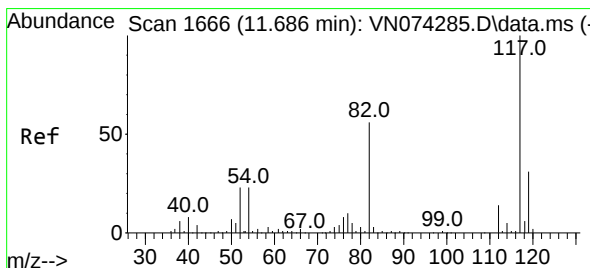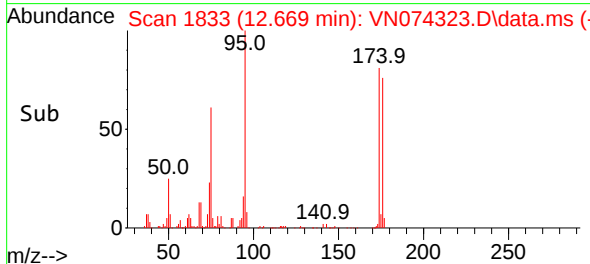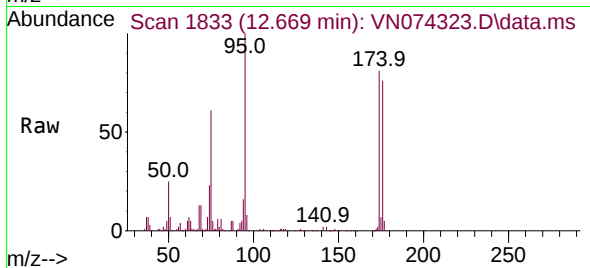

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1666
Delta R.T. 0.000 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44

Tgt Ion: 117 Resp: 554857
Ion Ratio Lower Upper
117 100
82 55.6 44.2 66.2
119 34.4 25.4 38.0


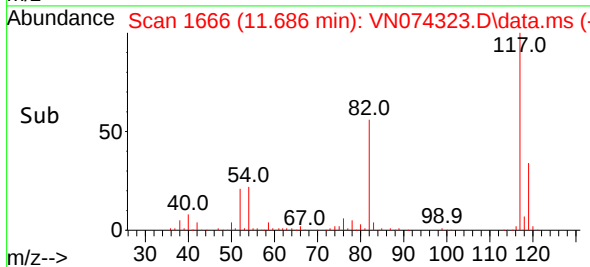

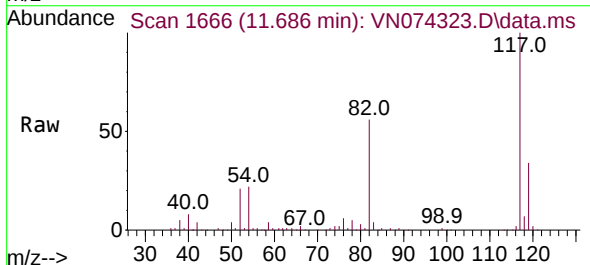




#68
m/p-Xylenes
Concen: 0.347 ug/l
RT: 11.886 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44




Instrument :
MSVOA_N
ClientSampleId :
MW-16R


Tgt Ion:106 Resp: 2893
Ion Ratio Lower Upper
106 100
91 249.6 158.9 238.3#

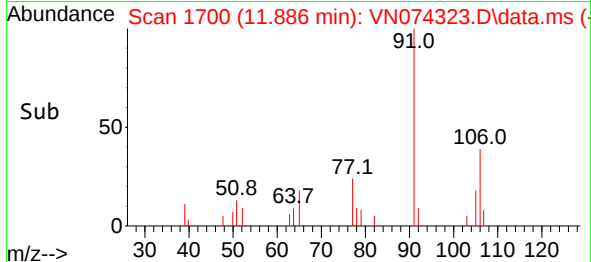

#71
Bromoform
Concen: 1.087 ug/l
RT: 12.663 min Scan# 1832
Delta R.T. 0.265 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44

Tgt Ion:173 Resp: 3548
Ion Ratio Lower Upper
173 100
175 344.3 24.6 73.6#
254 0.0 0.1 0.1#


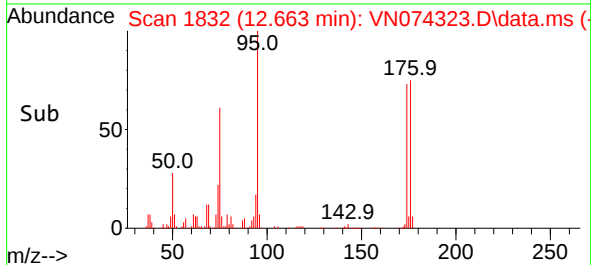

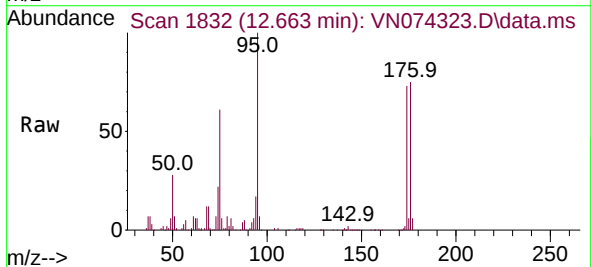


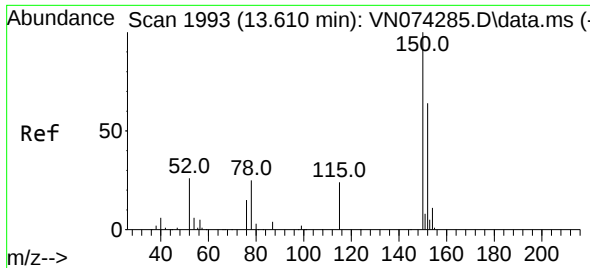

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.610 min Scan# 1993
 Delta R.T. -0.000 min
 Lab File: VN074323.D
 Acq: 03 Sep 2022 17:44




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-16R


Tgt Ion:152 Resp: 258848
 Ion Ratio Lower Upper
 152 100
 115 60.2 28.9 86.7
 150 154.9 0.0 356.2

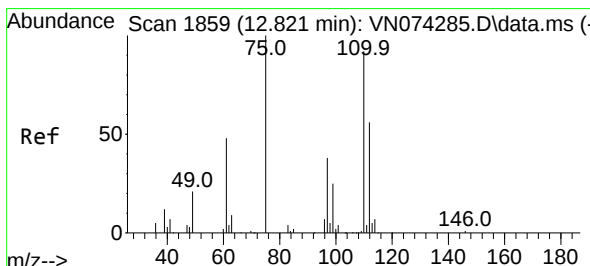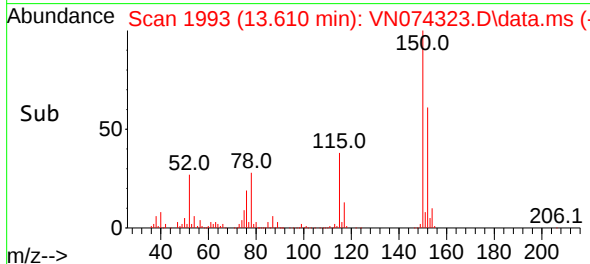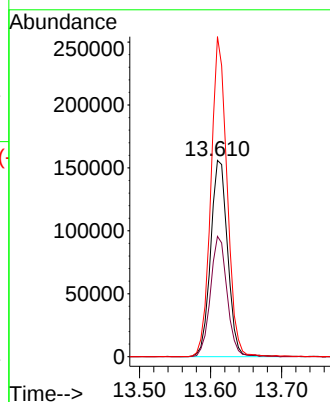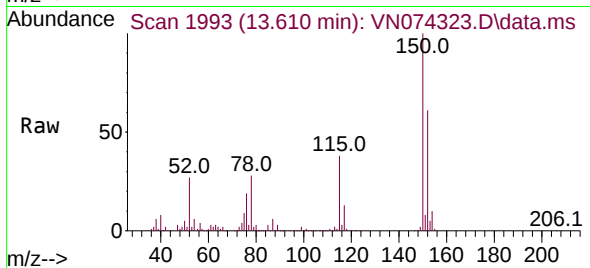

#76
 1,2,3-Trichloropropane
 Concen: 20.542 ug/l
 RT: 12.669 min Scan# 1833
 Delta R.T. -0.152 min
 Lab File: VN074323.D
 Acq: 03 Sep 2022 17:44

Tgt Ion: 75 Resp: 150598
 Ion Ratio Lower Upper
 75 100
 77 1.3 98.5 295.5#


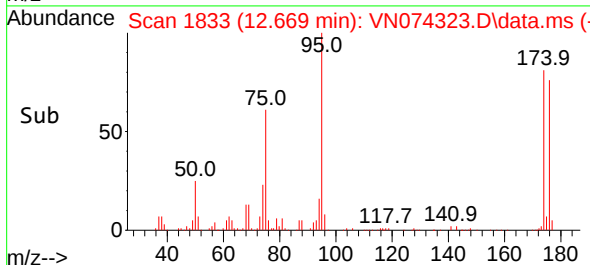

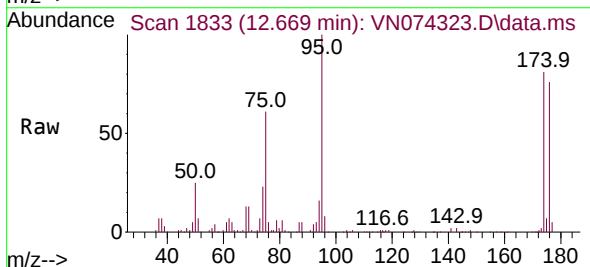


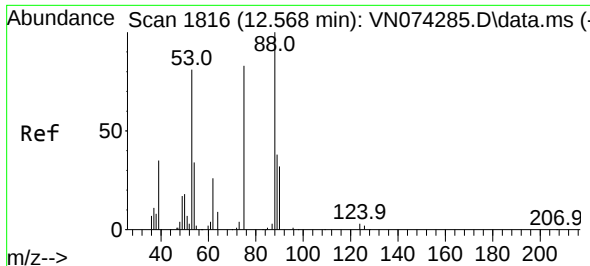

#81
trans-1,4-Dichloro-2-butene
Concen: 66.686 ug/l
RT: 12.669 min Scan# 1816
Delta R.T. 0.106 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44




Instrument :
MSVOA_N
ClientSampleId :
MW-16R


Tgt Ion: 75 Resp: 150598
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.1 37.2 55.8#

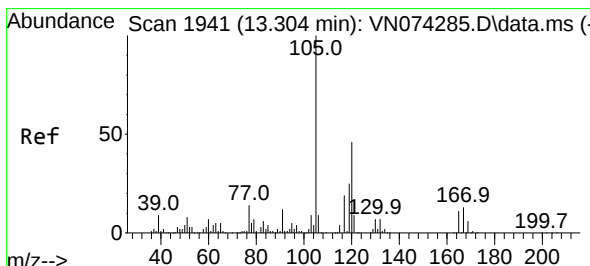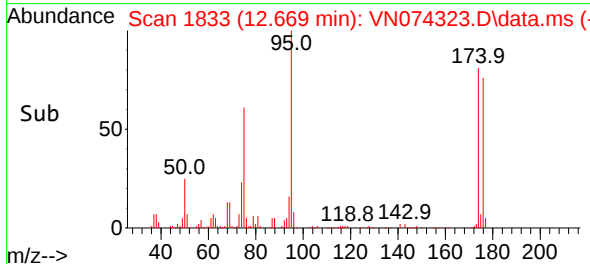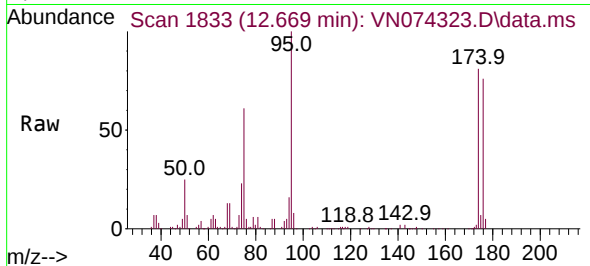

#84
1,2,4-Trimethylbenzene
Concen: 0.250 ug/l
RT: 13.298 min Scan# 1940
Delta R.T. -0.012 min
Lab File: VN074323.D
Acq: 03 Sep 2022 17:44

Tgt Ion: 105 Resp: 4609
Ion Ratio Lower Upper
105 100
120 39.3 23.3 69.8


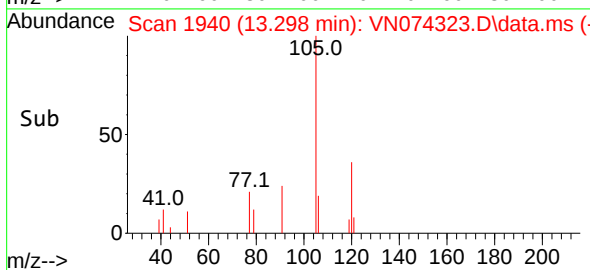

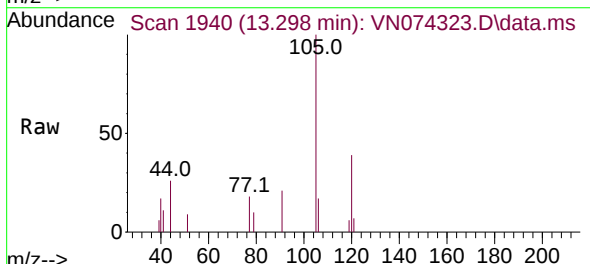




#88
 1,4-Dichlorobenzene
 Concen: 0.216 ug/l
 RT: 13.633 min Scan# 1997
 Delta R.T. 0.000 min
 Lab File: VN074323.D
 Acq: 03 Sep 2022 17:44




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-16R


Tgt Ion:146 Resp: 466
 Ion Ratio Lower Upper
 146 100
 111 0.0 19.1 57.1#
 148 0.0 31.4 94.3#

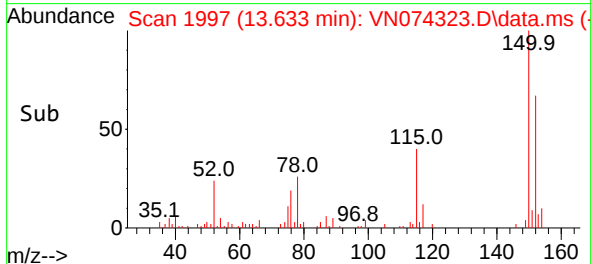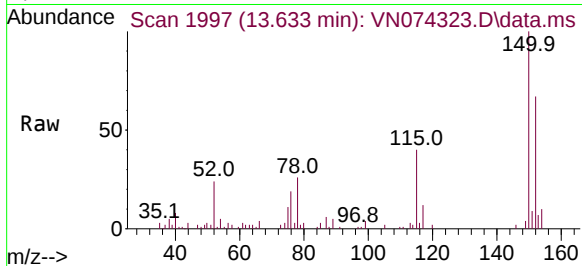

#93
 1,2,4-Trichlorobenzene
 Concen: 0.868 ug/l
 RT: 15.198 min Scan# 2263
 Delta R.T. -0.000 min
 Lab File: VN074323.D
 Acq: 03 Sep 2022 17:44

Tgt Ion:180 Resp: 66
 Ion Ratio Lower Upper
 180 100
 182 125.8 47.5 142.5
 145 0.0 14.5 43.5#

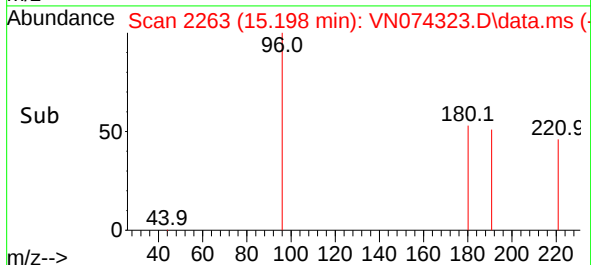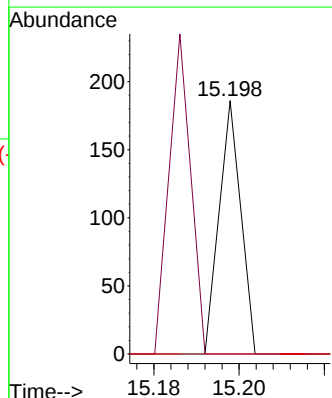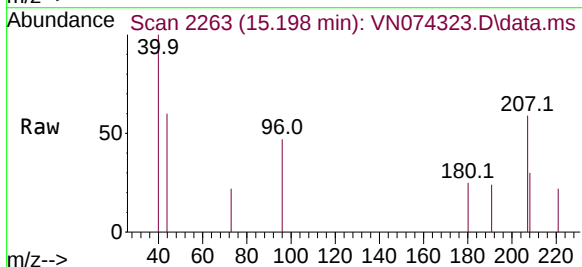



#95

Naphthalene

Concen: 1.193 ug/l

RT: 15.433 min Scan# 21

Delta R.T. 0.000 min

Lab File: VN074323.D


Acq: 03 Sep 2022 17:44

Instrument :

MSVOA_N

ClientSampleId :

MW-16R

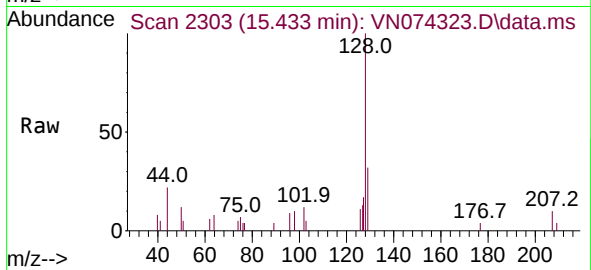

Tgt Ion:128 Resp: 8174

Ion Ratio Lower Upper

128 100

127 13.5 10.3 15.5

129 16.6 8.6 13.0#

