

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090322\
 Data File : VN074336.D
 Acq On : 03 Sep 2022 23:01
 Operator : JC\MD
 Sample : N4381-13
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-48

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090222W.M

Title : SW846 8260

Signal : TIC: VN074336.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.204	47	54	62	rBV2	28859	85408	4.80%	0.813%
2	2.287	62	68	69	rBV2	13518	22358	1.26%	0.213%
3	2.693	132	137	139	rBV4	42083	70790	3.98%	0.674%
4	3.104	205	207	214	rVB5	15054	29040	1.63%	0.277%
5	5.534	606	620	636	rBV4	74166	272459	15.32%	2.595%
6	7.951	1021	1031	1037	rBV	270965	666806	37.50%	6.351%
7	8.016	1037	1042	1060	rVB	434829	955553	53.74%	9.101%
8	8.369	1091	1102	1116	rBV	282806	642332	36.12%	6.118%
9	8.904	1184	1193	1214	rVB	661443	1324629	74.49%	12.616%
10	10.380	1435	1444	1459	rBV	987359	1778231	100.00%	16.936%
11	11.680	1657	1665	1679	rBV	963504	1724168	96.96%	16.421%
12	12.668	1825	1833	1844	rBV2	803818	1324475	74.48%	12.615%
13	13.609	1986	1993	2007	rBV	939166	1603245	90.16%	15.270%


Sum of corrected areas: 10499494

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090322\
Data File : VN074336.D
Acq On : 03 Sep 2022 23:01
Operator : JC\MD
Sample : N4381-13
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

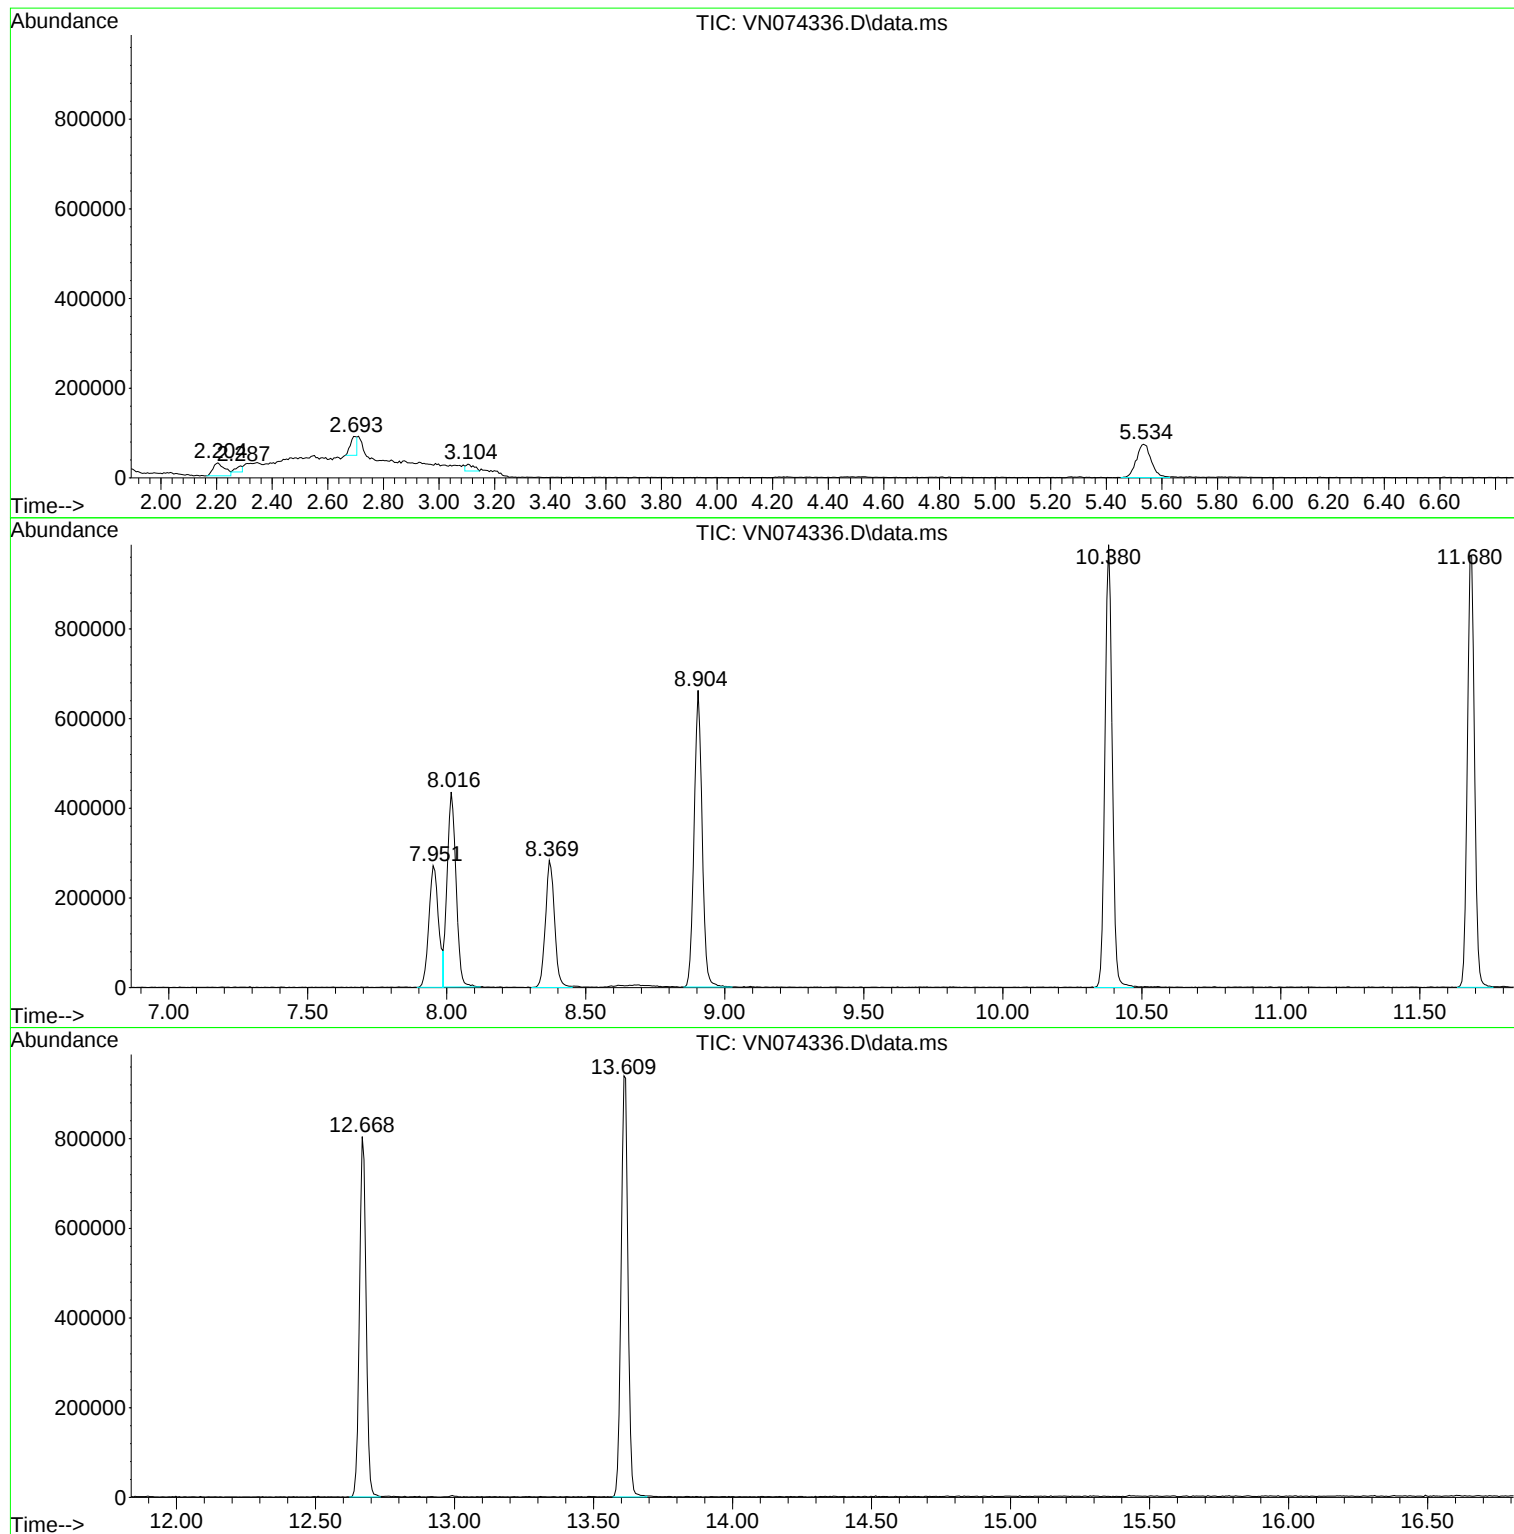

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090322\
Data File : VN074336.D
Acq On : 03 Sep 2022 23:01
Operator : JC\MD
Sample : N4381-13
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090322\
Data File : VN074336.D
Acq On : 03 Sep 2022 23:01
Operator : JC\MD
Sample : N4381-13
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc