
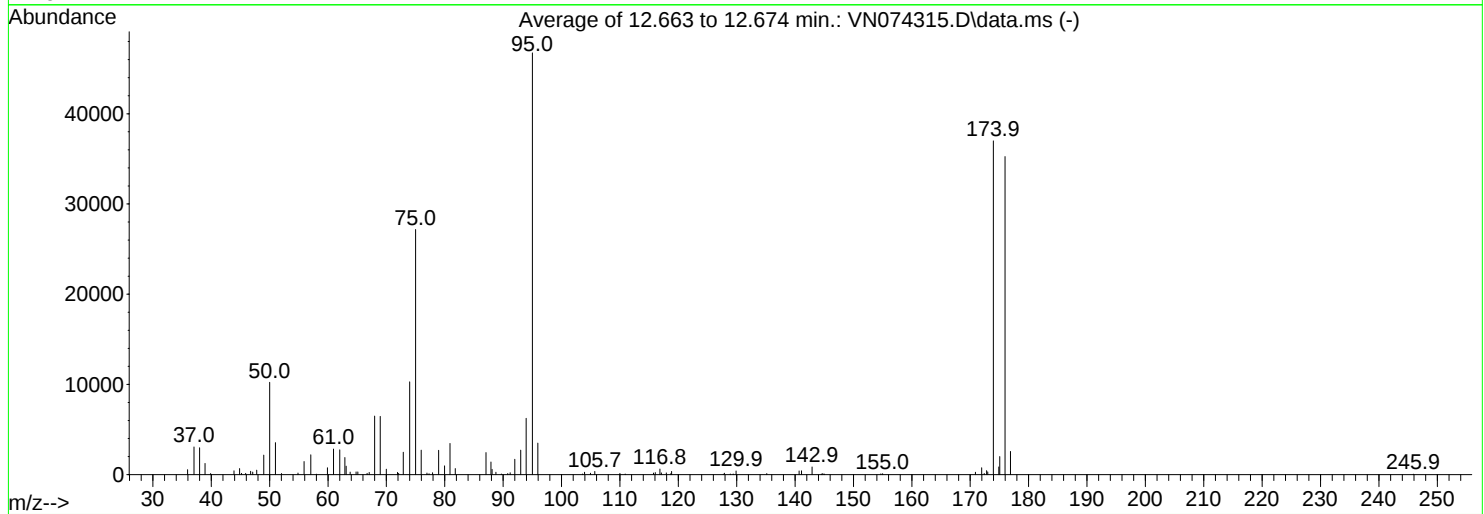


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090322\
 Data File : VN074315.D
 Acq On : 03 Sep 2022 13:44
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090222W.M
 Title : SW846 8260
 Last Update : Sat Sep 03 04:35:33 2022

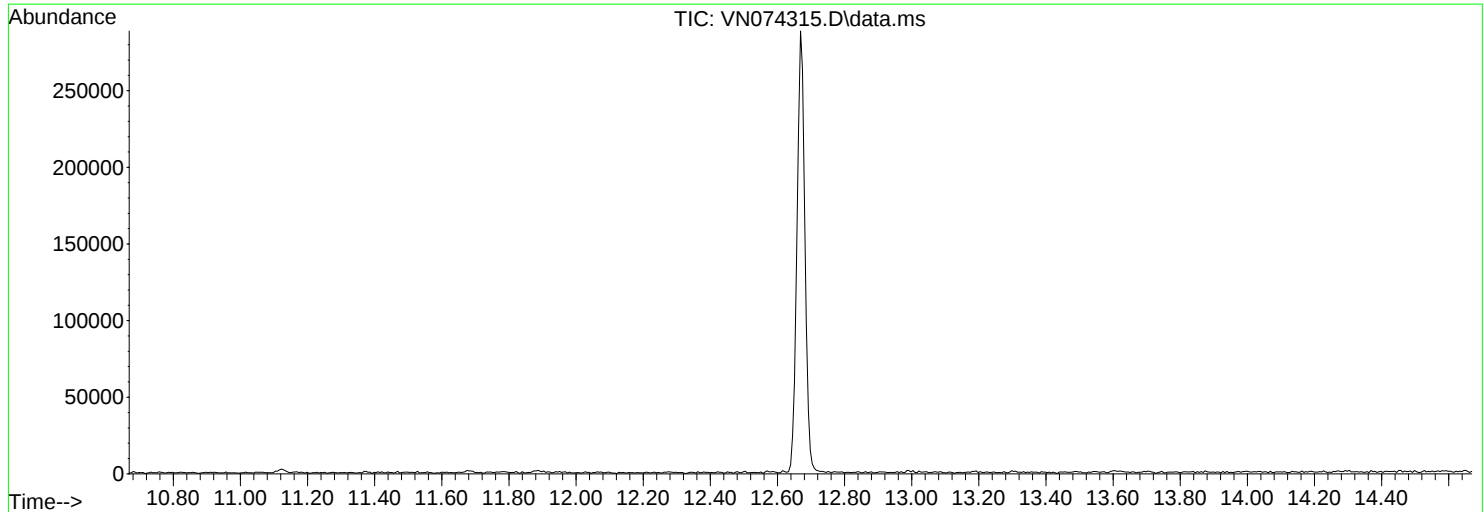

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	10230	PASS
75	95	30	60	58.1	27163	PASS
95	95	100	100	100.0	46752	PASS
96	95	5	9	7.5	3488	PASS
173	174	0.00	2	1.2	446	PASS
174	95	50	100	79.1	36992	PASS
175	174	5	9	5.4	2012	PASS
176	174	95	101	95.3	35253	PASS
177	176	5	9	7.3	2578	PASS