
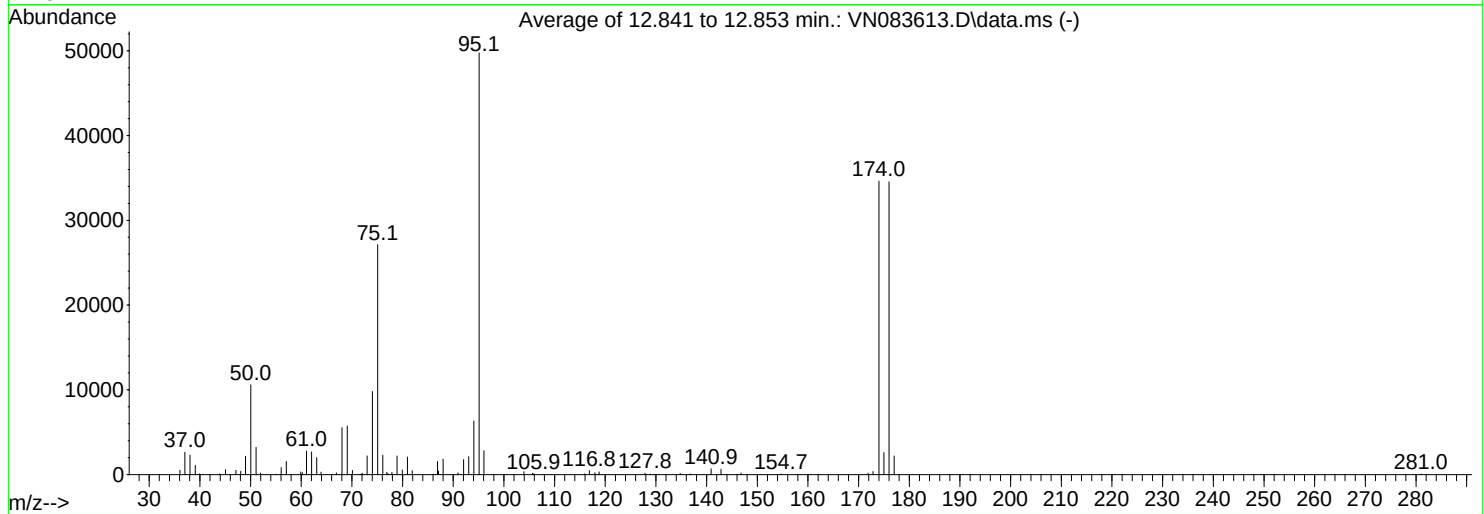


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083613.D
Data File : VN083613.D
Acq On : 03 Sep 2024 08:19
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083024W.M
Title : SW846 8260
Last Update : Sat Aug 31 00:48:10 2024

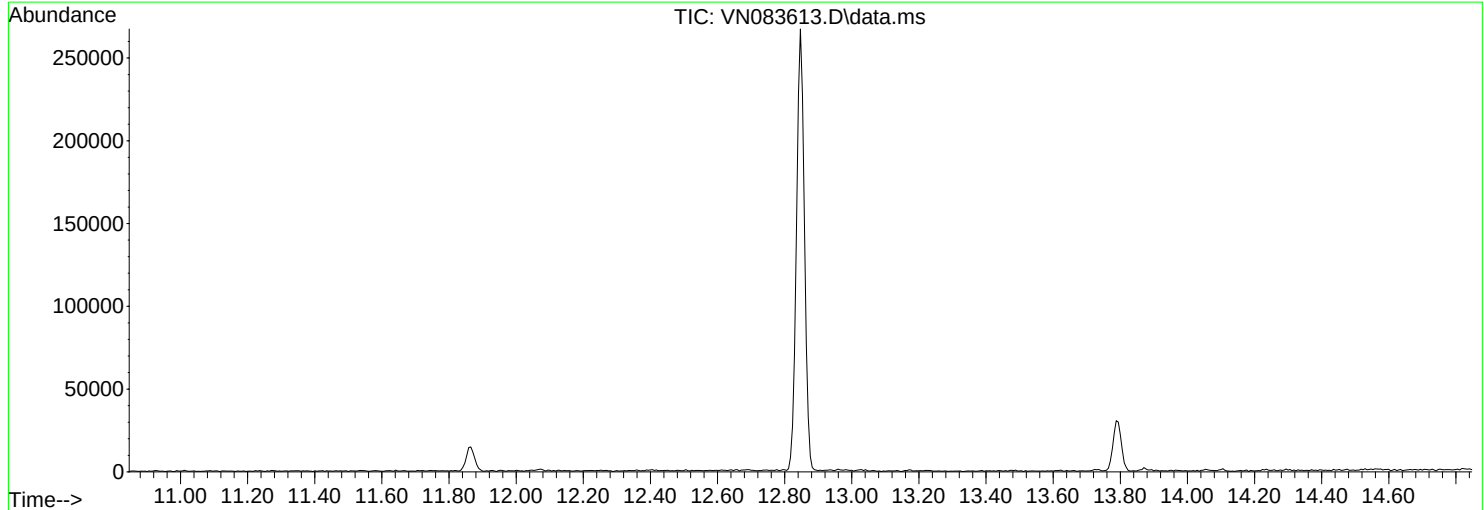

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	10581	PASS
75	95	30	60	54.5	27115	PASS
95	95	100	100	100.0	49755	PASS
96	95	5	9	5.7	2838	PASS
173	174	0.00	2	1.1	373	PASS
174	95	50	100	69.6	34629	PASS
175	174	5	9	7.5	2599	PASS
176	174	95	101	99.7	34533	PASS
177	176	5	9	6.4	2210	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	532	51.10	3227	66.95	204	77.10	121
37.05	2636	51.95	186	68.05	5552	77.90	261
38.05	2305	55.00	61	69.10	5740	78.90	220
39.10	1102	56.05	840	70.10	501	79.95	54
39.90	92	57.05	1557	71.80	77	80.95	2084
43.85	96	59.90	320	72.05	148	81.90	469
45.05	584	60.20	219	73.00	2201	86.90	1555
47.10	514	61.05	2780	74.05	9825	87.10	424
48.05	402	62.05	2682	75.10	27115	88.00	1837
49.00	2172	63.05	1998	76.10	2295	90.95	214
50.05	10581	63.90	313	76.90	289	92.05	1771

Average of 12.841 to 12.853 min.: VN083613.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.05	2107	127.85	174	174.00	34629		
94.05	6316	128.90	52	175.00	2599		
95.10	49755	129.70	55	176.00	34533		
96.05	2838	134.80	125	177.00	2210		
103.95	335	136.80	71	281.00	69		
105.65	151	140.90	690				
105.90	119	142.85	641				
115.90	99	146.80	197				
116.85	467	154.70	76				
117.95	225	171.85	187				
118.80	321	172.85	373				

Instrument :

MSVOA_N

ClientSampleId :

BFB