


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN090418\
 Data File : VN051002.D
 Acq On : 4 Sep 2018 7:39
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082118W.M
 Title : SW846 8260
 Last Update : Wed Aug 22 05:38:12 2018

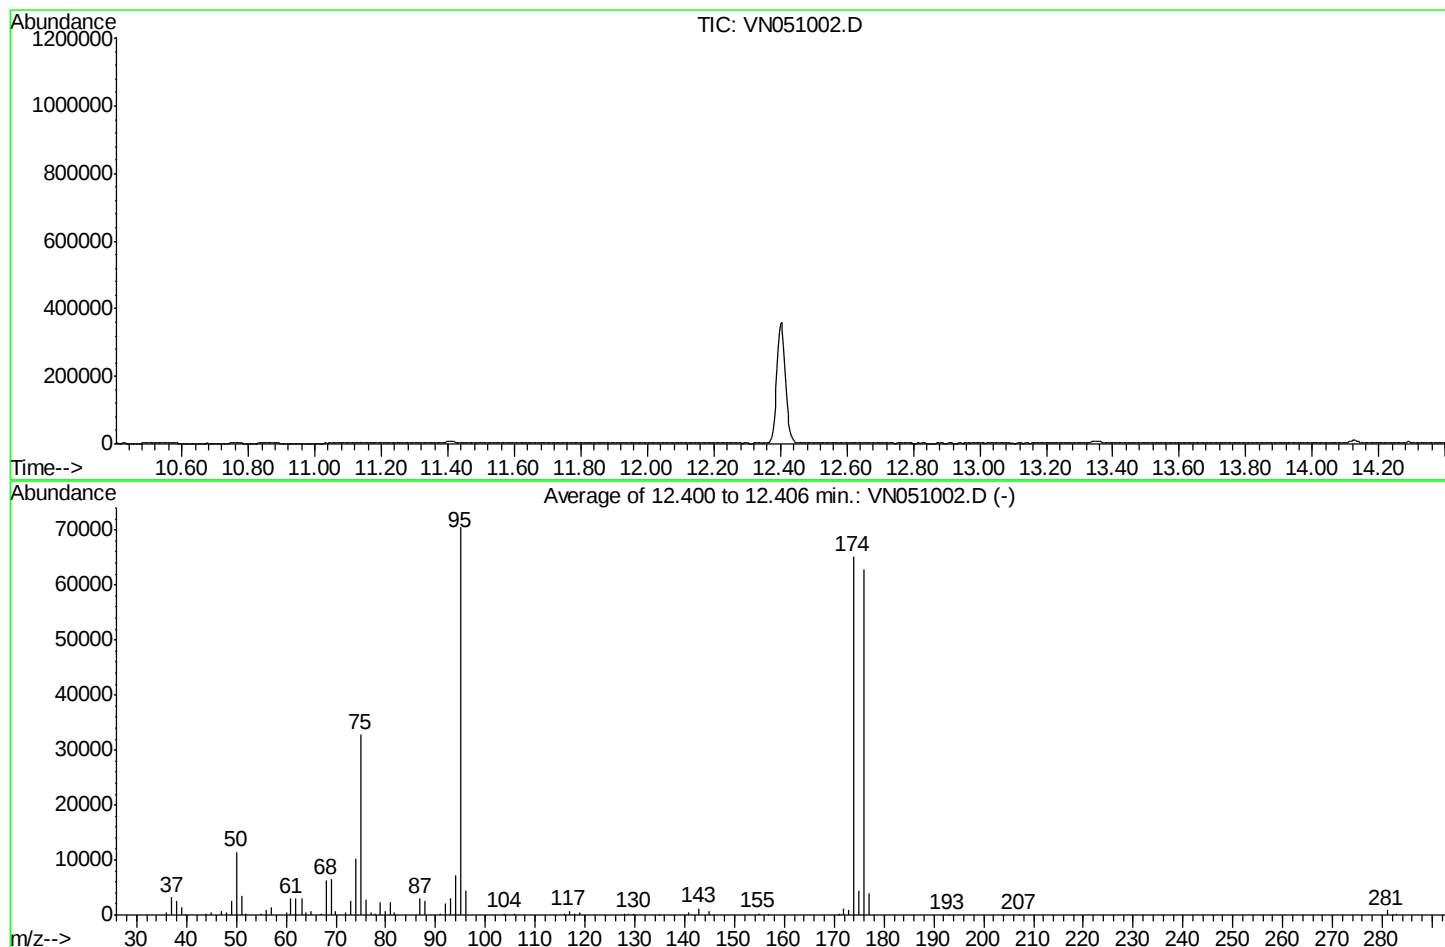

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	11478	PASS
75	95	30	60	46.5	32794	PASS
95	95	100	100	100.0	70498	PASS
96	95	5	9	6.2	4389	PASS
173	174	0.00	2	1.5	1008	PASS
174	95	50	100	92.4	65125	PASS
175	174	5	9	6.9	4472	PASS
176	174	95	101	96.7	62954	PASS
177	176	5	9	6.2	3902	PASS