


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN090519\
 Data File : VN057693.D
 Acq On : 5 Sep 2019 9:51
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N090319W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Sep 04 02:08:50 2019

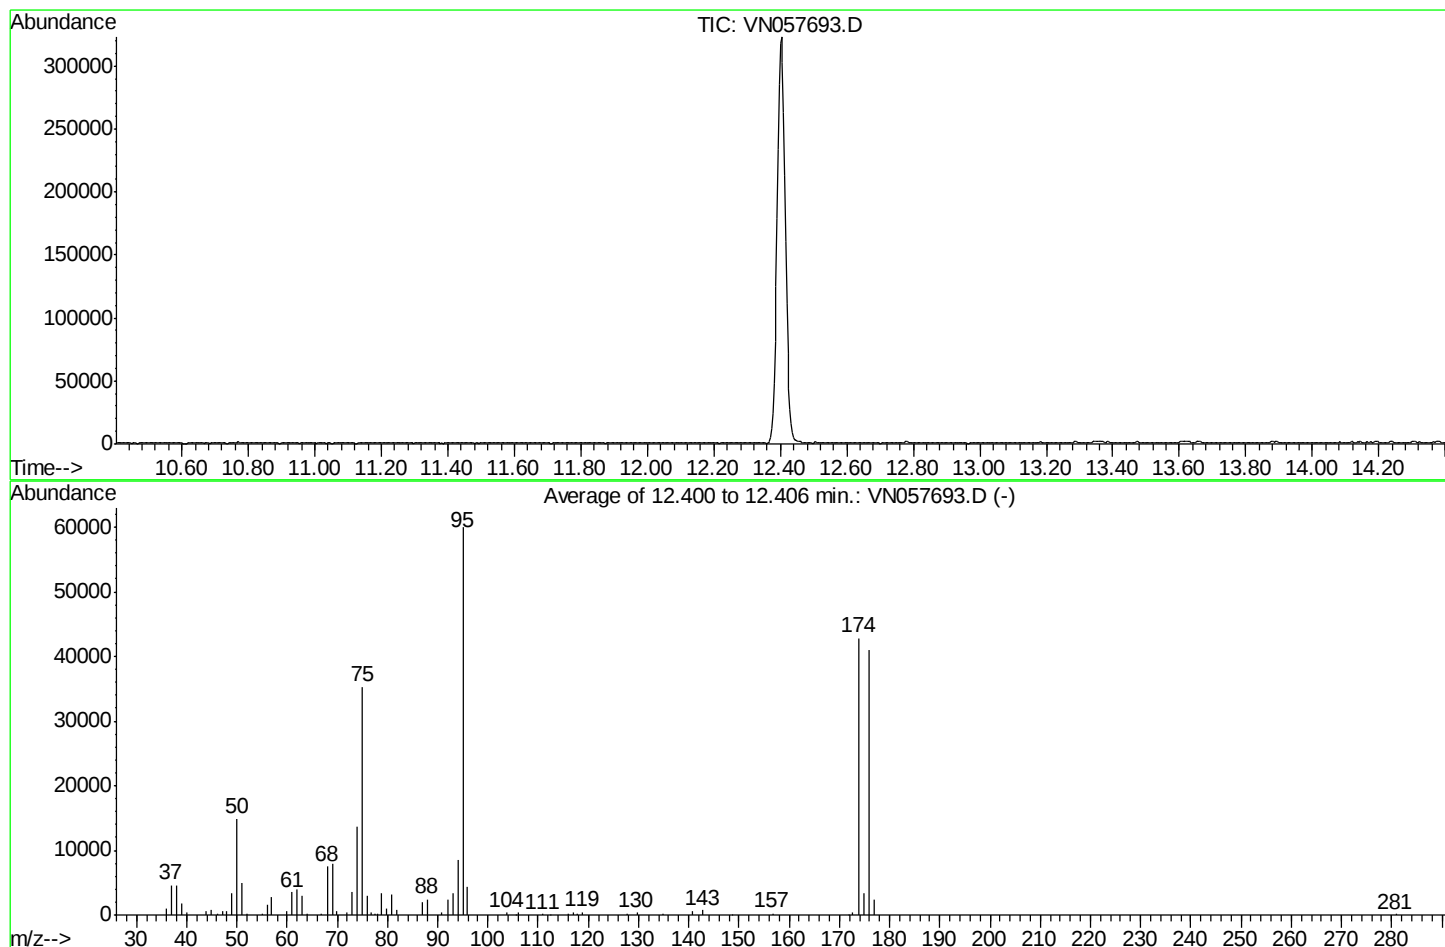

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.9	14950	PASS
75	95	30	60	58.8	35253	PASS
95	95	100	100	100.0	59970	PASS
96	95	5	9	7.2	4323	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.5	42850	PASS
175	174	5	9	7.9	3386	PASS
176	174	95	101	95.6	40970	PASS
177	176	5	9	6.0	2442	PASS