
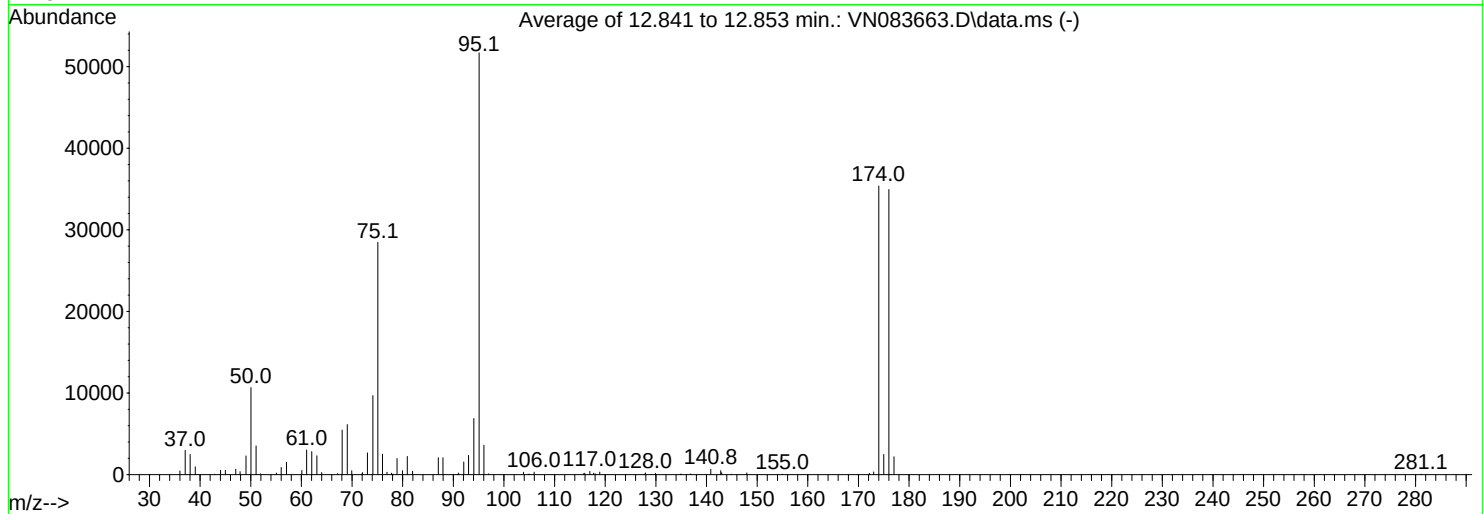


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090524\
Data File : VN083663.D
Acq On : 05 Sep 2024 08:26
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083024W.M
Title : SW846 8260
Last Update : Sat Aug 31 00:48:10 2024

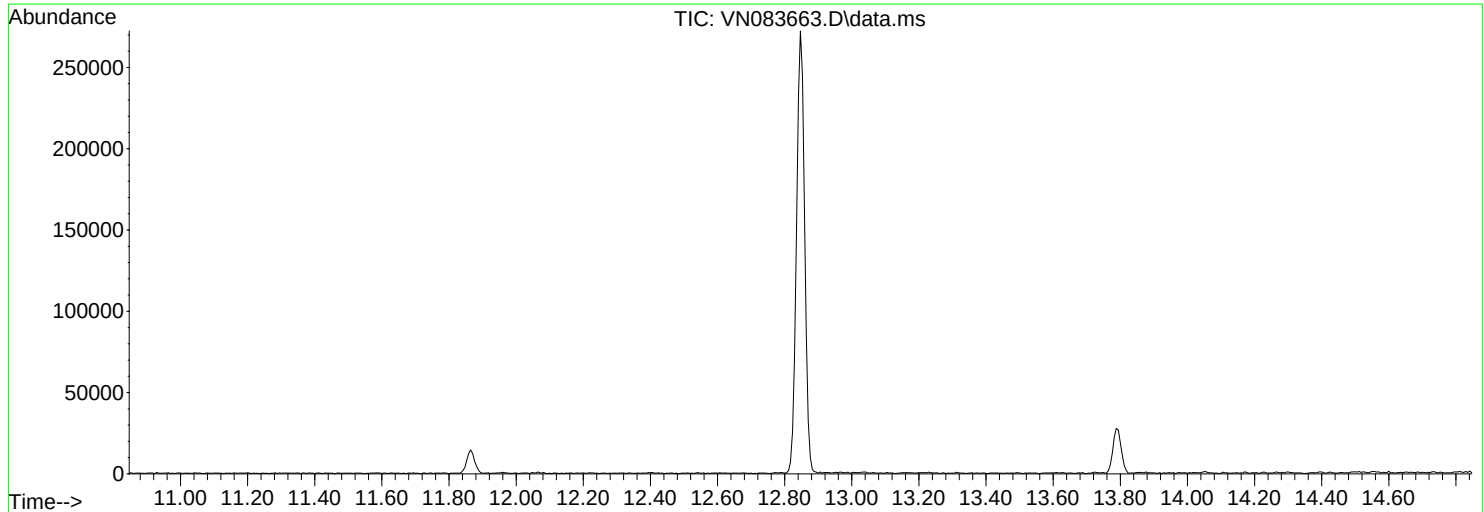

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	10662	PASS
75	95	30	60	55.1	28469	PASS
95	95	100	100	100.0	51693	PASS
96	95	5	9	7.0	3601	PASS
173	174	0.00	2	1.0	341	PASS
174	95	50	100	68.4	35373	PASS
175	174	5	9	7.0	2473	PASS
176	174	95	101	98.8	34952	PASS
177	176	5	9	6.3	2202	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	447	51.05	3523	68.05	5469	78.10	51
37.05	2980	51.95	106	69.05	6148	78.90	198
38.05	2469	55.05	201	69.95	499	79.95	49
39.05	963	56.00	889	71.90	78	80.90	223
42.90	52	57.05	1518	72.05	260	81.95	408
44.05	525	60.10	506	73.05	2672	87.05	2087
45.00	525	61.05	3031	74.10	9678	87.95	2081
47.05	674	62.05	2819	75.10	28469	90.80	50
47.90	378	63.05	2307	76.00	2502	91.05	191
49.05	2293	64.00	264	76.90	293	92.05	1547
50.05	10662	67.15	142	77.80	169	93.00	2354

Average of 12.841 to 12.853 min.: VN083663.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	6889	117.70	174	143.00	233		
95.10	51693	118.00	95	144.90	56		
96.05	3601	118.90	312	147.95	209		
96.95	106	127.80	70	155.00	53		
103.85	286	127.95	208	172.15	150		
104.80	51	129.90	150	173.00	341		
105.00	56	134.80	63	174.00	35373		
105.95	310	135.00	61	175.00	2473		
115.70	110	136.90	107	176.00	34952		
115.95	173	140.85	667	177.00	2202		
116.95	403	142.80	488	281.10	60		

Instrument :

MSVOA_N

ClientSampleId :

BFB