

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN090618\
 Data File : VN051039.D
 Acq On : 6 Sep 2018 18:08
 Operator : MD\SY
 Sample : J4817-02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 002M-35TH-AVE

Manual Integrations
 APPROVED

MMDadoda
 9/7/2018 11:23:29 AM

Quant Time: Sep 07 03:55:36 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA N\METHODS\624N082818W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Wed Aug 29 01:38:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	7.20	128	133858	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	8.59	114	682625	30.00	ug/l	0.00
57) Chlorobenzene-d5	11.41	117	607336	30.00	ug/l	0.00

System Monitoring Compounds

27) 1,2-Dichloroethane-d4	8.03	65	257261	30.12	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	100.40%
60) 4-Bromofluorobenzene	12.40	95	239355	26.50	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	88.33%
63) Toluene-d8	10.09	98	815262	28.79	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	95.97%

Target Compounds

						Ovalue
15) Acetone	3.82	58	1537865	2125.25	ug/l	92
30) 2-Butanone	6.85	43	66726	21.22	ug/l	97
58) 4-Methyl-2-Pentanone	9.99	43	16195	2.33	ug/l	97
62) Toluene	10.15	91	17873692m	527.51	ug/l	
82) p-Isopropyltoluene	13.29	119	308006	11.21	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN090618\
Data File : VN051039.D
Acq On : 6 Sep 2018 18:08
Operator : MD\SY
Sample : J4817-02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 13 Sample Multiplier: 1


Instrument :
MSVOA_N
ClientSampleId :
002M-35TH-AVE

Manual Integrations
APPROVED

MMDadoda
9/7/2018 11:23:29 AM

Quant Time: Sep 07 03:55:36 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA N\METHODS\624N082818W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Wed Aug 29 01:38:44 2018
Response via : Initial Calibration

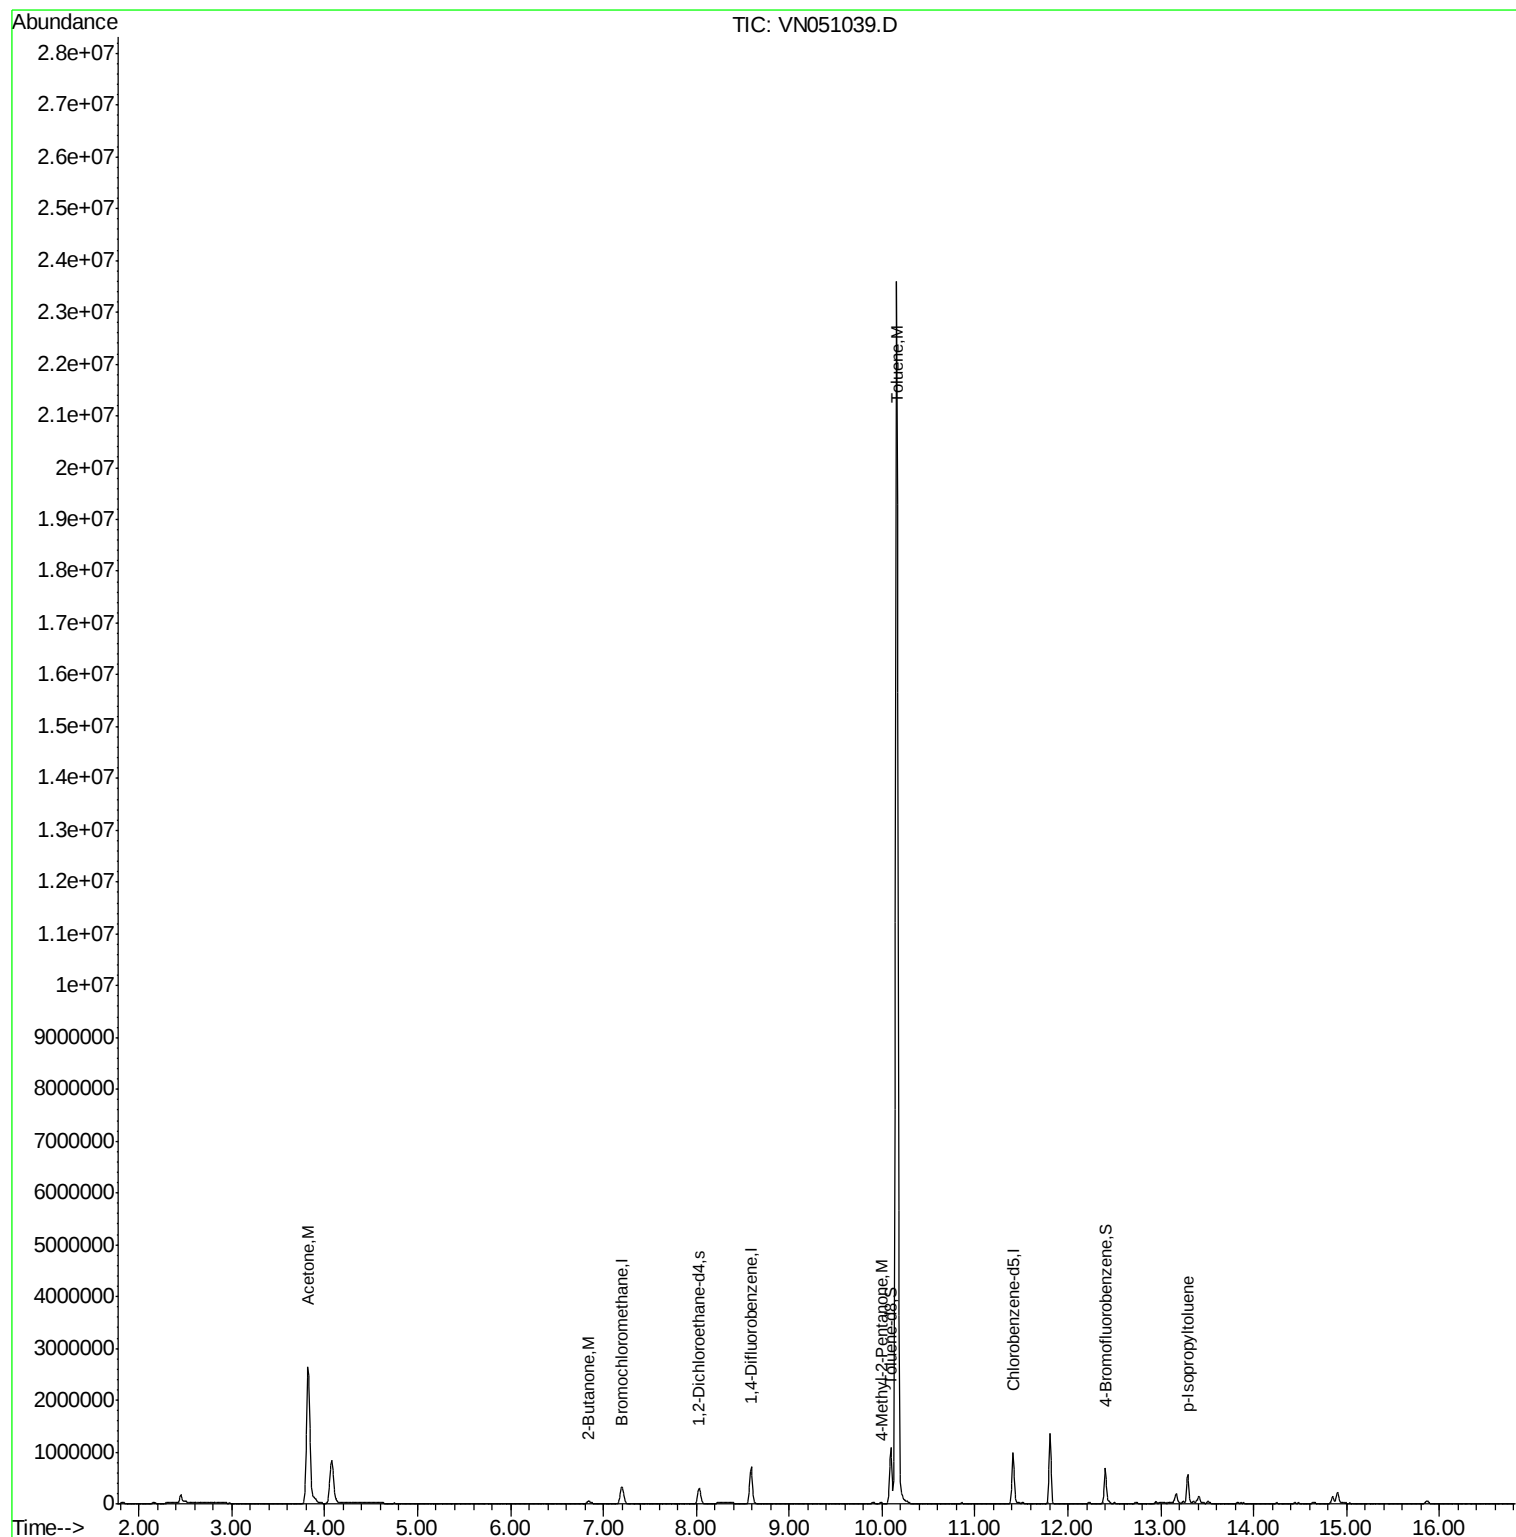

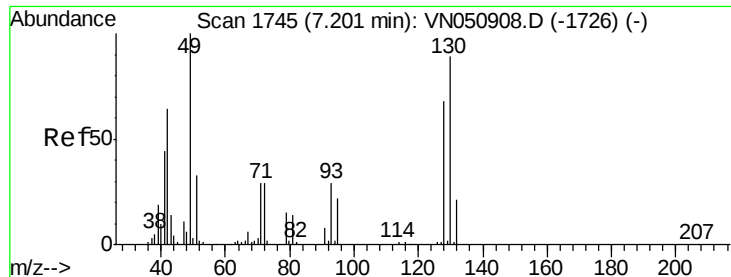

#1

Bromochloromethane

Concen: 30.00 ug/l

RT: 7.20 min Scan# 1687

Delta R.T. -0.00 min

Lab File: VN051039.D

Acq: 6 Sep 2018 18:08

Instrument :

MSVOA_N


ClientSampleId :

002M-35TH-AVE




Tot Ion:	128	Resp:	133858
Ion	Ratio	Lower	Upper
128	100		
49	147.5	0.0	380.3
130	128.5	0.0	325.3

Manual Integrations
APPROVED

MMDadoda
9/7/2018 11:23:29 AM

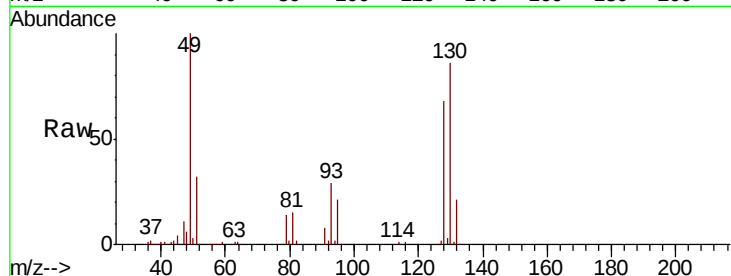

Abundance Ion 128.00 (127.70 to 128.70): V
Ion 49.00 (48.70 to 49.70): VN
Ion 130.00 (129.70 to 130.70): V

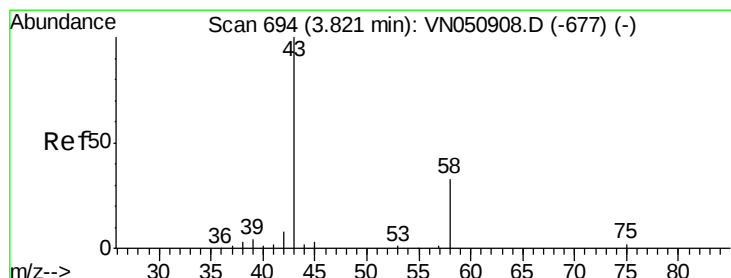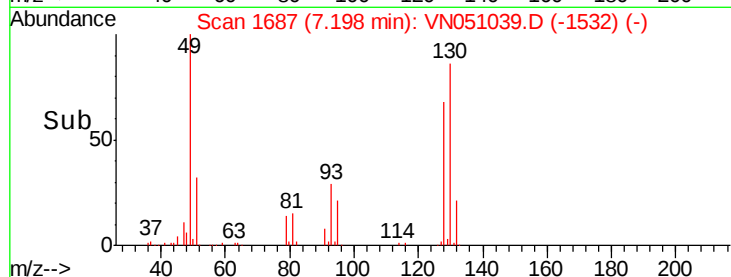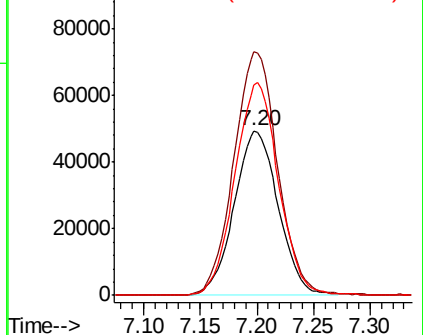

#15

Acetone

Concen: 2125.25 ug/l


RT: 3.82 min Scan# 637

Delta R.T. 0.00 min



Lab File: VN051039.D


Acq: 6 Sep 2018 18:08

Tgt Ion:	58	Resp:	1537865
Ion	Ratio	Lower	Upper
58	100		
43	284.0	239.4	359.0

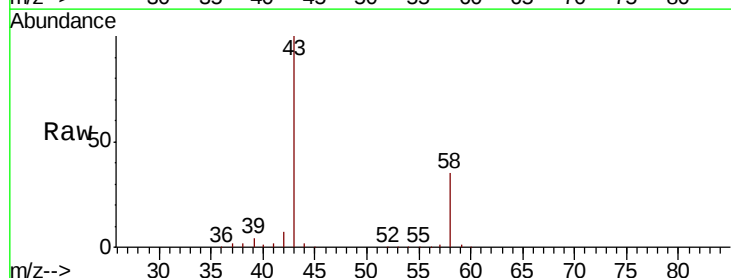

Abundance Ion 58.00 (57.70 to 58.70): VN
Ion 43.00 (42.70 to 43.70): VN

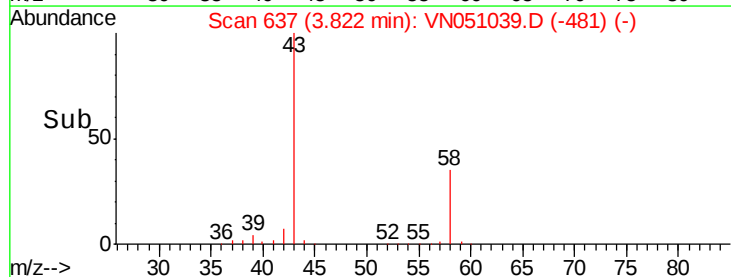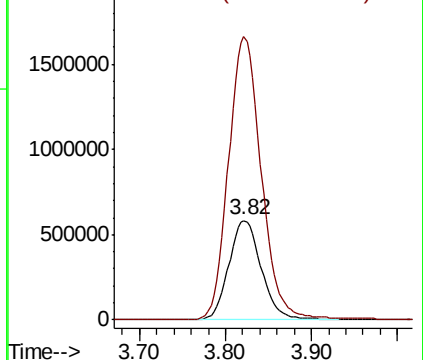

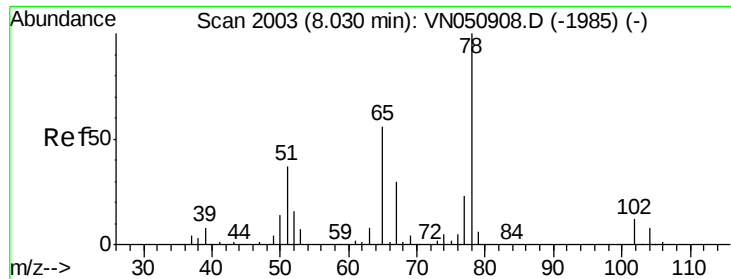

#27

1,2-Dichloroethane-d4

Concen: 30.12 ug/l

RT: 8.03 min Scan# 1946

Delta R.T. 0.00 min

Lab File: VN051039.D

Acq: 6 Sep 2018 18:08

Instrument :

MSVOA_N

ClientSampleId :

002M-35TH-AVE

Tot Ion: 65 Resp: 257261

Ion Ratio Lower Upper

65 100


67 54.4 43.7 65.5

Manual Integrations

APPROVED




MMDadoda

9/7/2018 11:23:29 AM

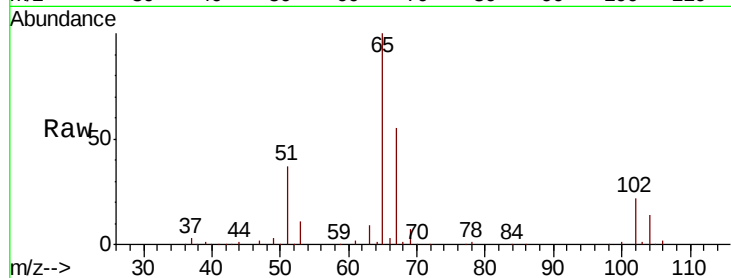

Abundance Ion 65.00 (64.70 to 65.70): VN0

Ion 67.00 (66.70 to 67.70): VN0

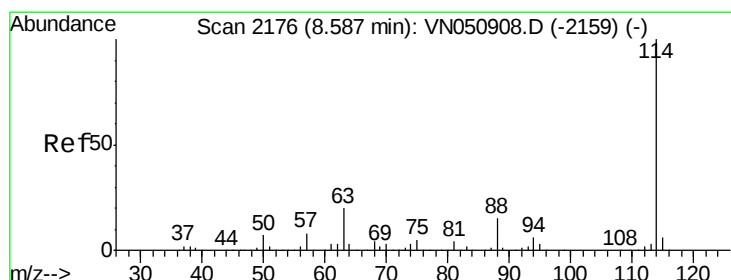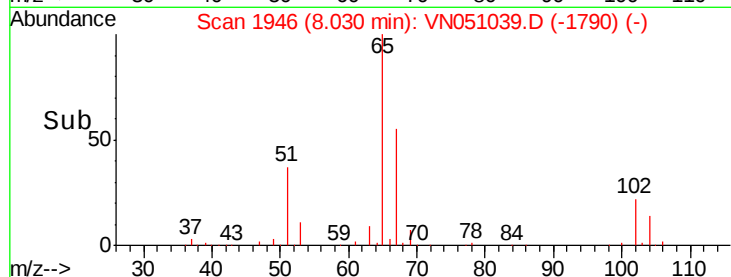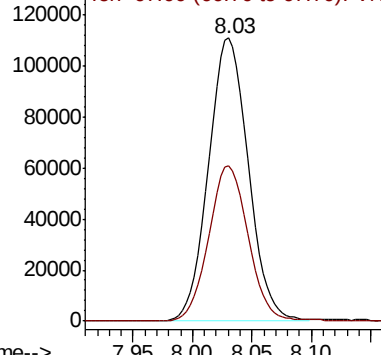

#28

1,4-Difluorobenzene

Concen: 30.00 ug/l

RT: 8.59 min Scan# 2120

Delta R.T. 0.00 min

Lab File: VN051039.D

Acq: 6 Sep 2018 18:08


Tgt Ion: 114 Resp: 682625

Ion Ratio Lower Upper

114 100

63 19.1 15.6 23.4



88 15.1 12.2 18.4

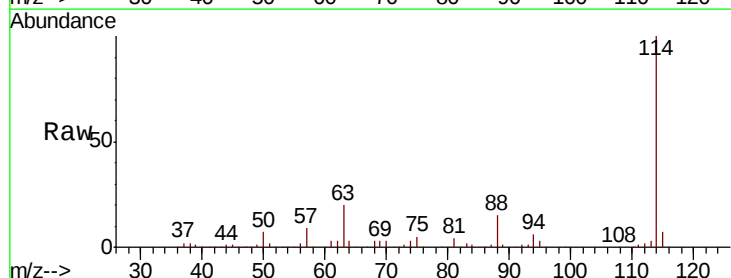


Abundance Ion 114.00 (113.70 to 114.70): V

Ion 63.00 (62.70 to 63.70): VN0

Ion 88.00 (87.70 to 88.70): VN0

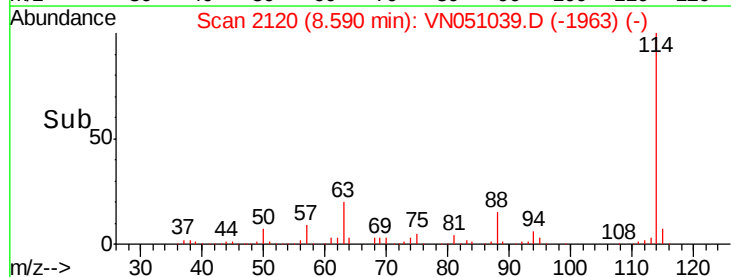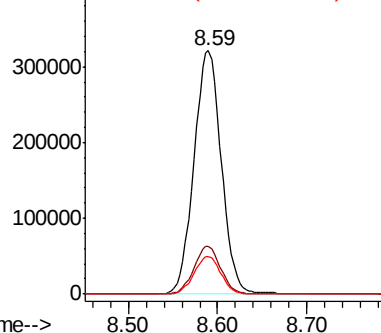

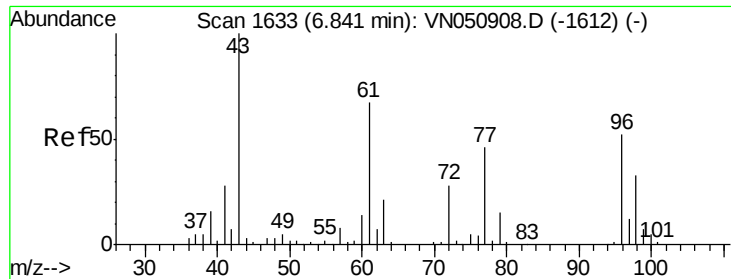





#30
2-Butanone
Concen: 21.22 ug/l
RT: 6.85 min Scan# 1578
Delta R.T. 0.01 min
Lab File: VN051039.D
Acq: 6 Sep 2018 18:08

Instrument :
MSVOA_N
ClientSampleId :
002M-35TH-AVE

Tot Ion	Ratio	Lower	Upper
43	100		
57	8.5	6.9	10.3
72	26.4	22.8	34.2




Manual Integrations
APPROVED


MMDadoda
9/7/2018 11:23:29 AM

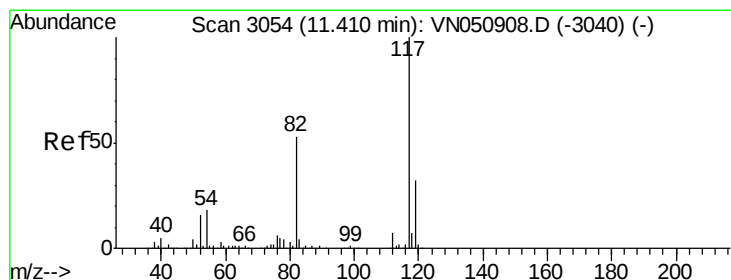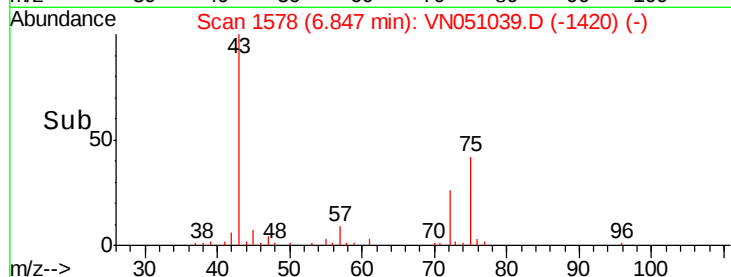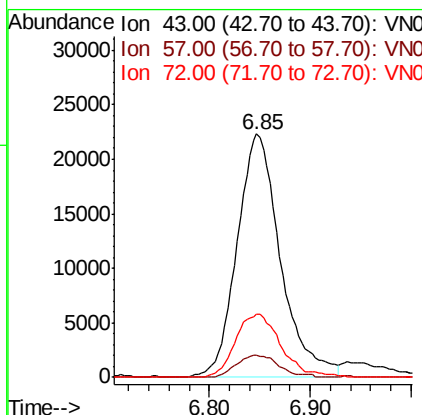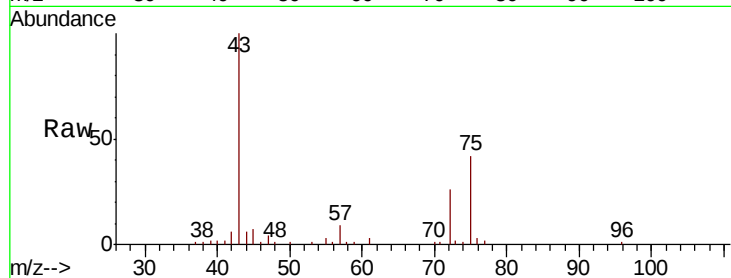

#57
Chlorobenzene-d5
Concen: 30.00 ug/l
RT: 11.41 min Scan# 2997
Delta R.T. 0.00 min
Lab File: VN051039.D
Acq: 6 Sep 2018 18:08

Tgt Ion	Ratio	Lower	Upper
117	100		
82	52.1	42.6	64.0
119	32.3	25.7	38.5

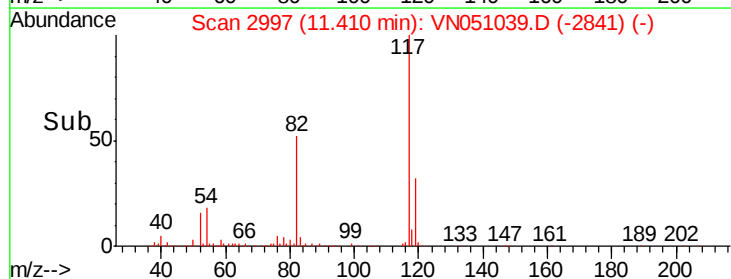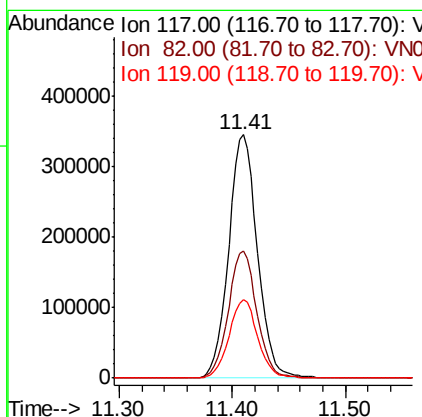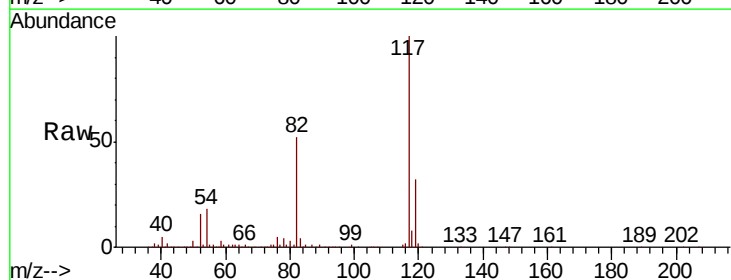

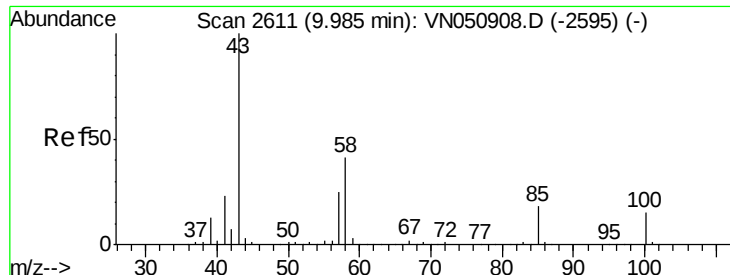





#58
4-Methyl-2-Pentanone
Concen: 2.33 ug/l
RT: 9.99 min Scan# 2555
Delta R.T. 0.00 min
Lab File: VN051039.D
Acq: 6 Sep 2018 18:08

Instrument :
MSVOA_N
ClientSampleId :
002M-35TH-AVE

Tot Ion	Ratio	Lower	Upper
43	100		
58	38.1	32.3	48.5
85	18.5	14.9	22.3




Manual Integrations
APPROVED


MMDadoda
9/7/2018 11:23:29 AM

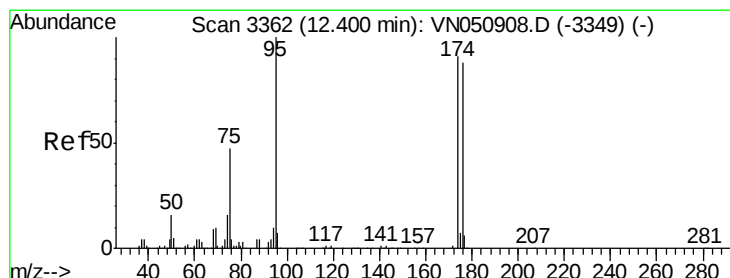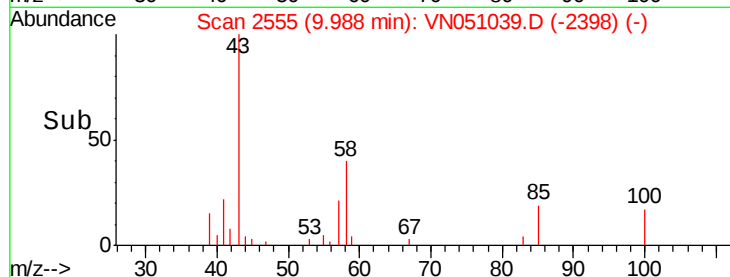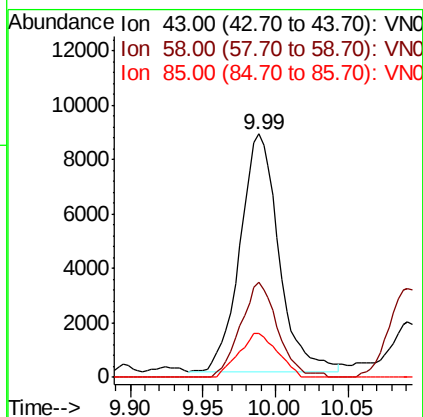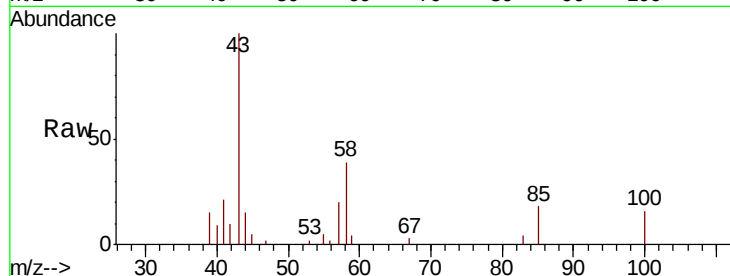

#60
4-Bromofluorobenzene
Concen: 26.50 ug/l
RT: 12.40 min Scan# 3306
Delta R.T. 0.00 min
Lab File: VN051039.D
Acq: 6 Sep 2018 18:08

Tgt Ion	Ratio	Lower	Upper
95	100		
174	92.3	74.6	112.0
176	89.2	71.5	107.3

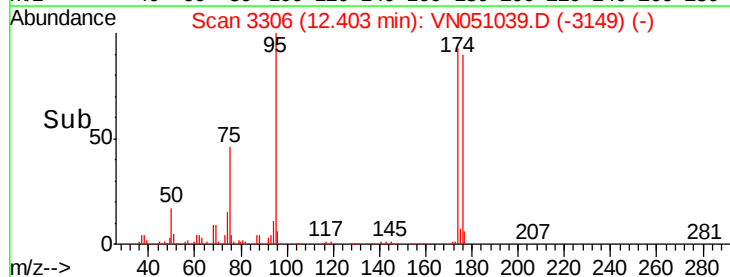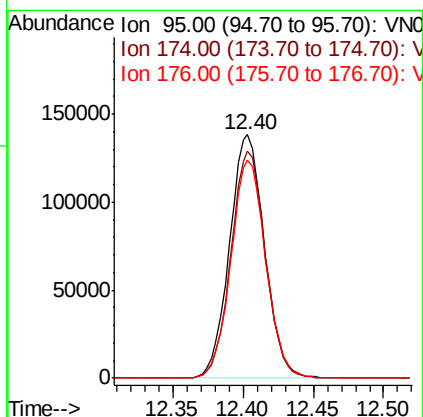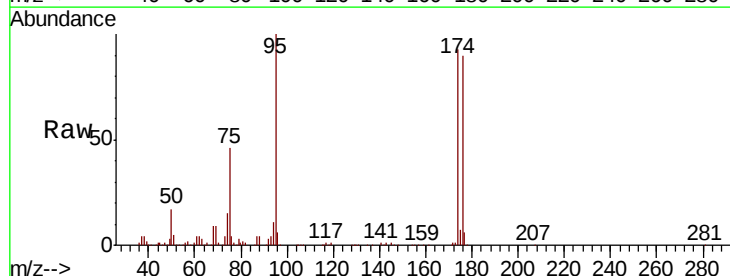

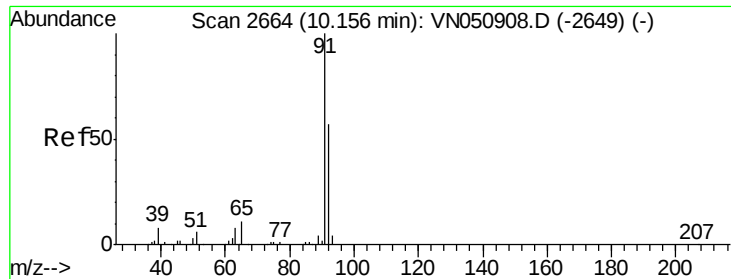

#62

Toluene

Concen: 527.51 ug/l m

RT: 10.15 min Scan# 2606

Delta R.T. -0.00 min

Lab File: VN051039.D

Acq: 6 Sep 2018 18:08

Instrument :

MSVOA_N

ClientSampleId :

002M-35TH-AVE

Tot Ion: 91 Resp:17873692

Ion Ratio Lower Upper

91 100





92 0.0 45.8 68.8#

Manual Integrations

APPROVED

MMDadoda

9/7/2018 11:23:29 AM

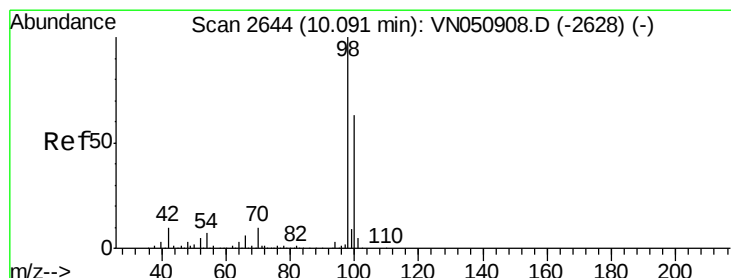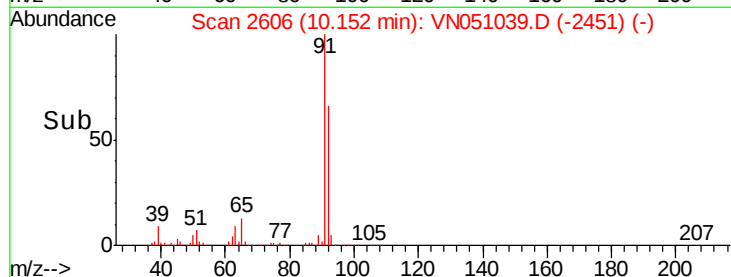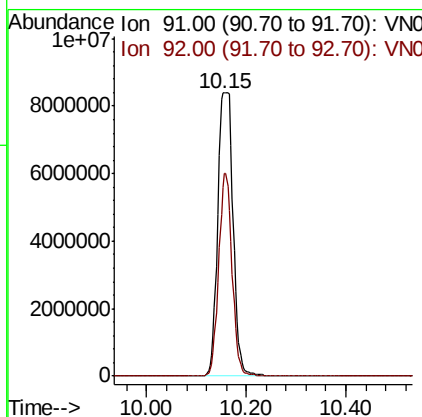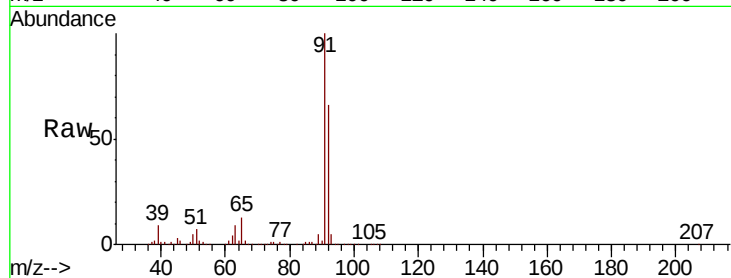

#63

Toluene-d8

Concen: 28.79 ug/l

RT: 10.09 min Scan# 2588

Delta R.T. 0.00 min

Lab File: VN051039.D




Acq: 6 Sep 2018 18:08


Tgt Ion: 98 Resp: 815262

Ion Ratio Lower Upper

98 100

100 63.1 50.6 75.8

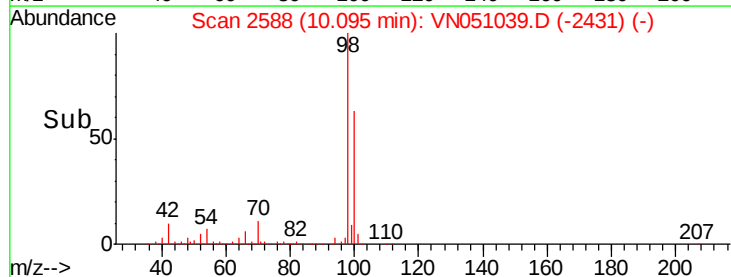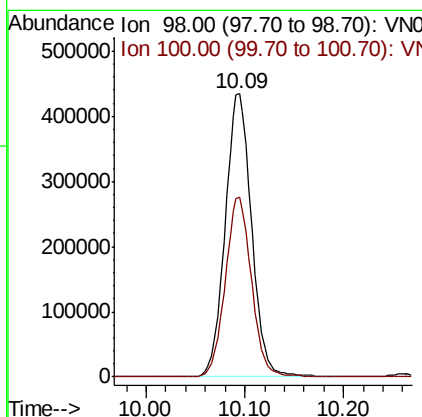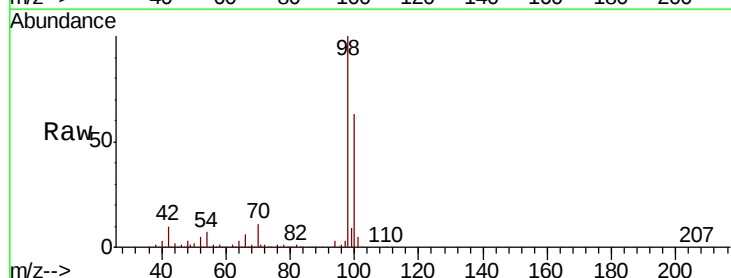

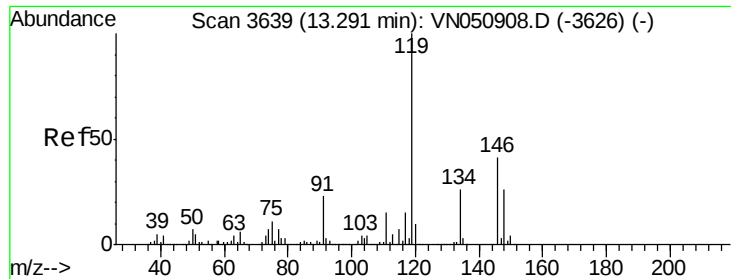

#82
 p-Isopropyltoluene
 Concen: 11.21 ug/l
 RT: 13.29 min Scan# 3582
 Delta R.T. 0.00 min
 Lab File: VN051039.D
 Acq: 6 Sep 2018 18:08

Instrument :
 MSVOA_N
 ClientSampleId :
 002M-35TH-AVE

Tot Ion	Ratio	Resp Lower	Upper
119	100		
134	27.5	0.0	53.2
91	23.4	0.0	46.0

Manual Integrations
 APPROVED

MMDadoda
 9/7/2018 11:23:29 AM

