

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN090619\
 Data File : VN057733.D
 Acq On : 6 Sep 2019 23:00
 Operator : JC/SP
 Sample : K4580-32
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PAR-12-C2-(0)

Quant Time: Sep 07 00:10:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N090619W.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 06 03:46:54 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.65	168	195785	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.57	114	321773	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	300221	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	153534	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.01	65	247159	51.89	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.78%	
35) Dibromofluoromethane	7.58	113	143210	48.86	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.72%	
50) Toluene-d8	10.08	98	559575	51.61	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.22%	
62) 4-Bromofluorobenzene	12.40	95	204283	45.36	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.72%	
Target Compounds						
16) Acetone	3.80	43	8746	5.967	ug/l	98
43) Isopropyl Acetate	8.15	43	69737	8.549	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN090619\
Data File : VN057733.D
Acq On : 6 Sep 2019 23:00
Operator : JC/SP
Sample : K4580-32
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PAR-12-C2-(0)

Quant Time: Sep 07 00:10:09 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N090619W.M
Quant Title : SW846 8260
QLast Update : Fri Sep 06 03:46:54 2019
Response via : Initial Calibration

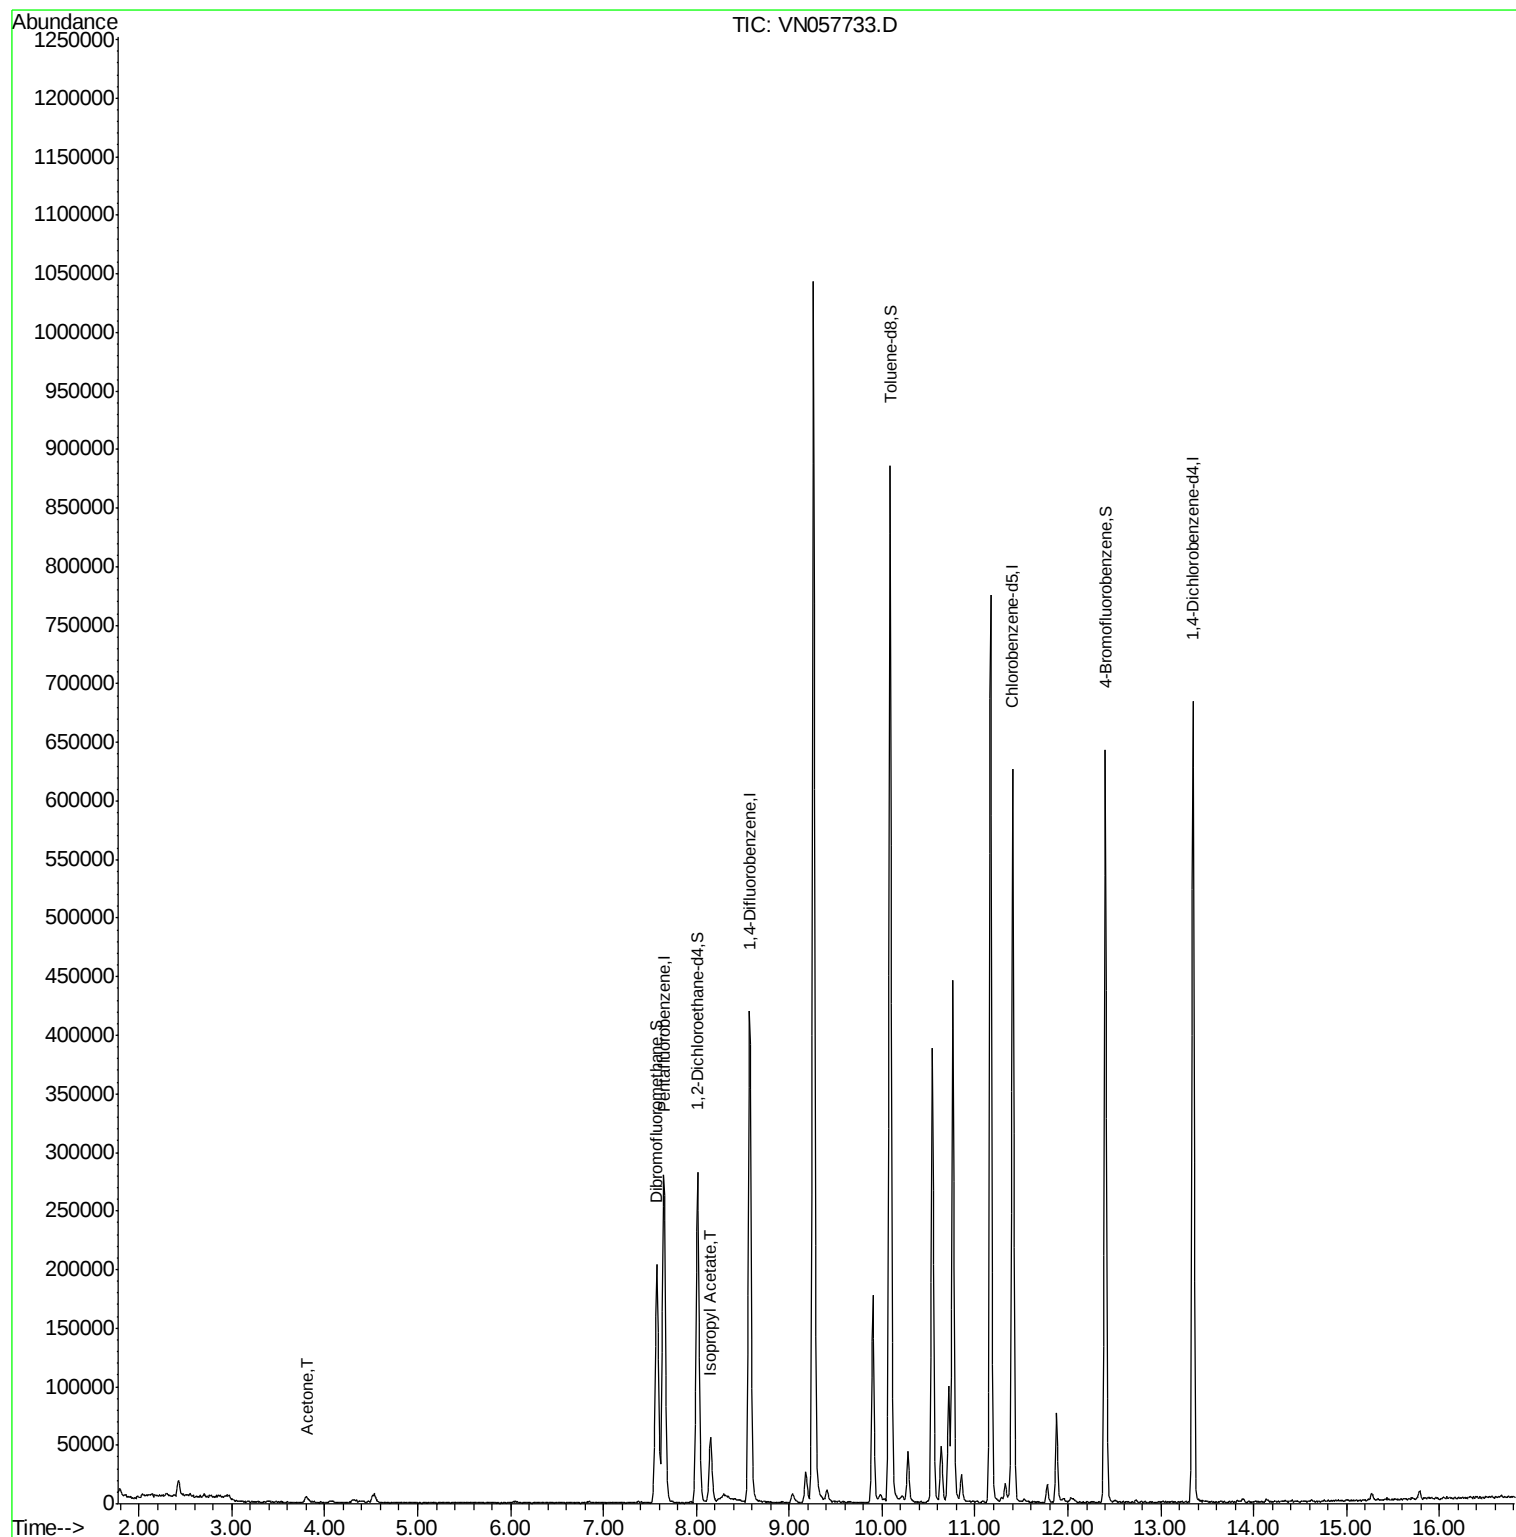

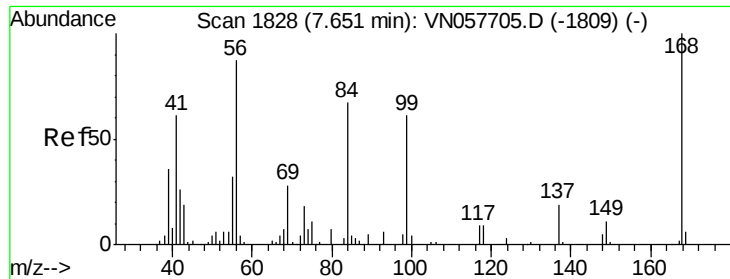

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.65 min Scan# 1828

Delta R.T. 0.00 min

Lab File: VN057733.D

Acq: 6 Sep 2019 23:00

Instrument :

MSVOA_N

ClientSampleId :


PAR-12-C2-(0)

Tot Ion:168 Resp: 195785

Ion Ratio Lower Upper




168 100

99 66.9 57.4 86.0

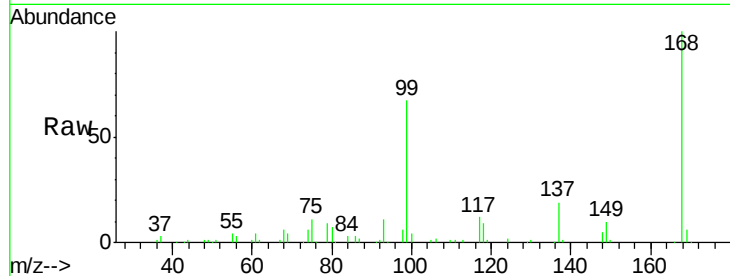

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

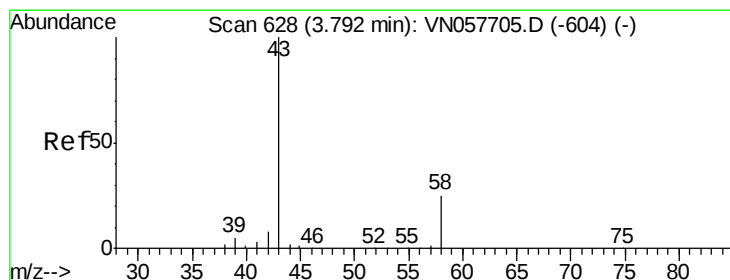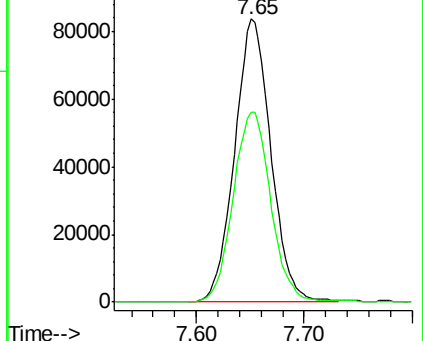

#16

Acetone

Concen: 5.967 ug/l

RT: 3.80 min Scan# 631

Delta R.T. 0.01 min

Lab File: VN057733.D


Acq: 6 Sep 2019 23:00

Tgt Ion: 43 Resp: 8746

Ion Ratio Lower Upper



43 100


58 23.6 19.8 29.8

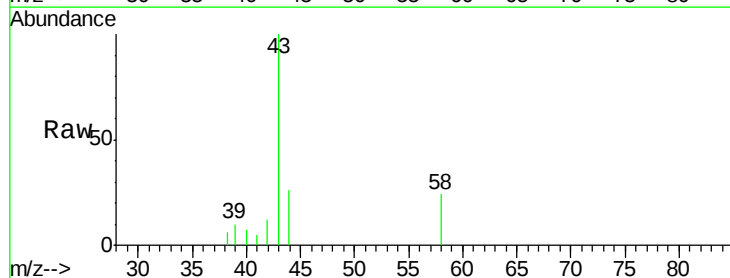

Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 58.00 (57.70 to 58.70): VNO




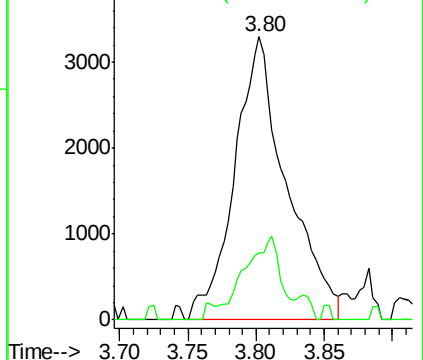


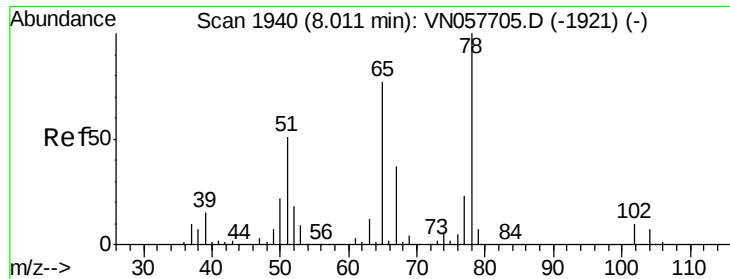

#33
 1,2-Dichloroethane-d4
 Concen: 51.893 ug/l
 RT: 8.01 min Scan# 1941
 Delta R.T. 0.00 min
 Lab File: VN057733.D
 Acq: 6 Sep 2019 23:00




Instrument :
 MSVOA_N
 ClientSampleId :
 PAR-12-C2-(0)


Tot Ion: 65 Resp: 247159
 Ion Ratio Lower Upper
 65 100
 67 49.5 0.0 98.2

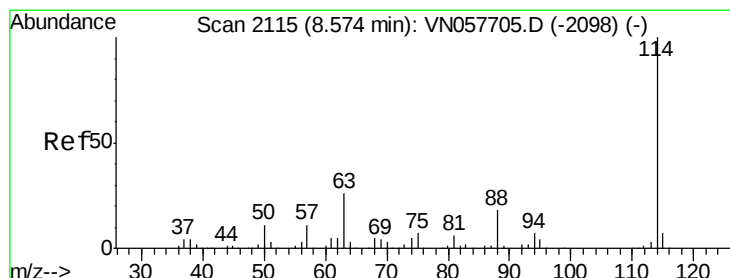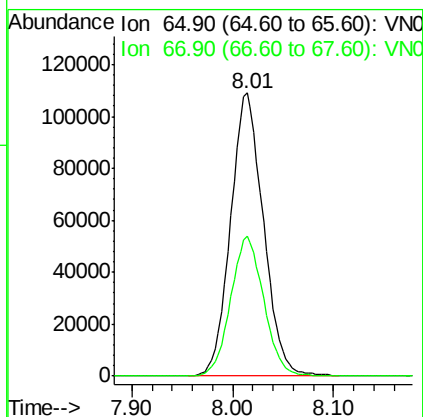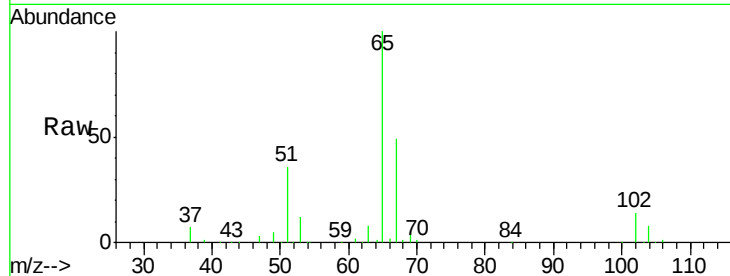

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.57 min Scan# 2115
 Delta R.T. 0.00 min
 Lab File: VN057733.D
 Acq: 6 Sep 2019 23:00

Tgt Ion: 114 Resp: 321773
 Ion Ratio Lower Upper
 114 100
 63 25.9 0.0 52.4
 88 17.5 0.0 35.4

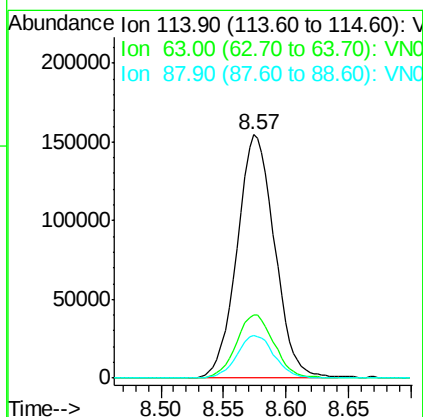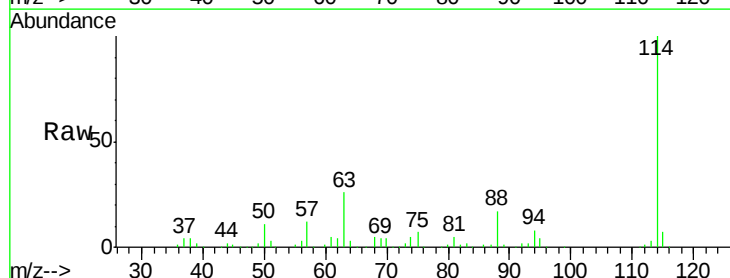







#35
 Dibromofluoromethane
 Concen: 48.863 ug/l
 RT: 7.58 min Scan# 1805
 Delta R.T. 0.00 min
 Lab File: VN057733.D
 Acq: 6 Sep 2019 23:00

Instrument :
 MSVOA_N
 ClientSampleId :
 PAR-12-C2-(0)

Tot Ion:113 Resp: 143210
 Ion Ratio Lower Upper
 113 100
 111 101.5 82.7 124.1
 192 17.8 13.8 20.6

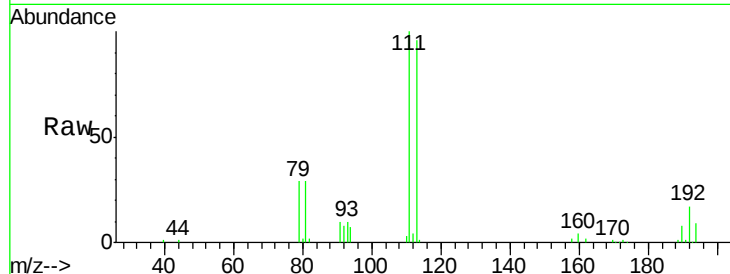


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

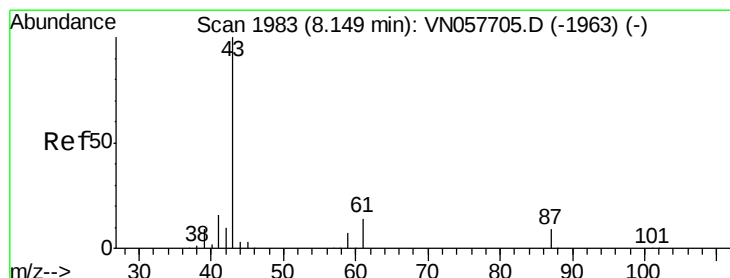
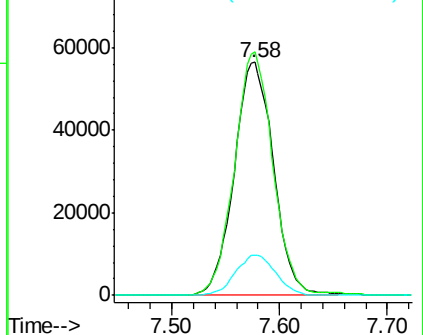



#43
 Isopropyl Acetate
 Concen: 8.549 ug/l
 RT: 8.15 min Scan# 1984
 Delta R.T. 0.00 min
 Lab File: VN057733.D
 Acq: 6 Sep 2019 23:00

Tgt Ion: 43 Resp: 69737
 Ion Ratio Lower Upper
 43 100
 61 15.5 12.8 19.2
 87 11.3 7.8 11.8

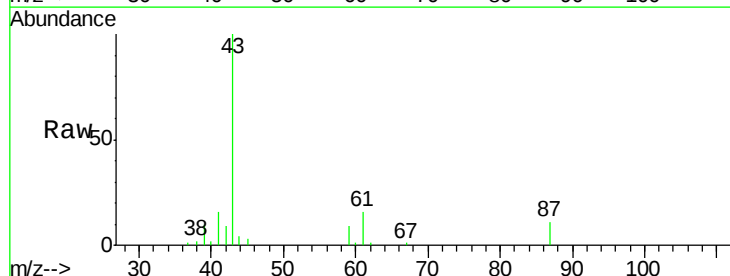

Abundance Ion 43.00 (42.70 to 43.70): V
 Ion 61.00 (60.70 to 61.70): V
 Ion 87.00 (86.70 to 87.70): V

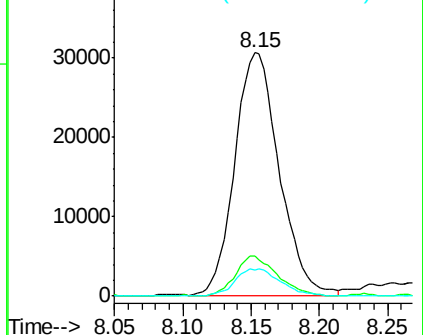



#50

Toluene-d8

Concen: 51.612 ug/l

RT: 10.08 min Scan# 2585

Delta R.T. 0.00 min

Lab File: VN057733.D

Acq: 6 Sep 2019 23:00

Instrument :

MSVOA_N

ClientSampleId :


PAR-12-C2-(0)

Tot Ion: 98 Resp: 559575

Ion Ratio Lower Upper

98 100

100 63.7 50.7 76.1

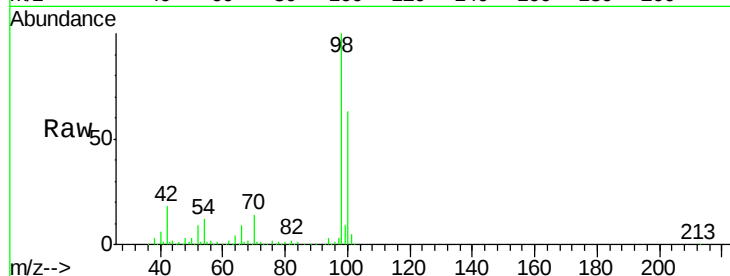

Abundance Ion 98.00 (97.70 to 98.70): VN057733.D (-2492) (-)

Ion 100.00 (99.70 to 100.70): VN057733.D (-2492) (-)

10.08



300000

200000

100000

0

Time-->

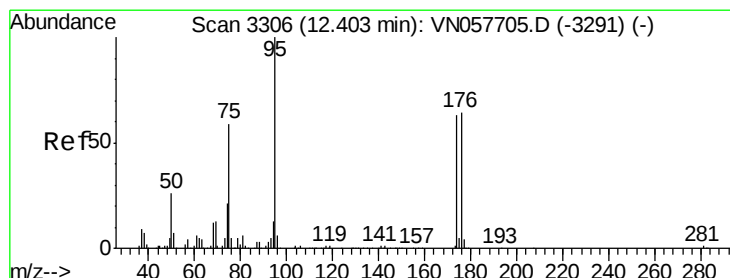

#62

4-Bromofluorobenzene

Concen: 45.364 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.00 min

Lab File: VN057733.D

Acq: 6 Sep 2019 23:00


Tgt Ion: 95 Resp: 204283

Ion Ratio Lower Upper

95 100

174 67.9 0.0 128.0

176 66.2 0.0 128.0

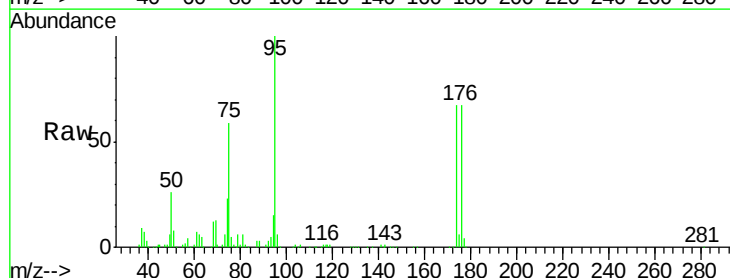

Abundance Ion 94.90 (94.60 to 95.60): VN057733.D (-3213) (-)

Ion 173.80 (173.50 to 174.50): VN057733.D (-3213) (-)

Ion 175.80 (175.50 to 176.50): VN057733.D (-3213) (-)

12.40


150000


100000

50000

0

Time-->



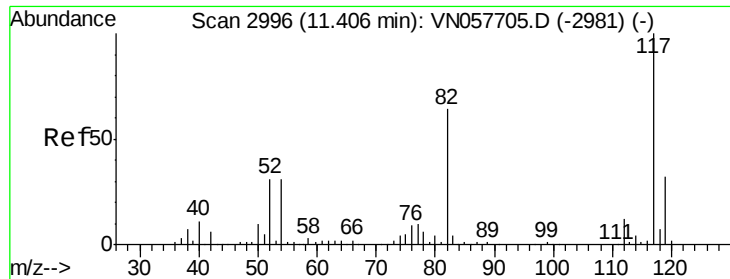

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2996

Delta R.T. 0.00 min

Lab File: VN057733.D

Acq: 6 Sep 2019 23:00

Instrument :

MSVOA_N

ClientSampleId :

PAR-12-C2-(0)


Tot Ion:117 Resp: 300221

Ion Ratio Lower Upper

117 100

82 63.6 51.4 77.0




119 31.7 25.4 38.2

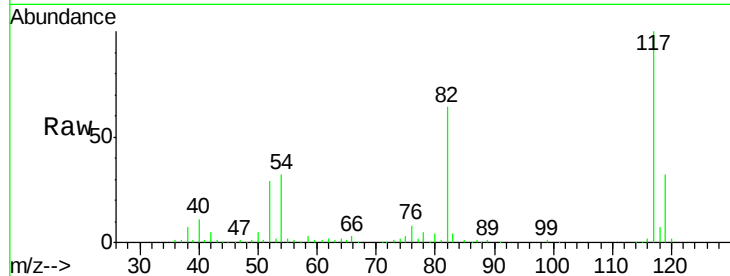

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

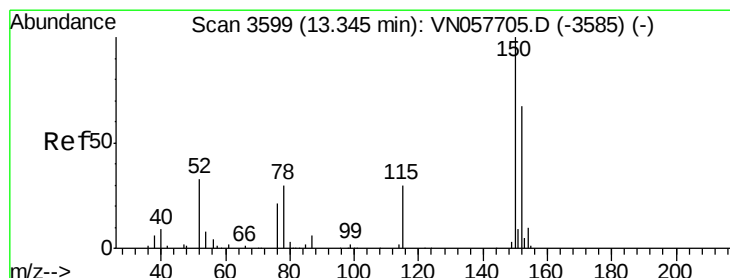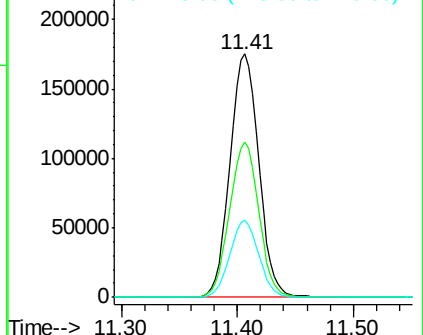

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3600

Delta R.T. 0.00 min

Lab File: VN057733.D

Acq: 6 Sep 2019 23:00


Tgt Ion:152 Resp: 153534

Ion Ratio Lower Upper

152 100

115 64.4 33.8 101.3

150 157.7 0.0 345.4

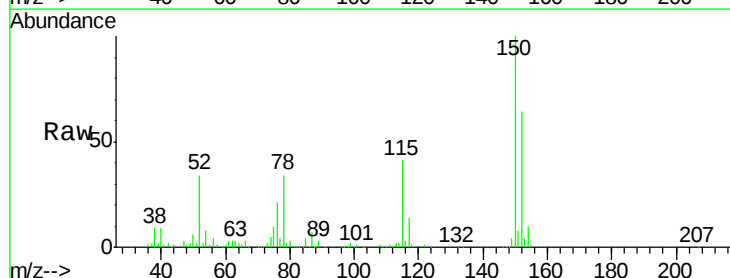

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

