


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN090619\
Data File : VN057701.D
Acq On : 5 Sep 2019 17:03
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N090619W.M
Title : SW846 8260
Last Update : Fri Sep 06 03:46:54 2019

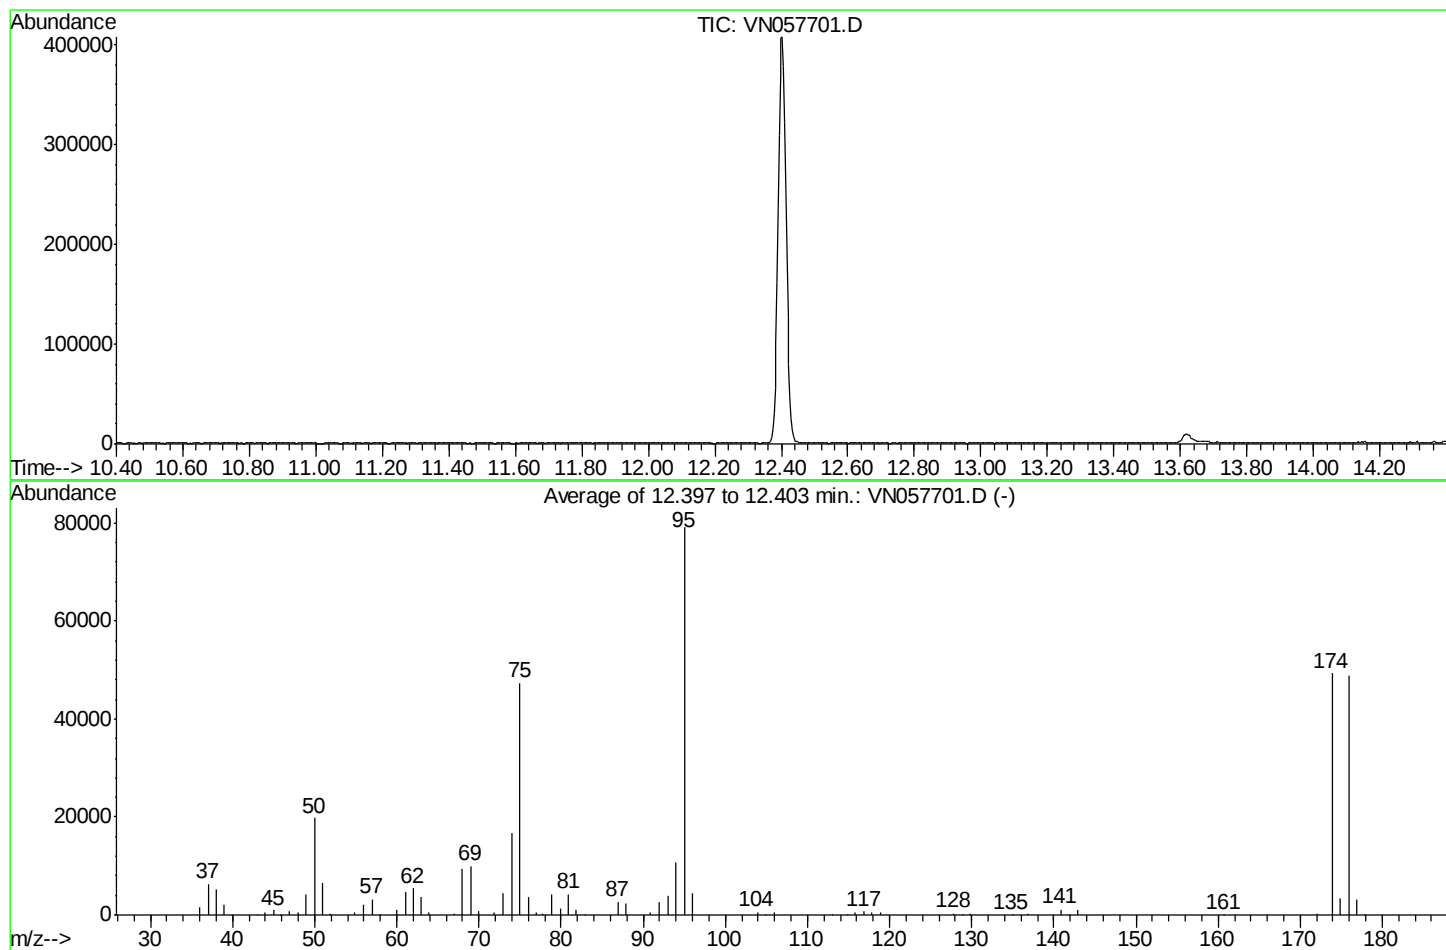

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.0	19797	PASS
75	95	30	60	59.9	47384	PASS
95	95	100	100	100.0	79125	PASS
96	95	5	9	5.7	4528	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	62.3	49288	PASS
175	174	5	9	7.1	3518	PASS
176	174	95	101	99.0	48797	PASS
177	176	5	9	6.6	3226	PASS