


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN090718\
 Data File : VN051040.D
 Acq On : 7 Sep 2018 8:05
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N082818W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Aug 29 01:38:44 2018

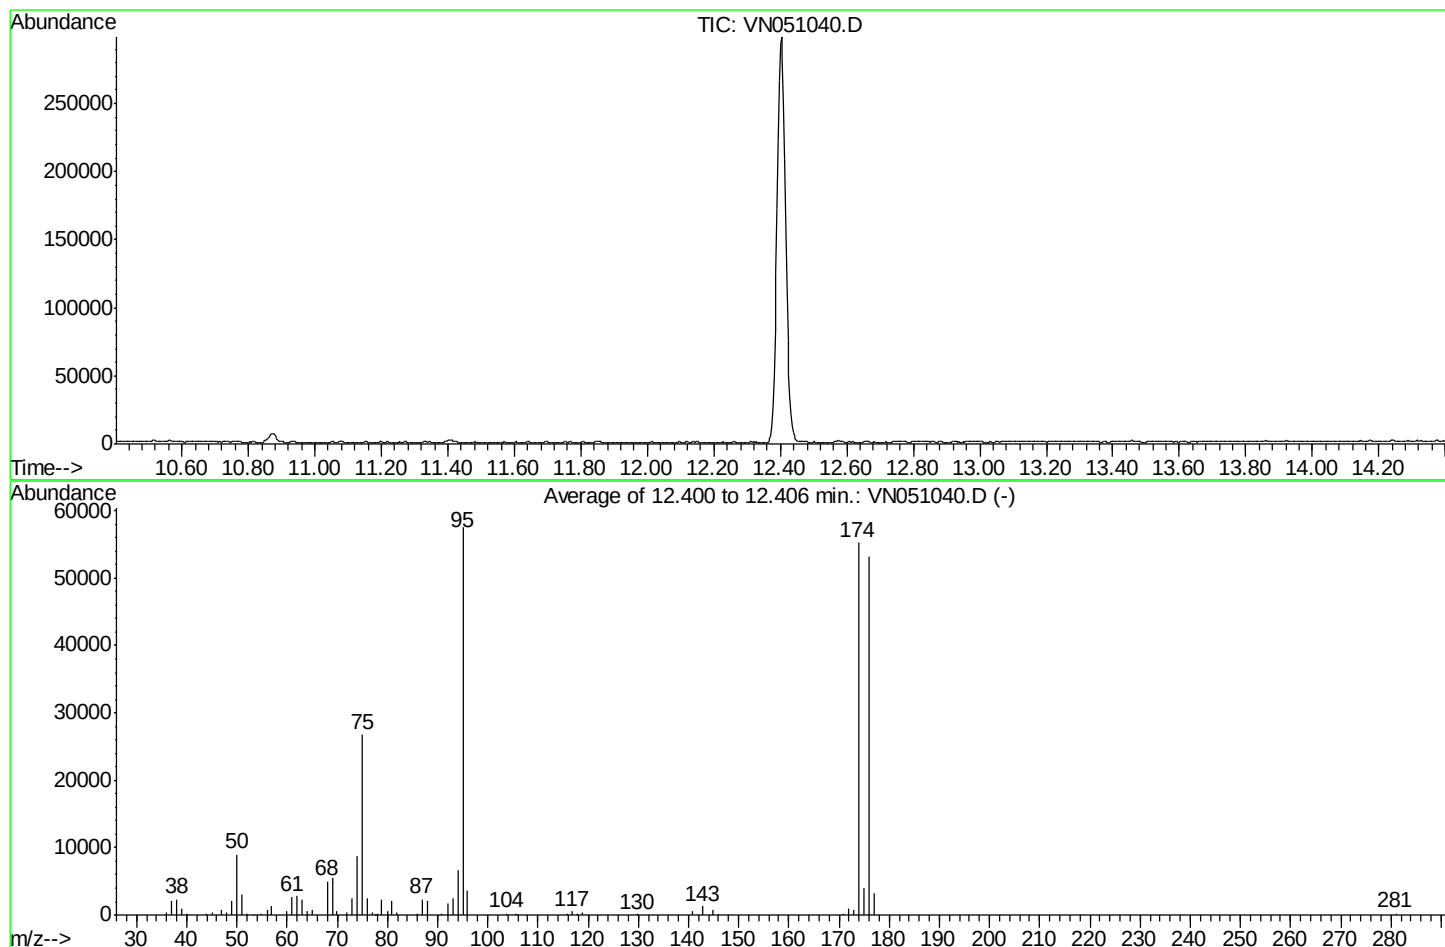

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	9002	PASS
75	95	30	60	46.5	26781	PASS
95	95	100	100	100.0	57538	PASS
96	95	5	9	6.2	3589	PASS
173	174	0.00	2	1.5	850	PASS
174	95	50	100	96.0	55240	PASS
175	174	5	9	7.2	3969	PASS
176	174	95	101	96.3	53208	PASS
177	176	5	9	6.2	3317	PASS