


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN090719\
 Data File : VN057740.D
 Acq On : 7 Sep 2019 10:02
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N090619W.M
 Title : SW846 8260
 Last Update : Fri Sep 06 03:46:54 2019

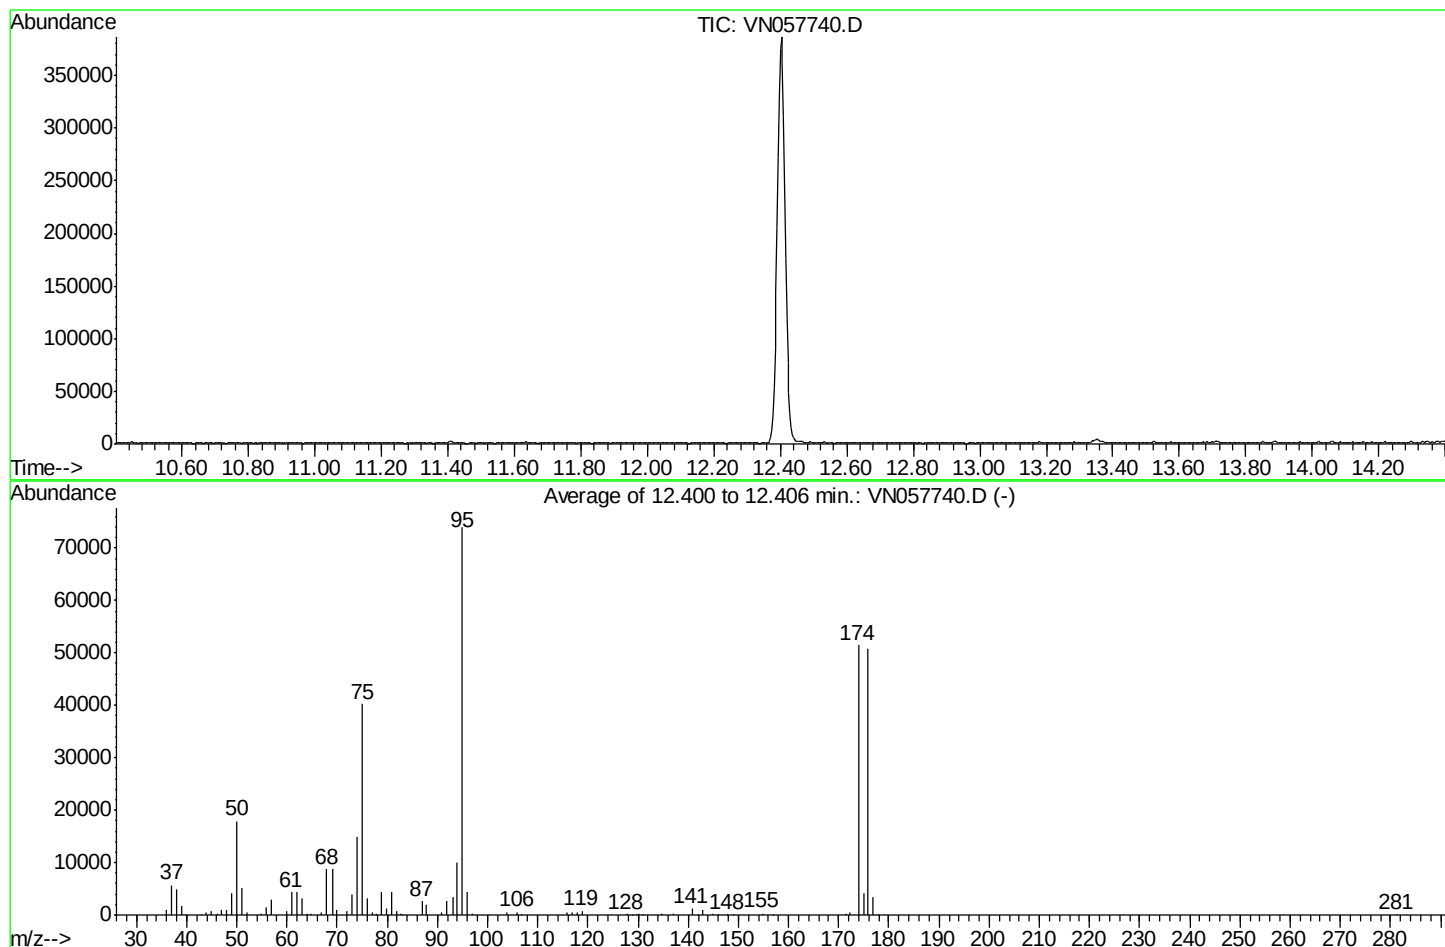

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.3	17936	PASS
75	95	30	60	54.3	40189	PASS
95	95	100	100	100.0	73962	PASS
96	95	5	9	5.9	4398	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	69.6	51464	PASS
175	174	5	9	8.0	4126	PASS
176	174	95	101	98.7	50813	PASS
177	176	5	9	6.7	3415	PASS