



Chloromethane

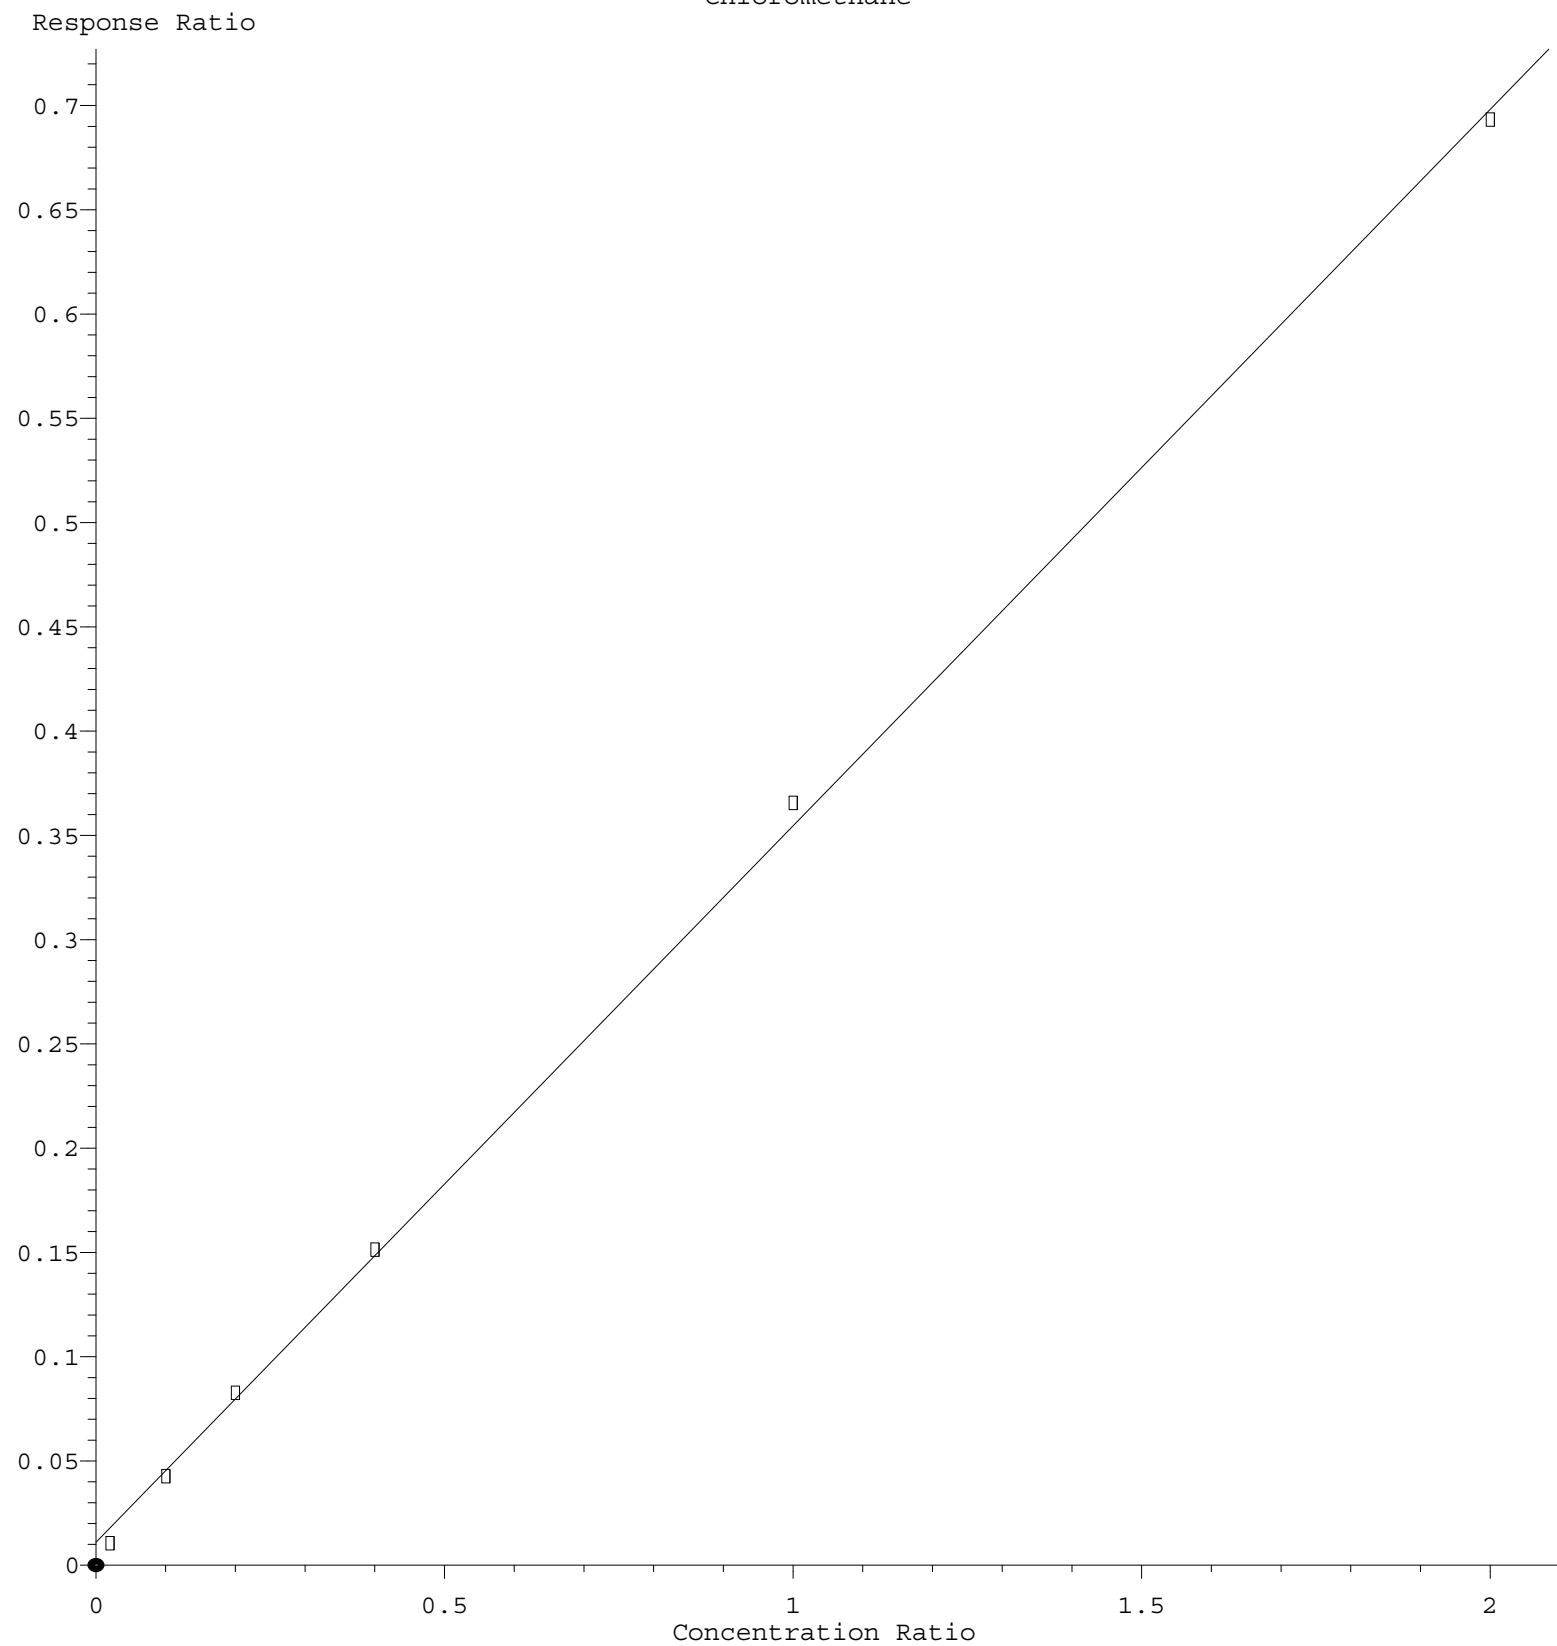

Response = $3.440 \times 10^{-1} \times \text{Amt} + 1.102 \times 10^{-2}$
Coef of Det (r^2) = 0.999358 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090721W.M
Calibration Table Last Updated: Fri Sep 17 11:02:11 2021


Bromoform

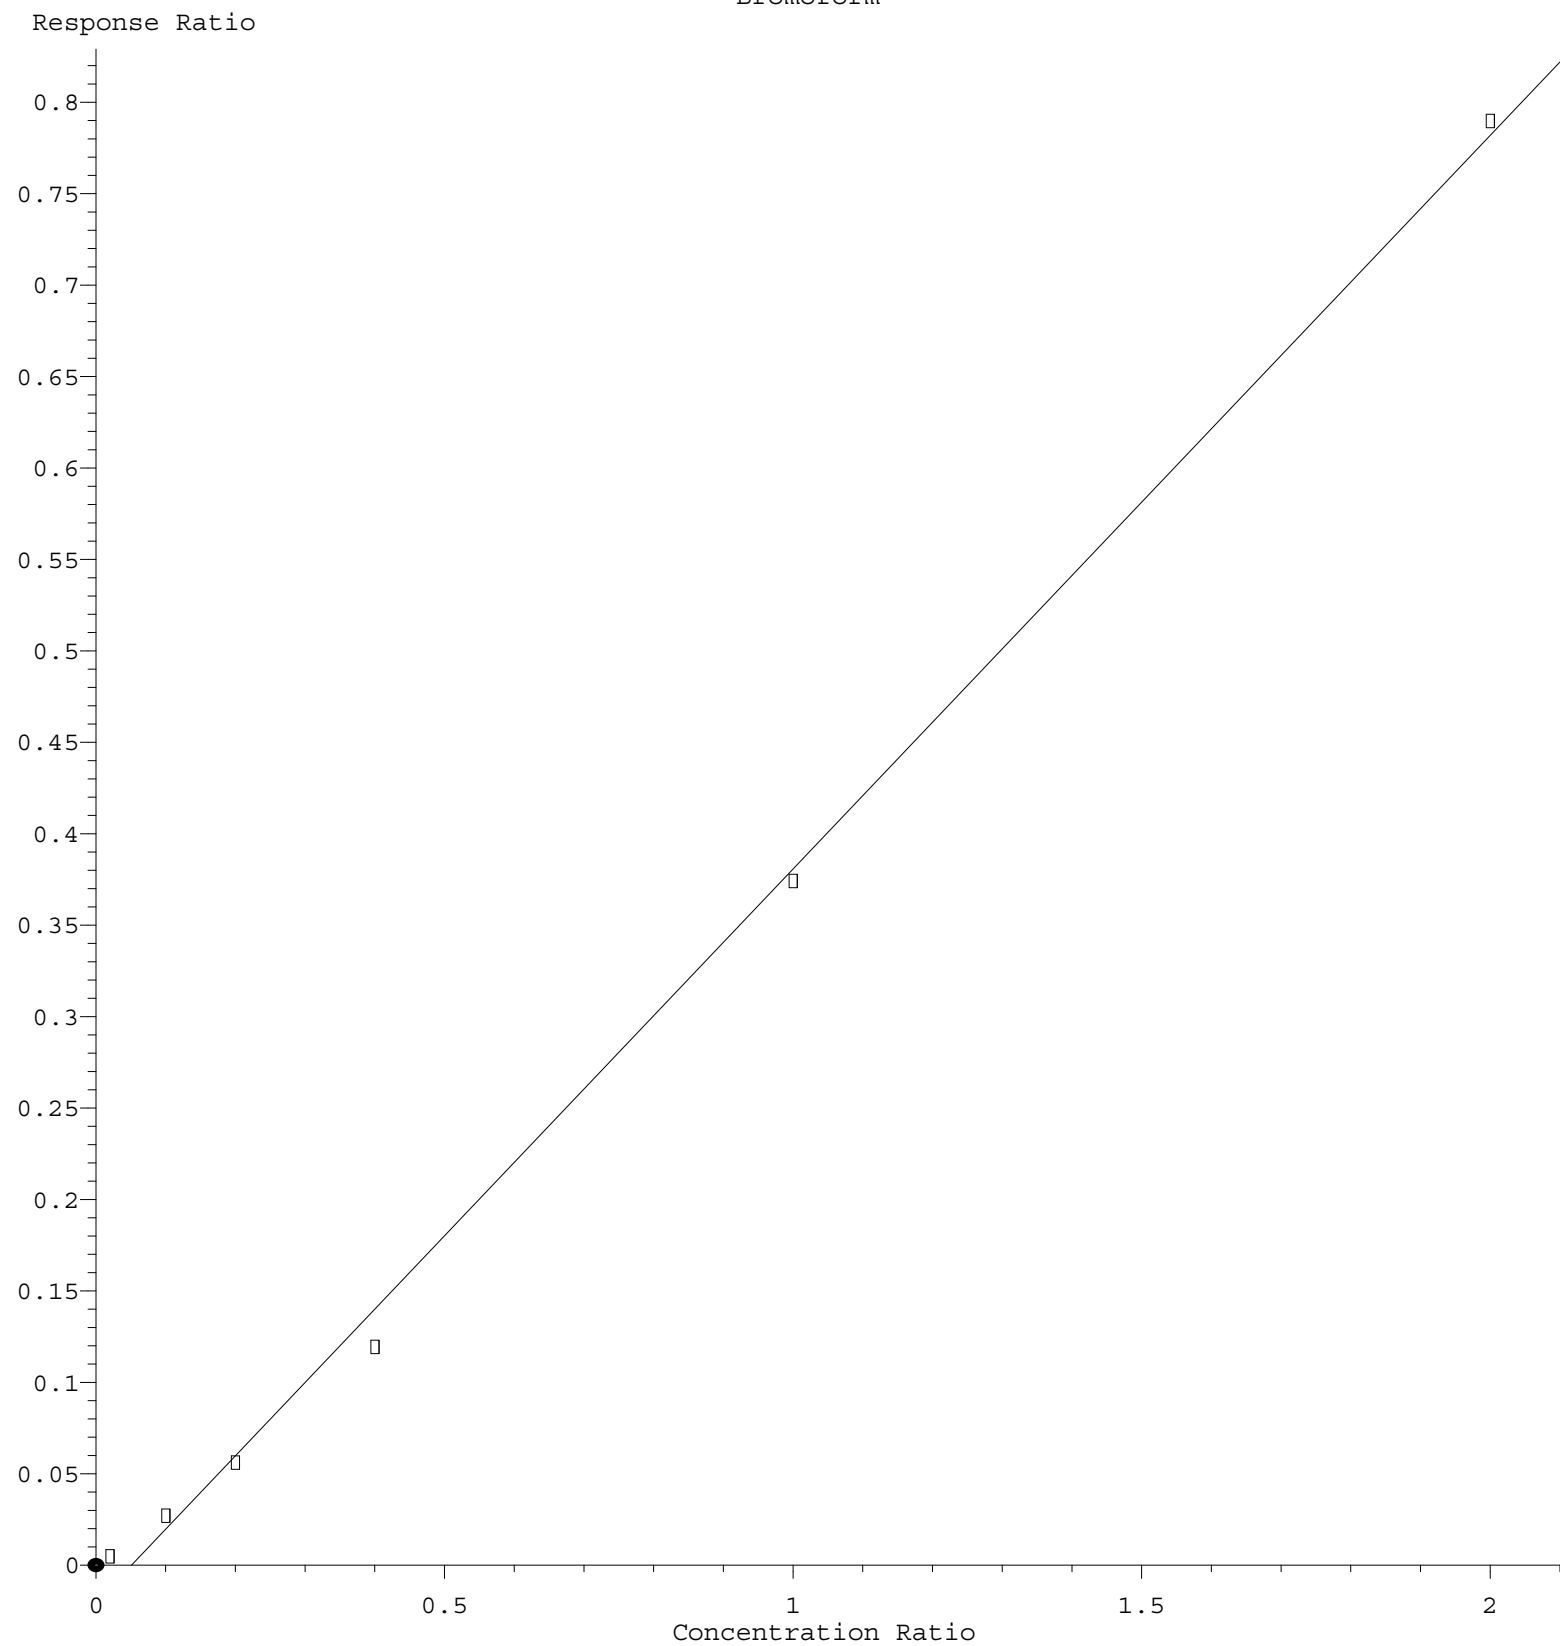

Response = $4.012 \times 10^{-1} \times \text{Amt} - 2.027 \times 10^{-2}$
 Coef of Det (r^2) = 0.998086 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090721W.M
 Calibration Table Last Updated: Fri Sep 17 11:02:11 2021

1,2,3-Trichloropropane

Response Ratio

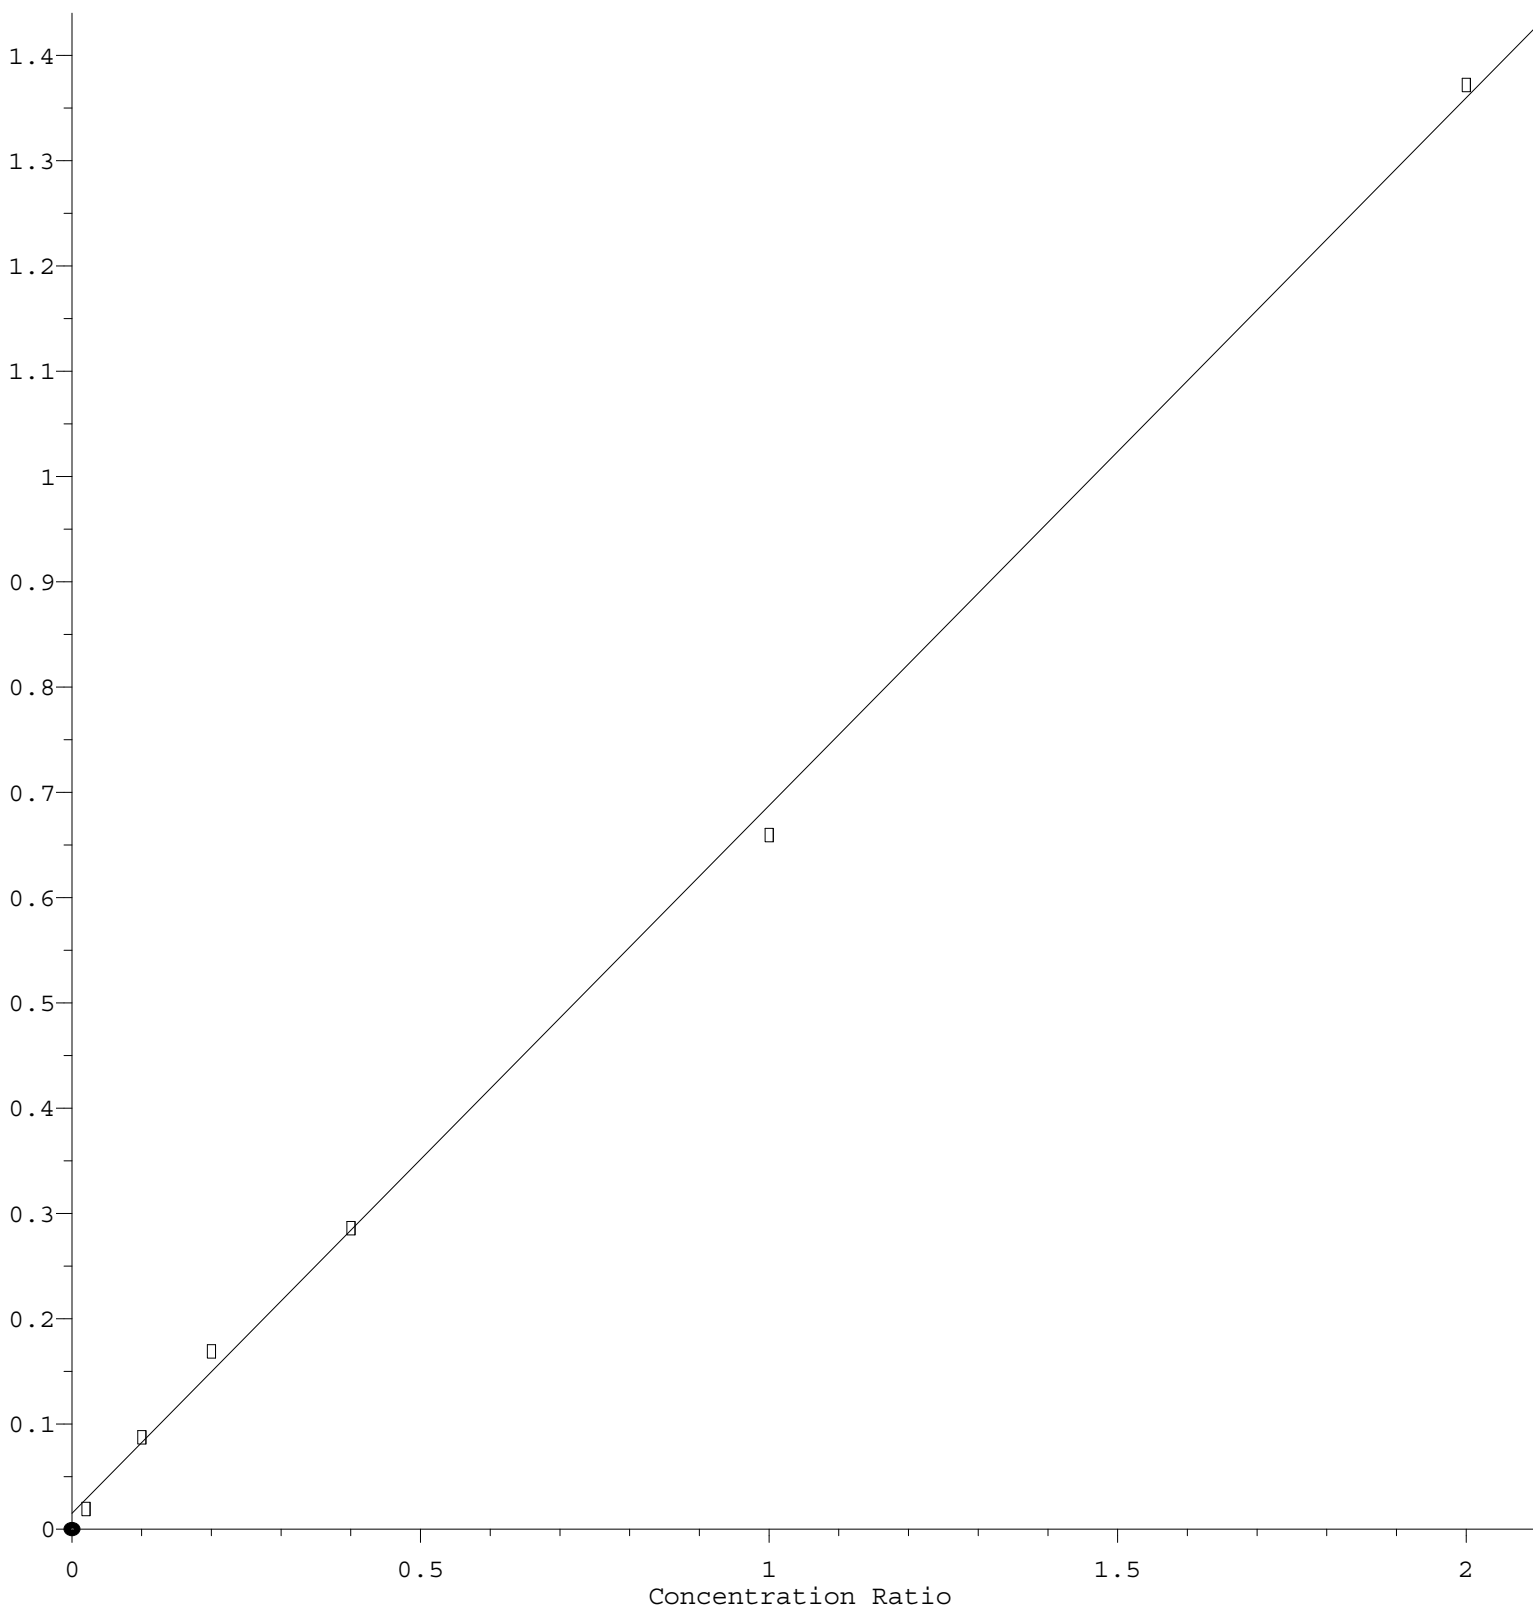

$$\text{Response} = 6.725\text{e-}001 * \text{Amt} + 1.510\text{e-}002$$


Coef of Det (r^2) = 0.998917 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090721W.M

Calibration Table Last Updated: Fri Sep 17 11:02:11 2021

1,2,4-Trichlorobenzene

Response Ratio

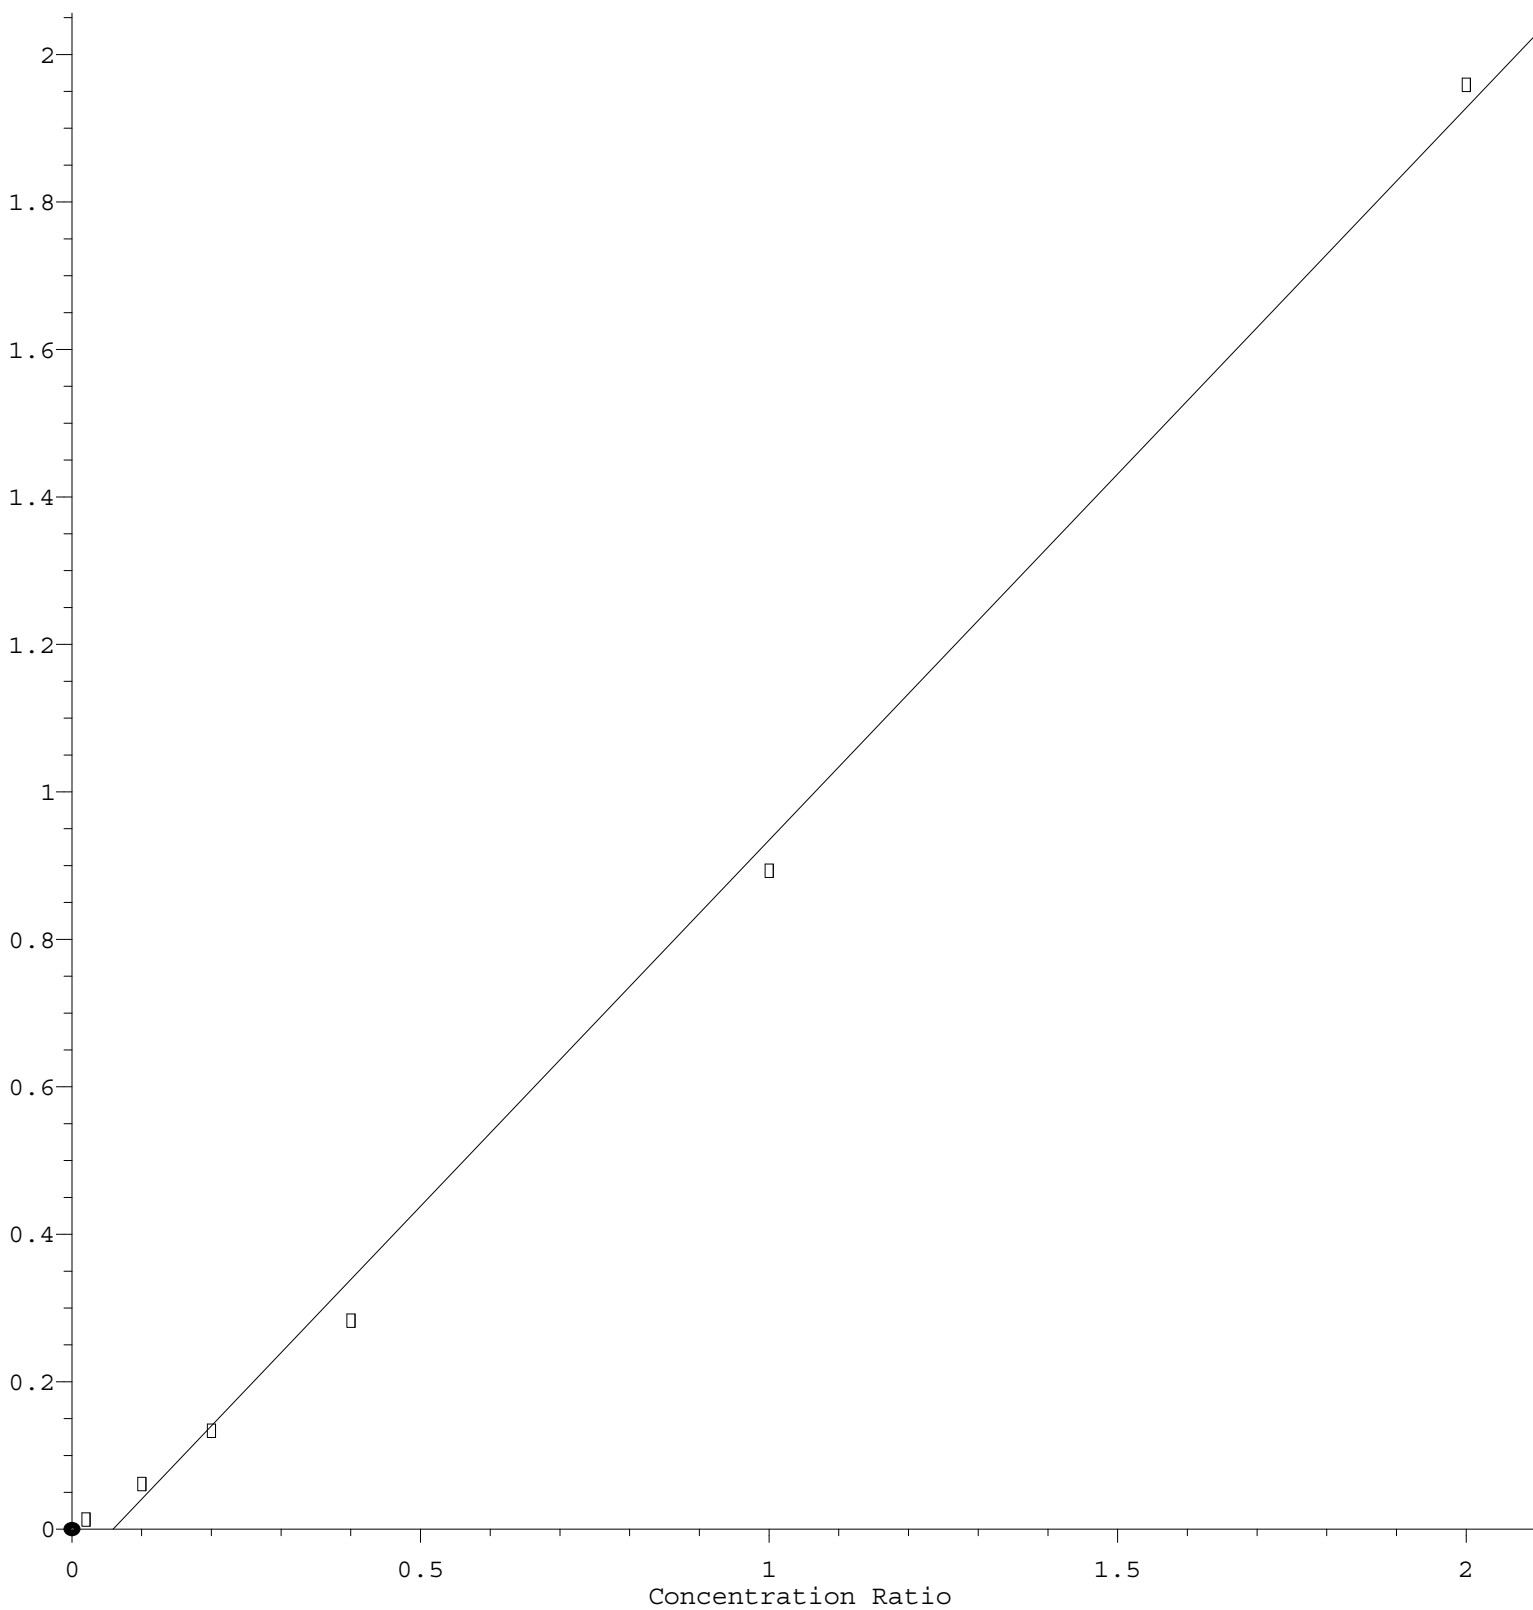

$$\text{Response} = 9.933\text{e-}001 * \text{Amt} - 5.878\text{e-}002$$


Coef of Det (r^2) = 0.996882 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090721W.M

Calibration Table Last Updated: Fri Sep 17 11:02:11 2021

Naphthalene


Response Ratio

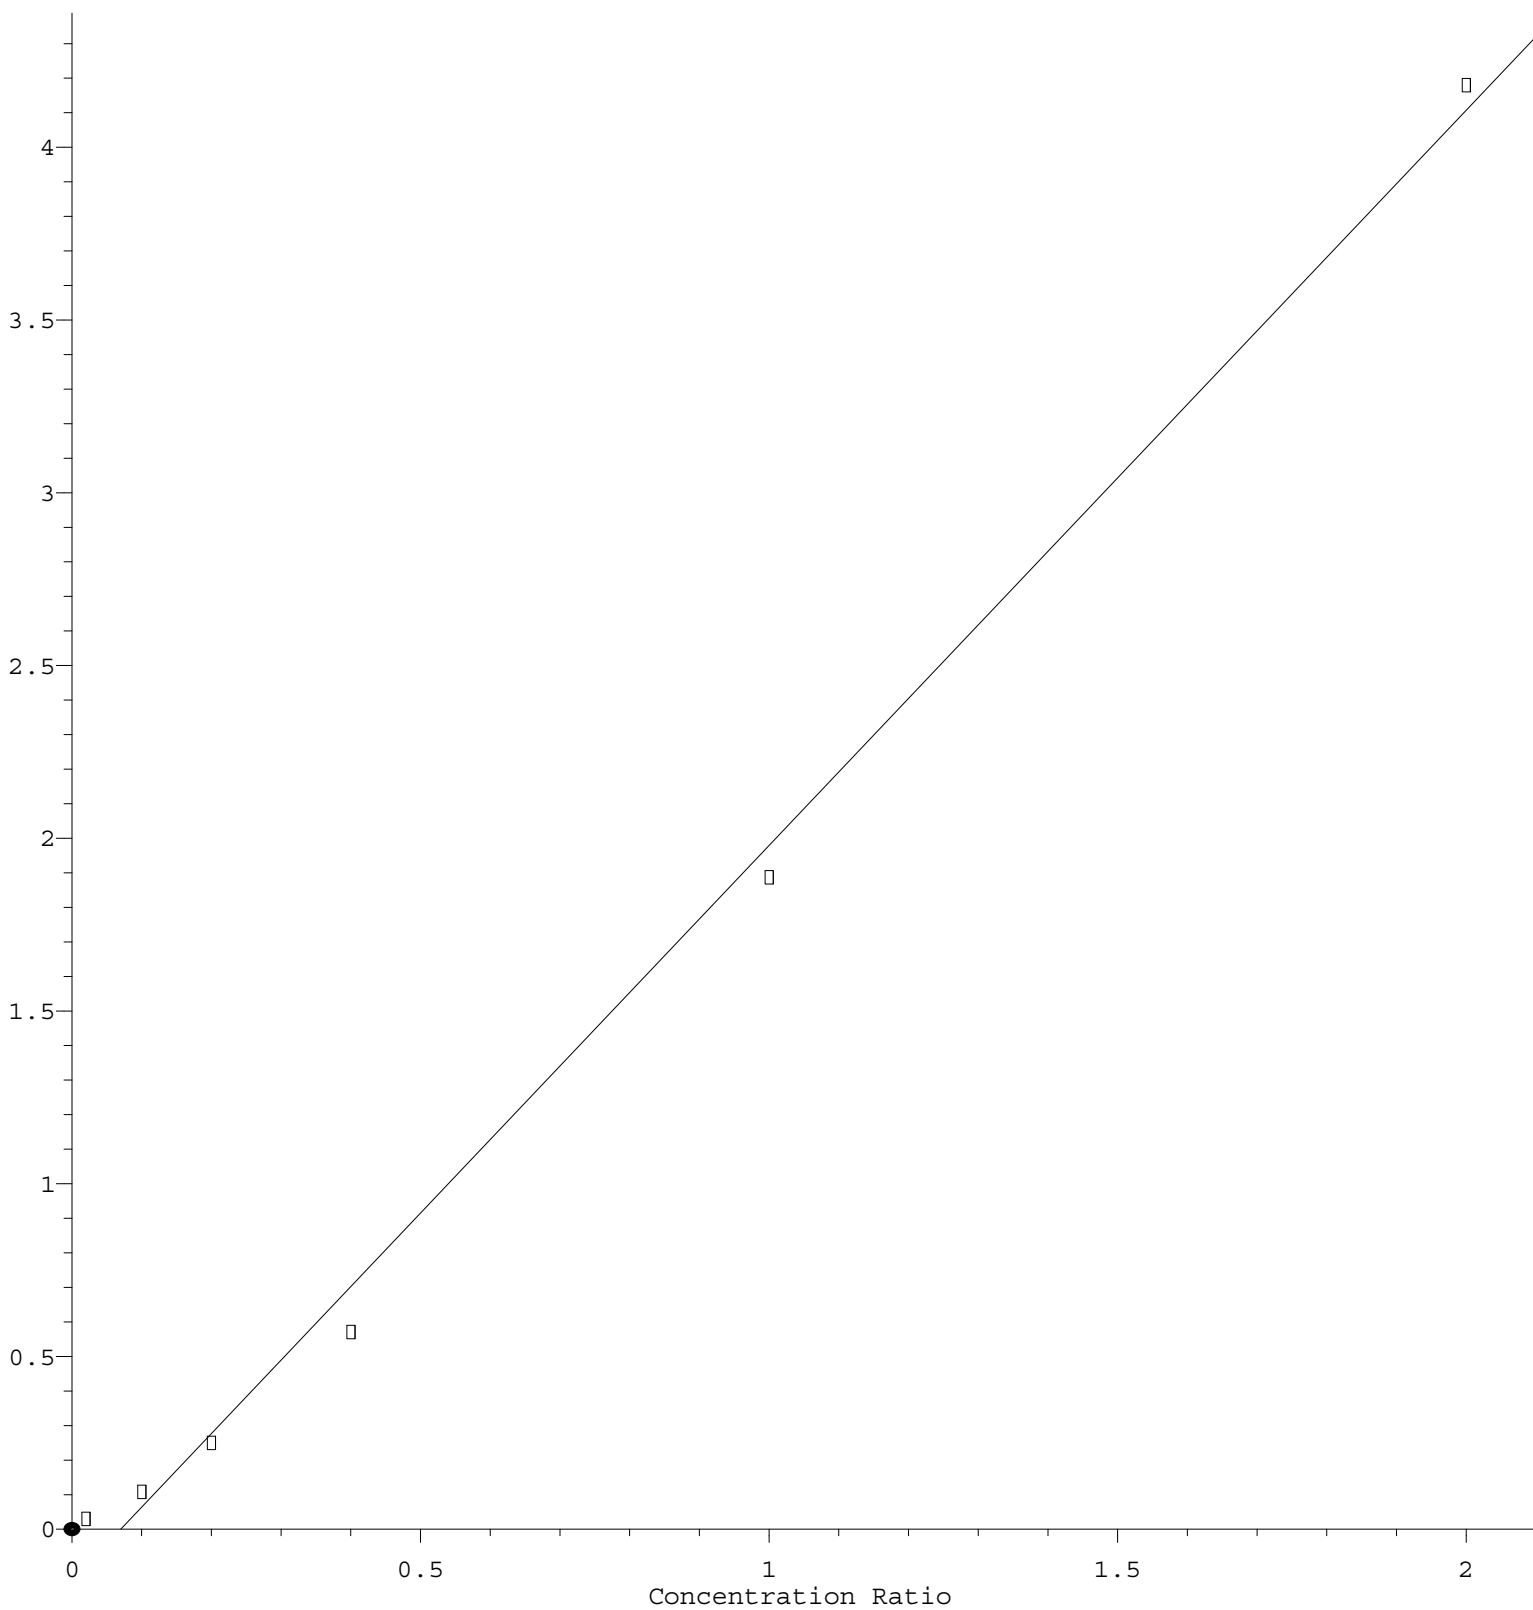

Response = 2.128e+000 * Amt - 1.488e-001
Coef of Det (r^2) = 0.996040 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090721W.M
Calibration Table Last Updated: Fri Sep 17 11:02:11 2021

1,2,3-Trichlorobenzene

Response Ratio

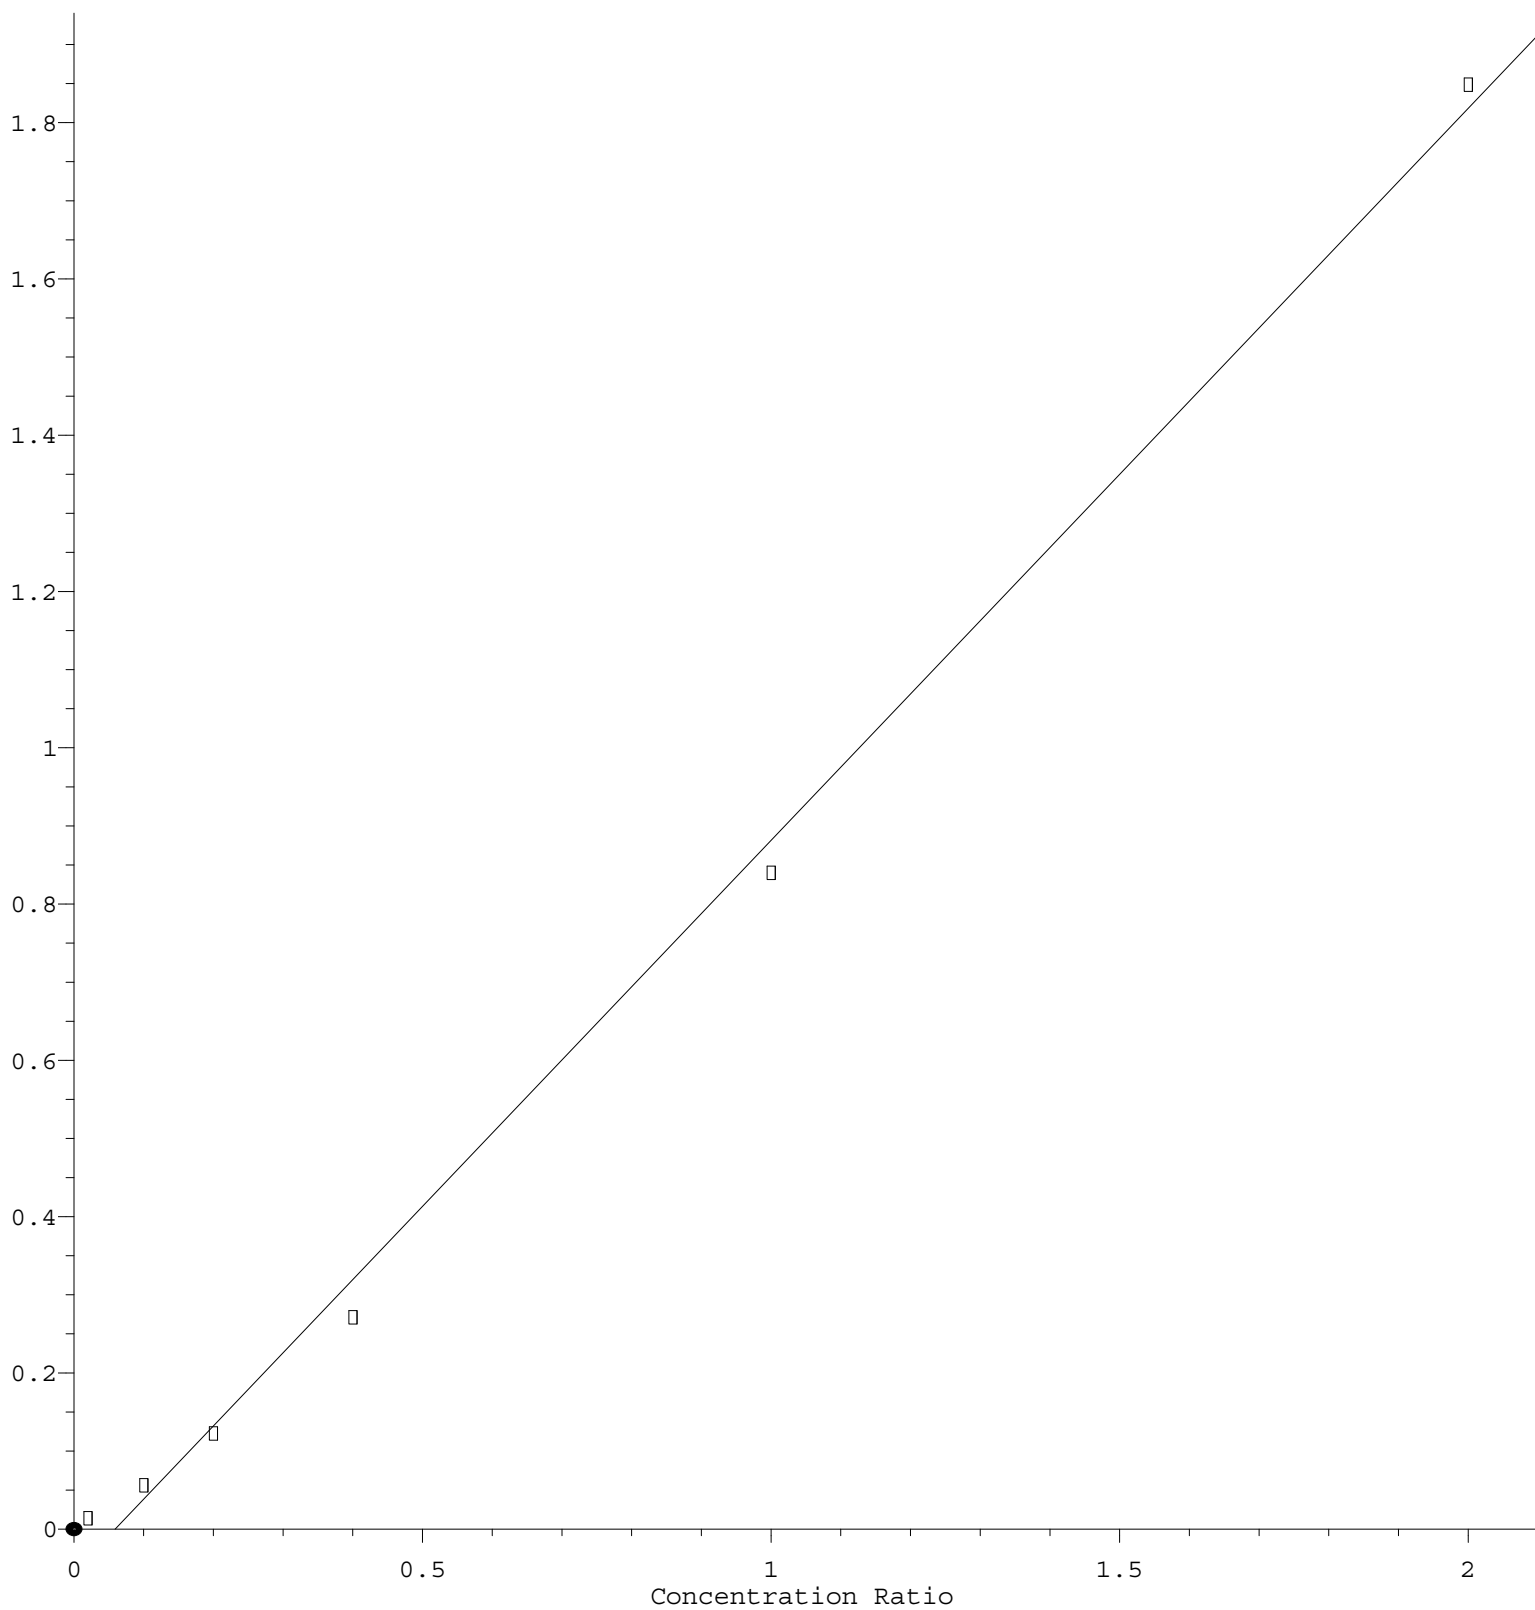

$$\text{Response} = 9.372\text{e-}001 * \text{Amt} - 5.575\text{e-}002$$


Coef of Det (r^2) = 0.996898 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090721W.M

Calibration Table Last Updated: Fri Sep 17 11:02:11 2021

Bromomethane


Response Ratio

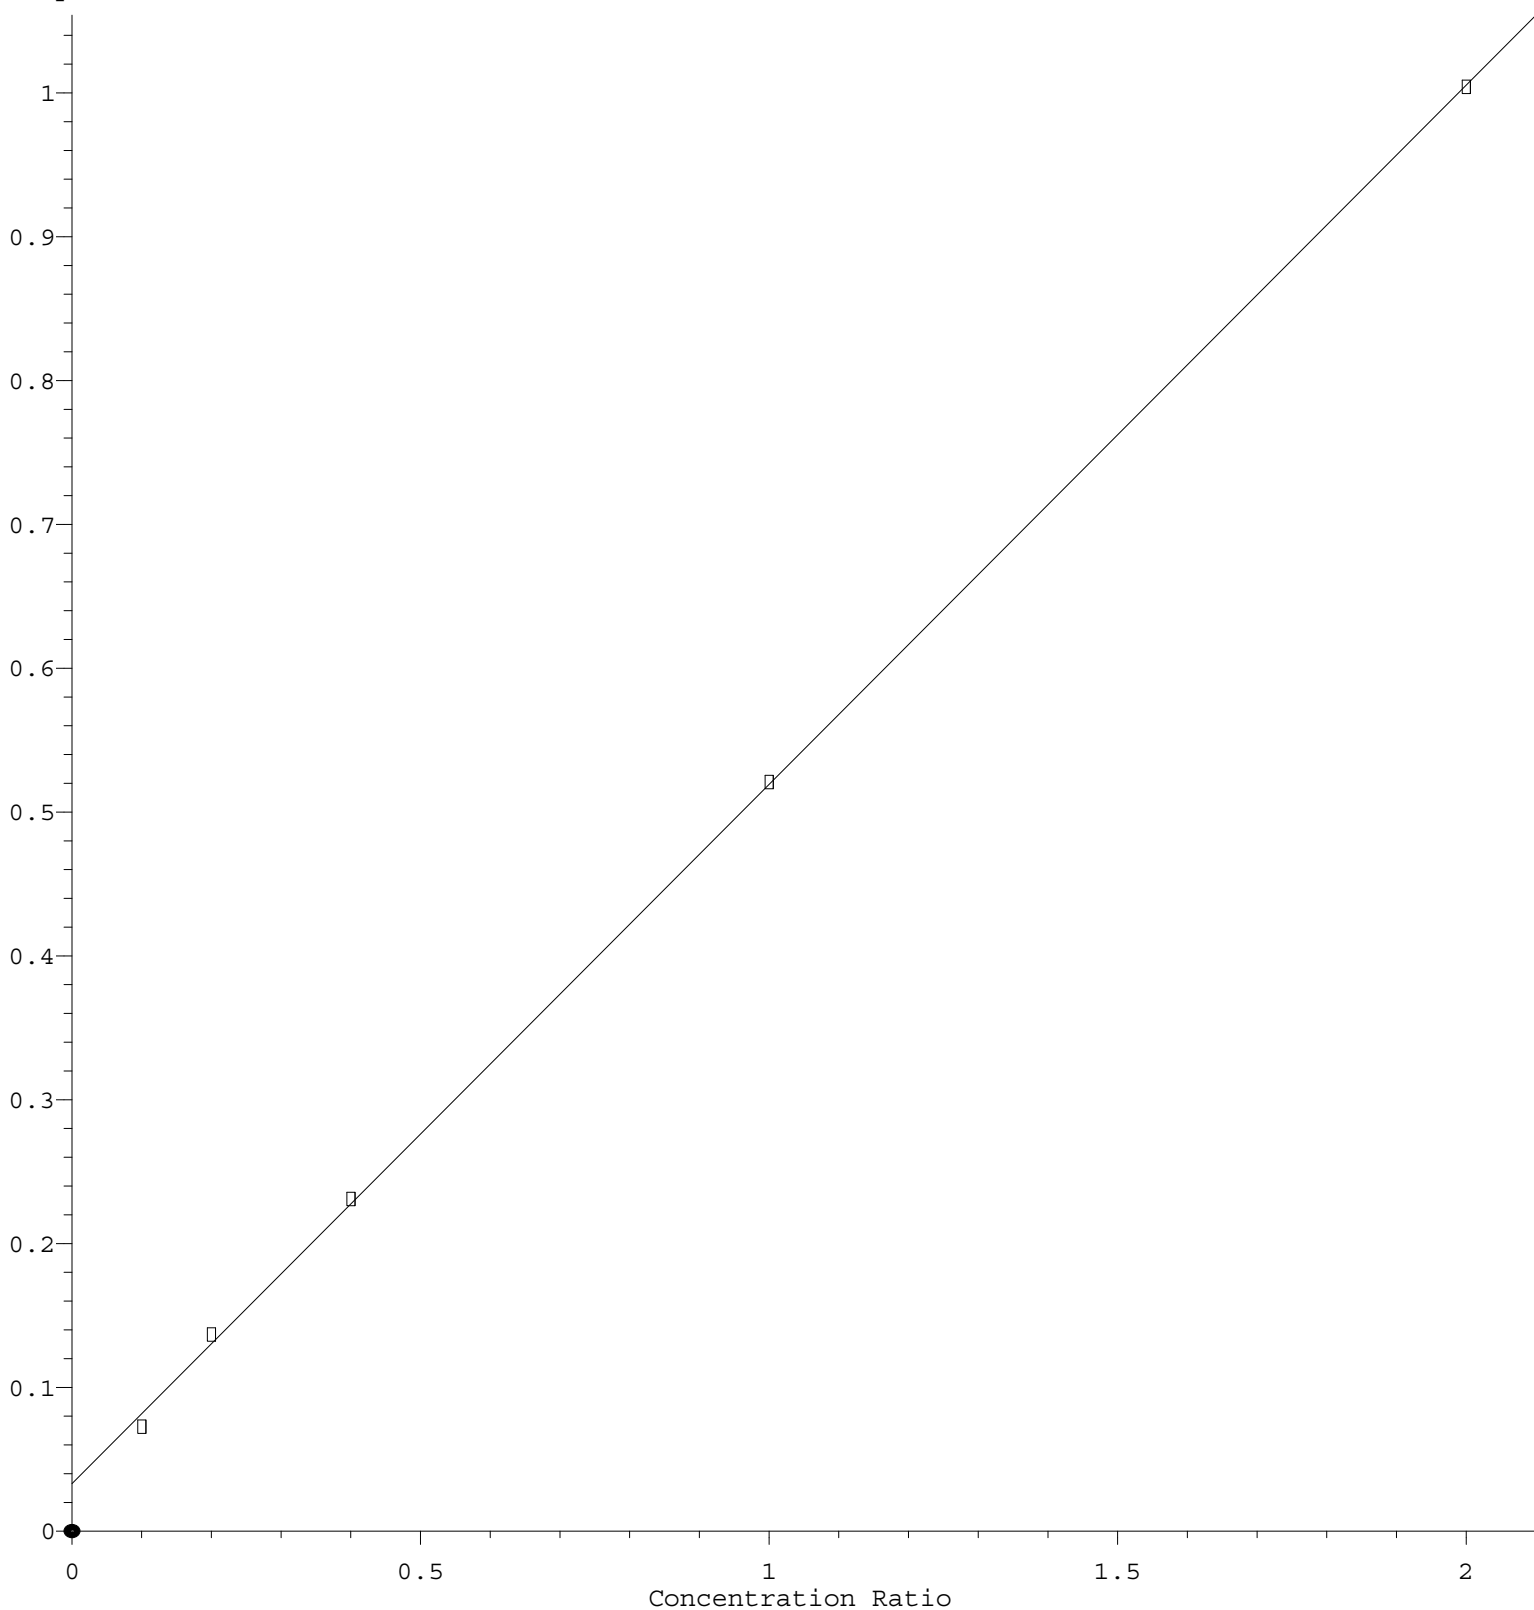

$\text{Response} = 4.862\text{e-}001 * \text{Amt} + 3.327\text{e-}002$
 Coef of Det (r^2) = 0.999762 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090721W.M
 Calibration Table Last Updated: Fri Sep 17 11:02:11 2021

Tert butyl alcohol

Response Ratio

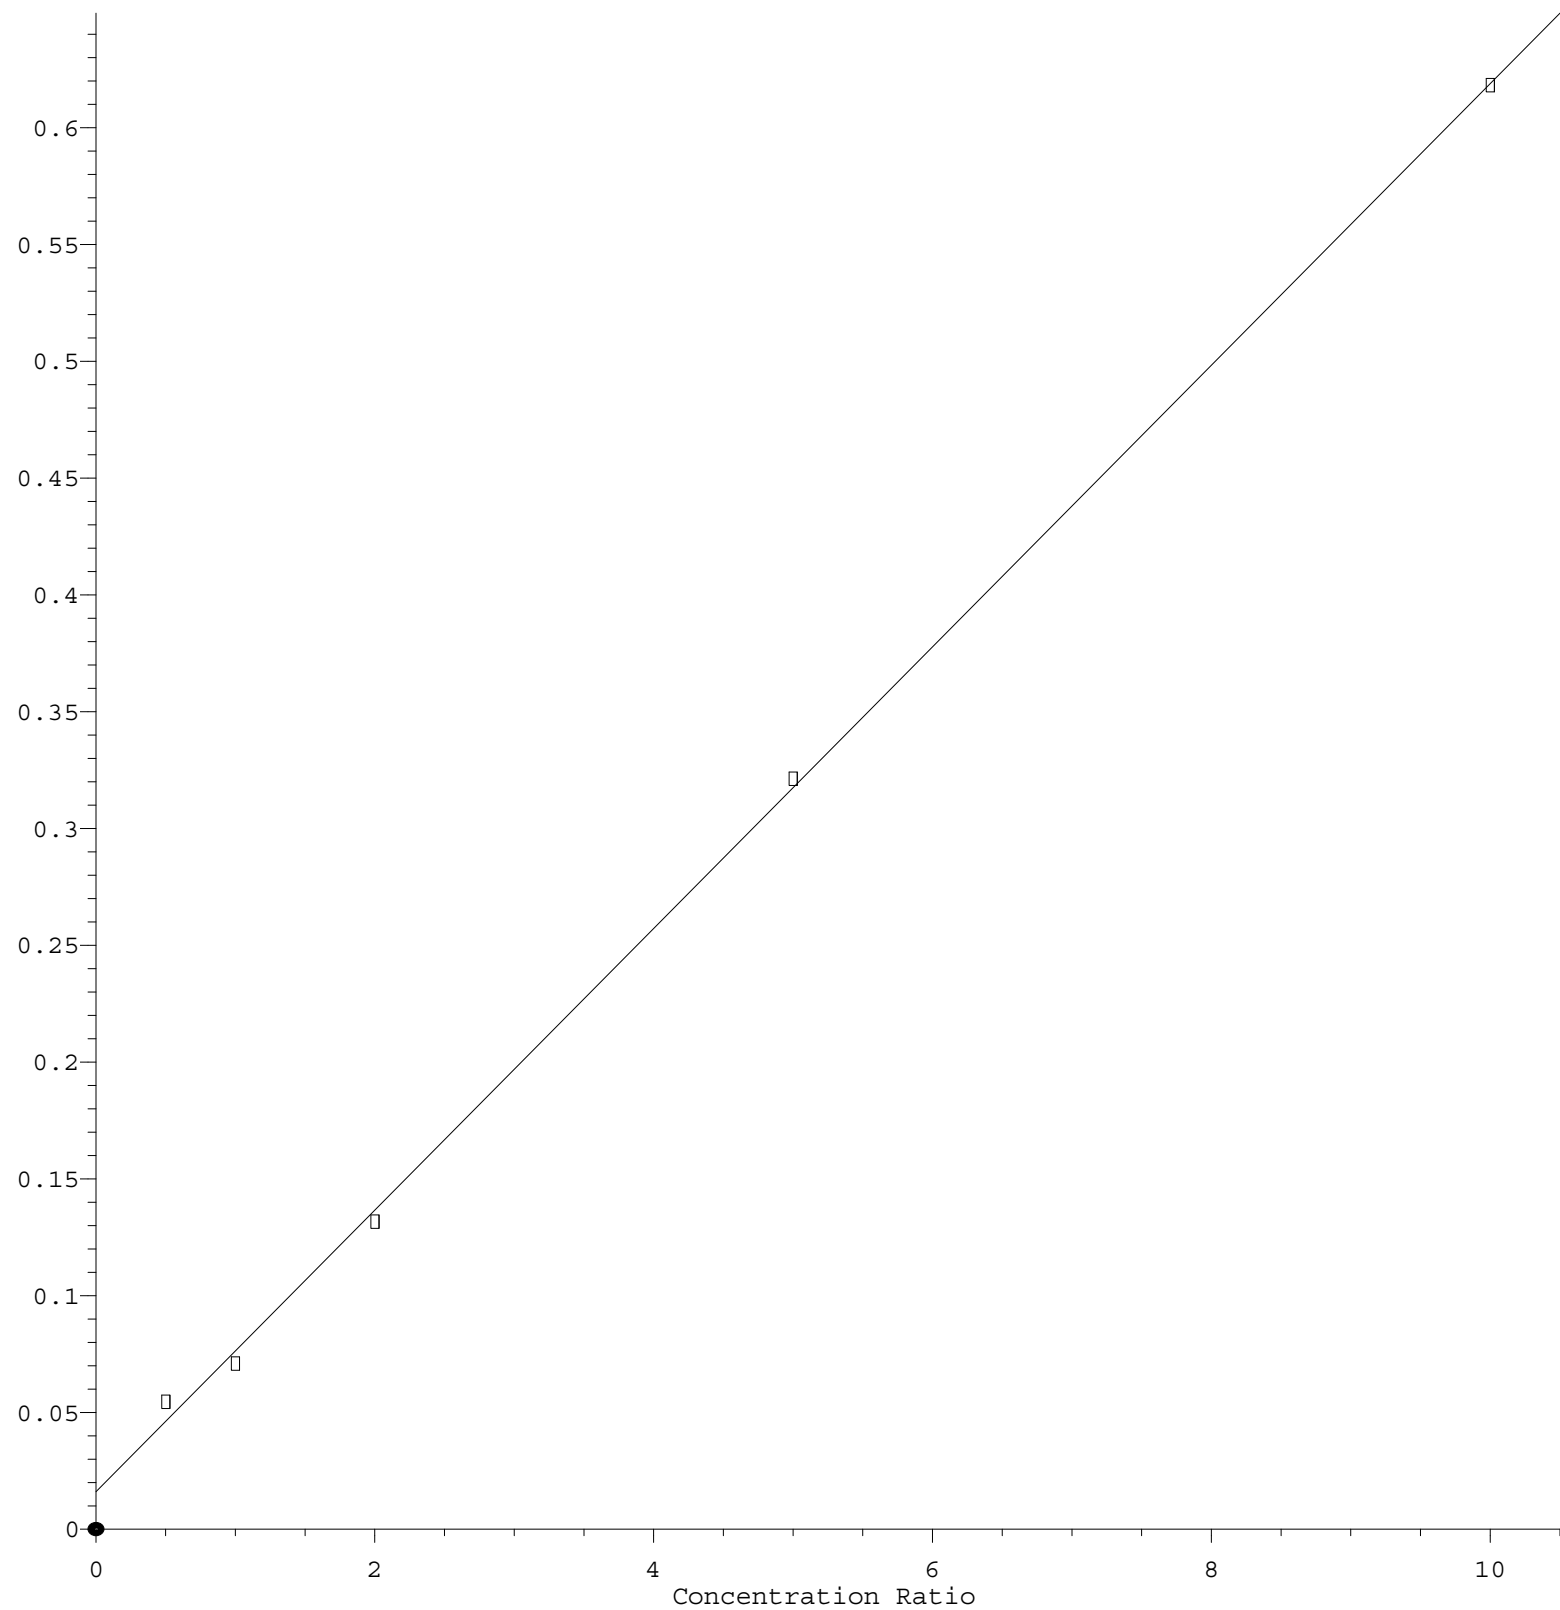

$$\text{Response} = 6.023\text{e-}002 * \text{Amt} + 1.644\text{e-}002$$


Coef of Det (r^2) = 0.999382 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090721W.M

Calibration Table Last Updated: Fri Sep 17 11:02:11 2021

Acetone

Response Ratio

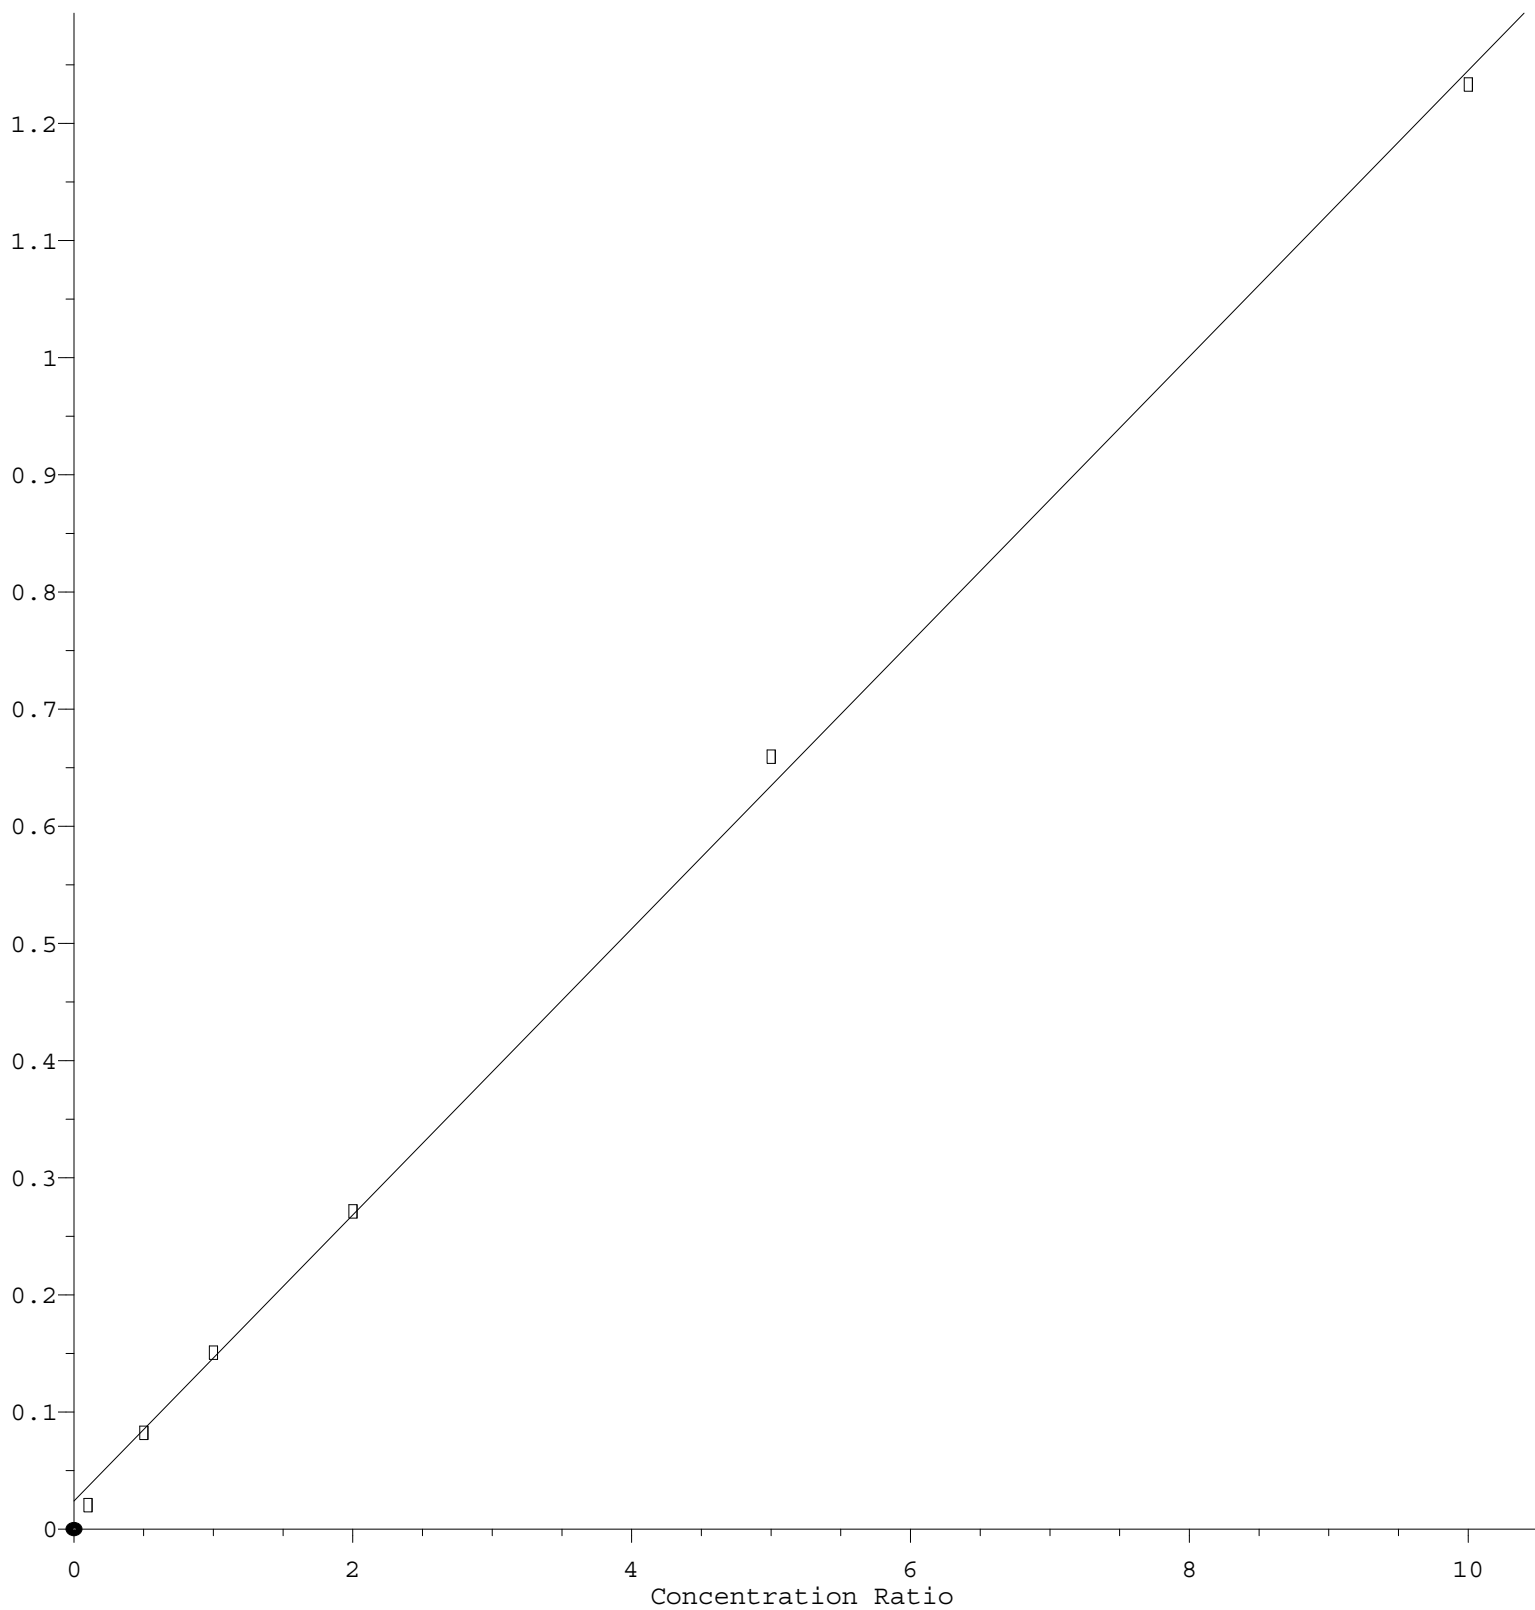


$$\text{Response} = 1.222\text{e-}001 * \text{Amt} + 2.403\text{e-}002$$

Coef of Det (r^2) = 0.999037 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090721W.M

Calibration Table Last Updated: Fri Sep 17 11:02:11 2021


Methyl Acetate

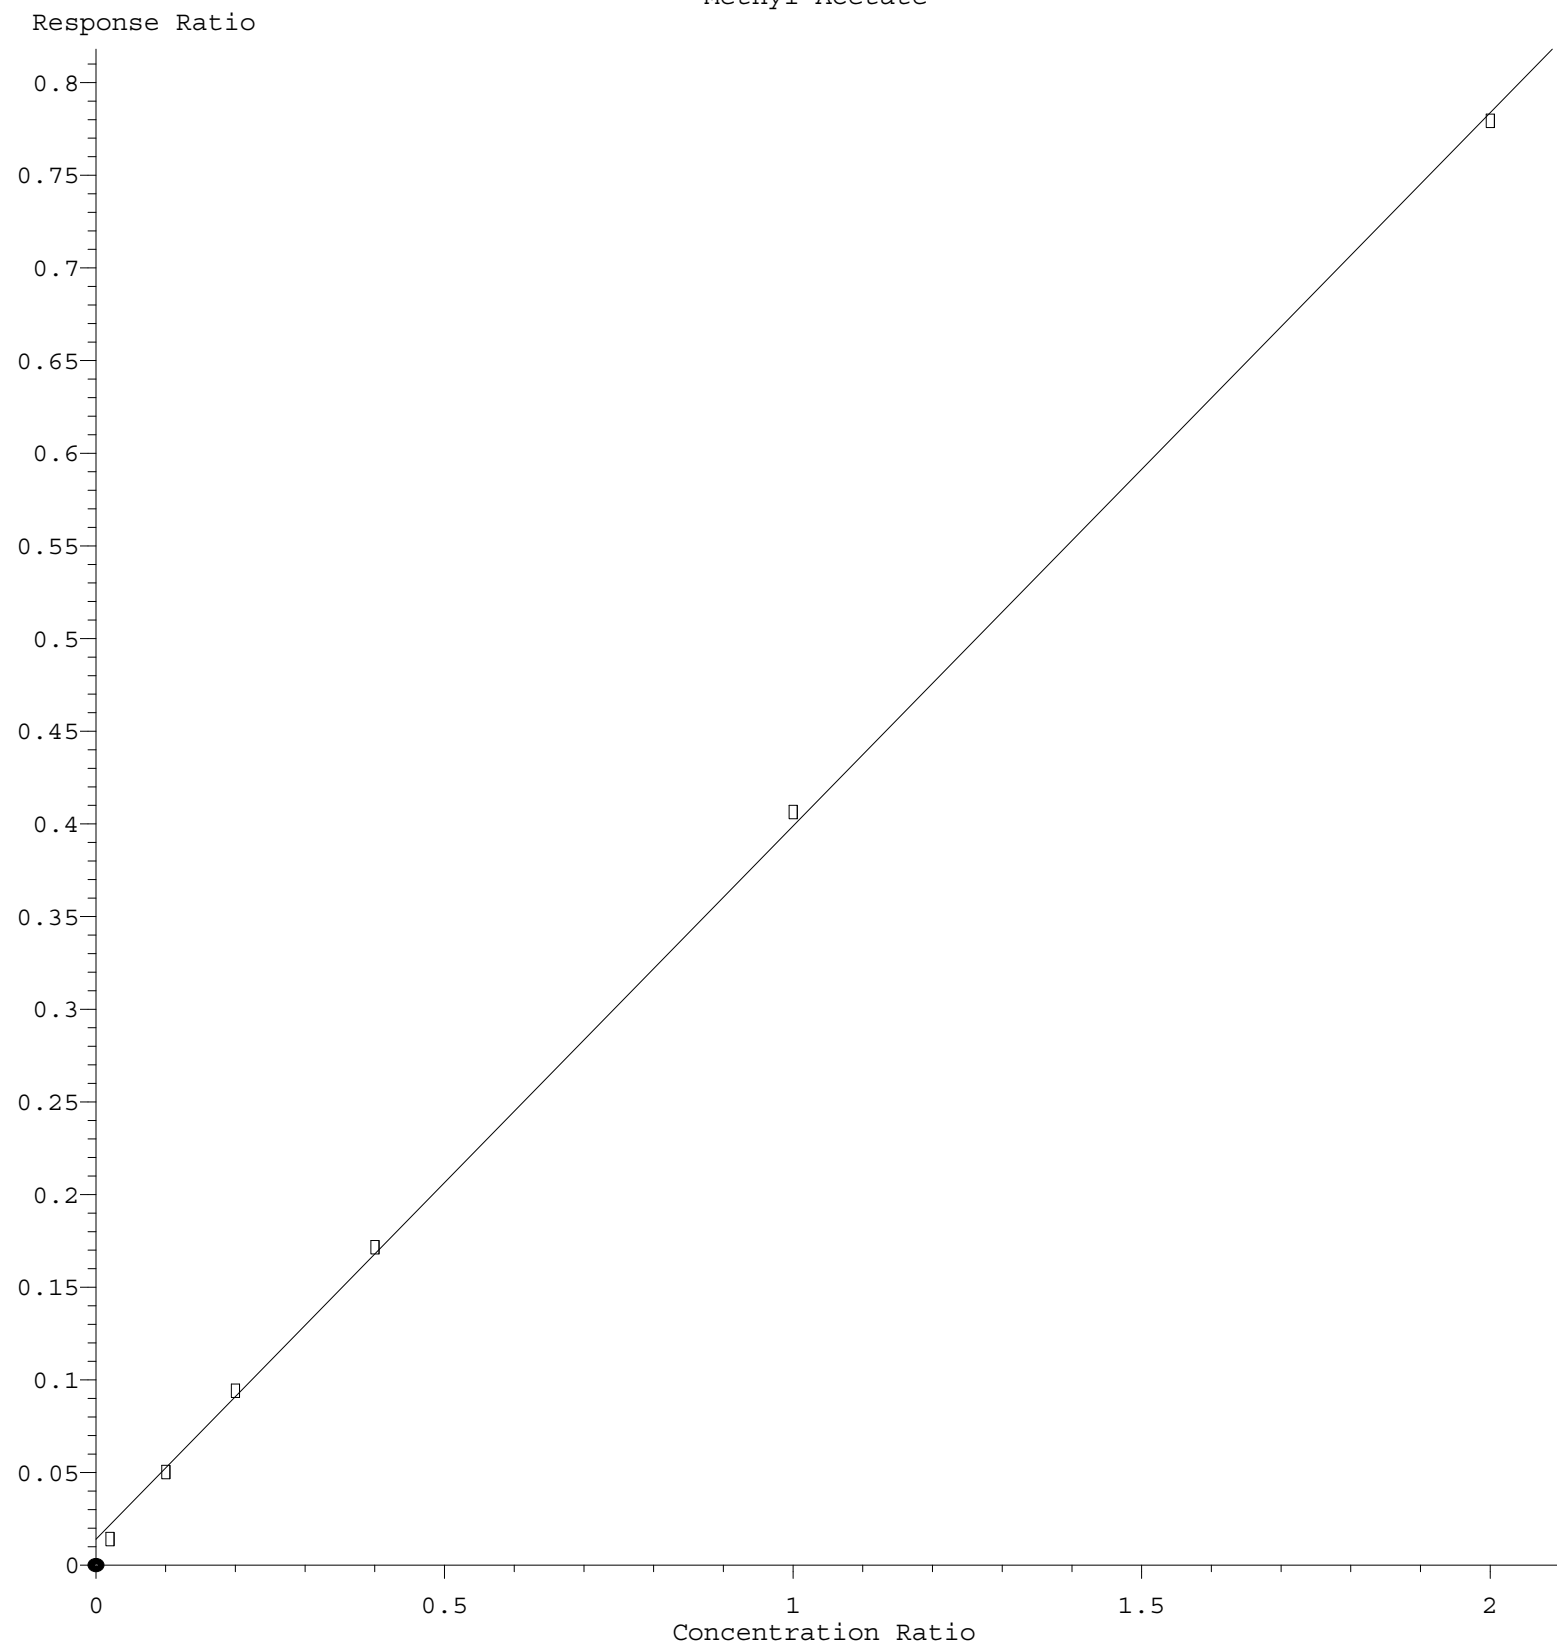

Response = $3.850 \times 10^{-1} \times \text{Amt} + 1.393 \times 10^{-2}$
Coef of Det (r^2) = 0.999625 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090721W.M
Calibration Table Last Updated: Fri Sep 17 11:02:11 2021

Methylene Chloride


Response Ratio

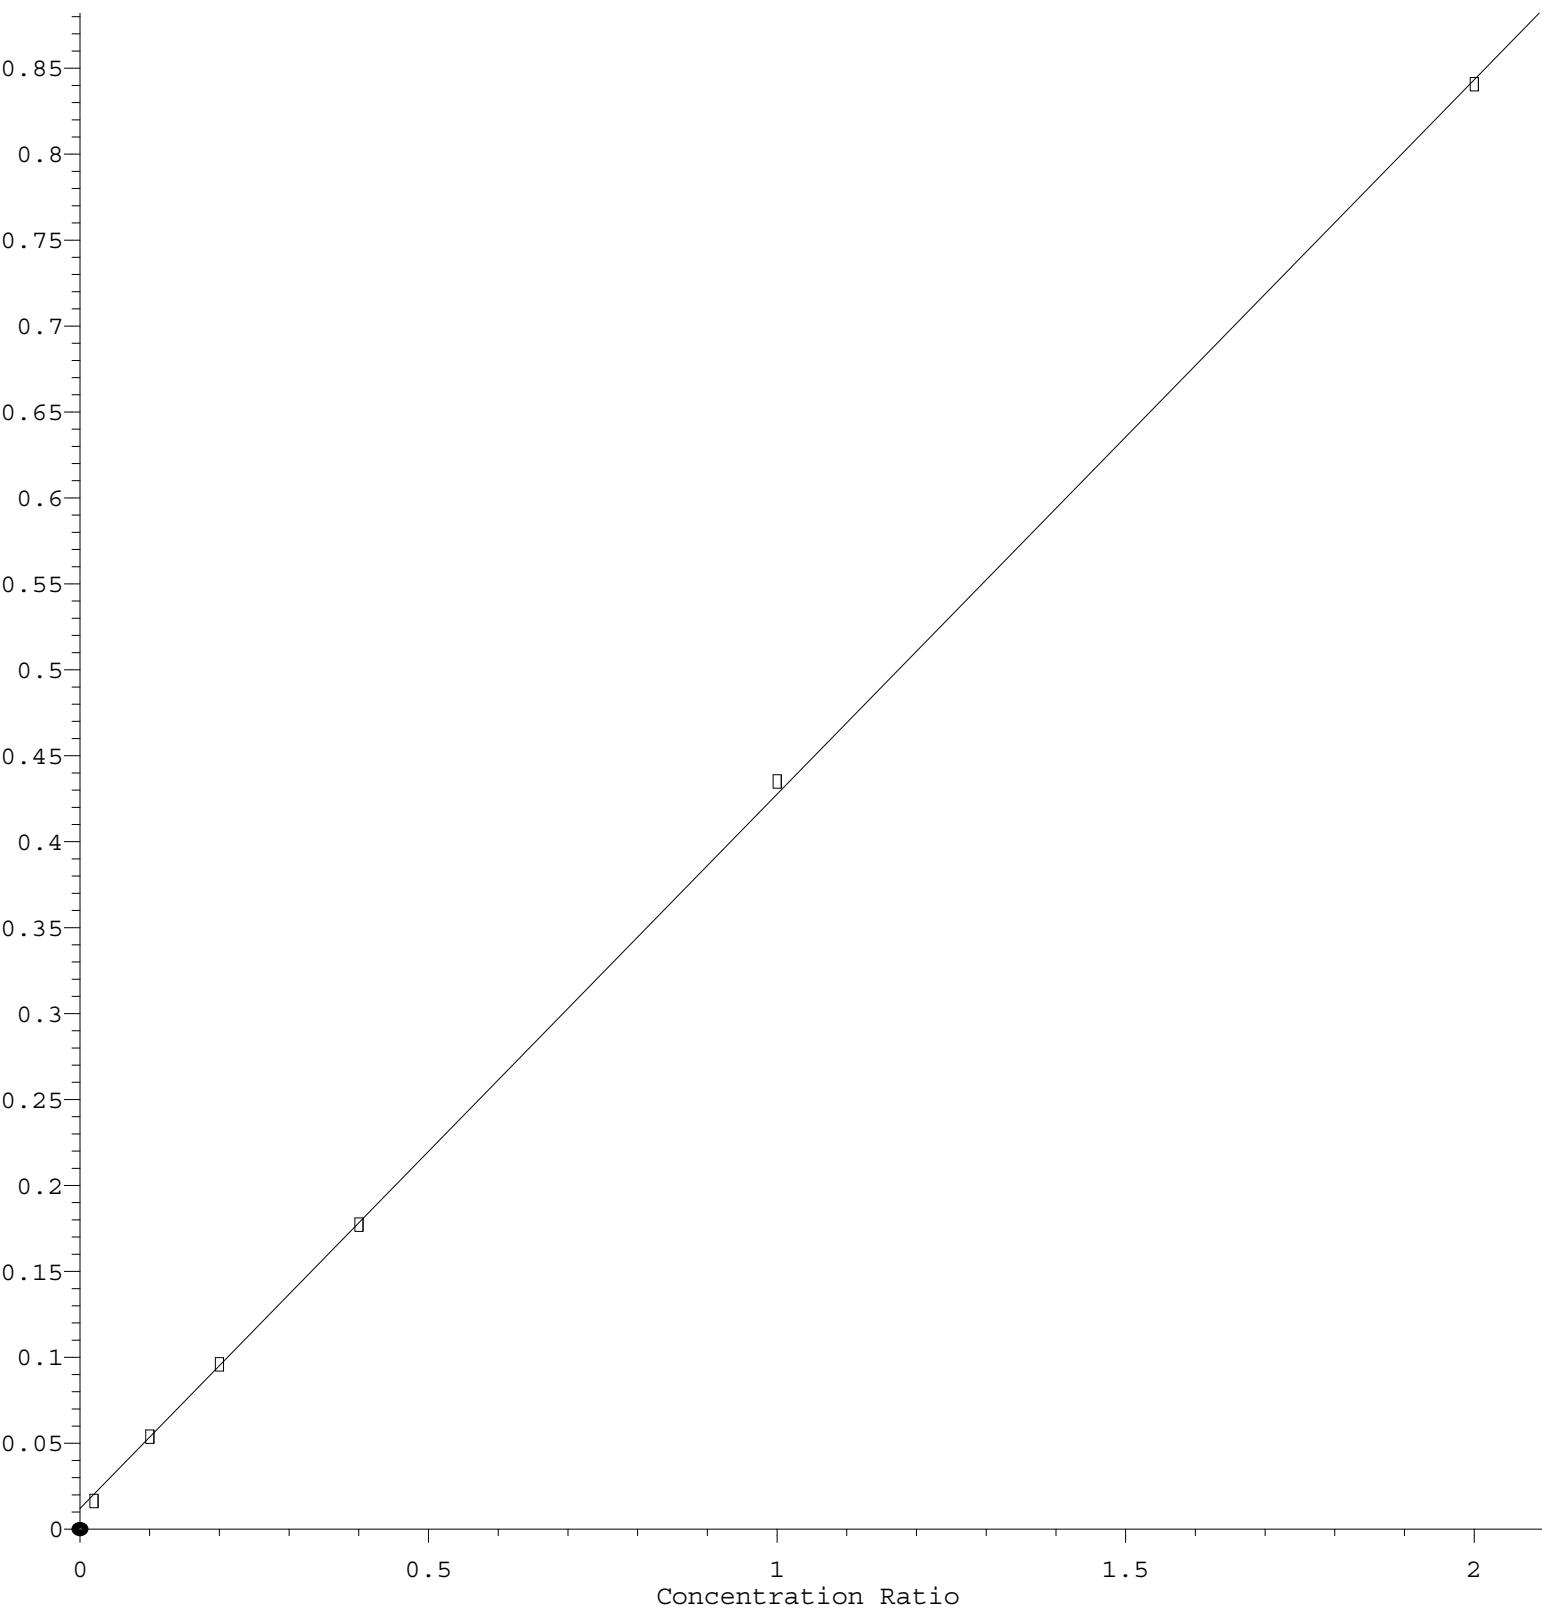

Response = 4.161e-001 * Amt + 1.181e-002
 Coef of Det (r^2) = 0.999844 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090721W.M
 Calibration Table Last Updated: Fri Sep 17 11:02:11 2021

Toluene-d8

Response Ratio

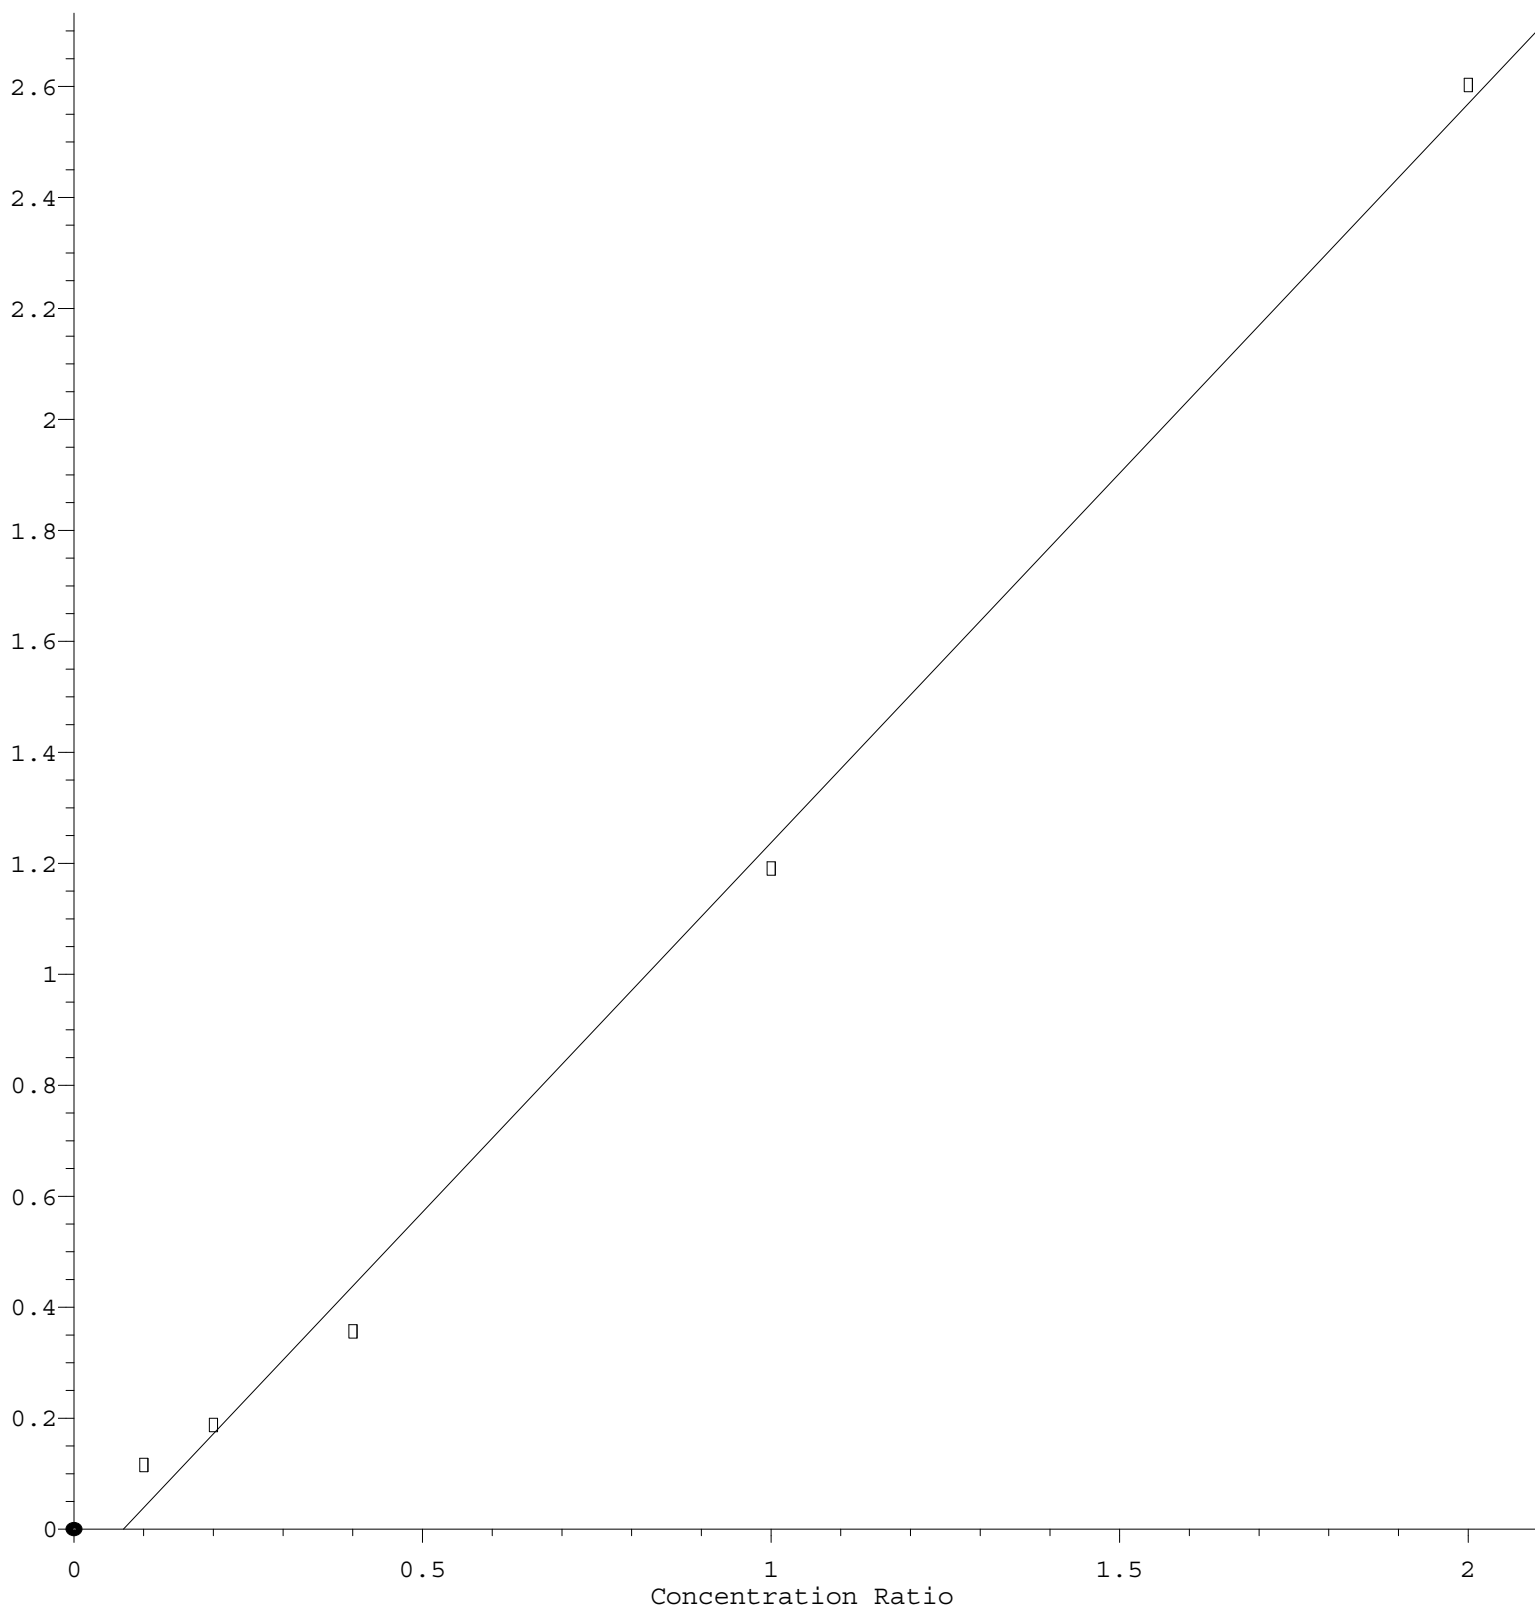

$$\text{Response} = 1.332\text{e}+000 * \text{Amt} - 9.506\text{e}-002$$


Coef of Det (r^2) = 0.996317 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090721W.M

Calibration Table Last Updated: Fri Sep 17 11:02:11 2021

2-Chloroethyl Vinyl ether


Response Ratio

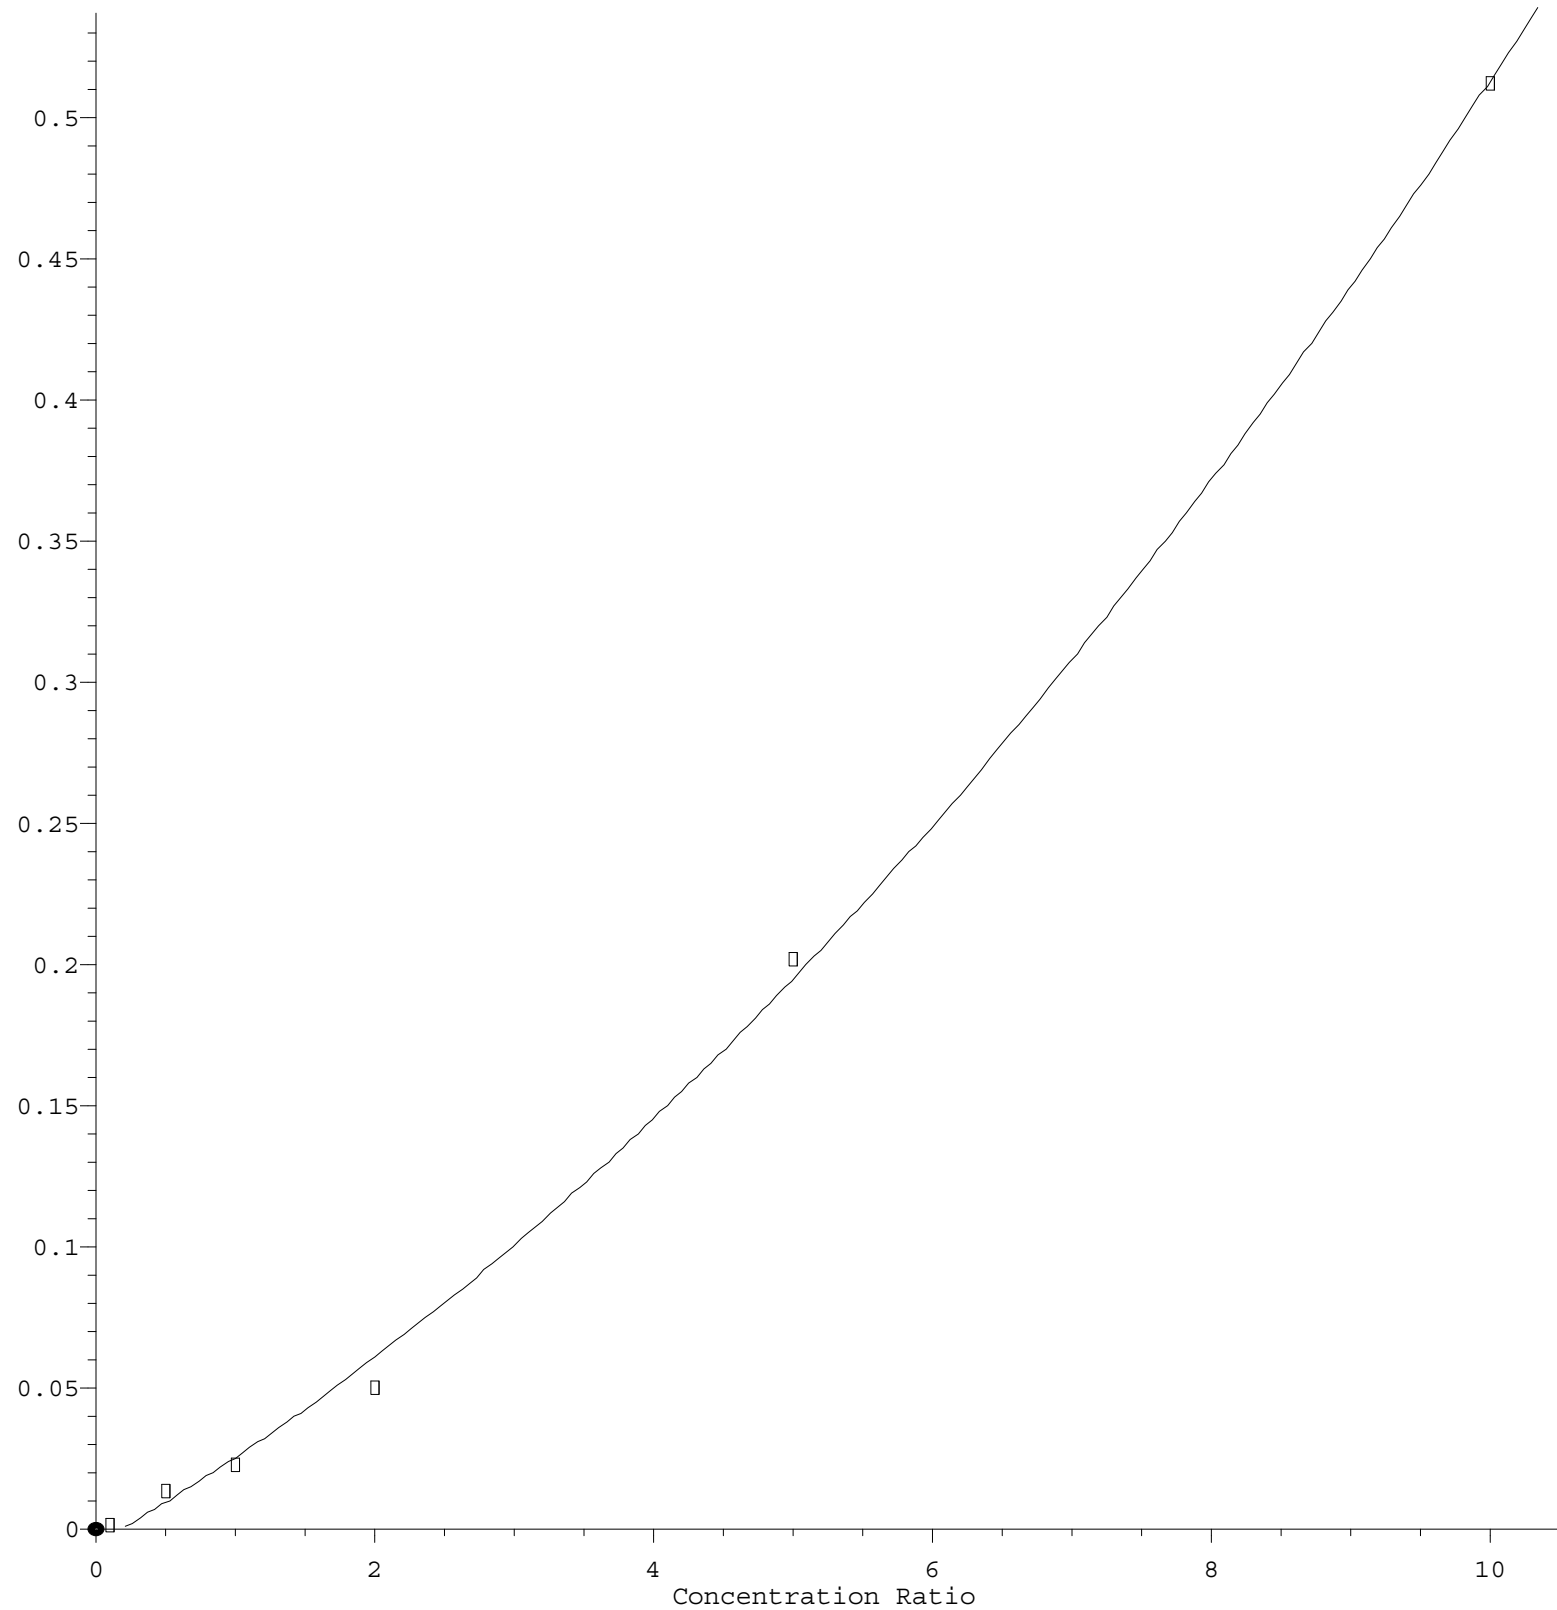

$R = 2.365e-003 A^2 + 2.820e-002 A - 5.136e-003$
 Coef of Det (r^2) = 0.999003 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090721W.M
 Calibration Table Last Updated: Fri Sep 17 11:02:11 2021

Dibromochloromethane

Response Ratio

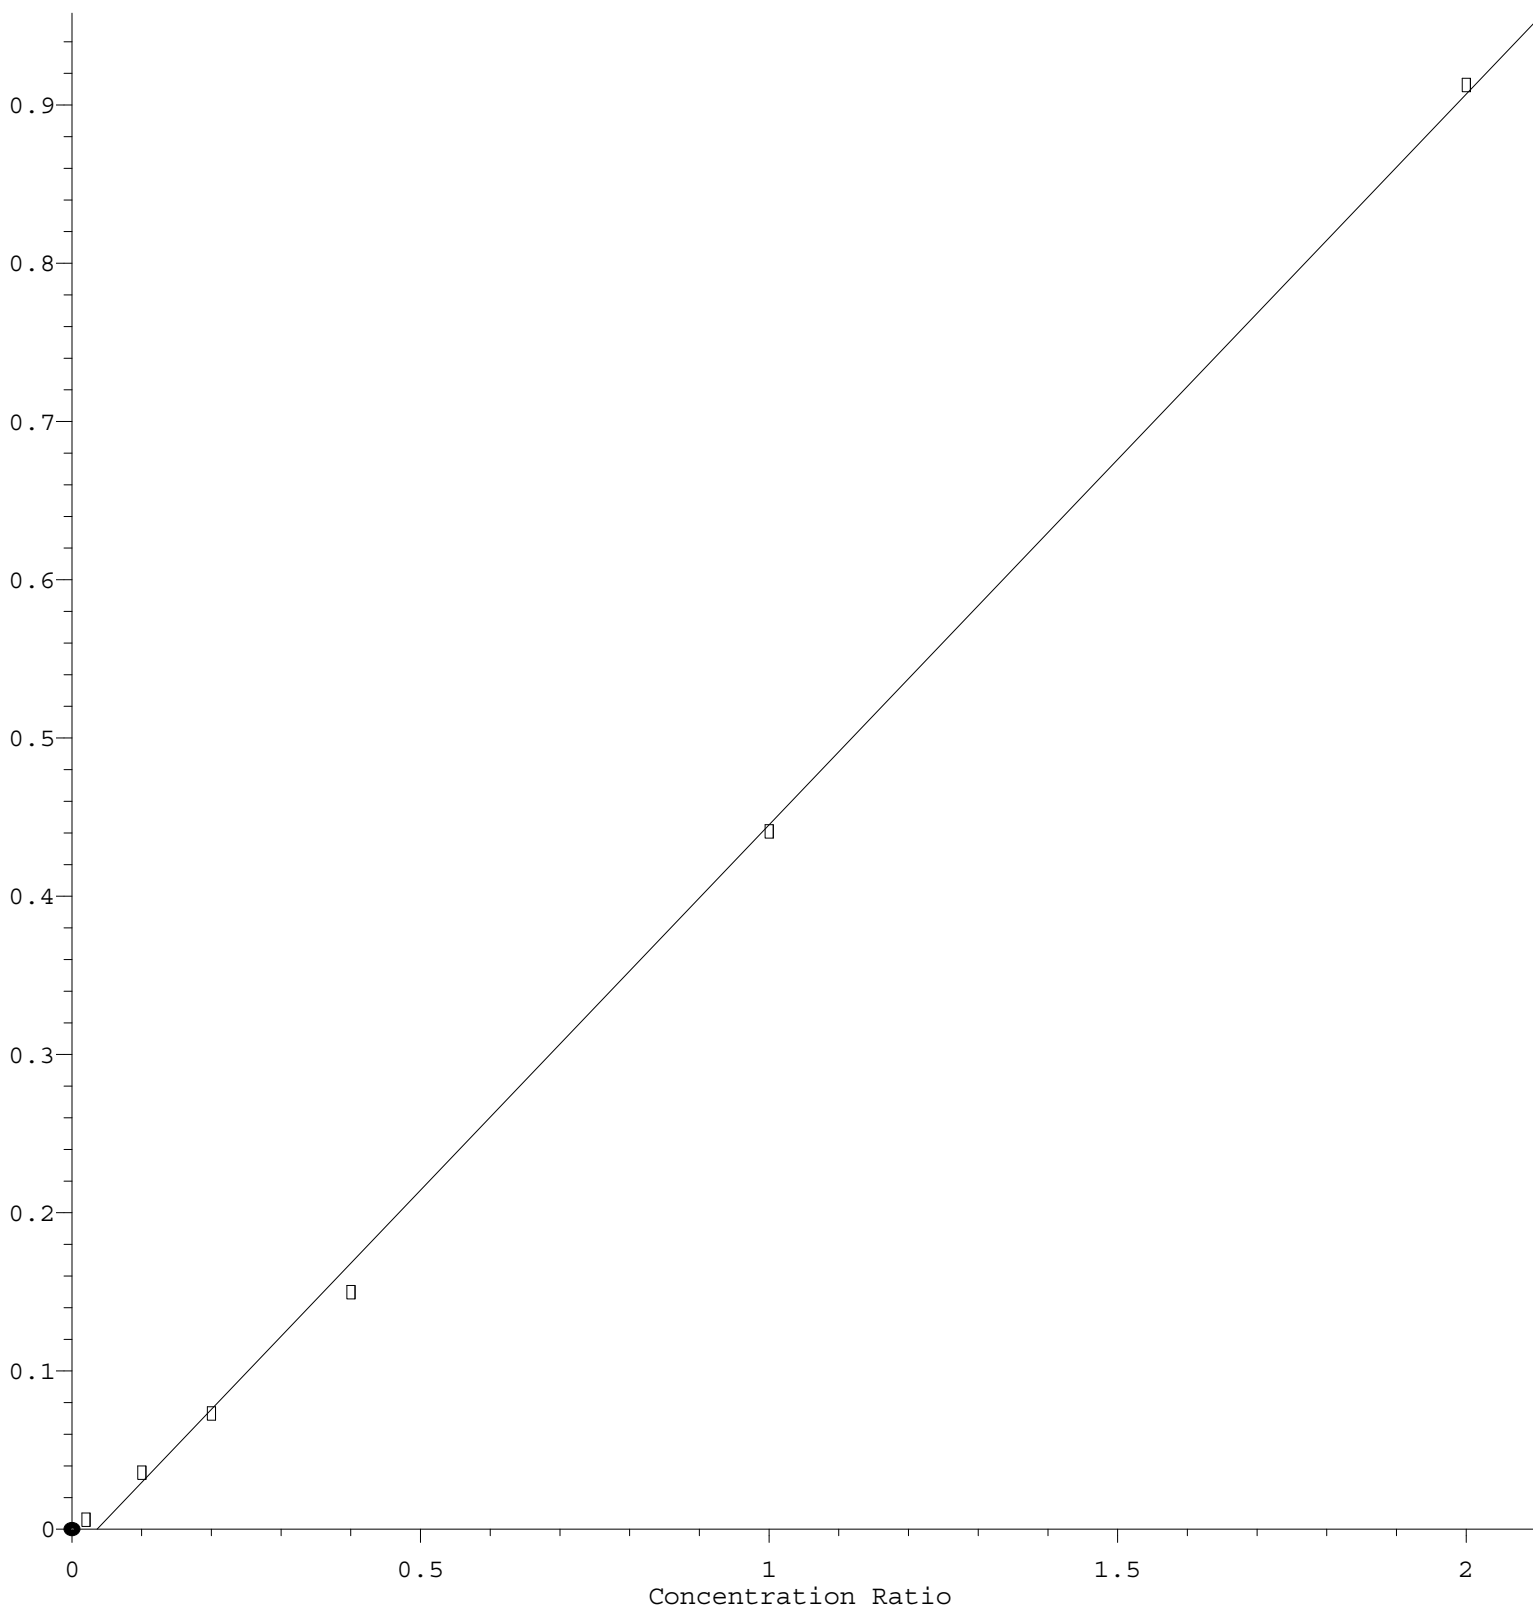


$$\text{Response} = 4.618\text{e-}001 * \text{Amt} - 1.665\text{e-}002$$

Coef of Det (r^2) = 0.999015 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090721W.M

Calibration Table Last Updated: Fri Sep 17 11:02:11 2021


4-Bromofluorobenzene

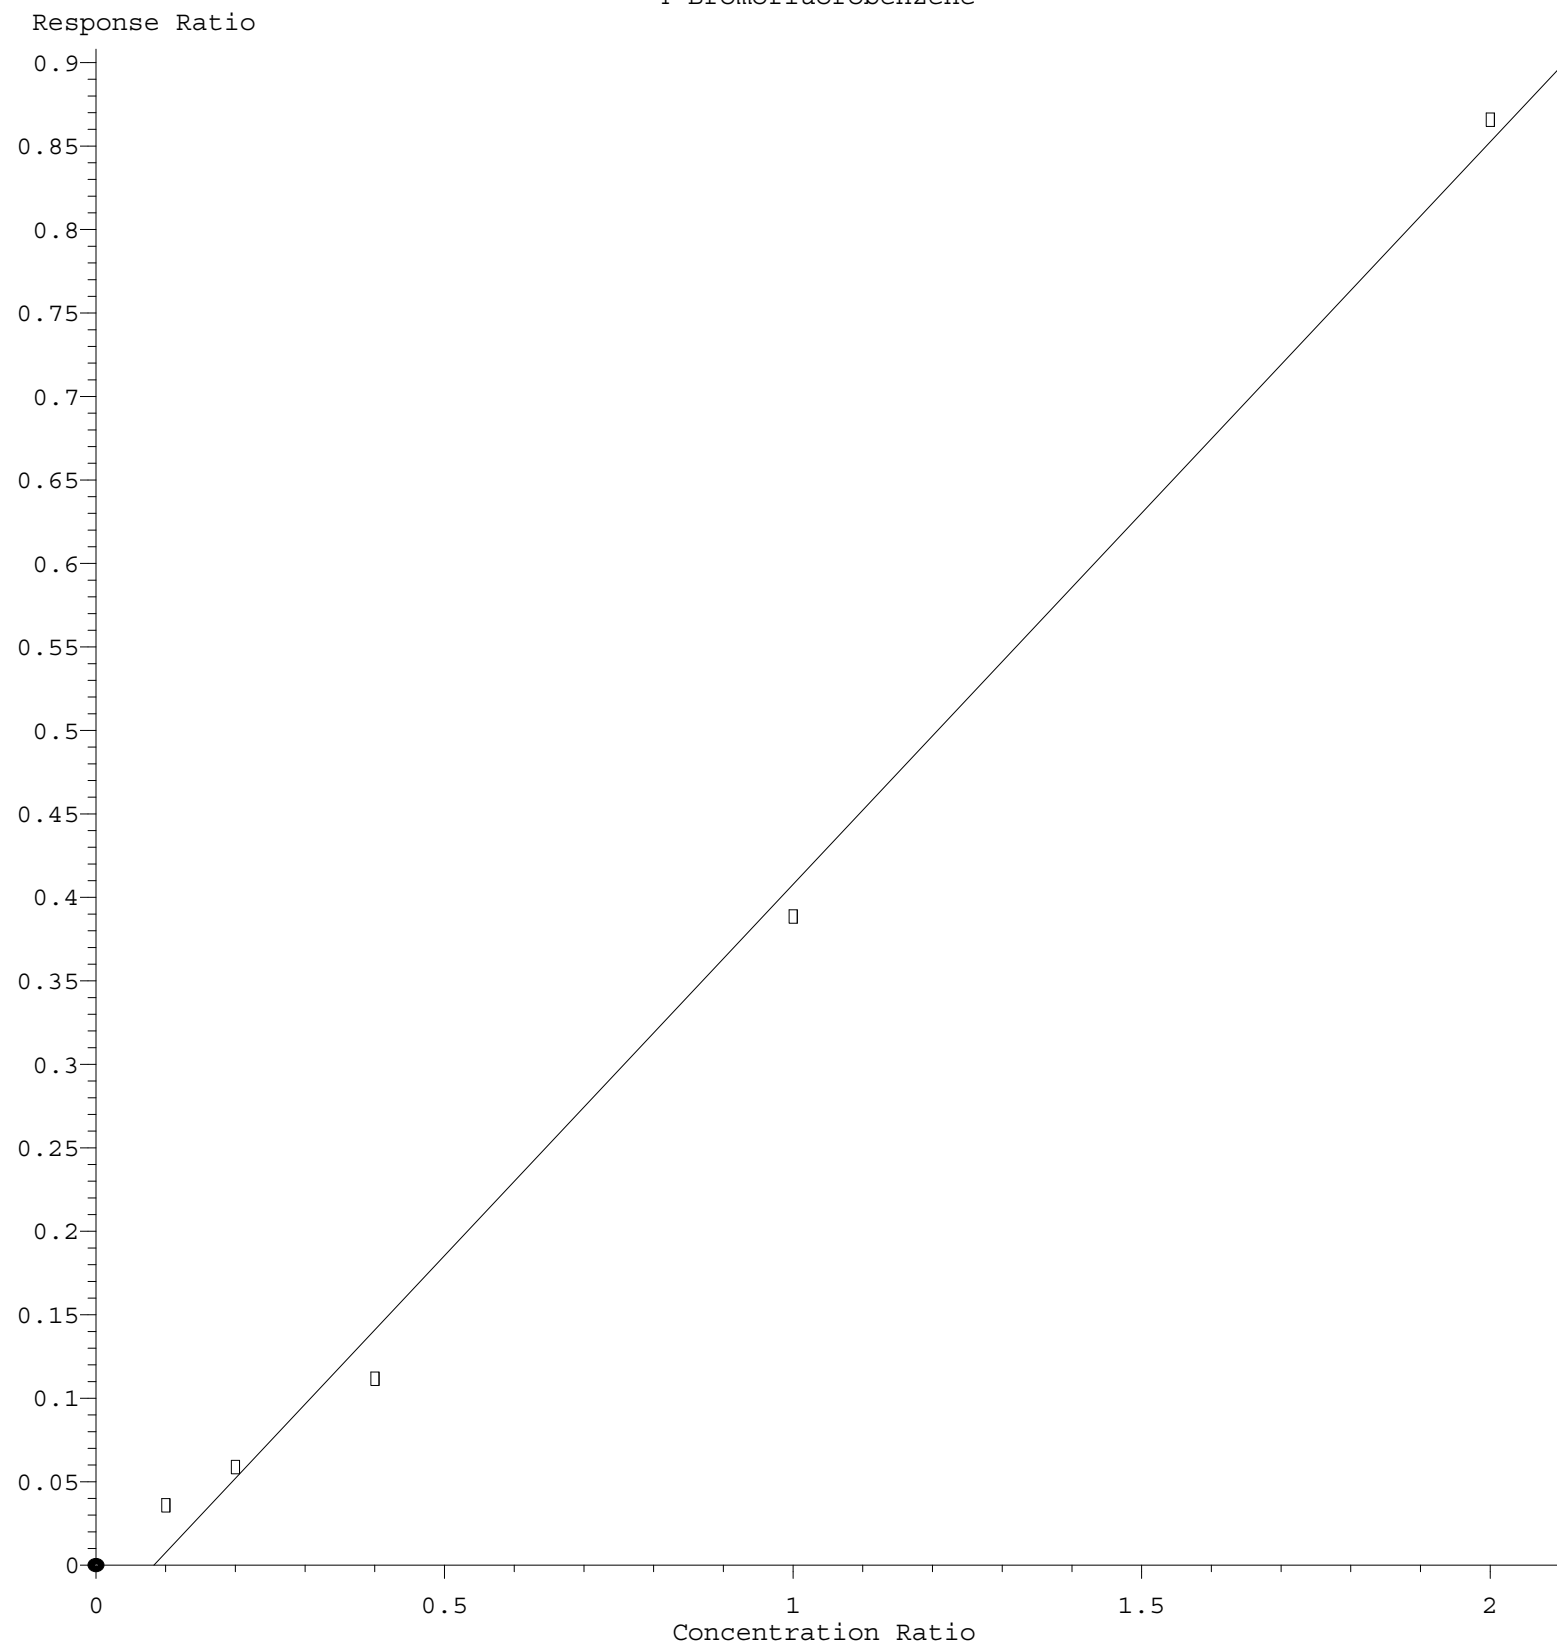

Response = $4.446 \times 10^{-1} \times \text{Amt} - 3.695 \times 10^{-2}$
Coef of Det (r^2) = 0.995416 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090721W.M
Calibration Table Last Updated: Fri Sep 17 11:02:11 2021

Styrene

Response Ratio

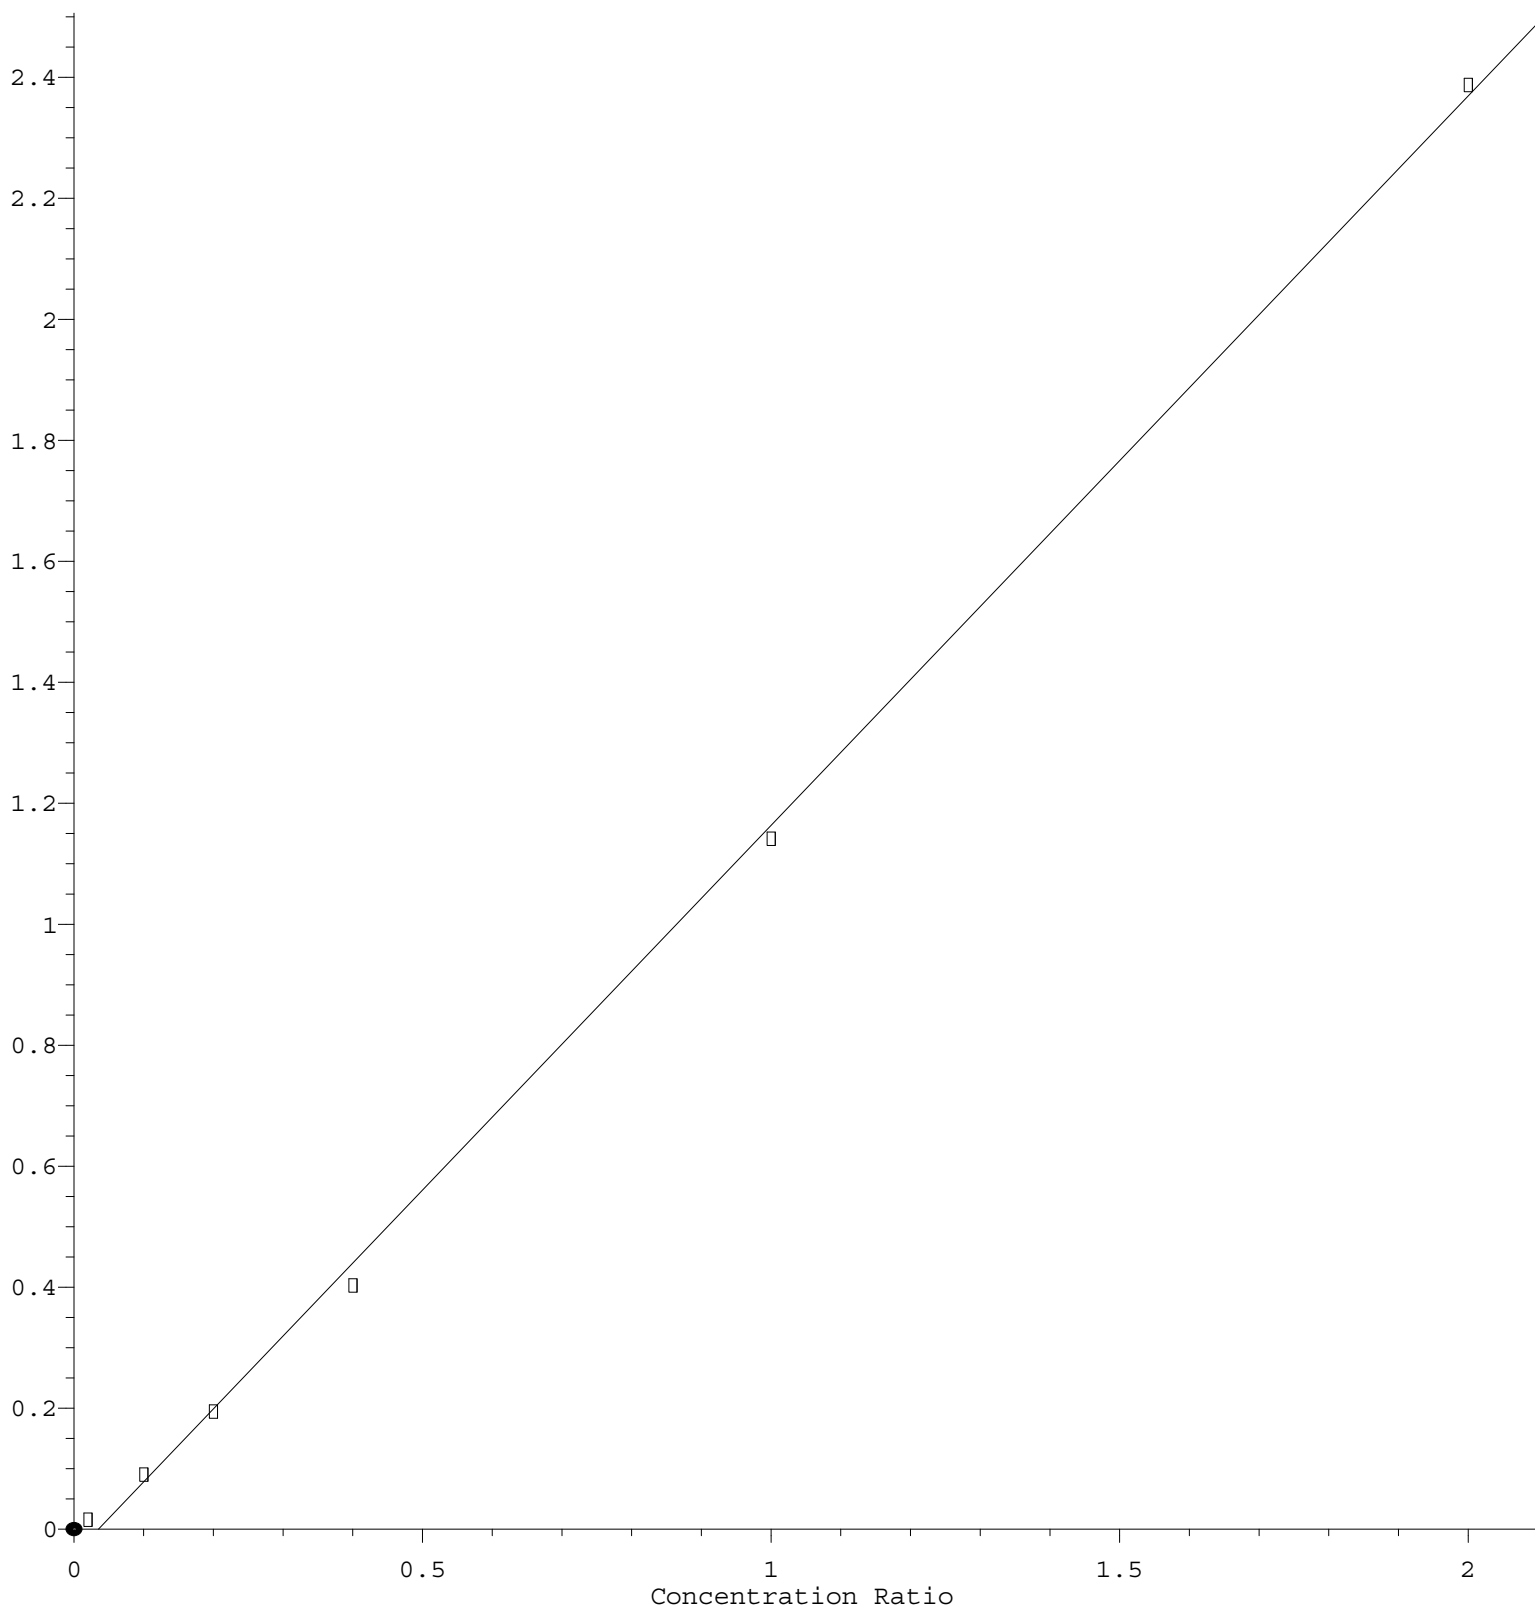

$$\text{Response} = 1.206\text{e}+000 * \text{Amt} - 4.229\text{e}-002$$

Coef of Det (r^2) = 0.999169 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N090721W.M

Calibration Table Last Updated: Fri Sep 17 11:02:11 2021