


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN090721\  
 Data File : VN068416.D  
 Acq On : 7 Sep 2021 10:08  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N090721W.M  
 Title : SW846 8260  
 Last Update : Wed Sep 08 20:01:41 2021

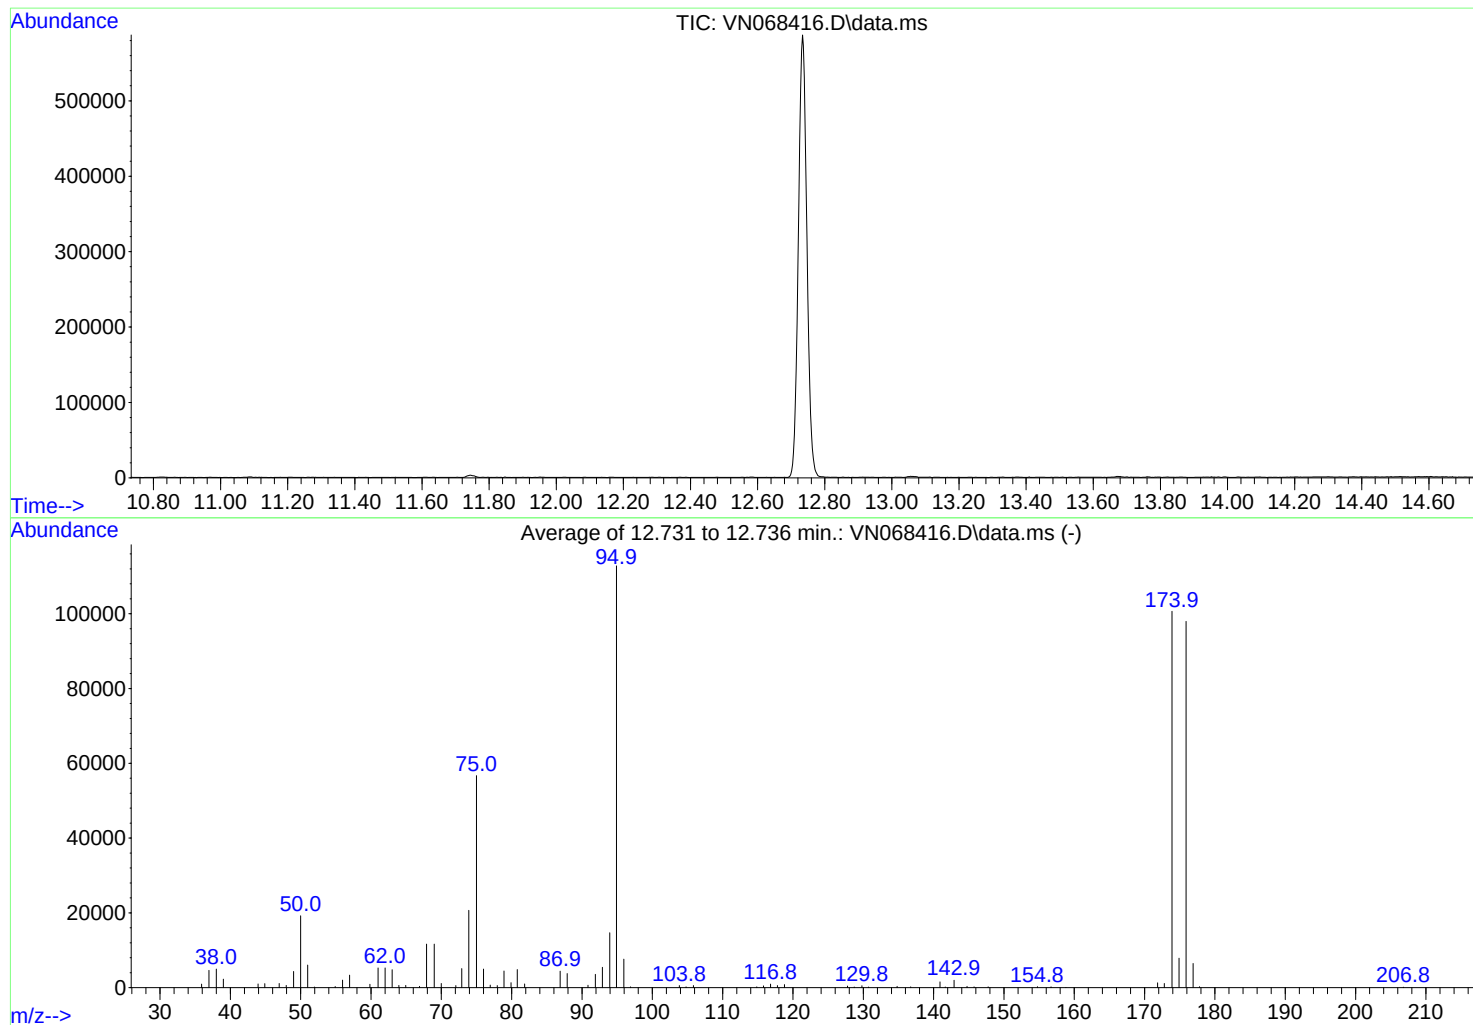

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3987

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 17.0         | 19224      | PASS                |
| 75             | 95              | 30              | 60              | 50.3         | 56725      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 112816     | PASS                |
| 96             | 95              | 5               | 9               | 6.7          | 7603       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.1          | 1134       | PASS                |
| 174            | 95              | 50              | 100             | 89.2         | 100637     | PASS                |
| 175            | 174             | 5               | 9               | 7.8          | 7871       | PASS                |
| 176            | 174             | 95              | 101             | 97.4         | 97976      | PASS                |
| 177            | 176             | 5               | 9               | 6.6          | 6447       | PASS                |