
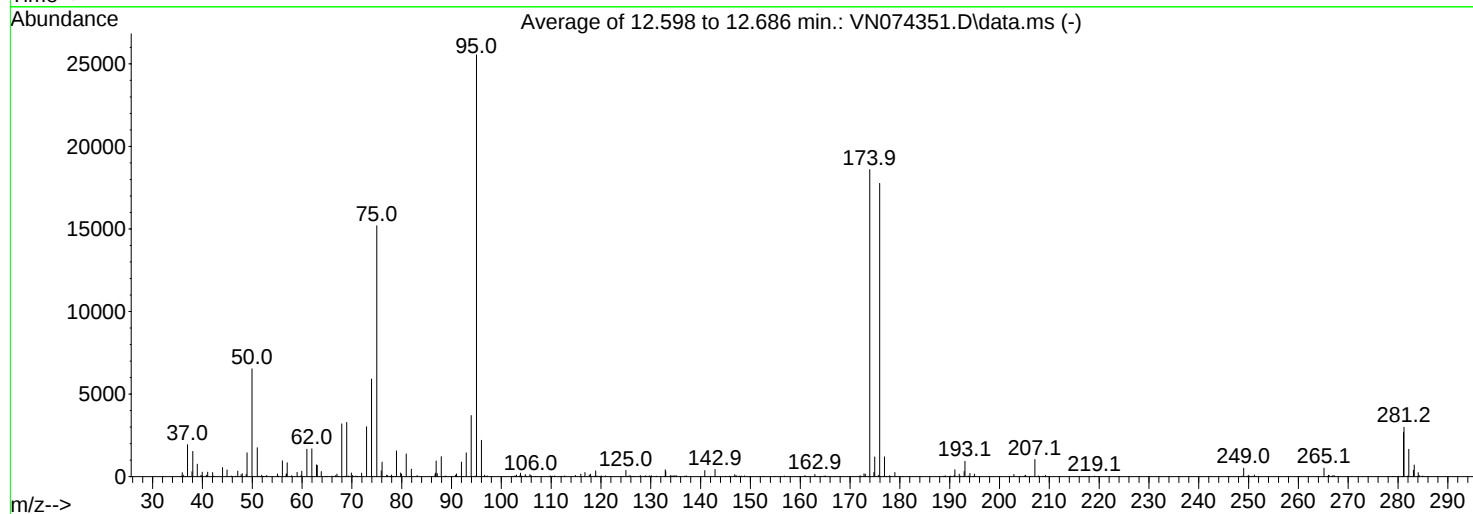


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090822\
 Data File : VN074351.D
 Acq On : 08 Sep 2022 11:39
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N090822W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Sep 09 05:24:20 2022

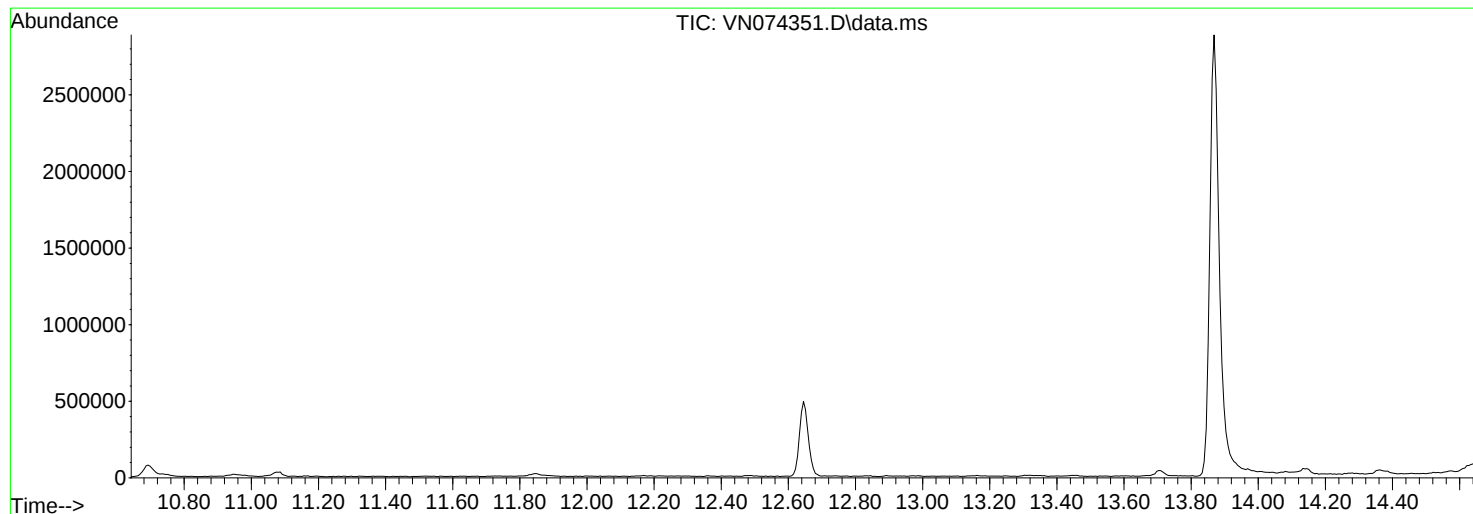

Spectrum Information: Average of 12.598 to 12.686 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.6	6528	PASS
75	95	30	60	59.5	15196	PASS
95	95	100	100	100.0	25546	PASS
96	95	5	9	8.6	2201	PASS
173	174	0.00	2	0.9	175	PASS
174	95	50	100	72.8	18600	PASS
175	174	5	9	6.4	1194	PASS
176	174	95	101	95.5	17766	PASS
177	176	5	9	6.7	1198	PASS