


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090823\
Data File : VN079188.D
Acq On : 08 Sep 2023 10:37
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N090723W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Sep 08 05:09:17 2023

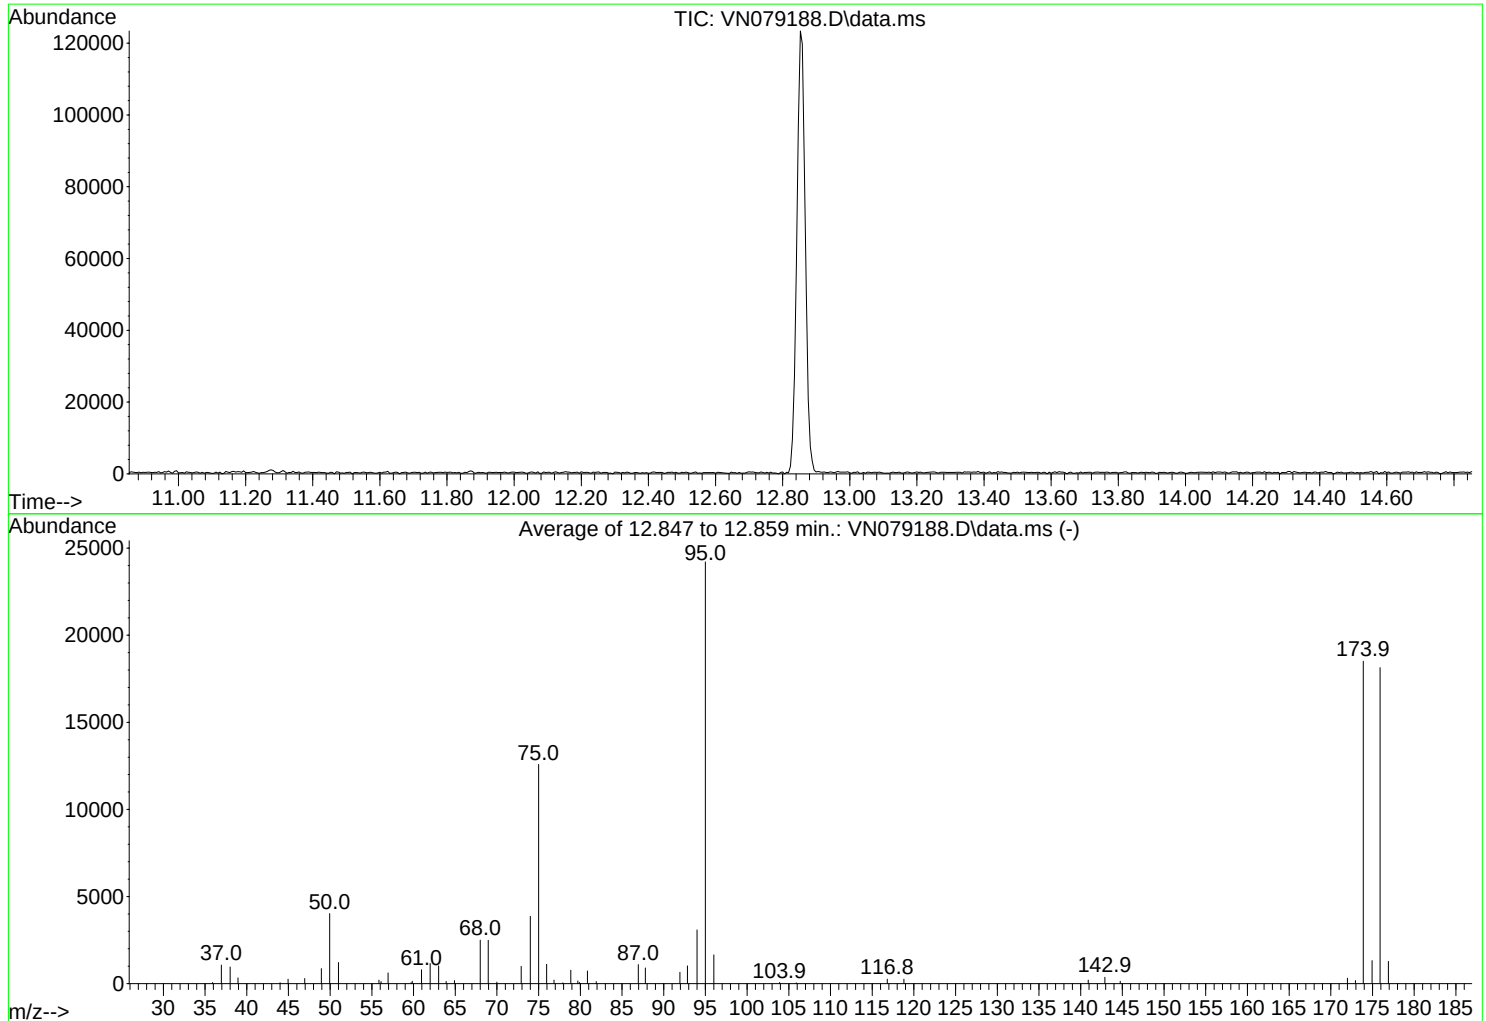

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1846

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	4024	PASS
75	95	30	60	52.0	12581	PASS
95	95	100	100	100.0	24211	PASS
96	95	5	9	6.8	1653	PASS
173	174	0.00	2	0.9	174	PASS
174	95	50	100	76.4	18507	PASS
175	174	5	9	7.1	1319	PASS
176	174	95	101	98.0	18137	PASS
177	176	5	9	7.0	1277	PASS