


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN090919\
 Data File : VN057786.D
 Acq On : 9 Sep 2019 8:17
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N090919W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Mon Sep 09 12:14:07 2019

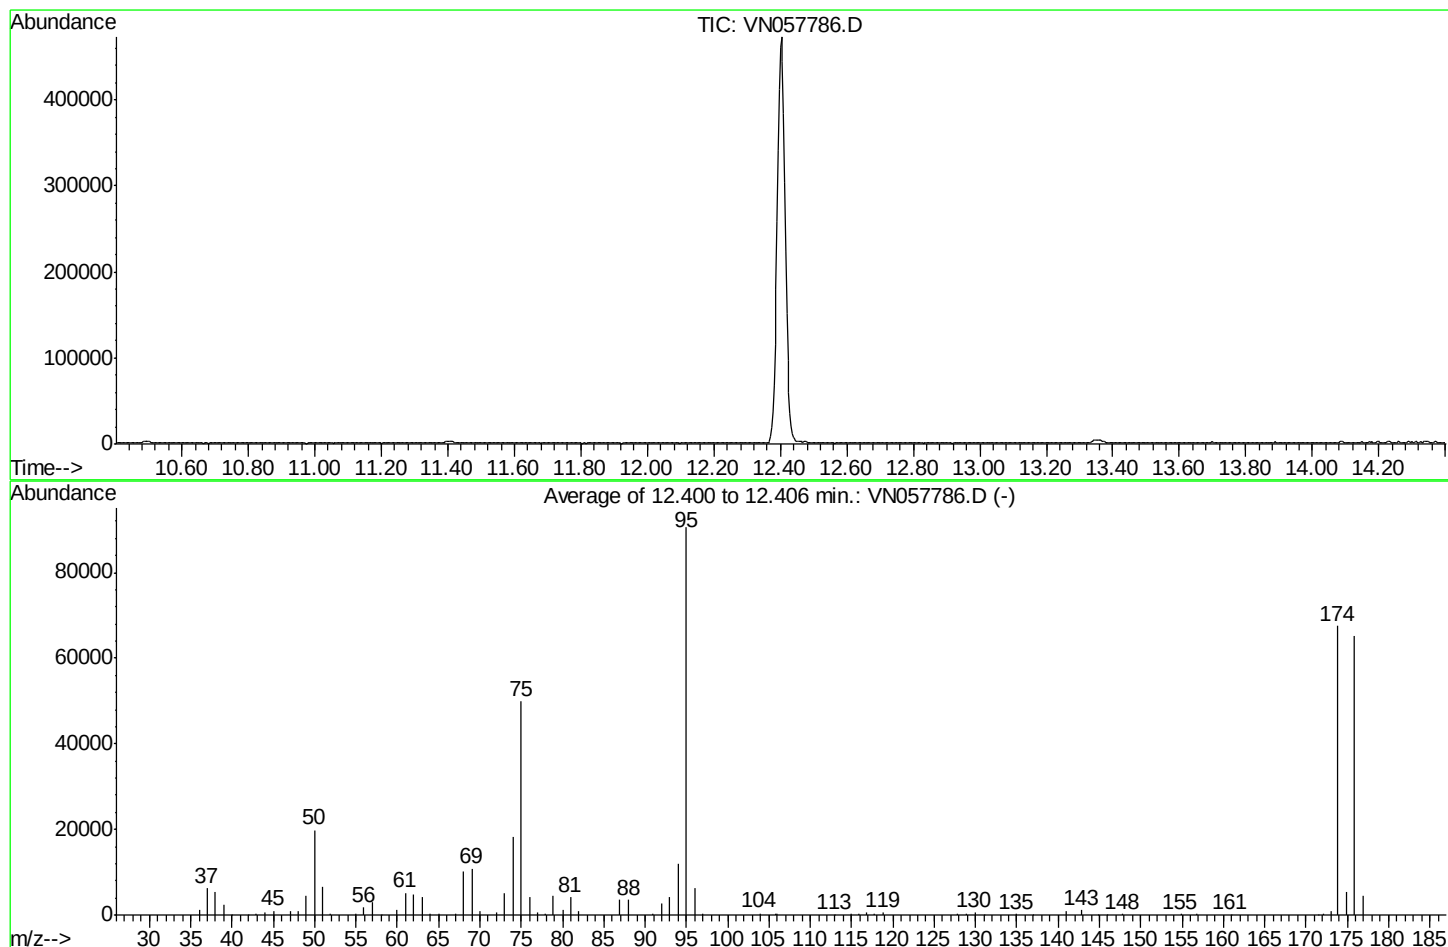

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	19808	PASS
75	95	30	60	55.1	49917	PASS
95	95	100	100	100.0	90573	PASS
96	95	5	9	7.1	6411	PASS
173	174	0.00	2	1.2	806	PASS
174	95	50	100	74.5	67461	PASS
175	174	5	9	7.8	5255	PASS
176	174	95	101	96.8	65320	PASS
177	176	5	9	6.7	4383	PASS