


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN090920\
 Data File : VN063270.D
 Acq On : 9 Sep 2020 9:30
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N083120W.M
 Title : SW846 8260
 Last Update : Tue Sep 01 04:21:28 2020

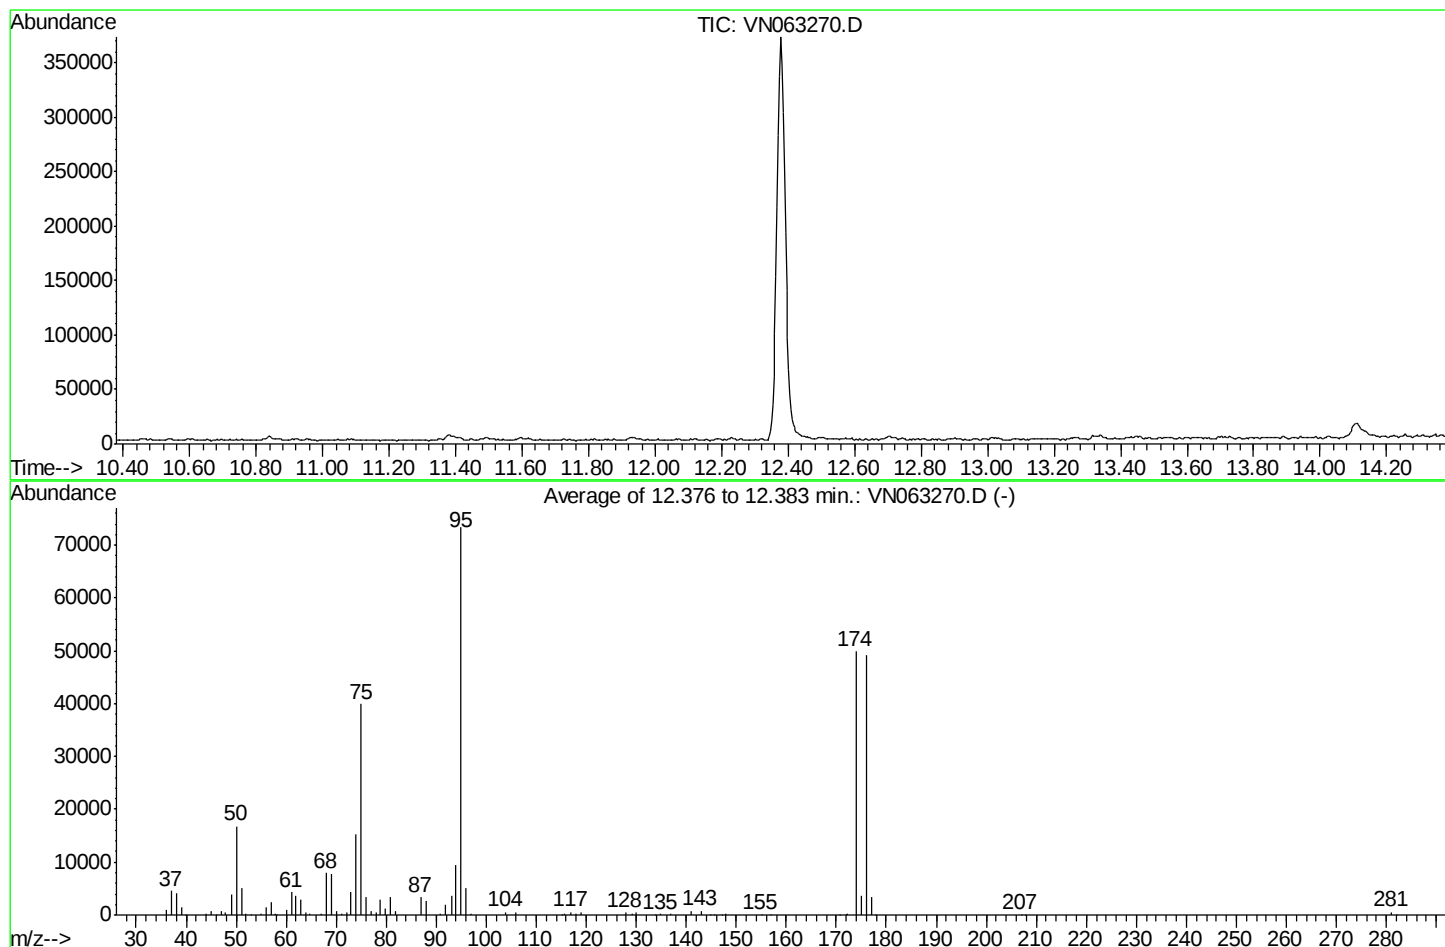

AutoFind: Scans 3308, 3309, 3310; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	16755	PASS
75	95	30	60	54.4	39901	PASS
95	95	100	100	100.0	73368	PASS
96	95	5	9	7.1	5195	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	68.0	49861	PASS
175	174	5	9	7.4	3673	PASS
176	174	95	101	98.6	49165	PASS
177	176	5	9	6.7	3311	PASS