
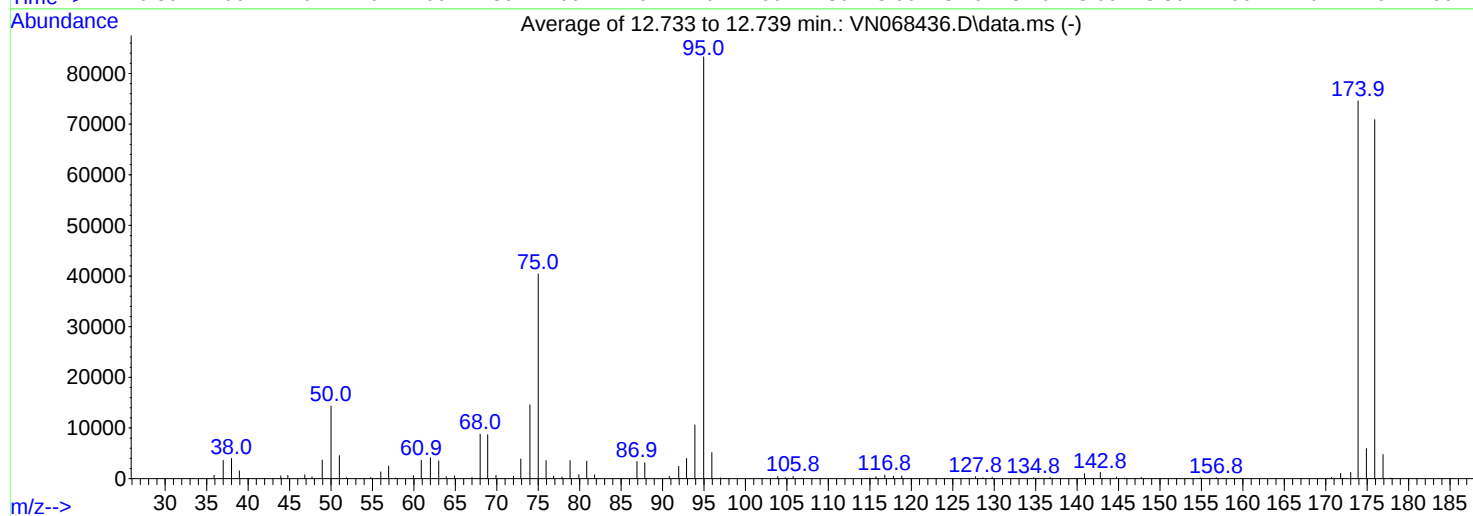


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090921\
 Data File : VN068436.D
 Acq On : 9 Sep 2021 9:52
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
 Title : SW846 8260
 Last Update : Fri Sep 10 04:04:05 2021

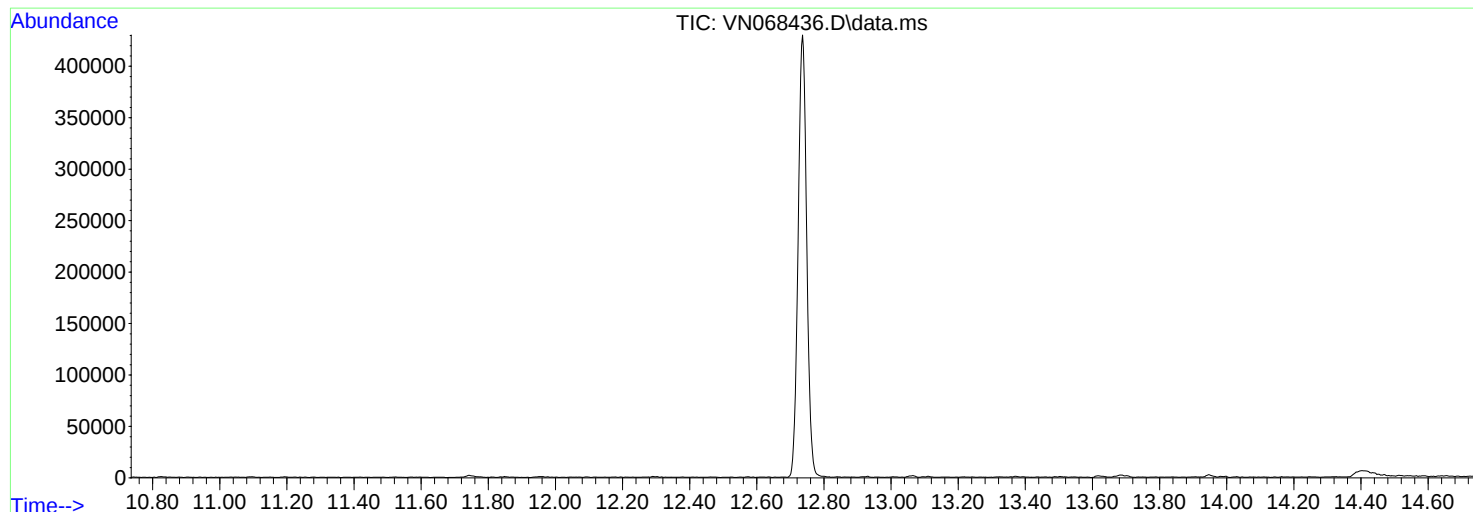

AutoFind: Scans 4006, 4007, 4008; Background Corrected with Scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	14352	PASS
75	95	30	60	48.5	40395	PASS
95	95	100	100	100.0	83277	PASS
96	95	5	9	6.2	5159	PASS
173	174	0.00	2	1.6	1228	PASS
174	95	50	100	89.6	74589	PASS
175	174	5	9	8.0	5942	PASS
176	174	95	101	95.0	70880	PASS
177	176	5	9	6.8	4785	PASS