

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090922\
 Data File : VN074382.D
 Acq On : 09 Sep 2022 18:56
 Operator : JC\MD
 Sample : N4471-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-10B-40-45-083022

Quant Time: Sep 10 07:24:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090922W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 10 06:10:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.016	168	338705	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	594463	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	587312	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.615	152	264939	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	237287	40.492	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	80.980%		
35) Dibromofluoromethane	7.951	113	196035	48.847	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	97.700%		
50) Toluene-d8	10.380	98	678572	43.394	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	86.780%		
62) 4-Bromofluorobenzene	12.674	95	279841	49.291	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	98.580%		
Target Compounds						Qvalue
3) Chloromethane	2.269	50	2122	Below Cal	#	86
4) Vinyl Chloride	2.404	62	8949	1.220	ug/l	97
5) Bromomethane	2.781	94	2204	0.430	ug/l #	24
6) Chloroethane	2.693	64	70316	12.223	ug/l #	51
11) Tert butyl alcohol	5.263	59	1607	1.048	ug/l #	71
12) 1,1-Dichloroethene	4.110	96	70395	16.672	ug/l	95
13) Acrolein	3.987	56	970	0.953	ug/l #	62
15) Acrylonitrile	5.469	53	895	0.255	ug/l #	73
16) Acetone	4.234	43	4460	1.410	ug/l #	86
17) Carbon Disulfide	4.451	76	2963	0.258	ug/l #	77
18) Methyl Acetate	4.775	43	4581	0.491	ug/l #	65
20) Methylene Chloride	5.028	84	143	Below Cal	#	38
21) trans-1,2-Dichloroethene	5.516	96	7596	1.606	ug/l	82
24) 1,1-Dichloroethane	6.304	63	22911	2.391	ug/l #	92
27) cis-1,2-Dichloroethene	7.245	96	190679	32.713	ug/l	90
28) Bromochloromethane	7.622	49	134	Below Cal	#	20
31) Cyclohexane	8.016	56	10301	1.105	ug/l #	1
36) 1,1-Dichloropropene	8.010	75	33656	5.091	ug/l #	51
38) Carbon Tetrachloride	8.022	117	37751	5.531	ug/l #	14
42) 1,2-Dichloroethane	8.463	62	19889	2.570	ug/l	99
44) Trichloroethene	9.151	130	159282	35.098	ug/l	96
49) 1,4-Dioxane	9.516	88	4883	33.521	ug/l #	72
51) 4-Methyl-2-Pentanone	10.269	43	2421	0.236	ug/l #	84
59) 2-Hexanone	11.027	43	2876	0.363	ug/l	86
74) N-amyl acetate	12.327	43	1571	Below Cal	#	53
76) 1,2,3-Trichloropropane	12.674	75	166685	24.067	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.674	75	166685	53.644	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	14.562	75	191	Below Cal	#	13
93) 1,2,4-Trichlorobenzene	15.204	180	1913	0.361	ug/l	79
95) Naphthalene	15.439	128	12220	0.590	ug/l #	87
96) 1,2,3-Trichlorobenzene	15.633	180	2144	0.391	ug/l	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090922\
Data File : VN074382.D
Acq On : 09 Sep 2022 18:56
Operator : JC\MD
Sample : N4471-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-10B-40-45-083022

Quant Time: Sep 10 07:24:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090922W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 10 06:10:29 2022
Response via : Initial Calibration




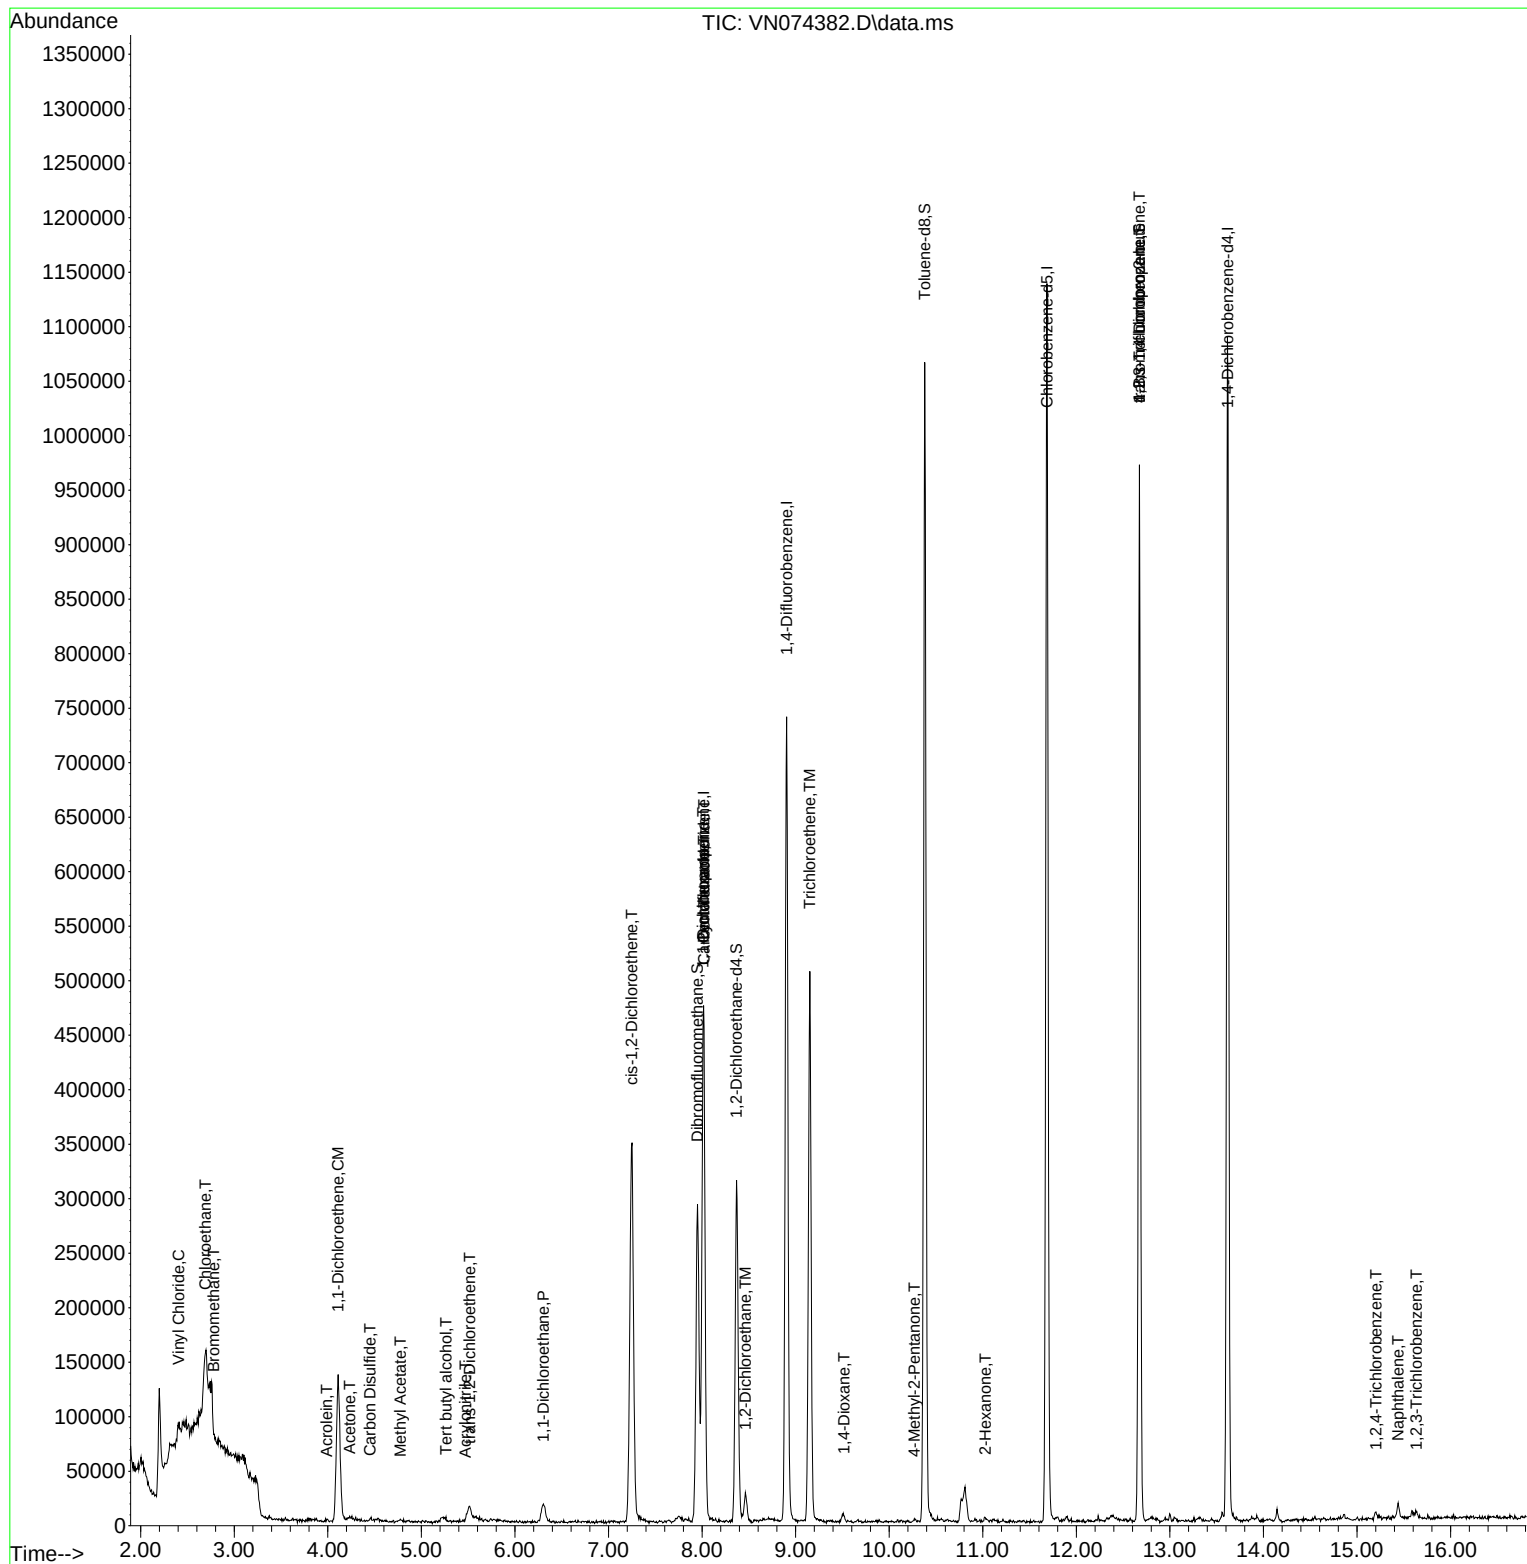




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56




Instrument :
MSVOA_N
ClientSampleId :
MW-10B-40-45-083022


Tgt Ion:168 Resp: 338705
Ion Ratio Lower Upper
168 100
99 60.1 52.8 79.2

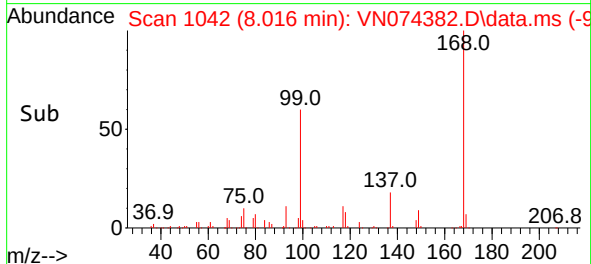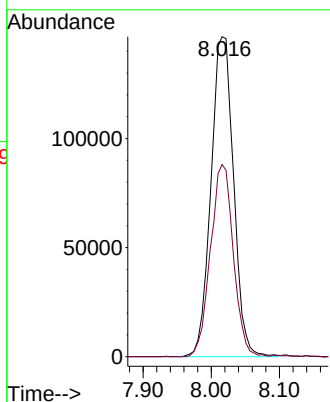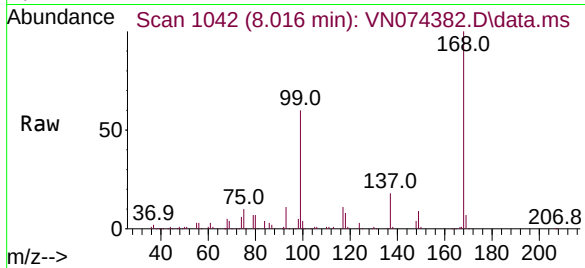

#3
Chloromethane
Concen: Below Cal
RT: 2.269 min Scan# 65
Delta R.T. 0.000 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56

Tgt Ion: 50 Resp: 2122
Ion Ratio Lower Upper
50 100
52 22.4 24.1 36.1#


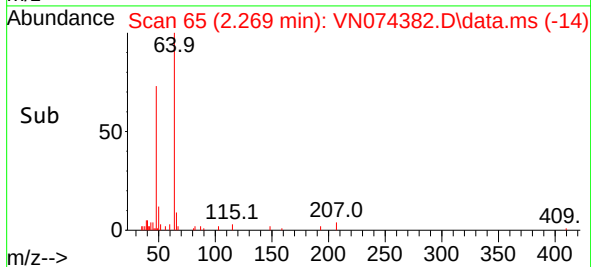
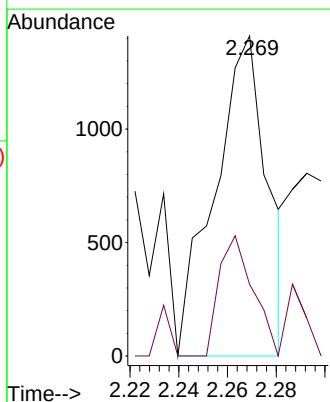
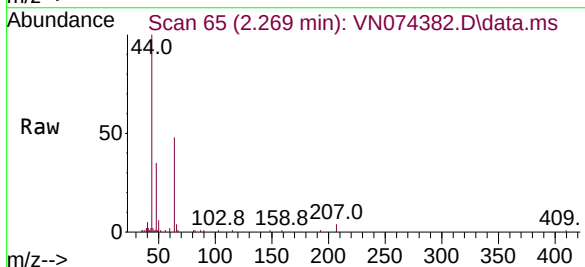


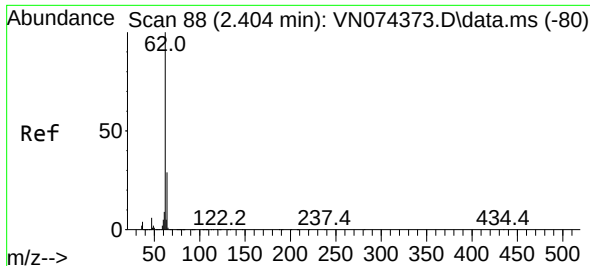

#4
 Vinyl Chloride
 Concen: 1.220 ug/l
 RT: 2.404 min Scan# 88
 Delta R.T. -0.000 min
 Lab File: VN074382.D
 Acq: 09 Sep 2022 18:56




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-10B-40-45-083022


Tgt Ion: 62 Resp: 8949
 Ion Ratio Lower Upper
 62 100
 64 27.8 23.5 35.3

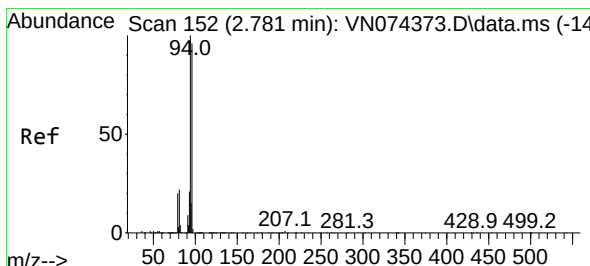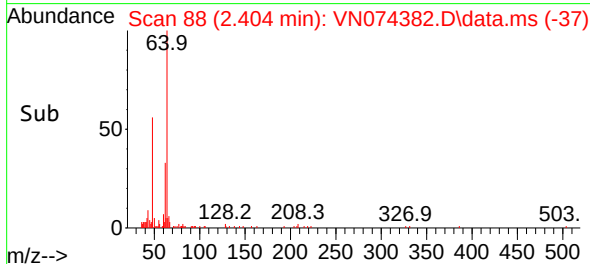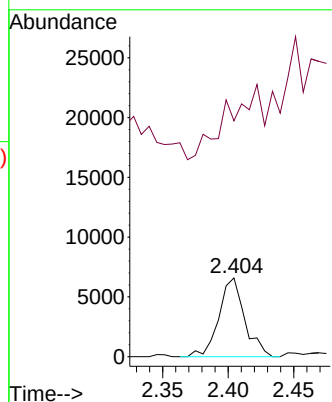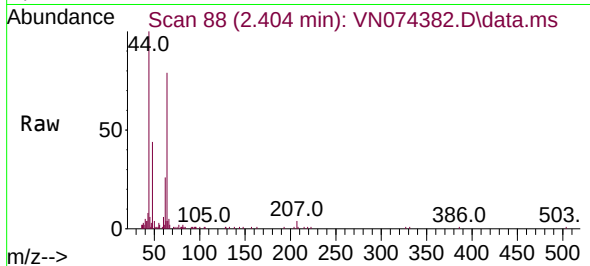

#5
 Bromomethane
 Concen: 0.430 ug/l
 RT: 2.781 min Scan# 152
 Delta R.T. -0.000 min
 Lab File: VN074382.D
 Acq: 09 Sep 2022 18:56

Tgt Ion: 94 Resp: 2204
 Ion Ratio Lower Upper
 94 100
 96 21.4 76.7 115.1#


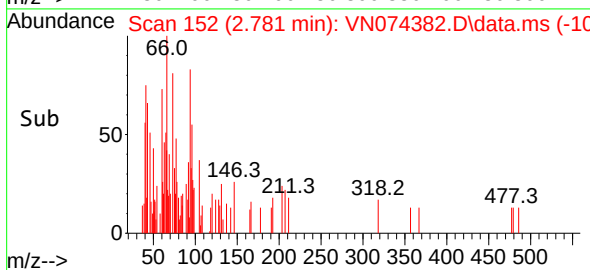
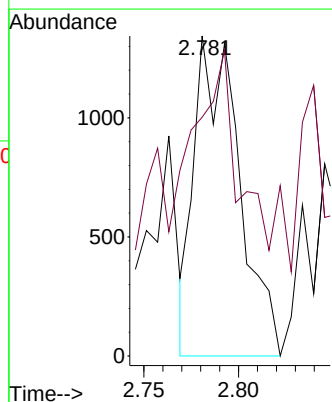
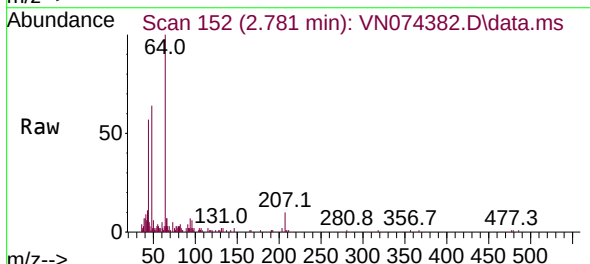




#6
Chloroethane
Concen: 12.223 ug/l
RT: 2.693 min Scan# 11
Delta R.T. -0.253 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56




Instrument :
MSVOA_N
ClientSampleId :
MW-10B-40-45-083022


Tgt Ion: 64 Resp: 70316
Ion Ratio Lower Upper
64 100
66 5.2 26.5 39.7#

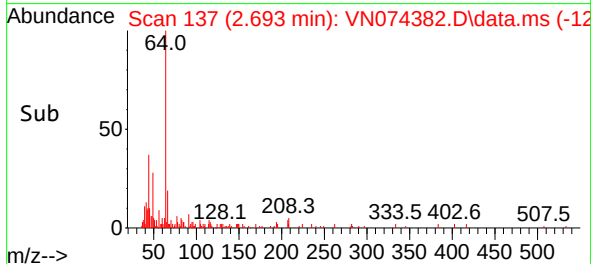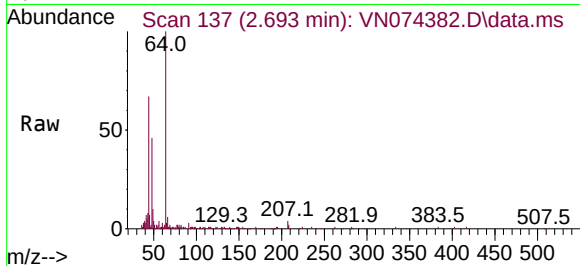

#11
Tert butyl alcohol
Concen: 1.048 ug/l
RT: 5.263 min Scan# 574
Delta R.T. -0.024 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56

Tgt Ion: 59 Resp: 1607
Ion Ratio Lower Upper
59 100
57 0.0 8.8 13.2#


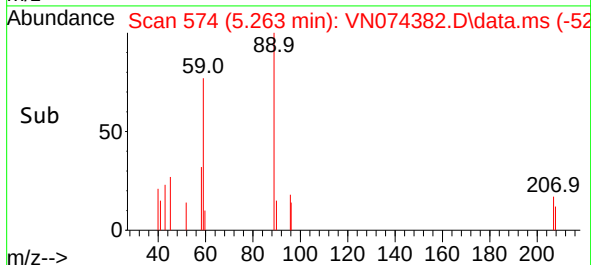

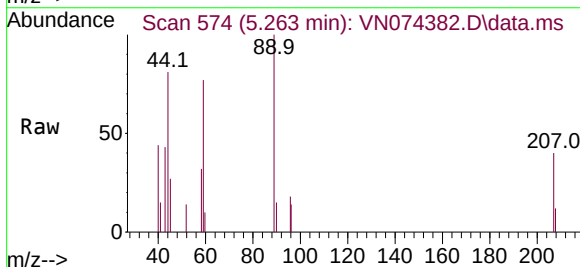




#12
1,1-Dichloroethene
Concen: 16.672 ug/l
RT: 4.110 min Scan# 31
Delta R.T. 0.006 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56




Instrument :
MSVOA_N
ClientSampleId :
MW-10B-40-45-083022


Tgt Ion: 96 Resp: 70395
Ion Ratio Lower Upper
96 100
61 159.8 134.7 202.1
98 61.3 50.2 75.4

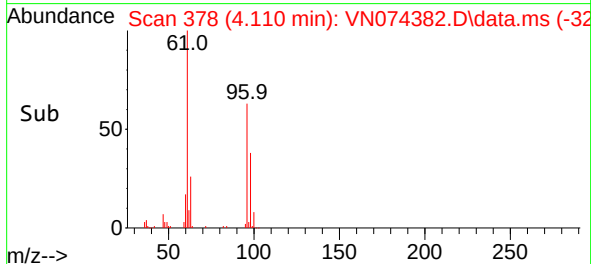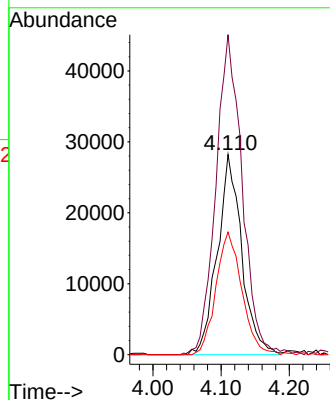

#13
Acrolein
Concen: 0.953 ug/l
RT: 3.987 min Scan# 357
Delta R.T. 0.012 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56

Tgt Ion: 56 Resp: 970
Ion Ratio Lower Upper
56 100
55 101.8 56.2 84.4#



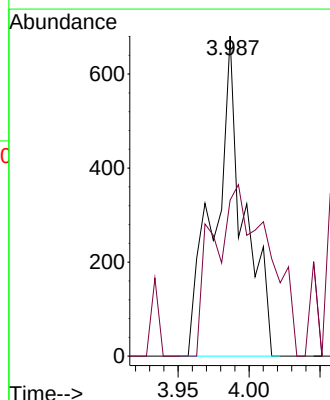
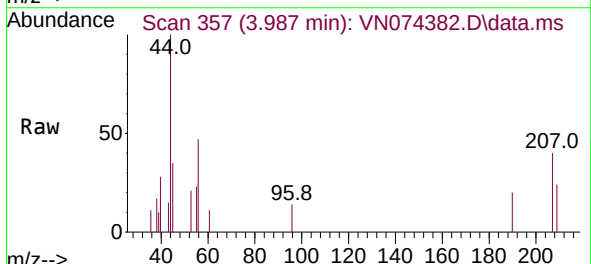




#15
Acrylonitrile
Concen: 0.255 ug/l
RT: 5.469 min Scan# 609
Delta R.T. -0.000 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56




Instrument :
MSVOA_N
ClientSampleId :
MW-10B-40-45-083022


Tgt Ion: 53 Resp: 895
Ion Ratio Lower Upper
53 100
52 55.5 65.9 98.9#
51 23.8 29.4 44.2#

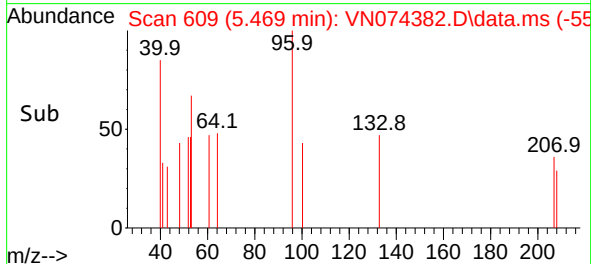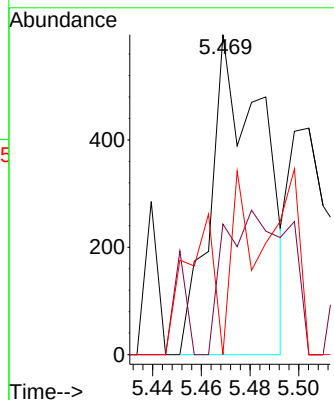

#16
Acetone
Concen: 1.410 ug/l
RT: 4.234 min Scan# 399
Delta R.T. 0.012 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56

Tgt Ion: 43 Resp: 4460
Ion Ratio Lower Upper
43 100
58 36.0 22.7 34.1#

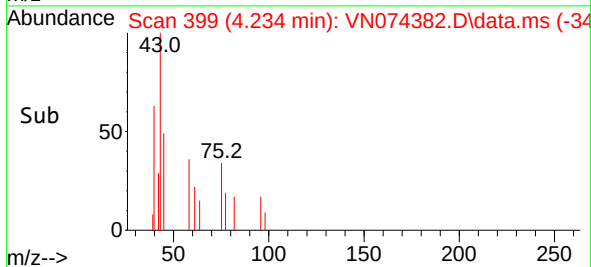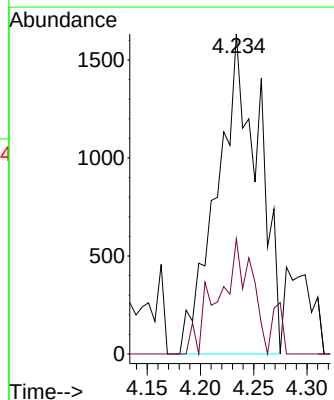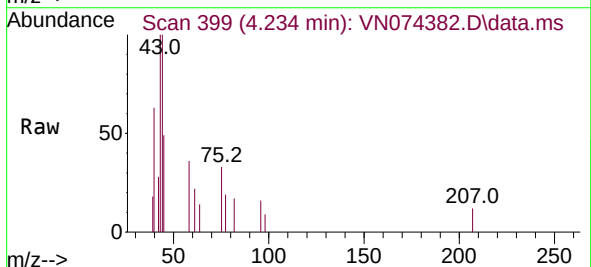



#17

Carbon Disulfide

Concen: 0.258 ug/l

RT: 4.451 min Scan# 41

Delta R.T. -0.000 min

Lab File: VN074382.D

Acq: 09 Sep 2022 18:56

Instrument :

MSVOA_N

ClientSampleId :





MW-10B-40-45-083022

Tgt Ion: 76 Resp: 2963

Ion Ratio Lower Upper

76 100

78 0.0 6.5 9.7#

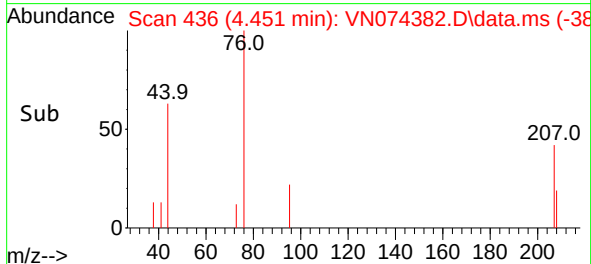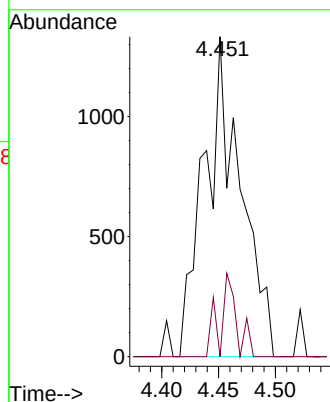

#18

Methyl Acetate

Concen: 0.491 ug/l

RT: 4.775 min Scan# 491

Delta R.T. 0.006 min

Lab File: VN074382.D




Acq: 09 Sep 2022 18:56


Tgt Ion: 43 Resp: 4581

Ion Ratio Lower Upper

43 100

74 4.7 16.7 25.1#



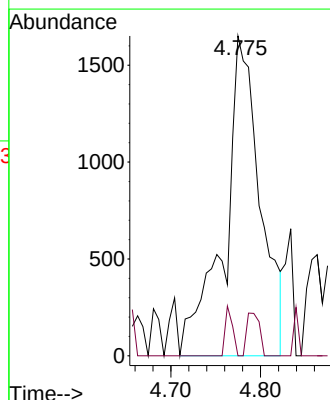



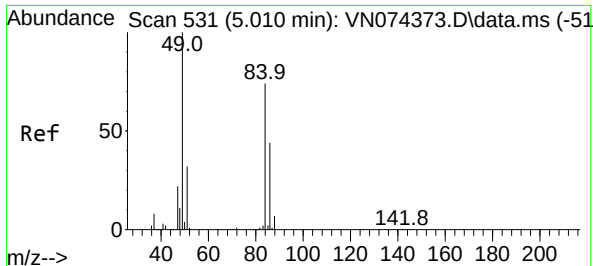

#20
Methylene Chloride
Concen: Below Cal
RT: 5.028 min Scan# 51
Delta R.T. 0.018 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56




Instrument :
MSVOA_N
ClientSampleId :
MW-10B-40-45-083022


Tgt Ion: 84 Resp: 143
Ion Ratio Lower Upper
84 100
49 71.6 108.2 162.4#
51 0.0 34.3 51.5#
86 0.0 48.2 72.2#

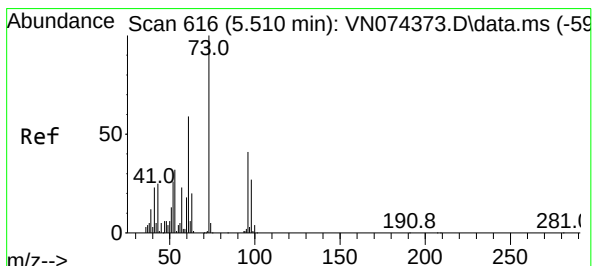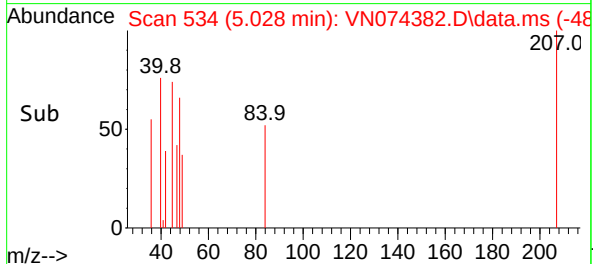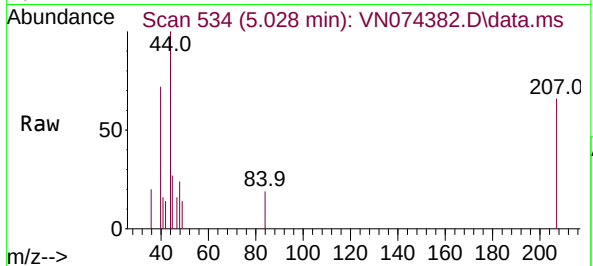

#21
trans-1,2-Dichloroethene
Concen: 1.606 ug/l
RT: 5.516 min Scan# 617
Delta R.T. 0.006 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56

Tgt Ion: 96 Resp: 7596
Ion Ratio Lower Upper
96 100
61 119.3 115.3 172.9
98 56.8 53.4 80.0


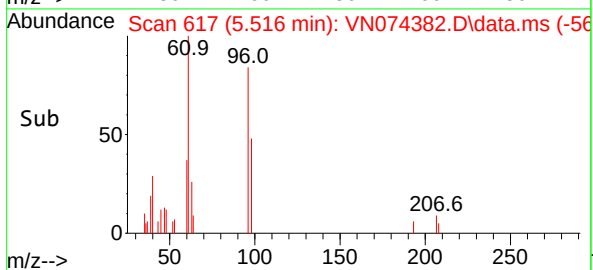

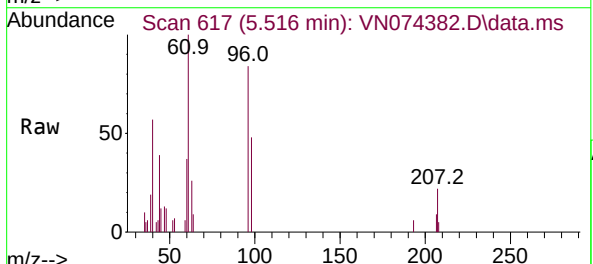




#24
 1,1-Dichloroethane
 Concen: 2.391 ug/l
 RT: 6.304 min Scan# 751
 Delta R.T. 0.006 min
 Lab File: VN074382.D
 Acq: 09 Sep 2022 18:56




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-10B-40-45-083022


Tgt Ion: 63	Resp: 22911
Ion Ratio	Lower Upper
63 100	
98 9.3	2.9 8.6#
100 5.1	2.0 5.8

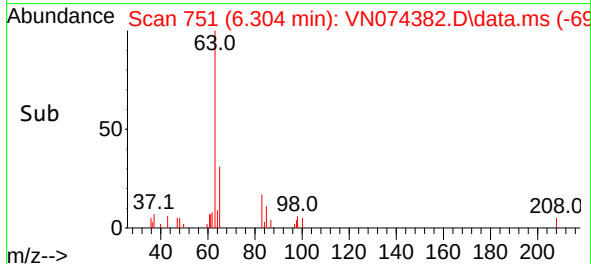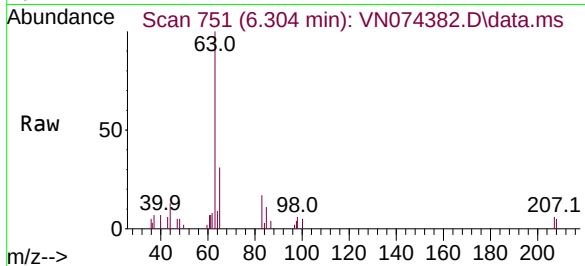

#27
 cis-1,2-Dichloroethene
 Concen: 32.713 ug/l
 RT: 7.245 min Scan# 911
 Delta R.T. -0.000 min
 Lab File: VN074382.D
 Acq: 09 Sep 2022 18:56

Tgt Ion: 96	Resp: 190679
Ion Ratio	Lower Upper
96 100	
61 135.4	0.0 306.2
98 65.8	0.0 129.8


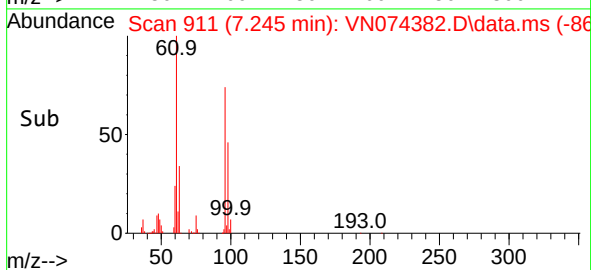

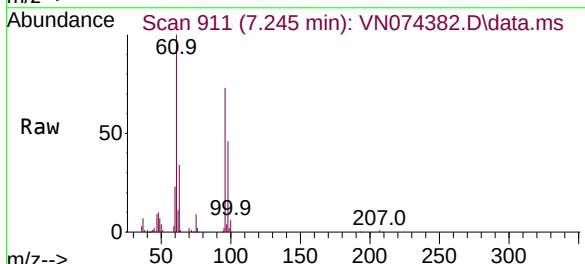




#28
Bromochloromethane
Concen: Below Cal
RT: 7.622 min Scan# 91
Delta R.T. 0.041 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56




Instrument :
MSVOA_N
ClientSampleId :
MW-10B-40-45-083022


Tgt Ion: 49 Resp: 134
Ion Ratio Lower Upper
49 100
129 0.0 0.0 2.2
130 0.0 50.0 75.0#

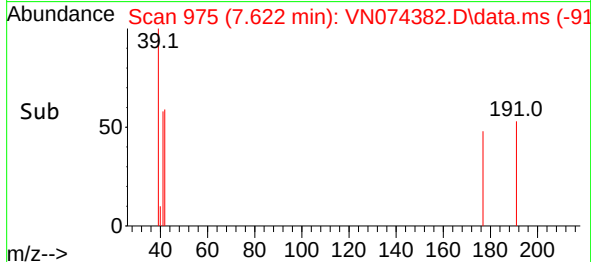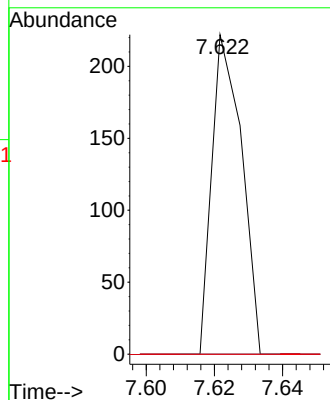

#31
Cyclohexane
Concen: 1.105 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.012 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56

Tgt Ion: 56 Resp: 10301
Ion Ratio Lower Upper
56 100
69 144.0 23.0 34.4#
84 137.2 66.3 99.5#

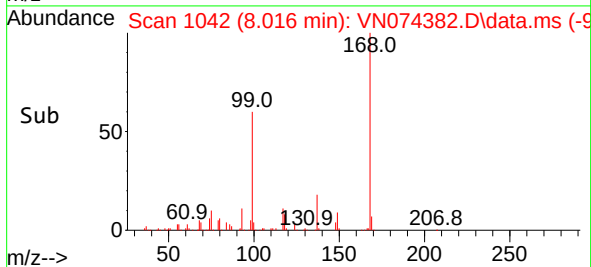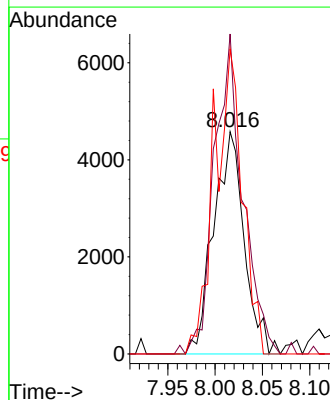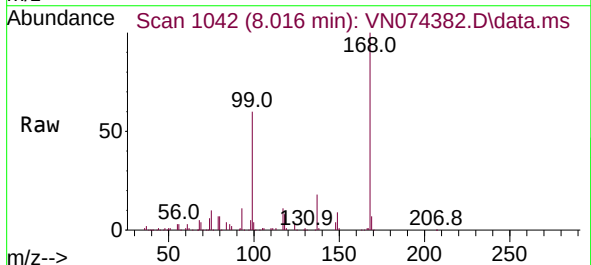

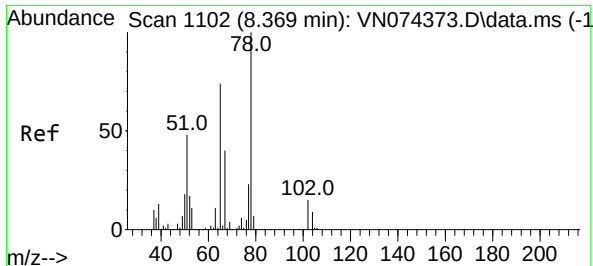

#33

1,2-Dichloroethane-d4

Concen: 40.492 ug/l

RT: 8.369 min Scan# 1102

Delta R.T. -0.000 min

Lab File: VN074382.D

Acq: 09 Sep 2022 18:56

Instrument :

MSVOA_N

ClientSampleId :





MW-10B-40-45-083022

Tgt Ion: 65 Resp: 237287

Ion Ratio Lower Upper

65 100

67 51.3 0.0 102.4

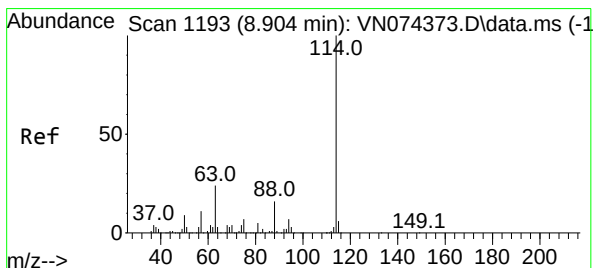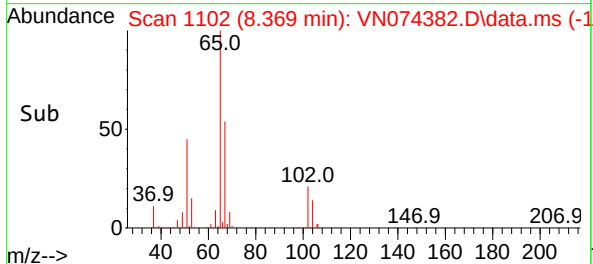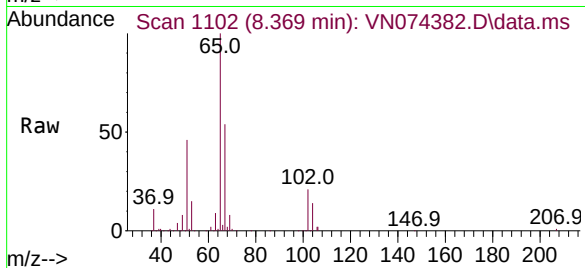

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. -0.000 min

Lab File: VN074382.D

Acq: 09 Sep 2022 18:56




Tgt Ion: 114 Resp: 594463


Ion Ratio Lower Upper

114 100

63 23.2 0.0 47.6

88 14.9 0.0 31.4


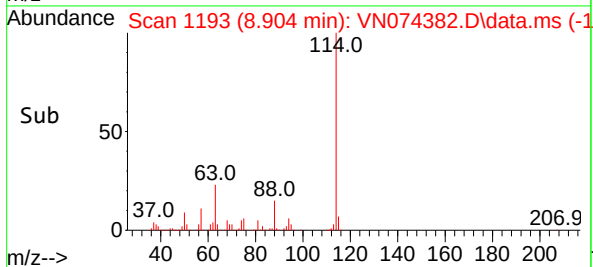

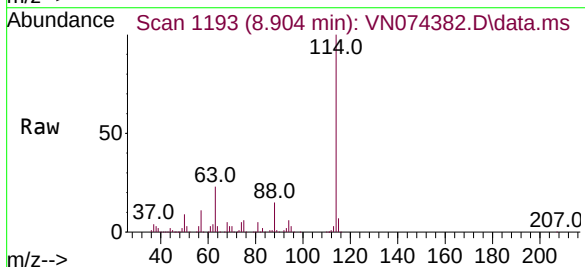




#35
Dibromofluoromethane
Concen: 48.847 ug/l
RT: 7.951 min Scan# 1041
Delta R.T. -0.000 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56




Instrument :
MSVOA_N
ClientSampleId :
MW-10B-40-45-083022


Tgt Ion:113 Resp: 196035
Ion Ratio Lower Upper
113 100
111 104.3 83.0 124.4
192 17.0 13.7 20.5

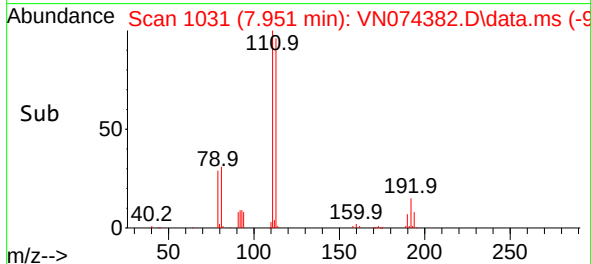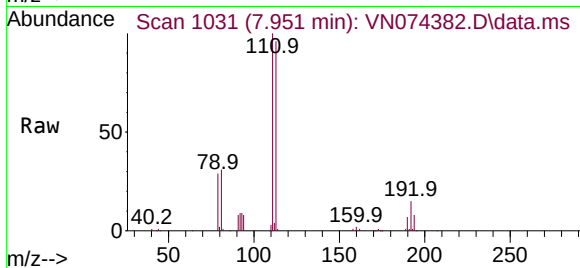

#36
1,1-Dichloropropene
Concen: 5.091 ug/l
RT: 8.010 min Scan# 1041
Delta R.T. -0.141 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56

Tgt Ion: 75 Resp: 33656
Ion Ratio Lower Upper
75 100
110 9.2 16.4 49.1#
77 0.0 25.4 38.2#


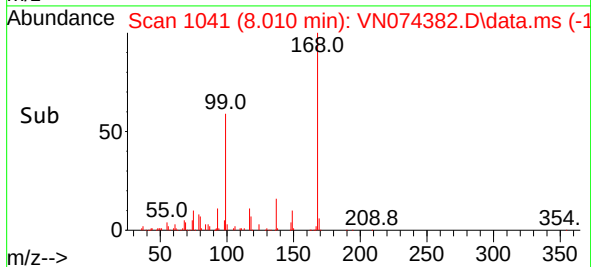

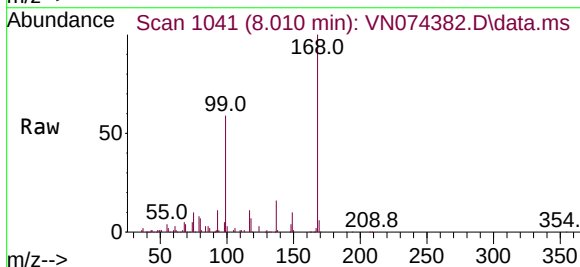


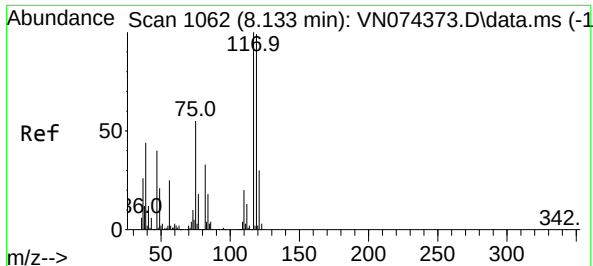

#38
Carbon Tetrachloride
Concen: 5.531 ug/l
RT: 8.022 min Scan# 1107
Delta R.T. -0.112 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56




Instrument :
MSVOA_N
ClientSampleId :
MW-10B-40-45-083022


Tgt Ion: 117 Resp: 37751
Ion Ratio Lower Upper
117 100
119 3.5 78.8 118.2#
121 0.0 24.1 36.1#

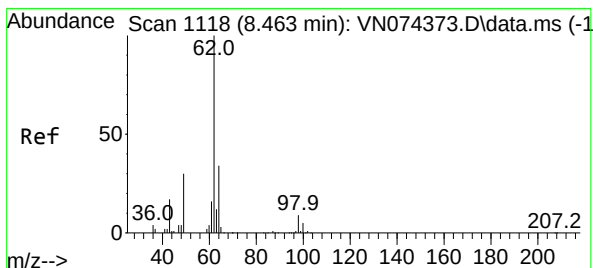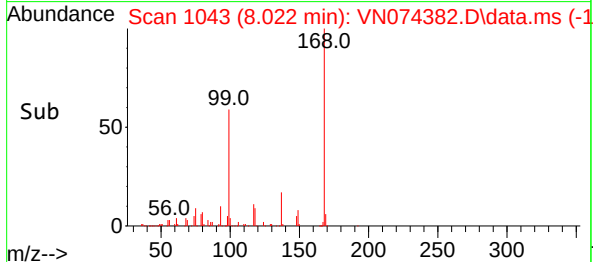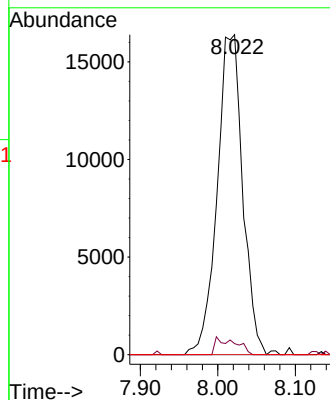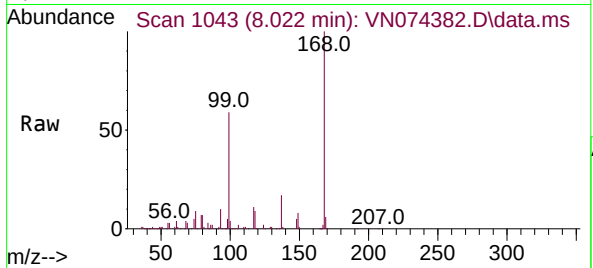

#42
1,2-Dichloroethane
Concen: 2.570 ug/l
RT: 8.463 min Scan# 1118
Delta R.T. -0.000 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56

Tgt Ion: 62 Resp: 19889
Ion Ratio Lower Upper
62 100
98 9.3 0.0 17.6


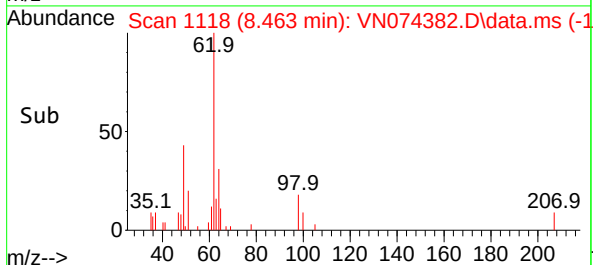
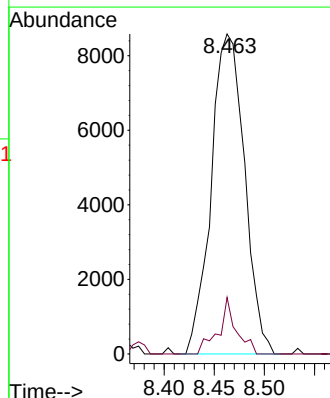
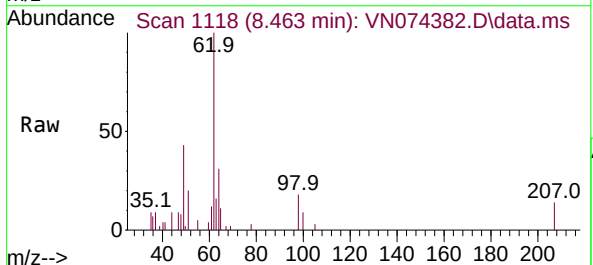


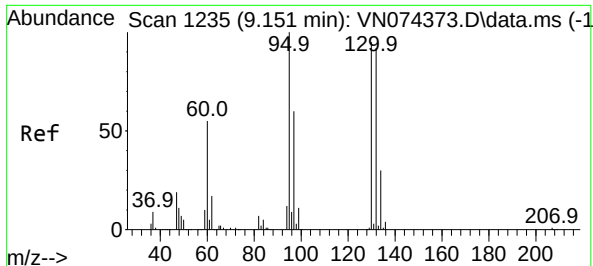

#44
Trichloroethene
Concen: 35.098 ug/l
RT: 9.151 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56




Instrument :
MSVOA_N
ClientSampleId :
MW-10B-40-45-083022


Tgt Ion:130 Resp: 159282
Ion Ratio Lower Upper
130 100
95 100.8 0.0 210.0

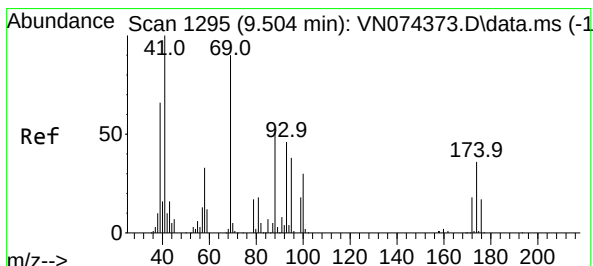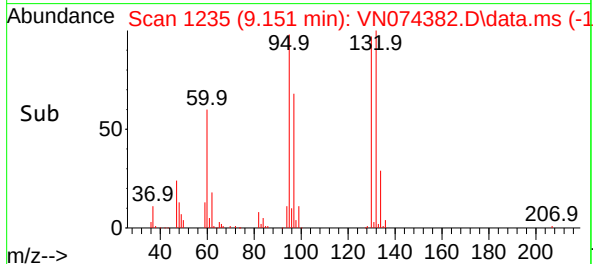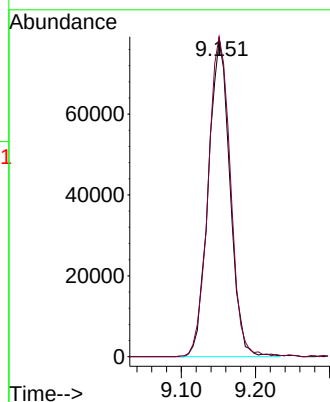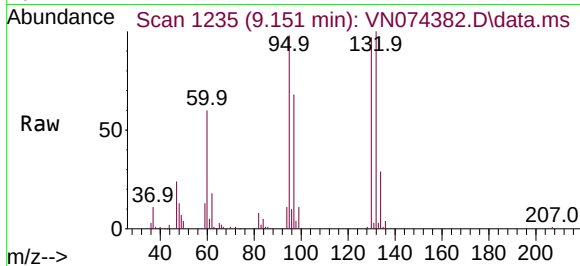

#49
1,4-Dioxane
Concen: 33.521 ug/l
RT: 9.516 min Scan# 1297
Delta R.T. 0.012 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56

Tgt Ion: 88 Resp: 4883
Ion Ratio Lower Upper
88 100
43 0.0 26.9 40.3#
58 75.4 52.7 79.1


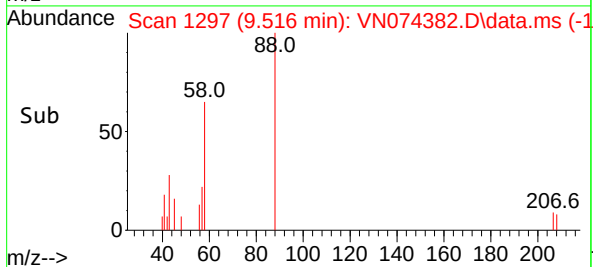
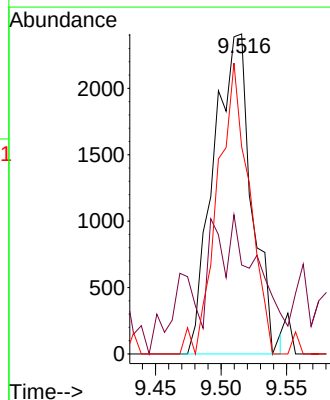
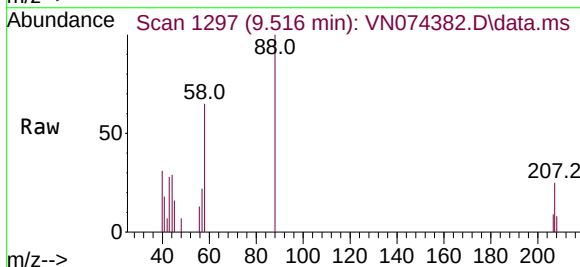




#50
Toluene-d8
Concen: 43.394 ug/l
RT: 10.380 min Scan# 1444
Delta R.T. -0.000 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56




Instrument :
MSVOA_N
ClientSampleId :
MW-10B-40-45-083022


Tgt Ion: 98 Resp: 678572
Ion Ratio Lower Upper
98 100
100 64.0 50.6 76.0

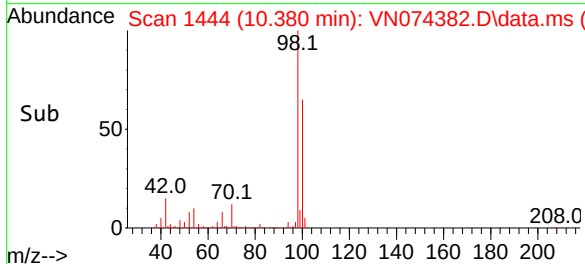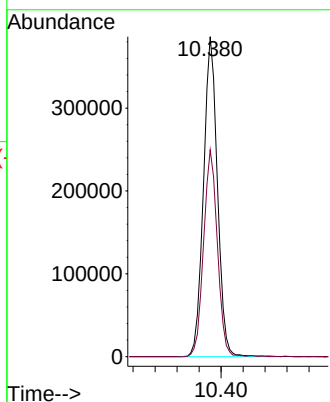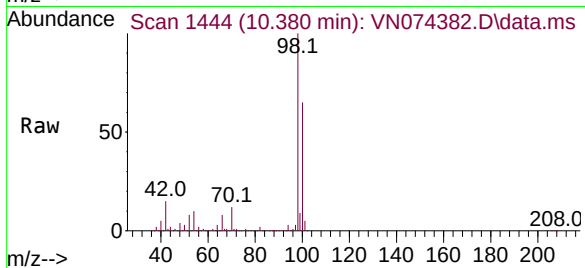

#51
4-Methyl-2-Pentanone
Concen: 0.236 ug/l
RT: 10.269 min Scan# 1425
Delta R.T. -0.000 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56

Tgt Ion: 43 Resp: 2421
Ion Ratio Lower Upper
43 100
58 26.8 29.0 43.6#


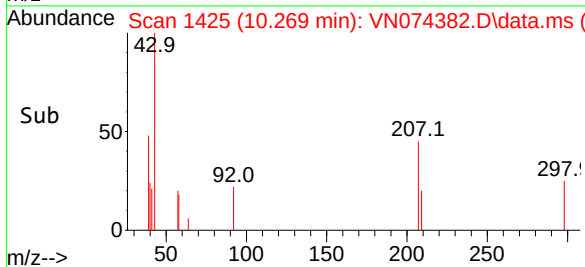
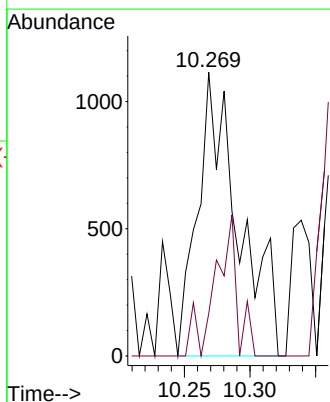
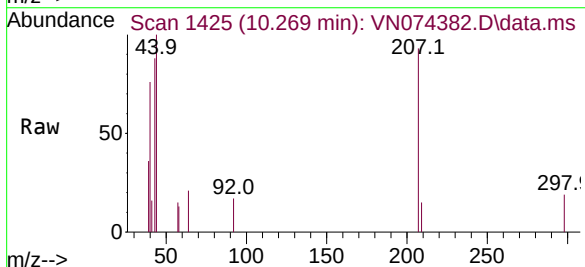




#59
2-Hexanone
Concen: 0.363 ug/l
RT: 11.027 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56




Instrument :
MSVOA_N
ClientSampleId :
MW-10B-40-45-083022


Tgt Ion: 43 Resp: 2876
Ion Ratio Lower Upper
43 100
58 61.4 25.8 77.3

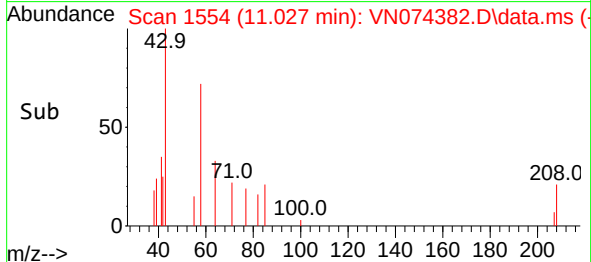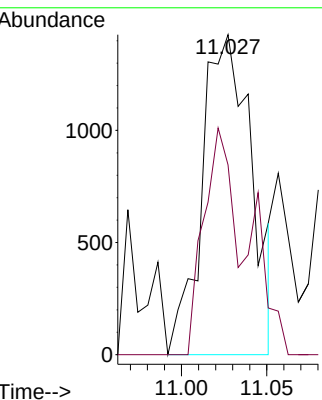

#62
4-Bromofluorobenzene
Concen: 49.291 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. -0.000 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56

Tgt Ion: 95 Resp: 279841
Ion Ratio Lower Upper
95 100
174 75.3 0.0 150.6
176 73.8 0.0 143.4


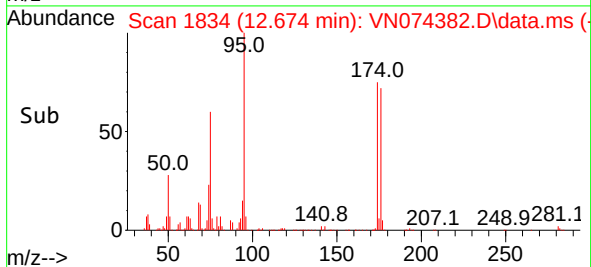
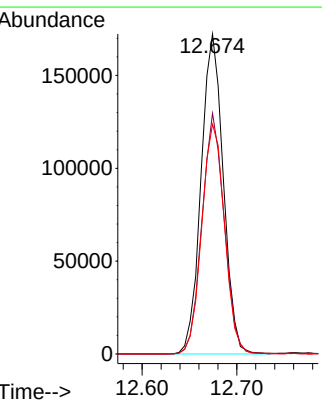
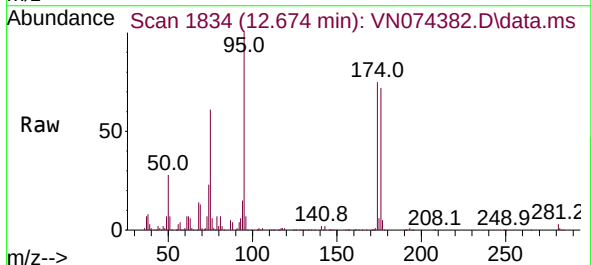


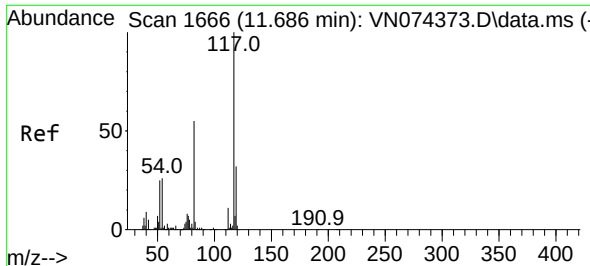

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1
Delta R.T. -0.000 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56




Instrument :
MSVOA_N
ClientSampleId :
MW-10B-40-45-083022


Tgt Ion:117 Resp: 587312
Ion Ratio Lower Upper
117 100
82 58.2 44.3 66.5
119 30.3 25.5 38.3

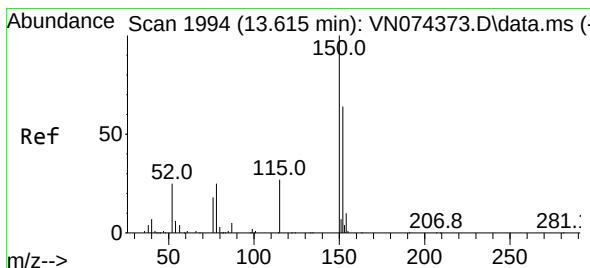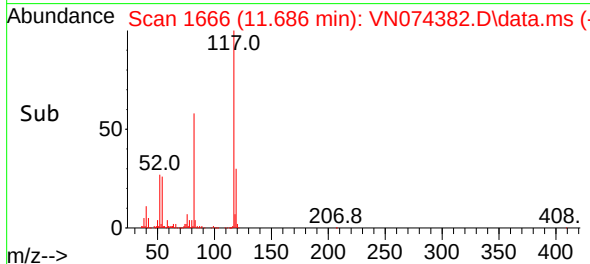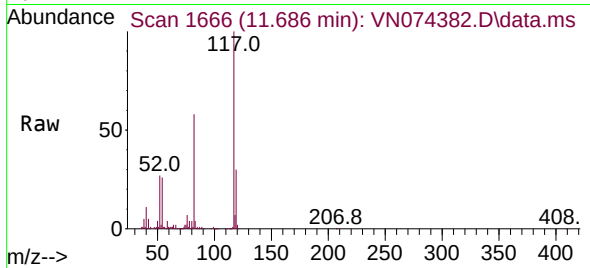

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.615 min Scan# 1994
Delta R.T. 0.000 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56

Tgt Ion:152 Resp: 264939
Ion Ratio Lower Upper
152 100
115 61.4 32.0 96.0
150 155.4 0.0 359.6


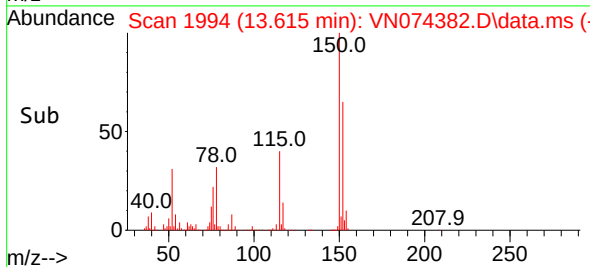

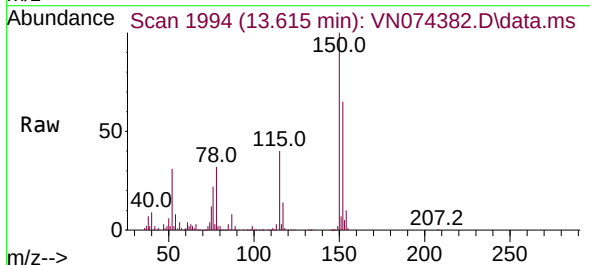


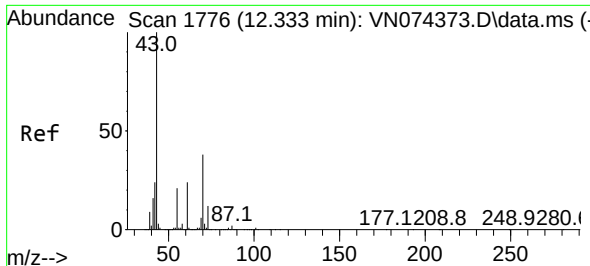

#74
N-amy1 acetate
Concen: Below Cal
RT: 12.327 min Scan# 1775
Delta R.T. -0.006 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56




Instrument :
MSVOA_N
ClientSampleId :
MW-10B-40-45-083022


Tgt Ion: 43	Resp: 1571
Ion Ratio	Lower Upper
43 100	
70 3.7	31.4 47.0#
55 0.0	17.0 25.6#
61 9.3	18.4 27.6#

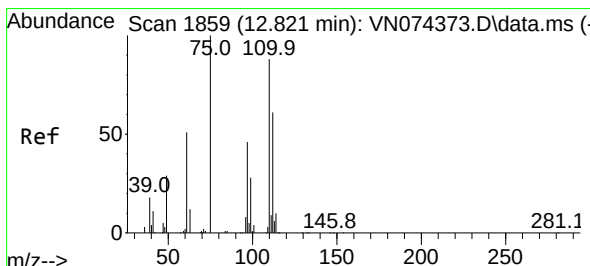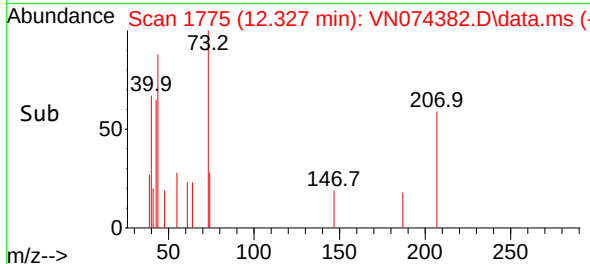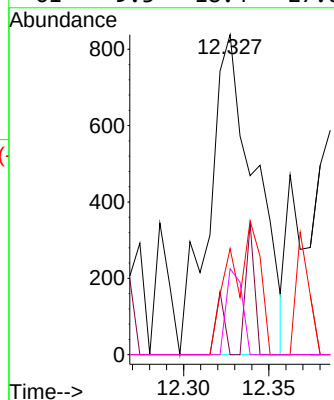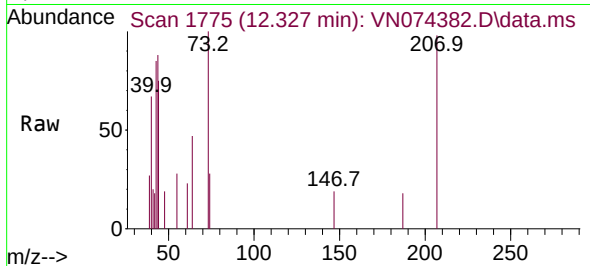

#76
1,2,3-Trichloropropane
Concen: 24.067 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. -0.147 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56

Tgt Ion: 75	Resp: 166685
Ion Ratio	Lower Upper
75 100	
77 1.2	78.9 236.7#


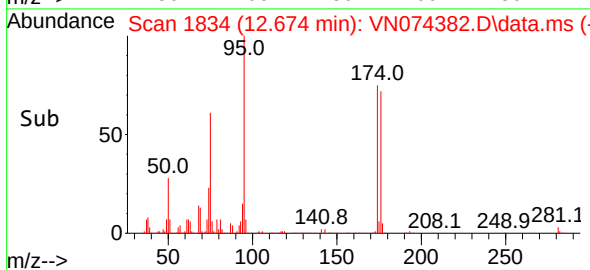
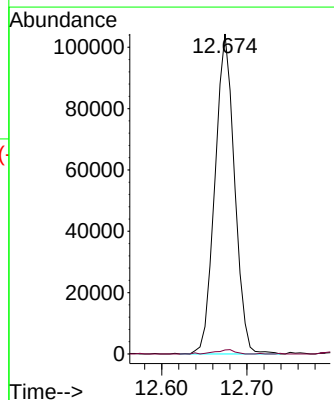
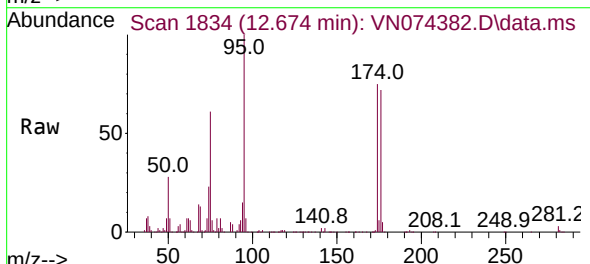




#81
 trans-1,4-Dichloro-2-butene
 Concen: 53.644 ug/l
 RT: 12.674 min Scan# 1816
 Delta R.T. 0.106 min
 Lab File: VN074382.D
 Acq: 09 Sep 2022 18:56




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-10B-40-45-083022


Tgt Ion: 75 Resp: 166685
 Ion Ratio Lower Upper
 75 100
 53 0.1 82.2 123.2#
 89 0.1 37.7 56.5#

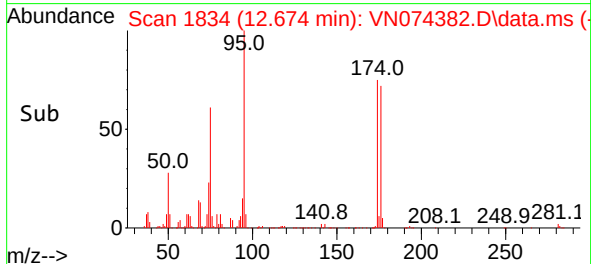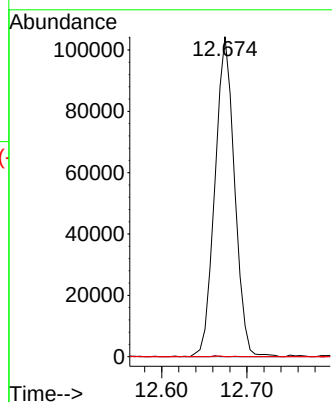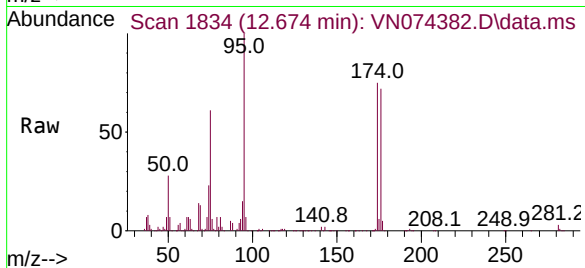

#92
 1,2-Dibromo-3-Chloropropane
 Concen: Below Cal
 RT: 14.562 min Scan# 2155
 Delta R.T. 0.017 min
 Lab File: VN074382.D
 Acq: 09 Sep 2022 18:56

Tgt Ion: 75 Resp: 191
 Ion Ratio Lower Upper
 75 100
 155 213.6 36.6 109.9#
 157 69.1 46.2 138.5


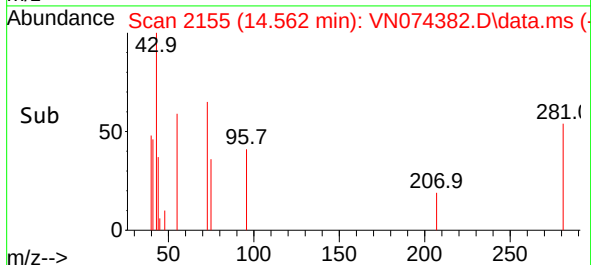

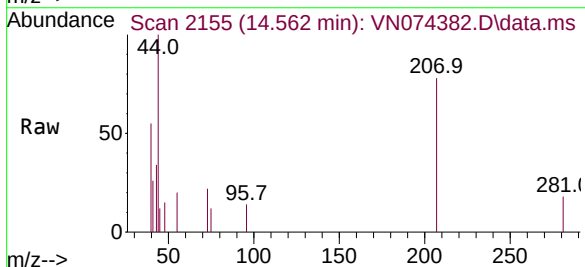


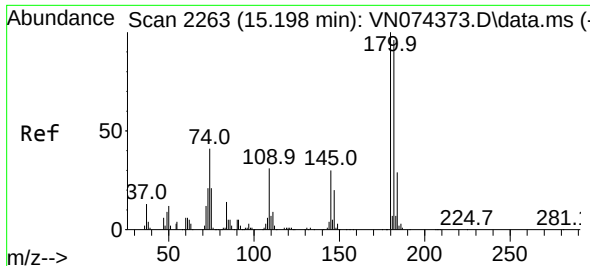

#93
1,2,4-Trichlorobenzene
Concen: 0.361 ug/l
RT: 15.204 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56




Instrument :
MSVOA_N
ClientSampleId :
MW-10B-40-45-083022


Tgt Ion	Ratio	Lower	Upper
180	100		
182	120.5	47.4	142.2
145	35.8	16.1	48.2

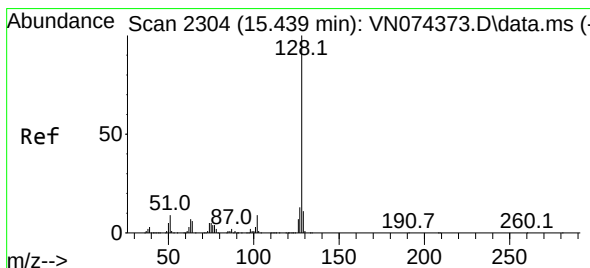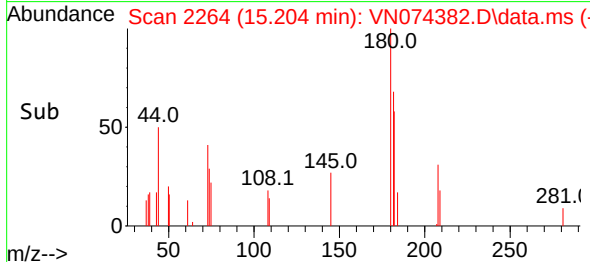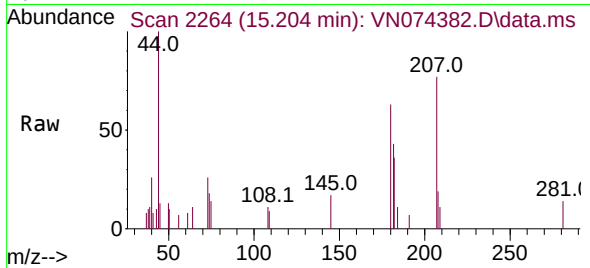

#95
Naphthalene
Concen: 0.590 ug/l
RT: 15.439 min Scan# 2304
Delta R.T. -0.000 min
Lab File: VN074382.D
Acq: 09 Sep 2022 18:56


Tgt Ion	Ratio	Lower	Upper
128	100		
127	3.8	10.6	16.0#
129	11.0	8.8	13.2

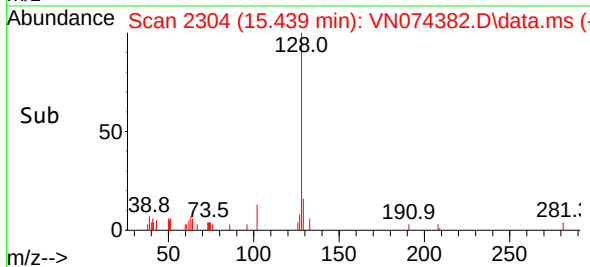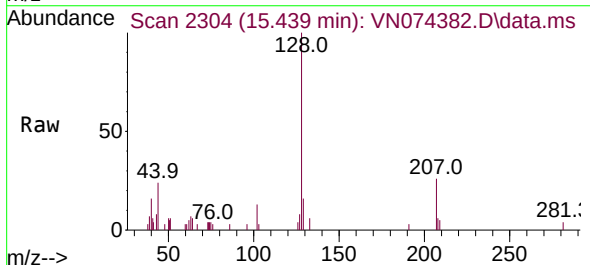



#96
 1,2,3-Trichlorobenzene
 Concen: 0.391 ug/l
 RT: 15.633 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN074382.D
 Acq: 09 Sep 2022 18:56

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-10B-40-45-083022

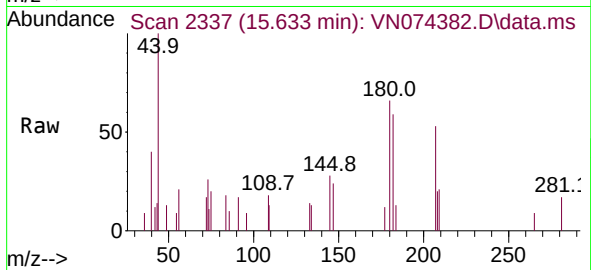

Tgt Ion:	180	Resp:	2144
Ion	Ratio	Lower	Upper
180	100		
182	120.1	47.6	142.8
145	20.3	17.3	52.0

