

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090922\
 Data File : VN074400.D
 Acq On : 10 Sep 2022 02:15
 Operator : JC\MD
 Sample : N4502-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SLUDGE-DRUM-1-4-COMP

Quant Time: Sep 10 07:31:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090922W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 10 06:10:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.016	168	321013	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	576549	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	576481	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.616	152	259938	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	230270	41.460	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	82.920%		
35) Dibromofluoromethane	7.951	113	190210	48.869	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	97.740%		
50) Toluene-d8	10.381	98	662086	43.656	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	87.320%		
62) 4-Bromofluorobenzene	12.674	95	267414	48.565	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	97.140%		
Target Compounds						Qvalue
3) Chloromethane	2.263	50	2116	Below Cal		94
6) Chloroethane	2.687	64	34424	4.022 ug/l #		51
9) 1,1,2-Trichlorotrifluo...	4.122	101	836	0.203 ug/l #		36
11) Tert butyl alcohol	5.287	59	629	0.433 ug/l #		71
13) Acrolein	3.999	56	593	0.615 ug/l #		69
16) Acetone	4.216	43	63715	21.249 ug/l		90
18) Methyl Acetate	4.775	43	8771	0.992 ug/l #		70
20) Methylene Chloride	5.010	84	14658	1.884 ug/l #		95
25) 2-Butanone	7.257	43	11455	2.276 ug/l #		76
28) Bromochloromethane	7.740	49	69	Below Cal #		20
29) Tetrahydrofuran	7.616	42	1048	0.315 ug/l #		90
31) Cyclohexane	8.022	56	9894	1.120 ug/l #		45
36) 1,1-Dichloropropene	8.022	75	29490	4.599 ug/l #		51
37) Ethyl Acetate	7.340	43	51921	5.582 ug/l		97
38) Carbon Tetrachloride	8.016	117	34571	5.222 ug/l #		15
43) Isopropyl Acetate	8.492	43	236927	15.575 ug/l #		90
44) Trichloroethene	9.151	130	10917	2.480 ug/l		96
45) 1,2-Dichloropropane	9.557	63	2528	0.485 ug/l #		44
48) Methyl methacrylate	9.492	41	9595	1.431 ug/l #		48
49) 1,4-Dioxane	9.510	88	228	1.614 ug/l #		25
51) 4-Methyl-2-Pentanone	10.275	43	22888	2.301 ug/l #		78
54) cis-1,3-Dichloropropene	10.186	75	78503	9.385 ug/l #		65
56) Ethyl methacrylate	10.816	69	2271	0.267 ug/l #		1
57) 1,3-Dichloropropane	11.033	76	7640	0.873 ug/l #		43
59) 2-Hexanone	11.033	43	94114	12.259 ug/l #		56
71) Bromoform	12.669	173	1040	0.256 ug/l #		29
74) N-amyl acetate	12.327	43	1223	Below Cal #		48
76) 1,2,3-Trichloropropane	12.674	75	166714	24.534 ug/l #		1
81) trans-1,4-Dichloro-2-b...	12.674	75	166714	54.686 ug/l #		9
92) 1,2-Dibromo-3-Chloropr...	14.586	75	66	Below Cal #		8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090922\
Data File : VN074400.D
Acq On : 10 Sep 2022 02:15
Operator : JC\MD
Sample : N4502-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-DRUM-1-4-COMP

Quant Time: Sep 10 07:31:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090922W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 10 06:10:29 2022
Response via : Initial Calibration

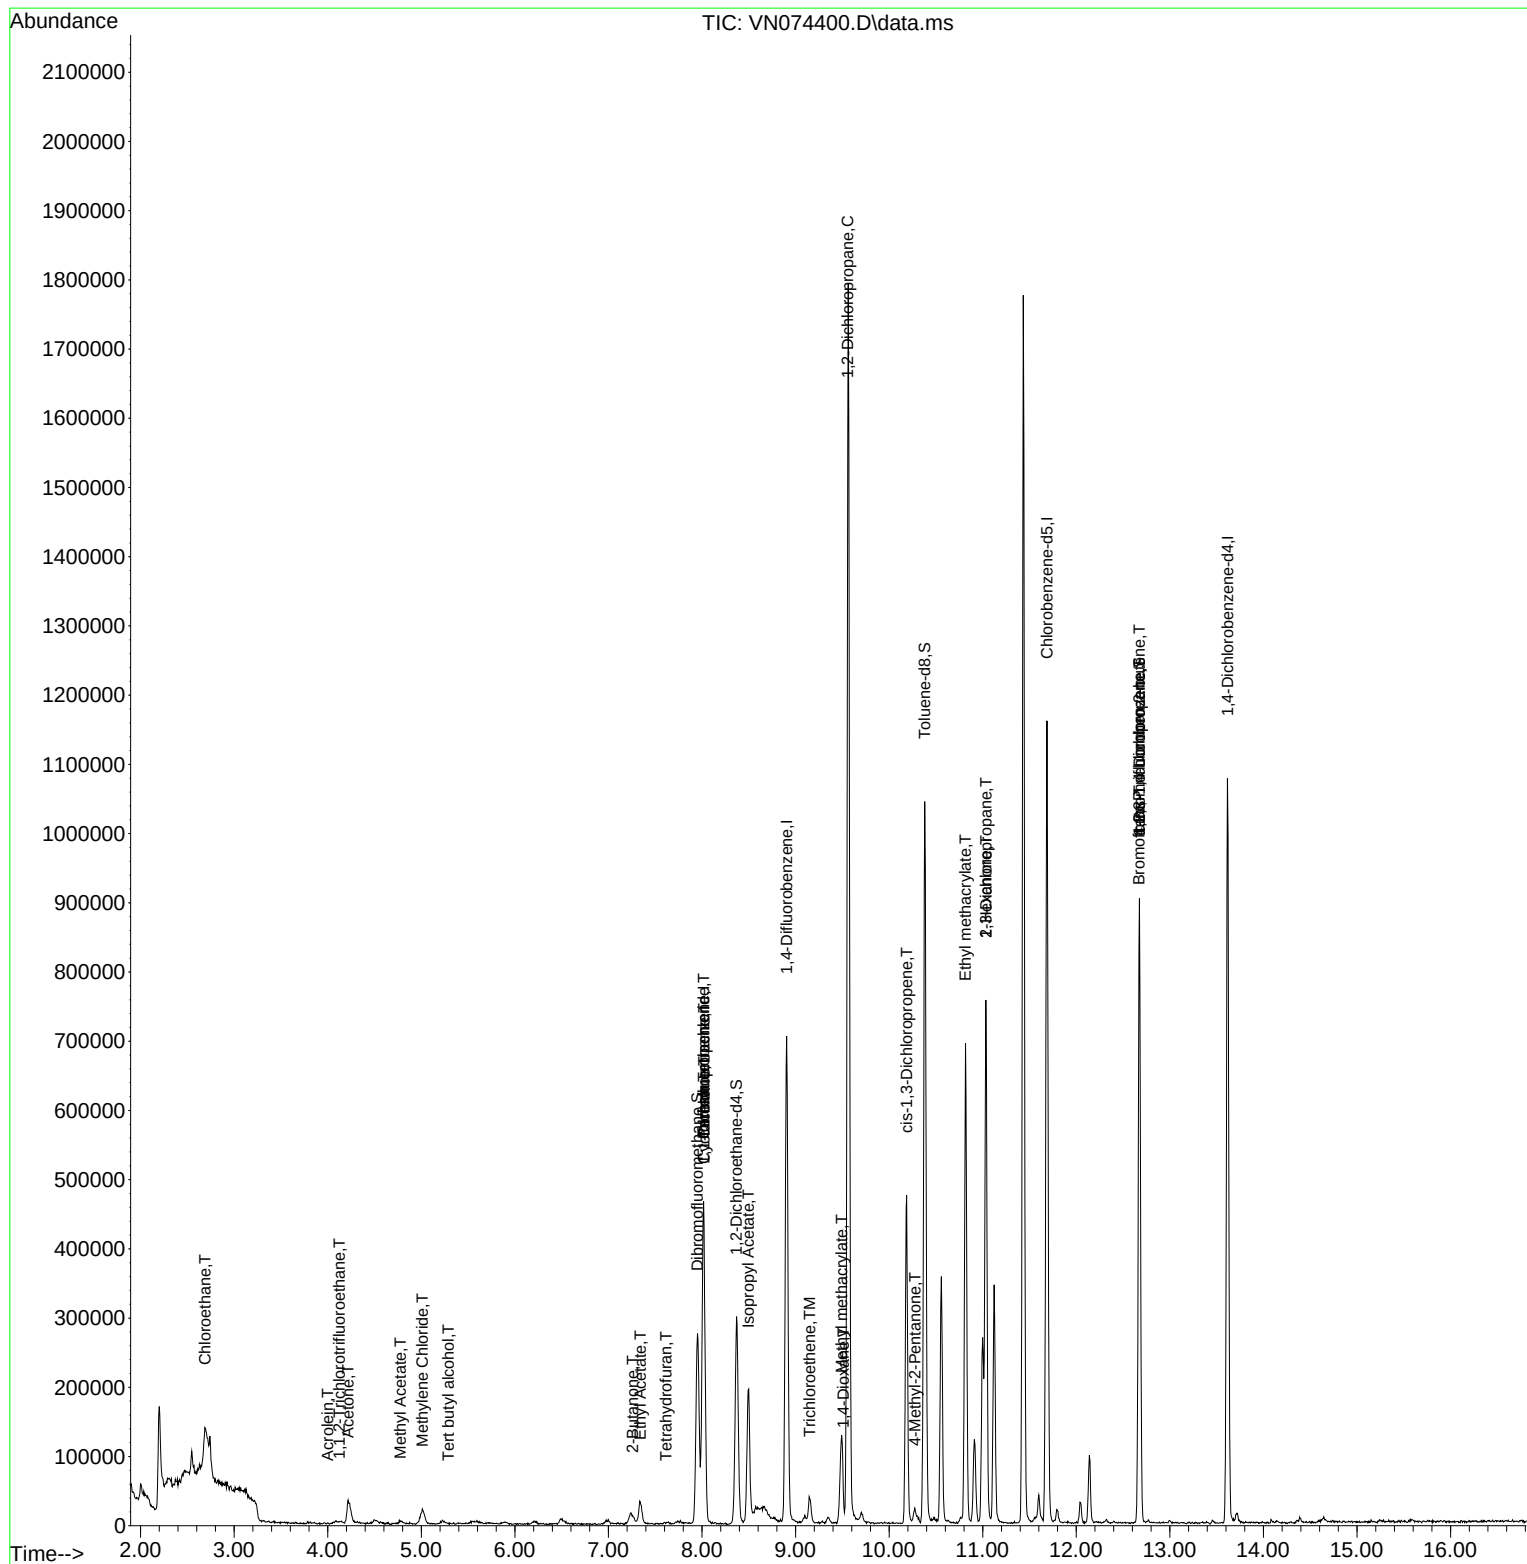



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.016 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN074400.D

Acq: 10 Sep 2022 02:15

Instrument :

MSVOA_N

ClientSampleId :





SLUDGE-DRUM-1-4-COMP

Tgt Ion:168 Resp: 321013

Ion Ratio Lower Upper

168 100

99 58.9 52.8 79.2

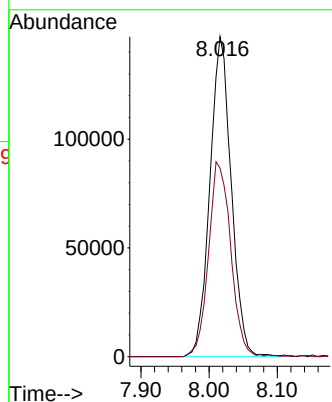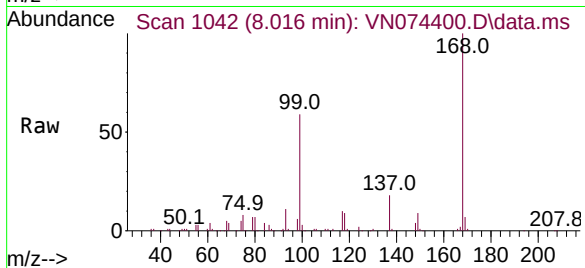

#3

Chloromethane

Concen: Below Cal

RT: 2.263 min Scan# 64

Delta R.T. -0.006 min

Lab File: VN074400.D




Acq: 10 Sep 2022 02:15


Tgt Ion: 50 Resp: 2116

Ion Ratio Lower Upper

50 100

52 33.6 24.1 36.1


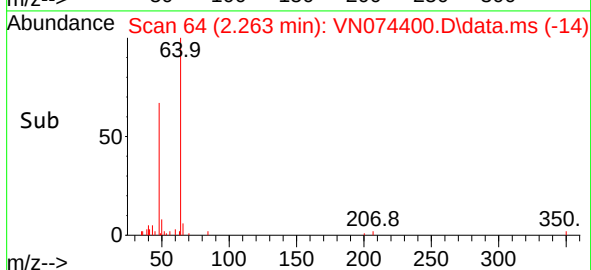

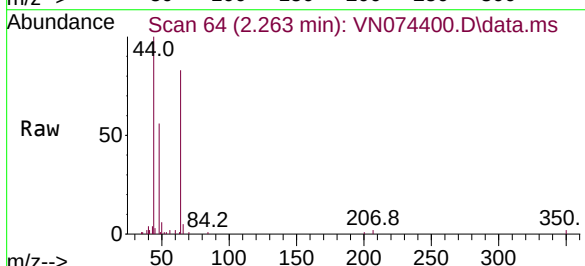




#6
Chloroethane
Concen: 4.022 ug/l
RT: 2.687 min Scan# 11
Delta R.T. -0.259 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15




Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-DRUM-1-4-COMP


Tgt Ion: 64 Resp: 34424
Ion Ratio Lower Upper
64 100
66 5.2 26.5 39.7#

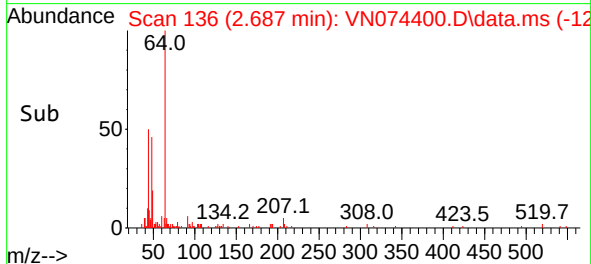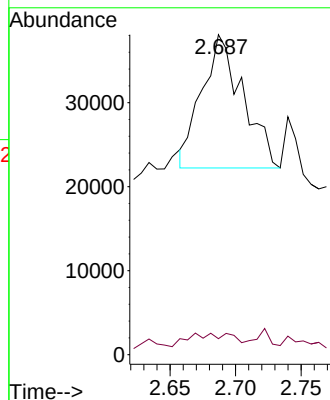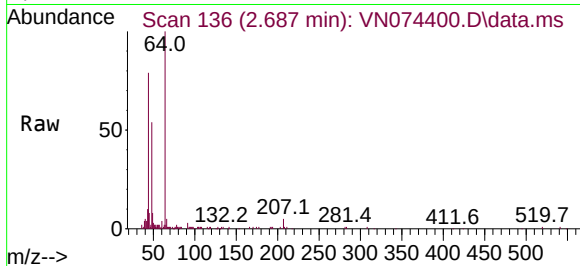

#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.203 ug/l
RT: 4.122 min Scan# 380
Delta R.T. -0.012 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15

Tgt Ion: 101 Resp: 836
Ion Ratio Lower Upper
101 100
85 140.3 39.5 59.3#
151 85.9 57.8 86.6

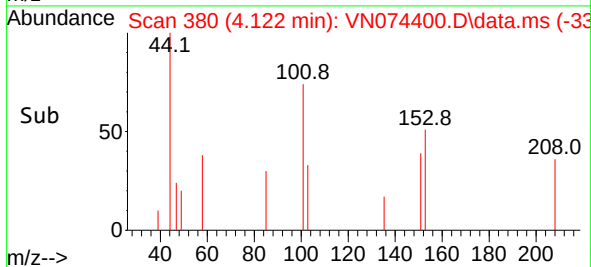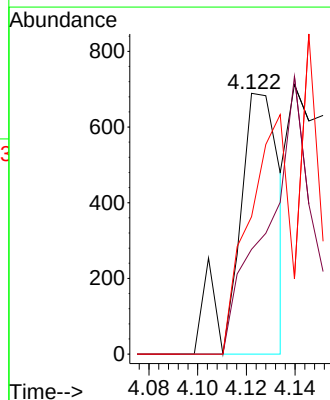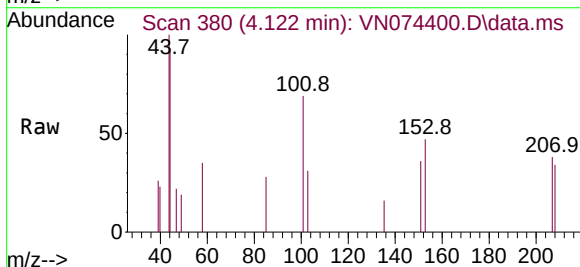



#11

Tert butyl alcohol

Concen: 0.433 ug/l

RT: 5.287 min Scan# 51

Delta R.T. 0.000 min

Lab File: VN074400.D

Acq: 10 Sep 2022 02:15

Instrument :

MSVOA_N

ClientSampleId :





SLUDGE-DRUM-1-4-COMP

Tgt Ion: 59 Resp: 629

Ion Ratio Lower Upper

59 100

57 0.0 8.8 13.2#

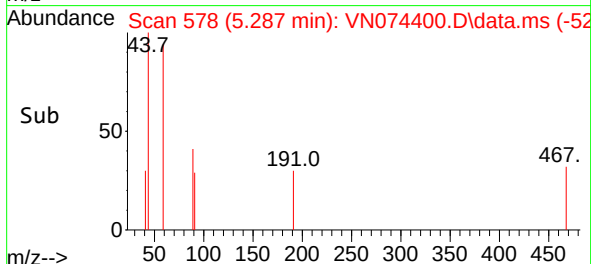

#13

Acrolein

Concen: 0.615 ug/l

RT: 3.999 min Scan# 359

Delta R.T. 0.024 min

Lab File: VN074400.D




Acq: 10 Sep 2022 02:15


Tgt Ion: 56 Resp: 593

Ion Ratio Lower Upper

56 100

55 44.7 56.2 84.4#


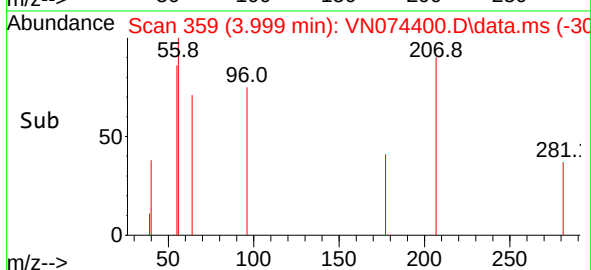






#16
Acetone
Concen: 21.249 ug/l
RT: 4.216 min Scan# 396
Delta R.T. -0.006 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15




Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-DRUM-1-4-COMP


Tgt Ion: 43 Resp: 63715
Ion Ratio Lower Upper
43 100
58 33.7 22.7 34.1

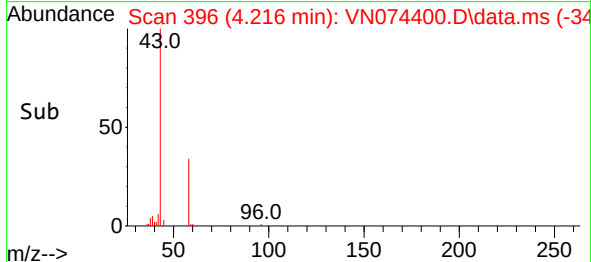

#18
Methyl Acetate
Concen: 0.992 ug/l
RT: 4.775 min Scan# 491
Delta R.T. 0.006 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15

Tgt Ion: 43 Resp: 8771
Ion Ratio Lower Upper
43 100
74 6.7 16.7 25.1#


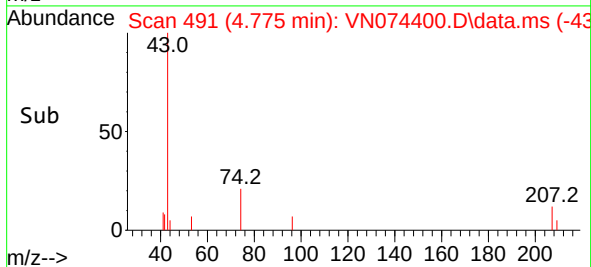

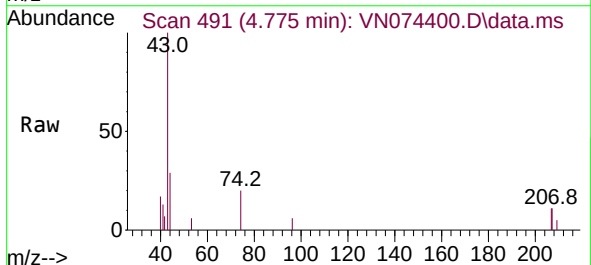




#20
Methylene Chloride
Concen: 1.884 ug/l
RT: 5.010 min Scan# 51
Delta R.T. 0.000 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15




Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-DRUM-1-4-COMP


Tgt Ion: 84 Resp: 14658
Ion Ratio Lower Upper
84 100
49 135.4 108.2 162.4
51 40.6 34.3 51.5
86 72.7 48.2 72.2#

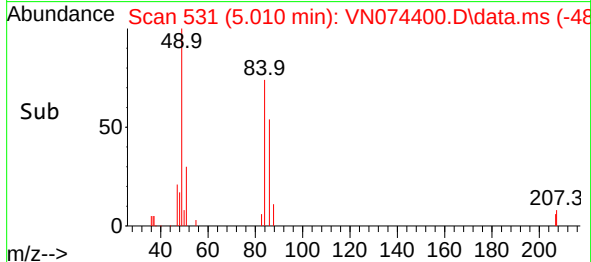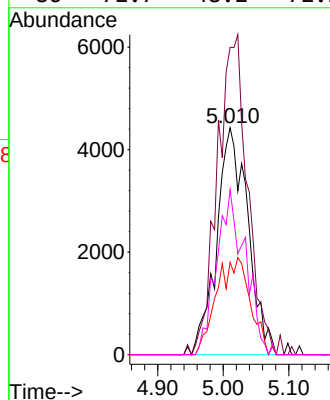

#25
2-Butanone
Concen: 2.276 ug/l
RT: 7.257 min Scan# 913
Delta R.T. 0.000 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15

Tgt Ion: 43 Resp: 11455
Ion Ratio Lower Upper
43 100
72 35.6 18.9 28.3#


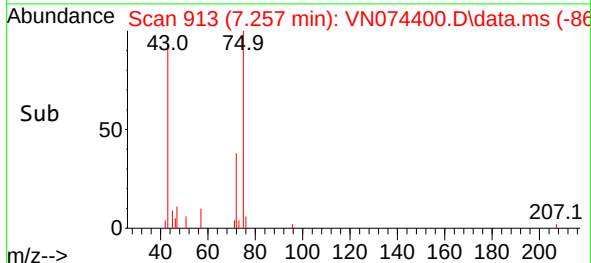
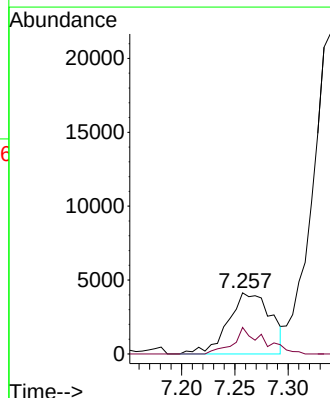
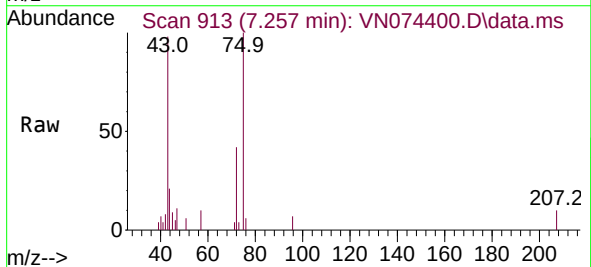




#28
Bromochloromethane
Concen: Below Cal
RT: 7.740 min Scan# 91
Delta R.T. 0.159 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15




Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-DRUM-1-4-COMP


Tgt Ion: 49 Resp: 69
Ion Ratio Lower Upper
49 100
129 0.0 0.0 2.2
130 0.0 50.0 75.0#

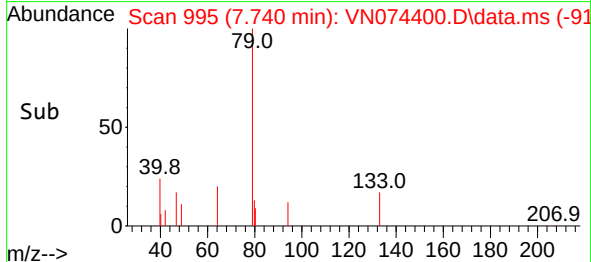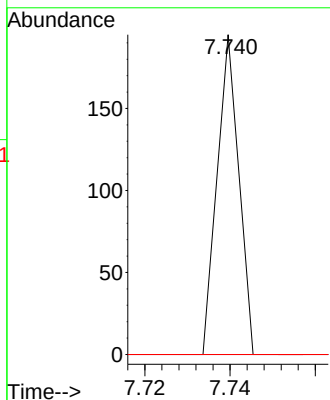

#29
Tetrahydrofuran
Concen: 0.315 ug/l
RT: 7.616 min Scan# 974
Delta R.T. 0.006 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15

Tgt Ion: 42 Resp: 1048
Ion Ratio Lower Upper
42 100
72 49.7 32.7 49.1#
71 34.8 31.0 46.6


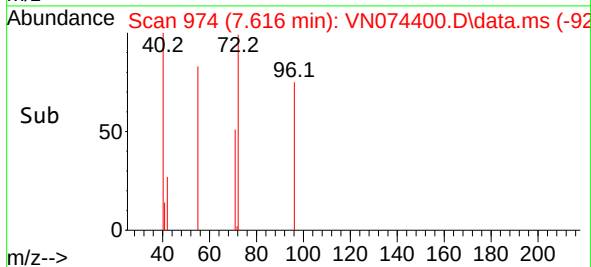
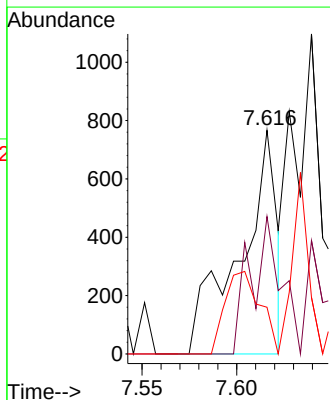
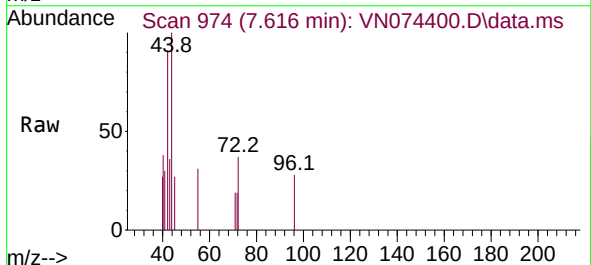




#31
Cyclohexane
Concen: 1.120 ug/l
RT: 8.022 min Scan# 1043
Delta R.T. -0.006 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15




Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-DRUM-1-4-COMP


Tgt Ion: 56 Resp: 9894
Ion Ratio Lower Upper
56 100
69 94.7 23.0 34.4#
84 111.2 66.3 99.5#

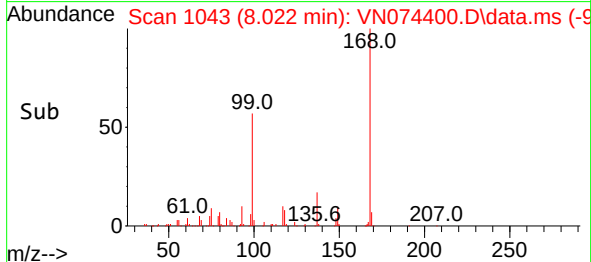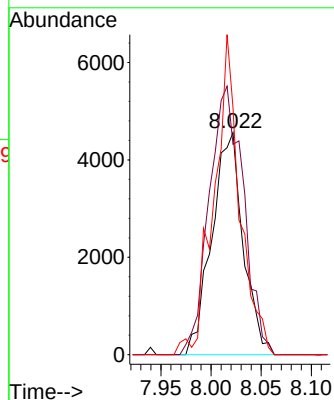

#33
1,2-Dichloroethane-d4
Concen: 41.460 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. 0.000 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15

Tgt Ion: 65 Resp: 230270
Ion Ratio Lower Upper
65 100
67 51.3 0.0 102.4

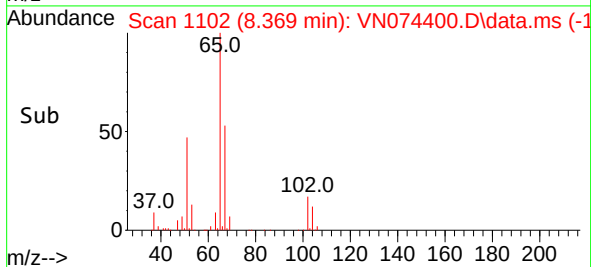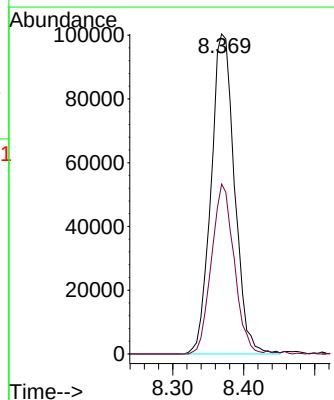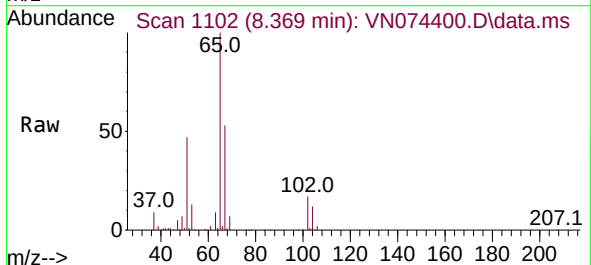

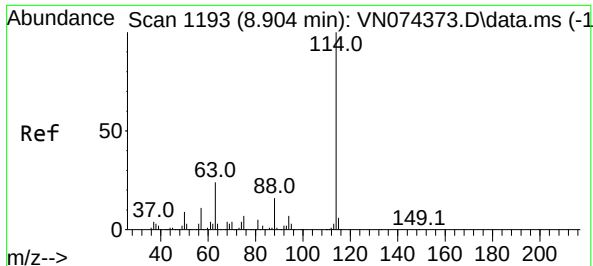

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.000 min

Lab File: VN074400.D

Acq: 10 Sep 2022 02:15

Instrument :

MSVOA_N

ClientSampleId :

SLUDGE-DRUM-1-4-COMP





Tgt Ion:114 Resp: 576549

Ion Ratio Lower Upper

114 100

63 24.5 0.0 47.6

88 16.5 0.0 31.4

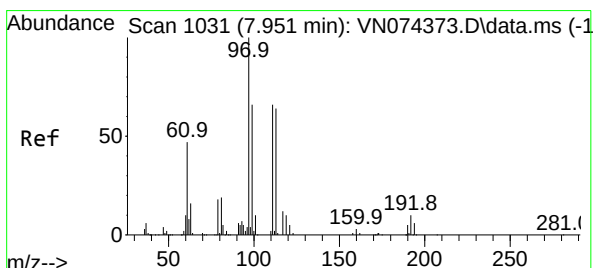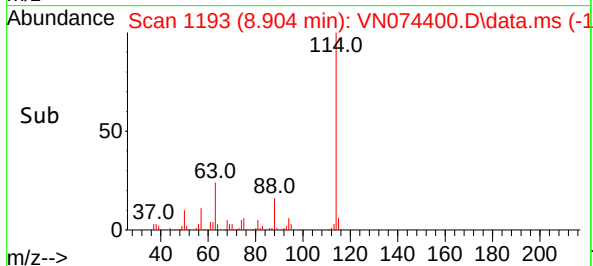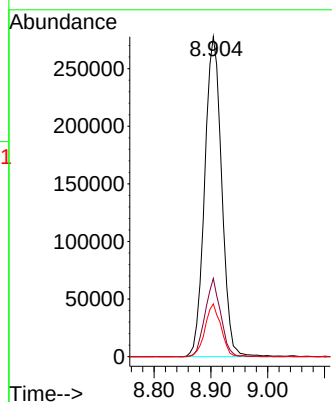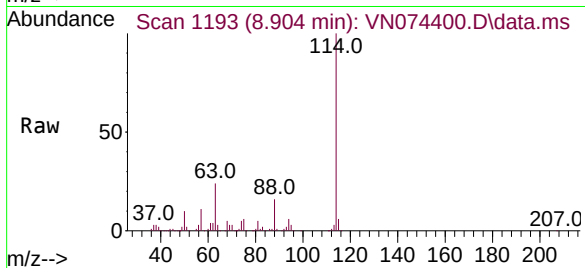

#35

Dibromofluoromethane

Concen: 48.869 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN074400.D

Acq: 10 Sep 2022 02:15




Tgt Ion:113 Resp: 190210


Ion Ratio Lower Upper

113 100

111 103.1 83.0 124.4

192 17.9 13.7 20.5

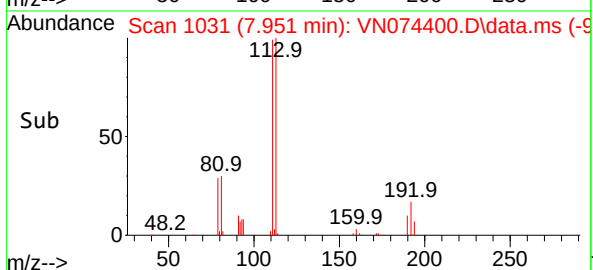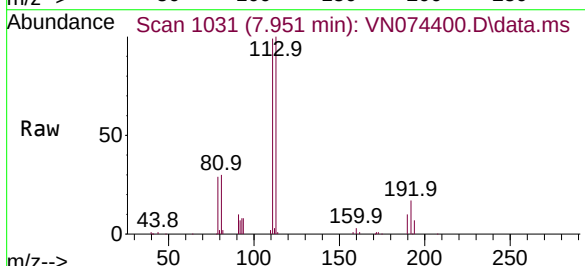

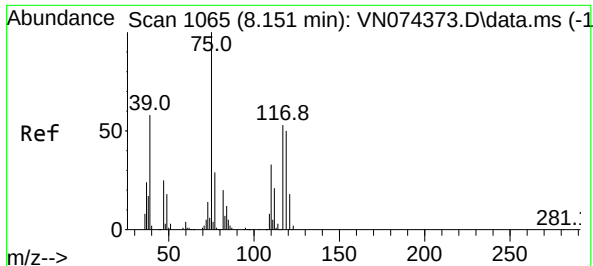

#36

1,1-Dichloropropene

Concen: 4.599 ug/l

RT: 8.022 min Scan# 1

Delta R.T. -0.129 min

Lab File: VN074400.D


Acq: 10 Sep 2022 02:15

Instrument :

MSVOA_N

ClientSampleId :

SLUDGE-DRUM-1-4-COMP

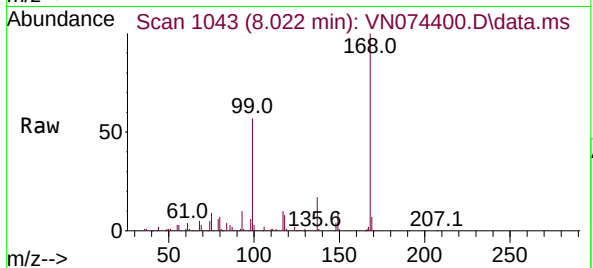




Tgt Ion: 75 Resp: 29490

Ion Ratio Lower Upper

75 100

110 9.5 16.4 49.1#

77 0.0 25.4 38.2#

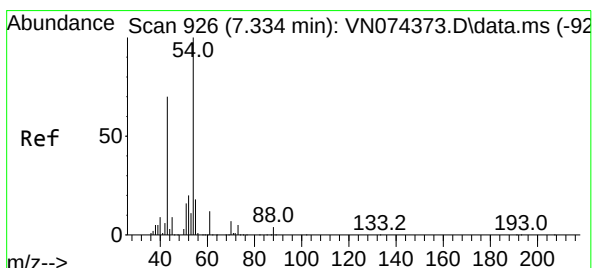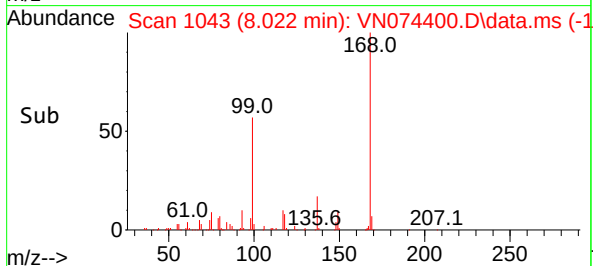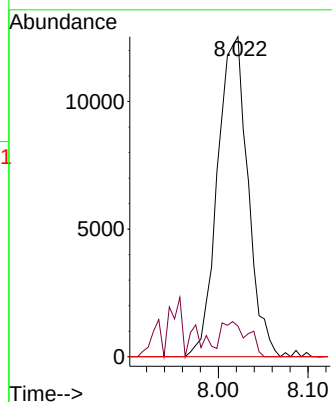

#37

Ethyl Acetate

Concen: 5.582 ug/l

RT: 7.340 min Scan# 927

Delta R.T. 0.006 min

Lab File: VN074400.D

Acq: 10 Sep 2022 02:15




Tgt Ion: 43 Resp: 51921


Ion Ratio Lower Upper

43 100

61 12.1 11.1 16.7

70 9.1 7.2 10.8


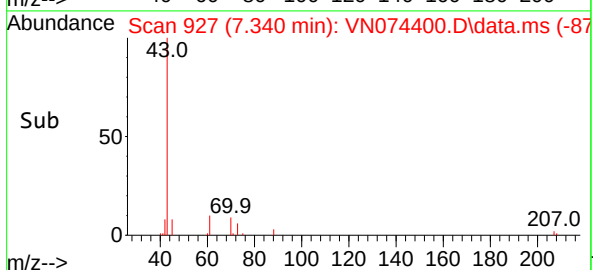
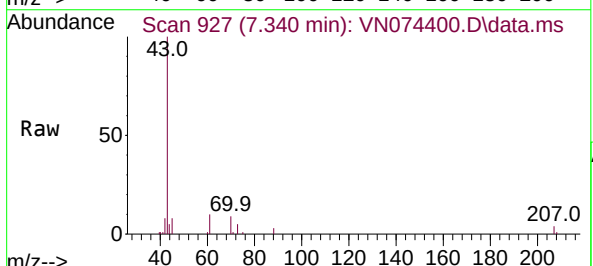



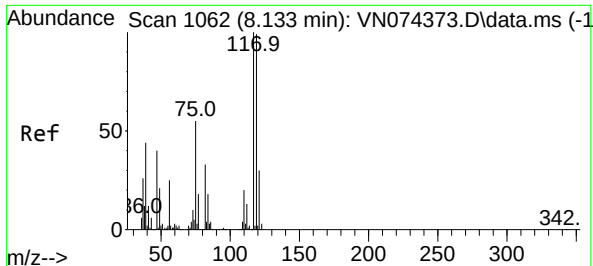

#38
Carbon Tetrachloride
Concen: 5.222 ug/l
RT: 8.016 min Scan# 117
Delta R.T. -0.117 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15




Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-DRUM-1-4-COMP


Tgt Ion:117 Resp: 34571
Ion Ratio Lower Upper
117 100
119 5.6 78.8 118.2#
121 0.0 24.1 36.1#

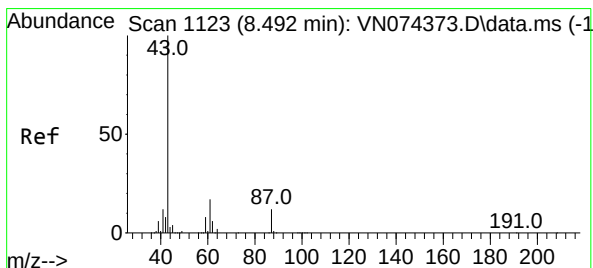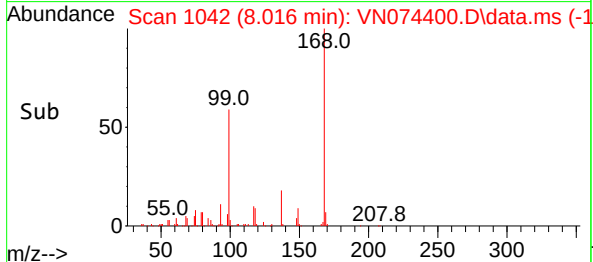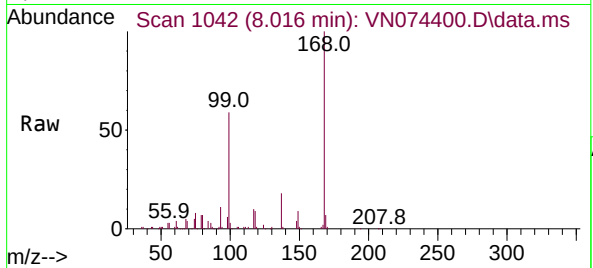

#43
Isopropyl Acetate
Concen: 15.575 ug/l
RT: 8.492 min Scan# 1123
Delta R.T. 0.000 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15

Tgt Ion: 43 Resp: 236927
Ion Ratio Lower Upper
43 100
61 16.4 18.6 27.8#
87 11.0 9.4 14.2


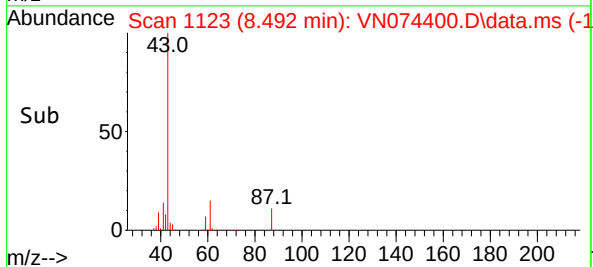

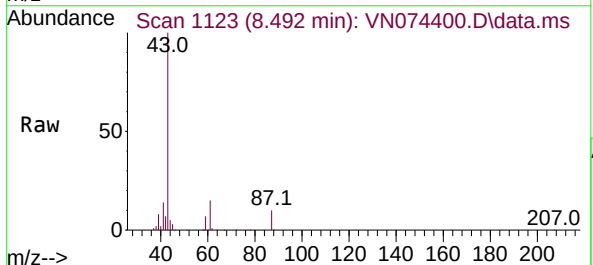


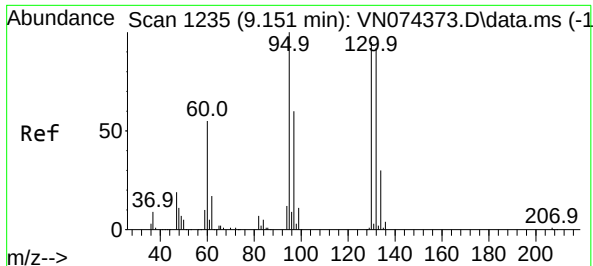

#44
Trichloroethene
Concen: 2.480 ug/l
RT: 9.151 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15




Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-DRUM-1-4-COMP


Tgt Ion:130 Resp: 10917
Ion Ratio Lower Upper
130 100
95 108.8 0.0 210.0

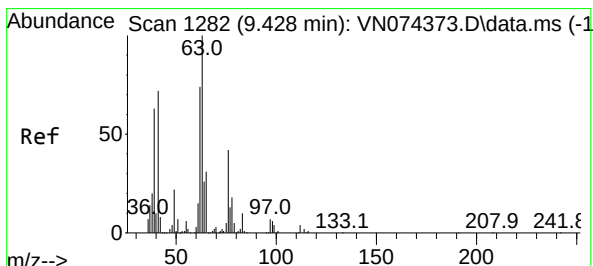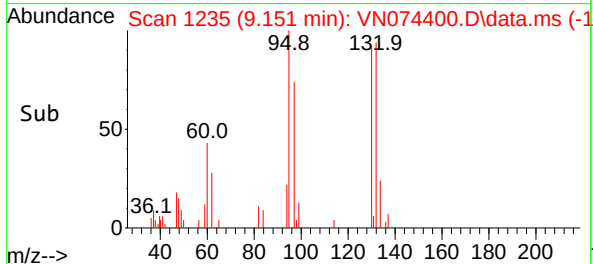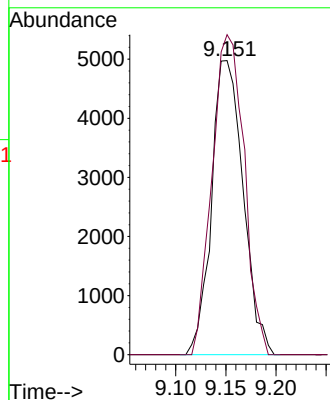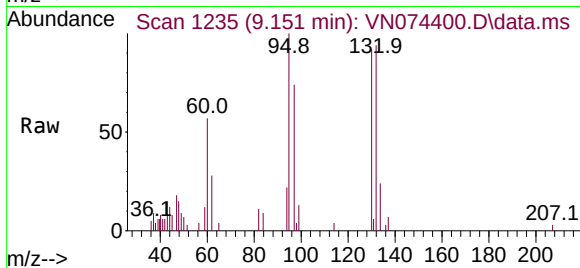

#45
1,2-Dichloropropane
Concen: 0.485 ug/l
RT: 9.557 min Scan# 1304
Delta R.T. 0.130 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15

Tgt Ion: 63 Resp: 2528
Ion Ratio Lower Upper
63 100
65 0.0 24.6 36.8#


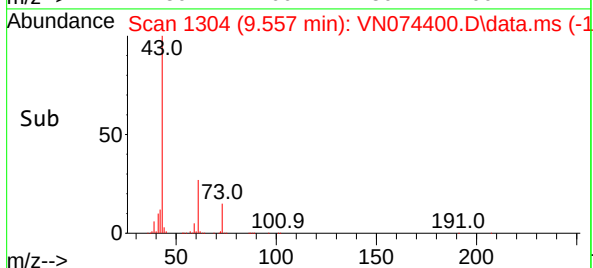
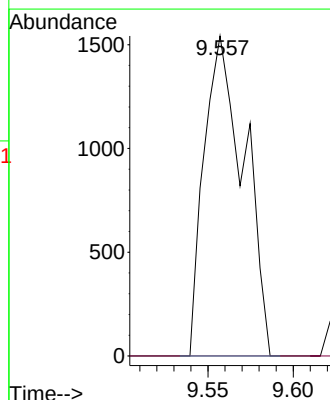
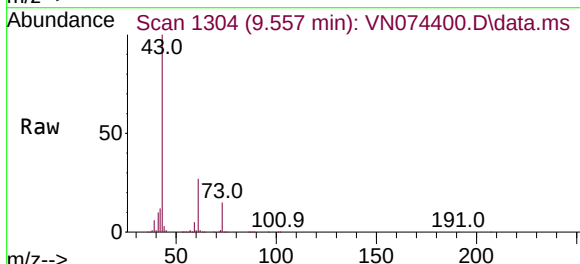




#48
Methyl methacrylate
Concen: 1.431 ug/l
RT: 9.492 min Scan# 1293
Delta R.T. -0.006 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15




Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-DRUM-1-4-COMP


Tgt Ion: 41 Resp: 9595
Ion Ratio Lower Upper
41 100
69 1.0 67.6 101.4#
39 68.7 58.2 87.4

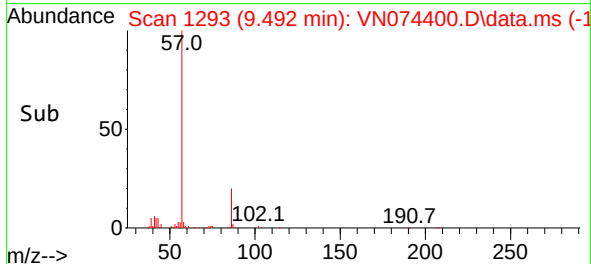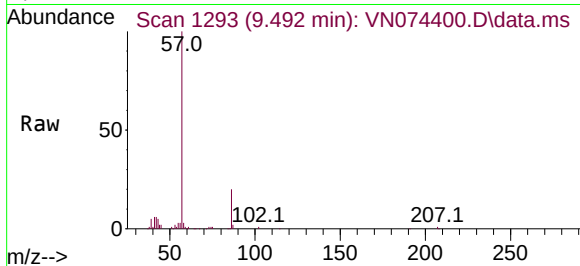

#49
1,4-Dioxane
Concen: 1.614 ug/l
RT: 9.510 min Scan# 1296
Delta R.T. 0.006 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15

Tgt Ion: 88 Resp: 228
Ion Ratio Lower Upper
88 100
43 0.0 26.9 40.3#
58 0.0 52.7 79.1#


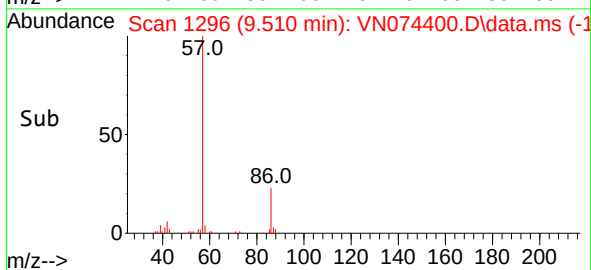

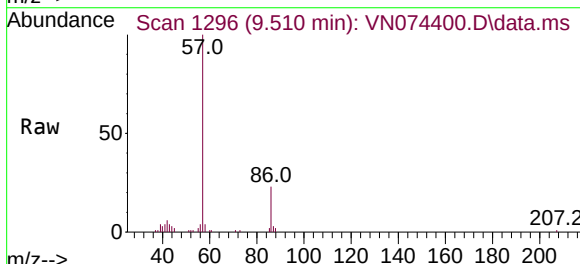




#50
Toluene-d8
Concen: 43.656 ug/l
RT: 10.381 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15




Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-DRUM-1-4-COMP


Tgt Ion: 98 Resp: 662086
Ion Ratio Lower Upper
98 100
100 65.5 50.6 76.0

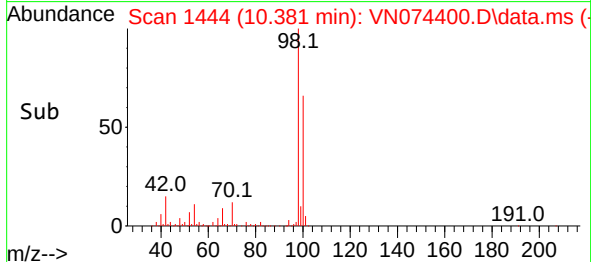

#51
4-Methyl-2-Pentanone
Concen: 2.301 ug/l
RT: 10.275 min Scan# 1426
Delta R.T. 0.006 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15

Tgt Ion: 43 Resp: 22888
Ion Ratio Lower Upper
43 100
58 23.5 29.0 43.6#


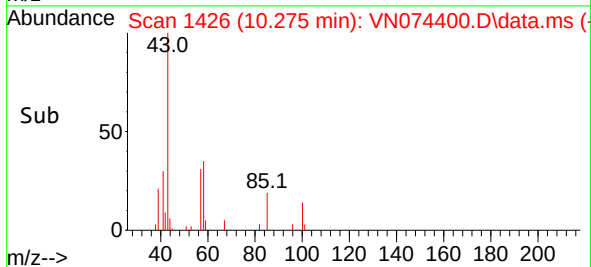

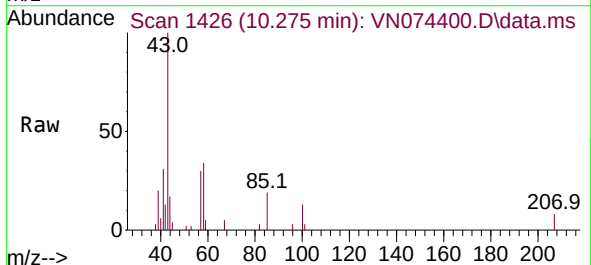




#54
 cis-1,3-Dichloropropene
 Concen: 9.385 ug/l
 RT: 10.186 min Scan# 1401
 Delta R.T. 0.059 min
 Lab File: VN074400.D
 Acq: 10 Sep 2022 02:15




Instrument :
 MSVOA_N
 ClientSampleId :
 SLUDGE-DRUM-1-4-COMP


Tgt Ion: 75 Resp: 78503
 Ion Ratio Lower Upper
 75 100
 77 0.8 24.5 36.7#
 39 41.1 48.0 72.0#

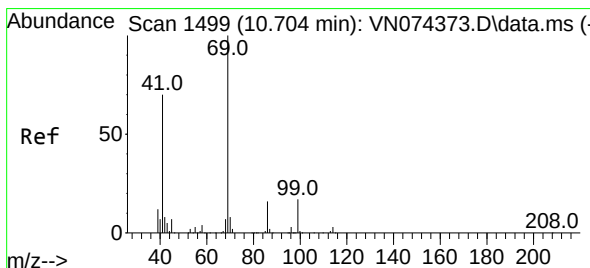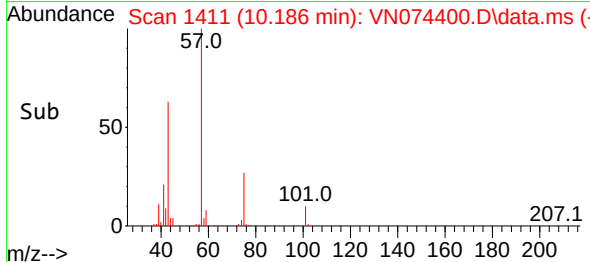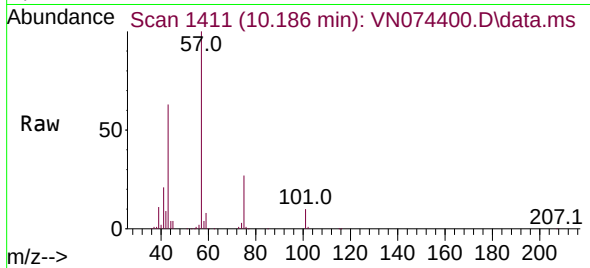

#56
 Ethyl methacrylate
 Concen: 0.267 ug/l
 RT: 10.816 min Scan# 1518
 Delta R.T. 0.112 min
 Lab File: VN074400.D
 Acq: 10 Sep 2022 02:15

Tgt Ion: 69 Resp: 2271
 Ion Ratio Lower Upper
 69 100
 41 5930.5 56.6 85.0#
 39 2868.7 37.4 56.2#

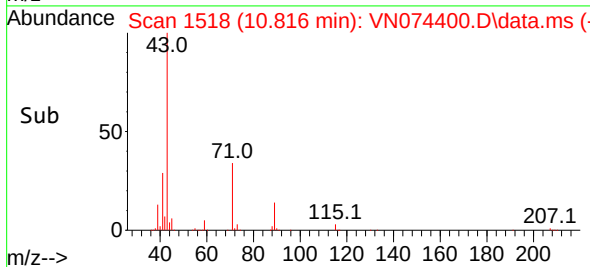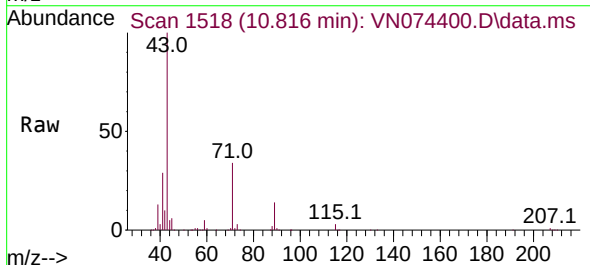



#57

1,3-Dichloropropane

Concen: 0.873 ug/l

RT: 11.033 min Scan# 1555

Delta R.T. 0.047 min

Lab File: VN074400.D

Acq: 10 Sep 2022 02:15

Instrument :

MSVOA_N

ClientSampleId :





SLUDGE-DRUM-1-4-COMP

Tgt Ion: 76 Resp: 7640

Ion Ratio Lower Upper

76 100

78 0.0 25.0 37.4#

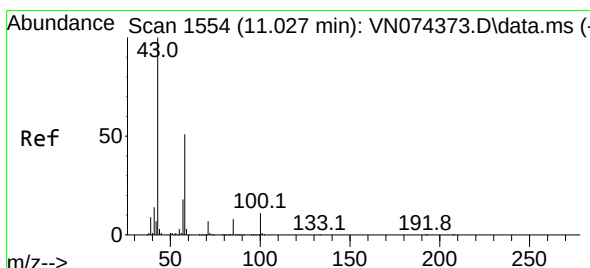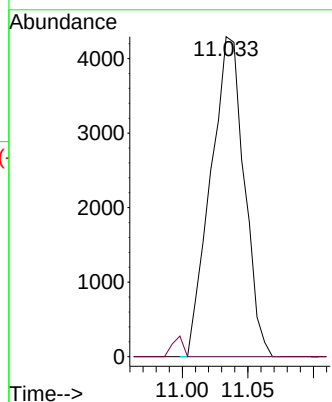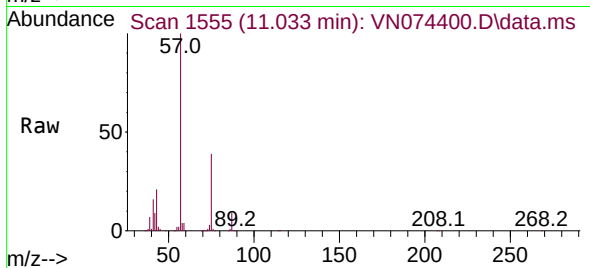

#59

2-Hexanone

Concen: 12.259 ug/l

RT: 11.033 min Scan# 1555

Delta R.T. 0.006 min

Lab File: VN074400.D




Acq: 10 Sep 2022 02:15


Tgt Ion: 43 Resp: 94114

Ion Ratio Lower Upper

43 100

58 20.9 25.8 77.3#


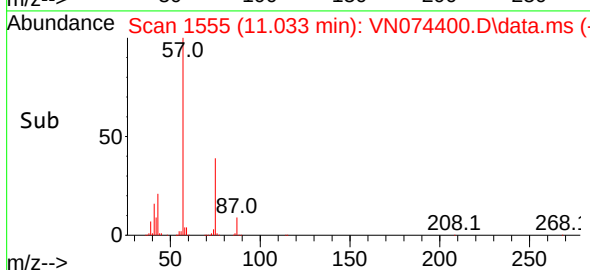






#62
4-Bromofluorobenzene
Concen: 48.565 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.000 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15




Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-DRUM-1-4-COMP


Tgt Ion: 95 Resp: 267414
Ion Ratio Lower Upper
95 100
174 77.0 0.0 150.6
176 74.3 0.0 143.4

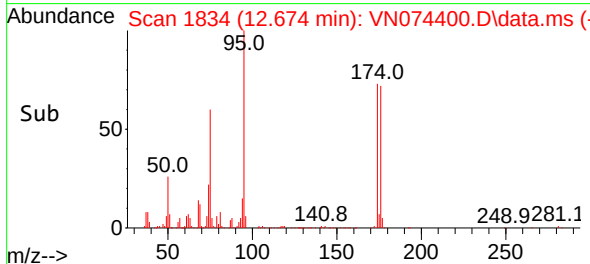

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1666
Delta R.T. 0.000 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15

Tgt Ion: 117 Resp: 576481
Ion Ratio Lower Upper
117 100
82 59.4 44.3 66.5
119 32.5 25.5 38.3


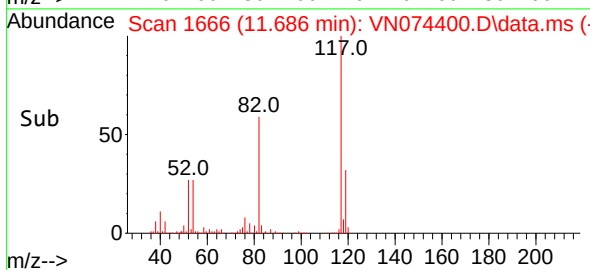

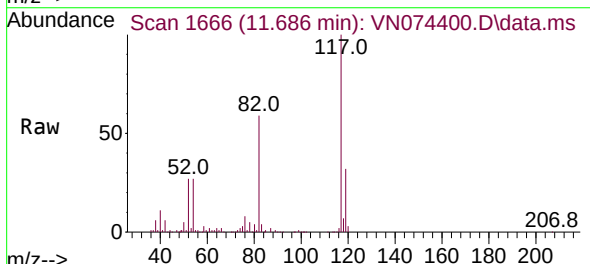




#71
Bromoform
Concen: 0.256 ug/l
RT: 12.669 min Scan# 11
Delta R.T. 0.271 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15




Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-DRUM-1-4-COMP


Tgt Ion:173 Resp: 1040
Ion Ratio Lower Upper
173 100
175 0.0 24.1 72.3#
254 0.0 0.0 0.0

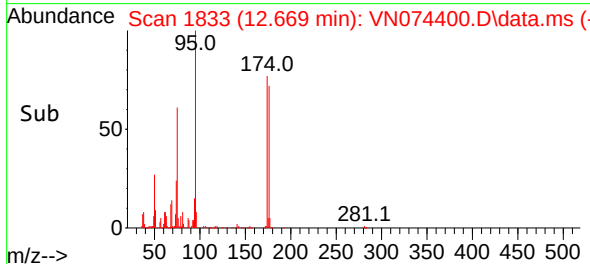

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.616 min Scan# 1994
Delta R.T. 0.001 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15

Tgt Ion:152 Resp: 259938
Ion Ratio Lower Upper
152 100
115 59.6 32.0 96.0
150 156.7 0.0 359.6


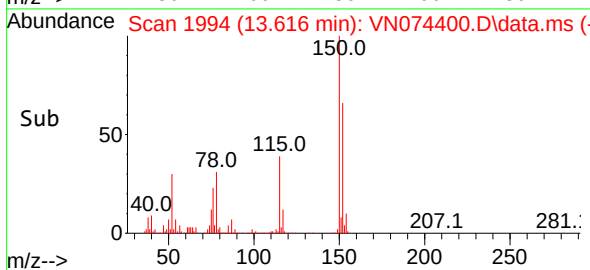

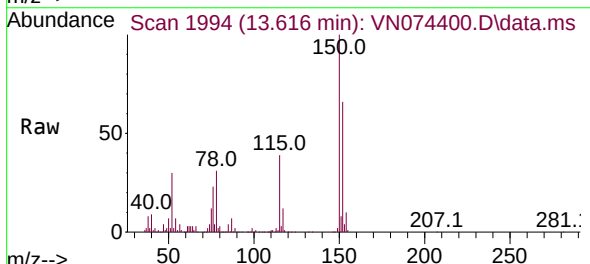




#74
N-amy1 acetate
Concen: Below Cal
RT: 12.327 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15




Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-DRUM-1-4-COMP


Tgt Ion: 43 Resp: 1223
Ion Ratio Lower Upper
43 100
70 0.0 31.4 47.0#
55 4.9 17.0 25.6#
61 0.0 18.4 27.6#

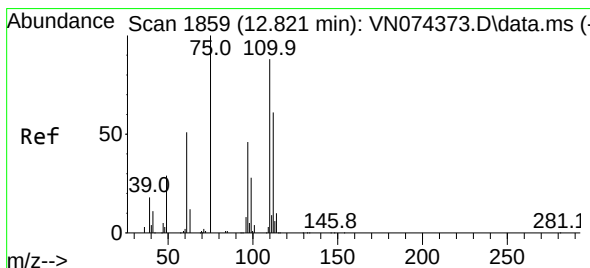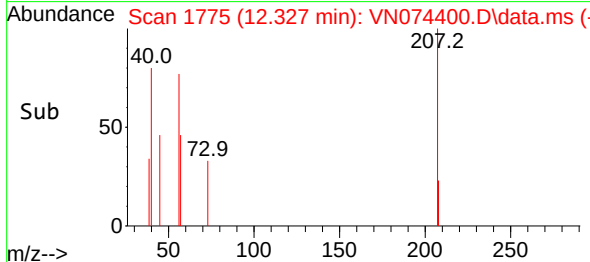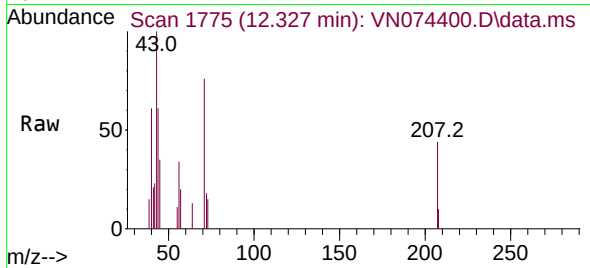

#76
1,2,3-Trichloropropane
Concen: 24.534 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. -0.147 min
Lab File: VN074400.D
Acq: 10 Sep 2022 02:15

Tgt Ion: 75 Resp: 166714
Ion Ratio Lower Upper
75 100
77 1.6 78.9 236.7#


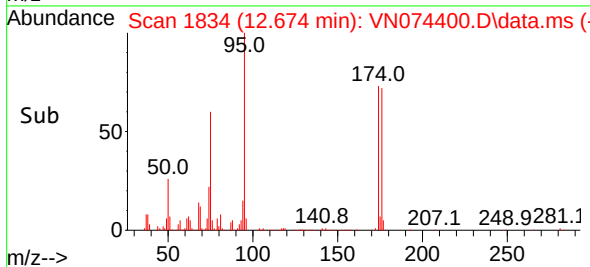

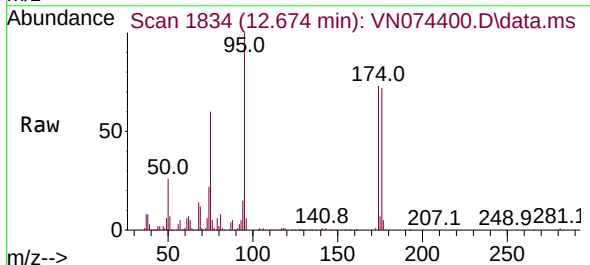




#81
 trans-1,4-Dichloro-2-butene
 Concen: 54.686 ug/l
 RT: 12.674 min Scan# 11
 Delta R.T. 0.106 min
 Lab File: VN074400.D
 Acq: 10 Sep 2022 02:15

Instrument :
 MSVOA_N
 ClientSampleId :
 SLUDGE-DRUM-1-4-COMP

Tgt Ion: 75 Resp: 166714
 Ion Ratio Lower Upper
 75 100
 53 0.0 82.2 123.2#
 89 0.1 37.7 56.5#

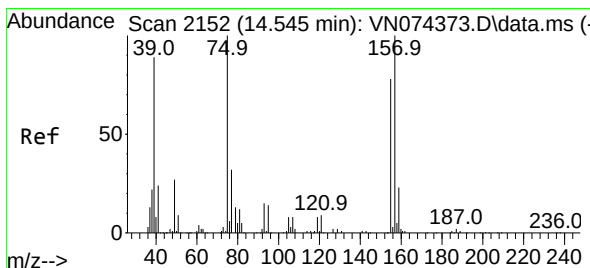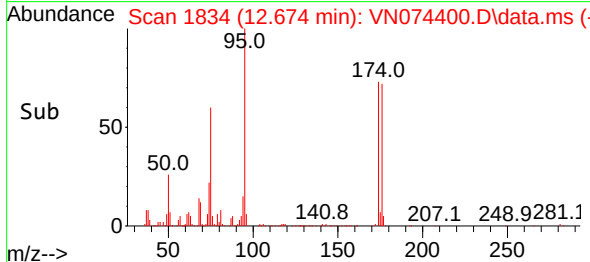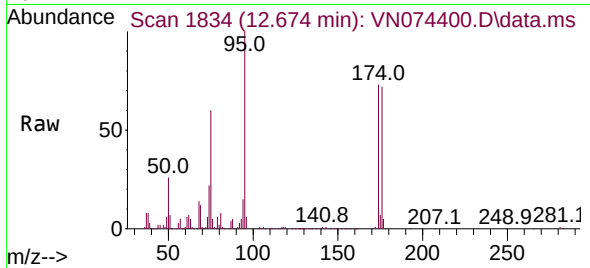

#92
 1,2-Dibromo-3-Chloropropane
 Concen: Below Cal
 RT: 14.586 min Scan# 2159
 Delta R.T. 0.041 min
 Lab File: VN074400.D
 Acq: 10 Sep 2022 02:15

Tgt Ion: 75 Resp: 66
 Ion Ratio Lower Upper
 75 100
 155 0.0 36.6 109.9#
 157 0.0 46.2 138.5#

