

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090922\
 Data File : VN074387.D
 Acq On : 09 Sep 2022 20:58
 Operator : JC\MD
 Sample : N4471-10
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-14A-15-20-083122

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090922W.M

Title : SW846 8260

Signal : TIC: VN074387.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.199	48	53	61	rBV	124347	262893	13.24%	2.186%
2	2.699	133	138	142	rBV3	47092	102191	5.14%	0.850%
3	7.951	1019	1031	1036	rBV2	293083	702936	35.39%	5.846%
4	8.016	1036	1042	1057	rVB	488758	1105705	55.67%	9.195%
5	8.369	1092	1102	1114	rBV2	306327	708814	35.68%	5.894%
6	8.904	1182	1193	1203	rBV	744620	1510394	76.04%	12.560%
7	9.157	1227	1236	1244	rBV4	37553	83821	4.22%	0.697%
8	10.381	1435	1444	1455	rBV	1062238	1911511	96.23%	15.896%
9	10.810	1504	1517	1524	rBV5	26593	103171	5.19%	0.858%
10	11.686	1658	1666	1678	rBV	1183840	1986339	100.00%	16.518%
11	12.674	1826	1834	1845	rVB	948209	1598781	80.49%	13.295%
12	13.616	1987	1994	2009	rBV	1168285	1948561	98.10%	16.204%


Sum of corrected areas: 12025117

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090922\
Data File : VN074387.D
Acq On : 09 Sep 2022 20:58
Operator : JC\MD
Sample : N4471-10
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-14A-15-20-083122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

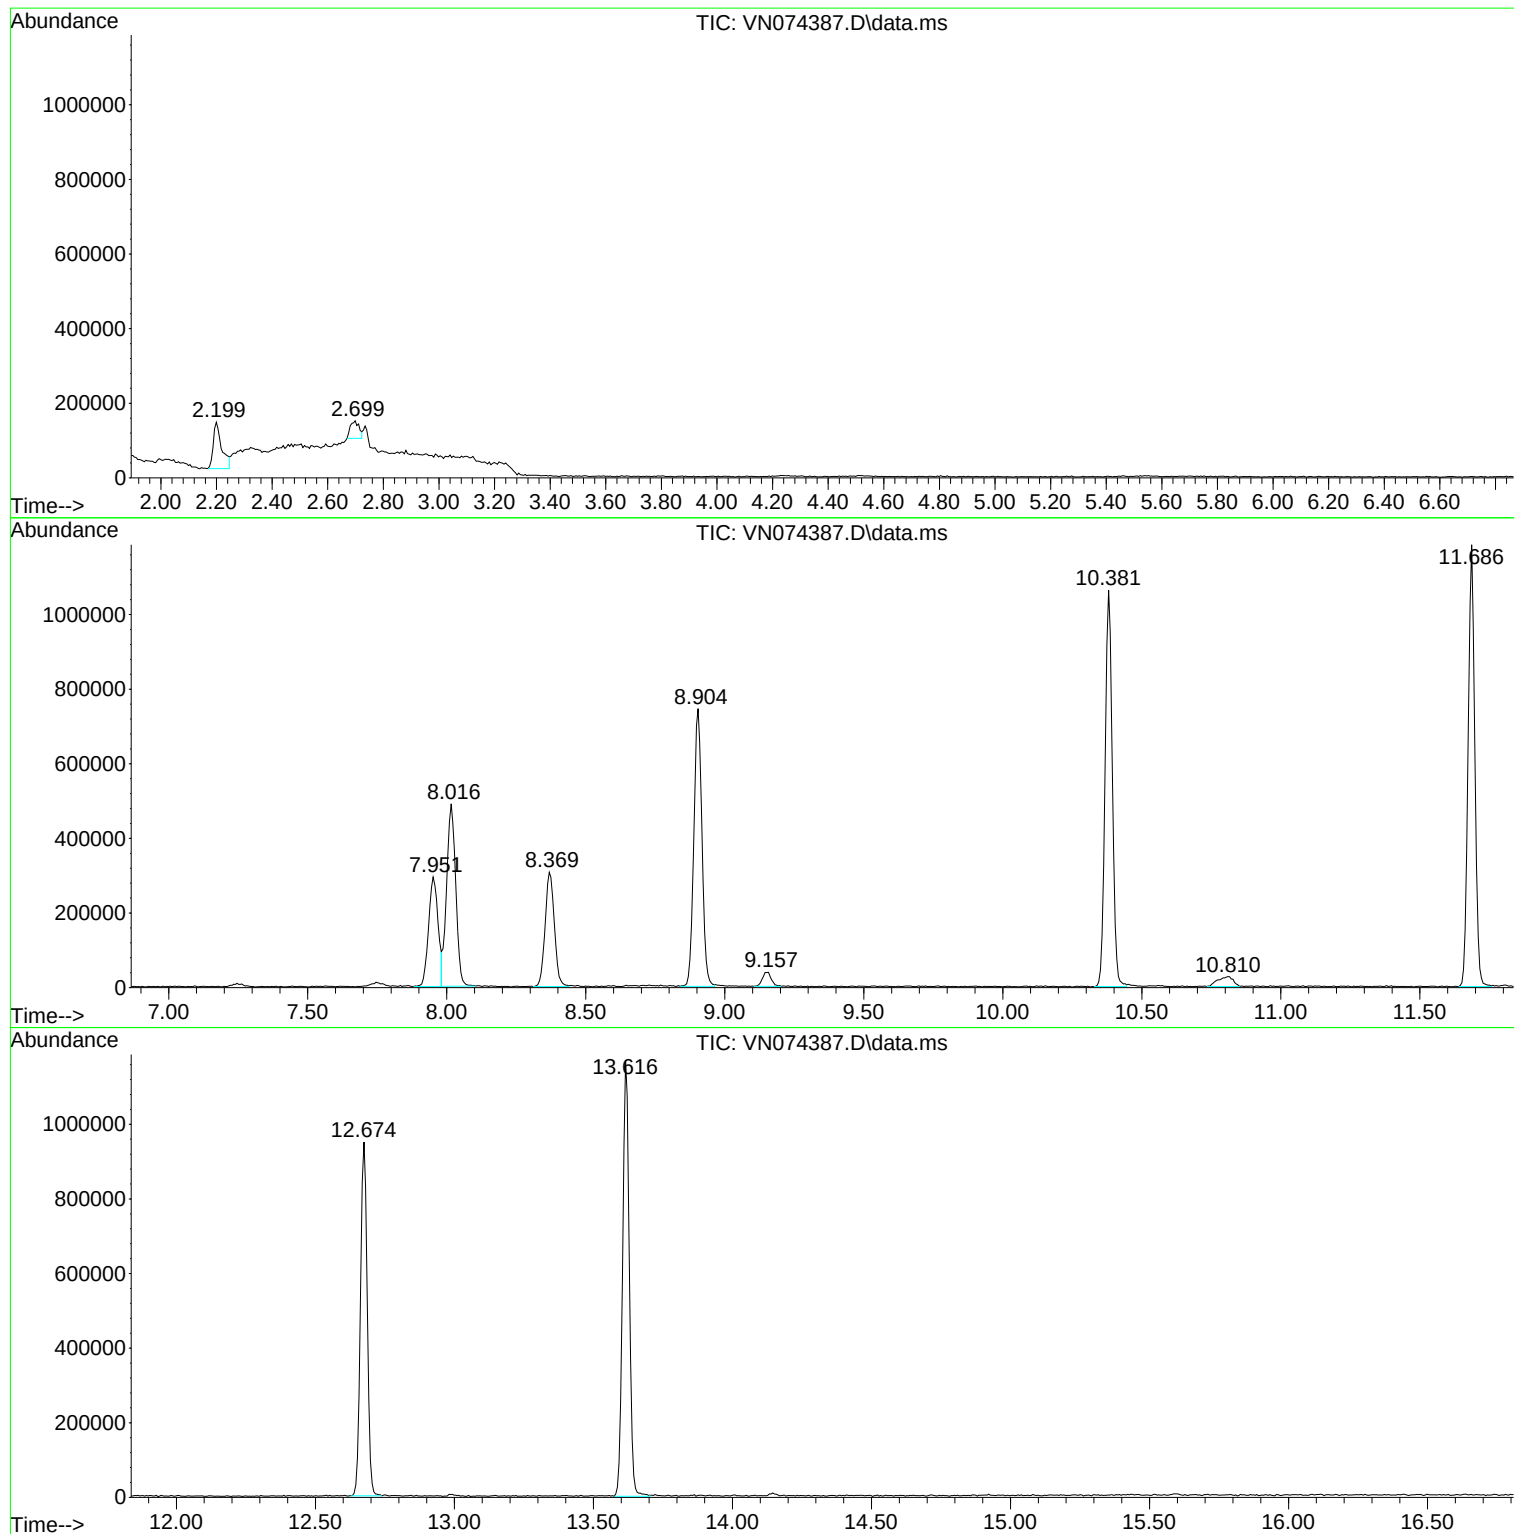

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090922\
Data File : VN074387.D
Acq On : 09 Sep 2022 20:58
Operator : JC\MD
Sample : N4471-10
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-14A-15-20-083122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	2.199	11.9	ug/l	262893	1	8.016	1105710	50.0