
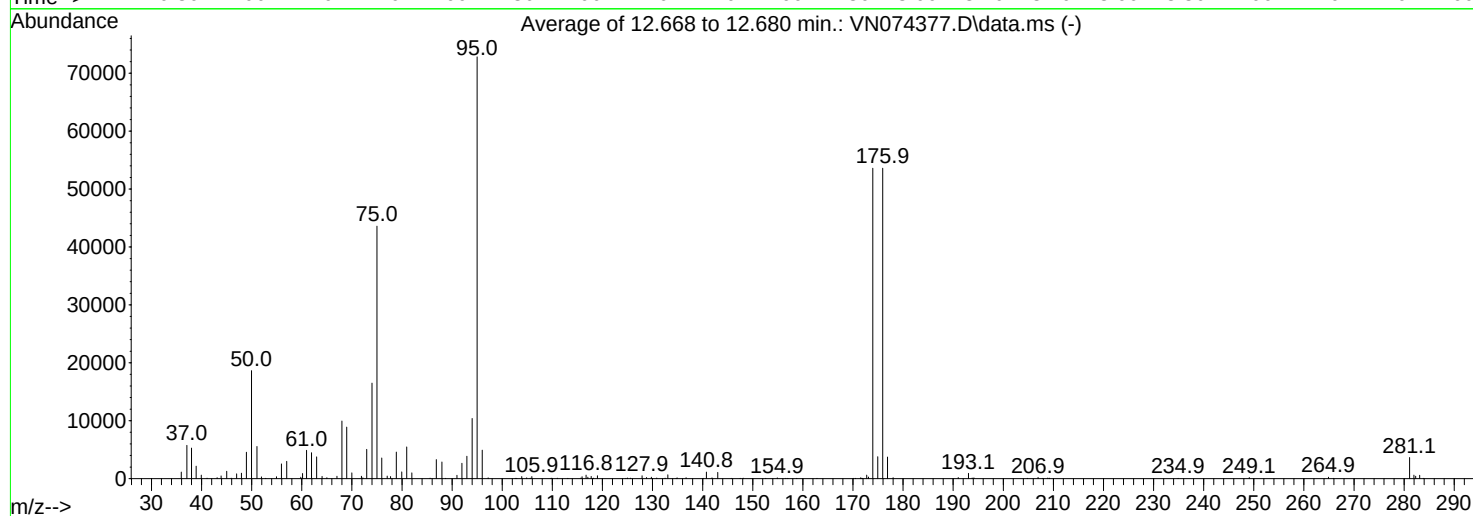


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090922\
 Data File : VN074377.D
 Acq On : 09 Sep 2022 16:25
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090922W.M
 Title : SW846 8260
 Last Update : Sat Sep 10 06:10:29 2022

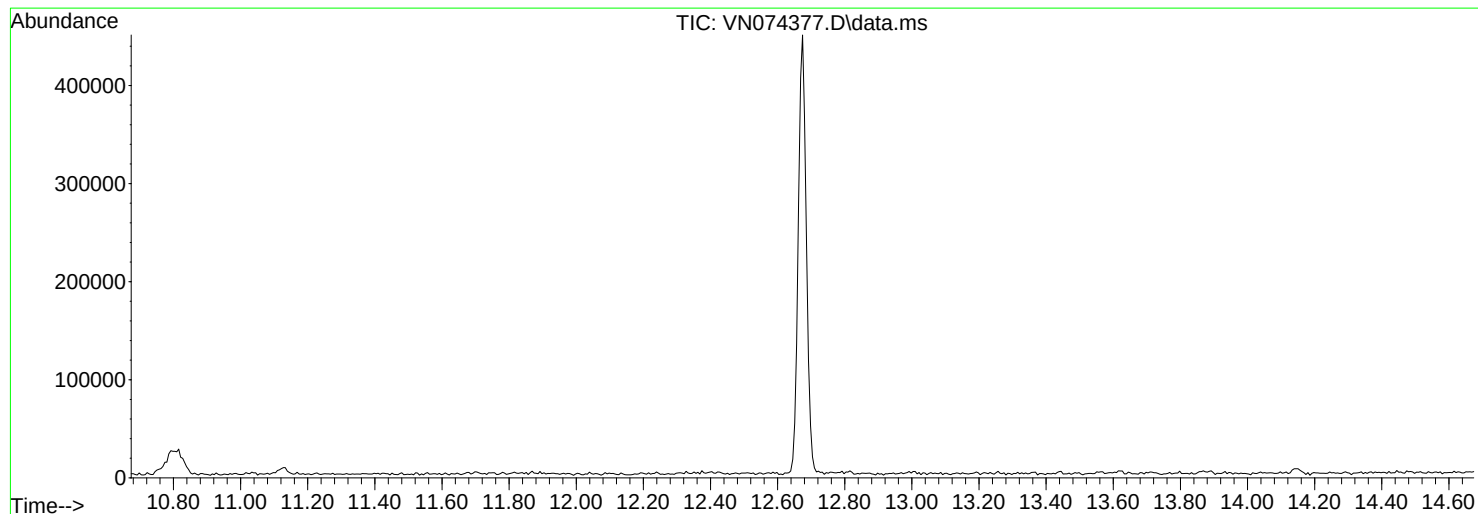

AutoFind: Scans 1833, 1834, 1835; Background Corrected with Scan 1825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.6	18659	PASS
75	95	30	60	59.9	43611	PASS
95	95	100	100	100.0	72829	PASS
96	95	5	9	6.7	4915	PASS
173	174	0.00	2	1.1	606	PASS
174	95	50	100	73.6	53584	PASS
175	174	5	9	7.1	3788	PASS
176	174	95	101	100.0	53587	PASS
177	176	5	9	7.0	3743	PASS