
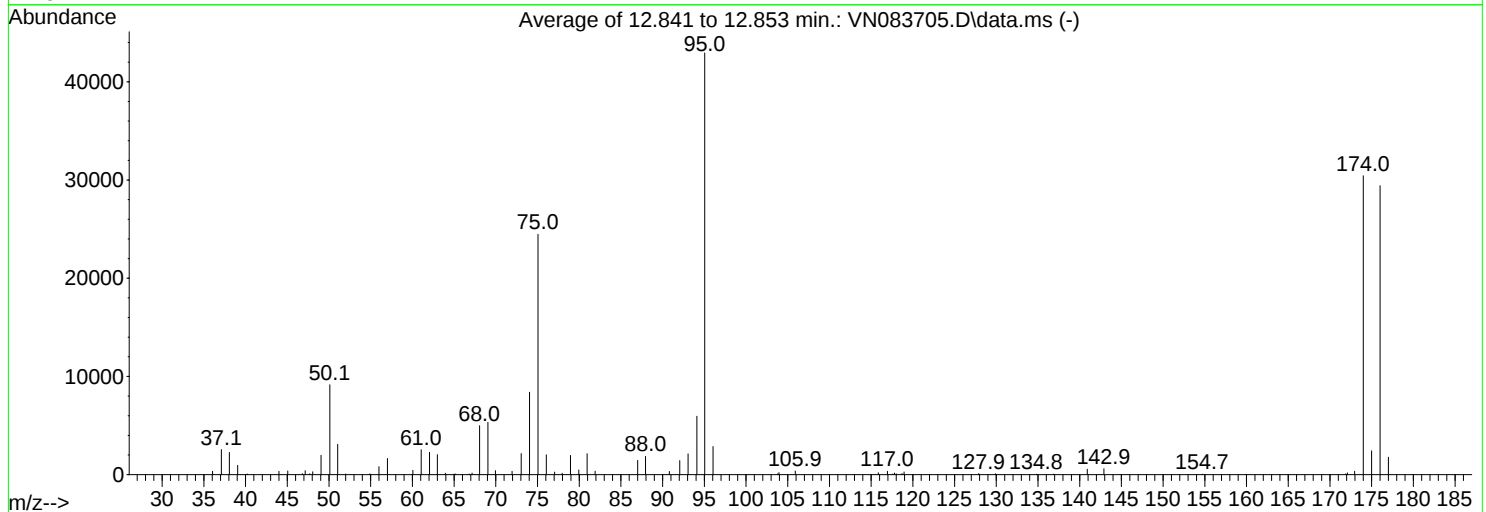


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090924\
Data File : VN083705.D
Acq On : 09 Sep 2024 07:56
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N090624W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Sep 06 23:42:47 2024

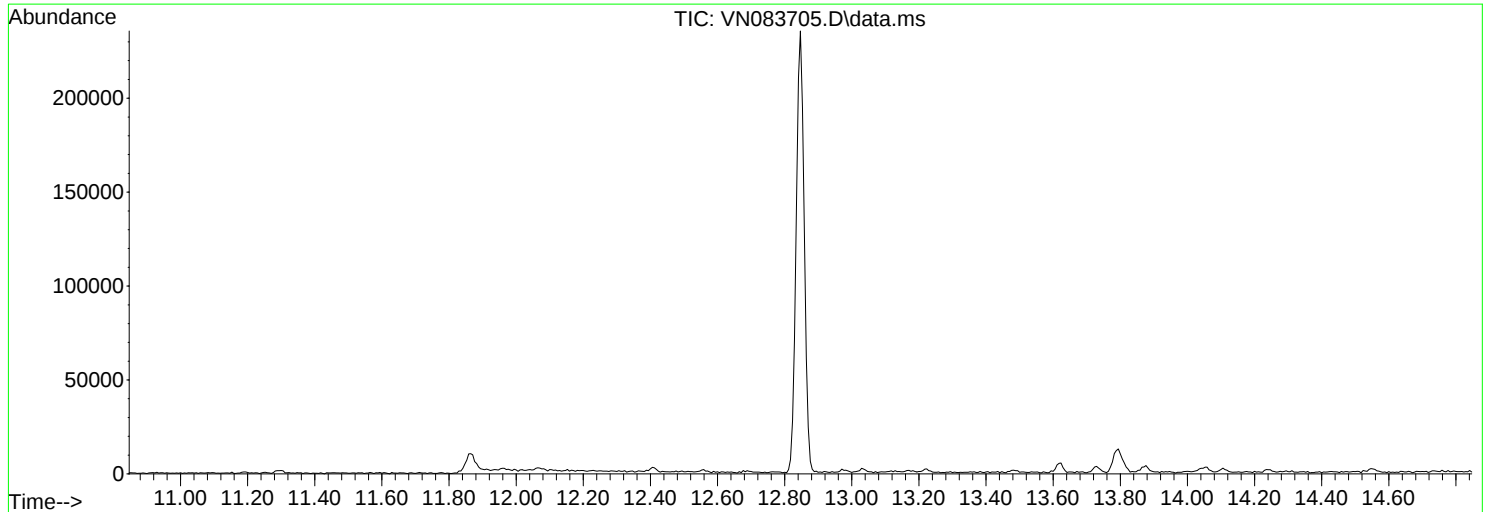

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	9154	PASS
75	95	30	60	57.0	24472	PASS
95	95	100	100	100.0	42949	PASS
96	95	5	9	6.7	2867	PASS
173	174	0.00	2	1.1	341	PASS
174	95	50	100	70.9	30437	PASS
175	174	5	9	8.0	2428	PASS
176	174	95	101	96.7	29427	PASS
177	176	5	9	6.0	1777	PASS