

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN091018\
 Data File : VN051078.D
 Acq On : 10 Sep 2018 15:21
 Operator : MD\SY
 Sample : J4832-04
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGEBLANK-SAMPLEMANAG

Quant Time: Sep 11 03:44:19 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091018W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 11 02:27:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	684083	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1035369	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	879277	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	272338	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	400564	52.62	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.24%	
35) Dibromofluoromethane	7.59	113	397372	51.08	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.16%	
50) Toluene-d8	10.09	98	1443772	48.90	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.80%	
62) 4-Bromofluorobenzene	12.40	95	382629	39.18	ug/l	0.00
Spiked Amount	50.000		Recovery	=	78.36%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN091018\
Data File : VN051078.D
Acq On : 10 Sep 2018 15:21
Operator : MD\SY
Sample : J4832-04
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGEBLANK-SAMPLEMANAG

Quant Time: Sep 11 03:44:19 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N091018W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 11 02:27:09 2018
Response via : Initial Calibration

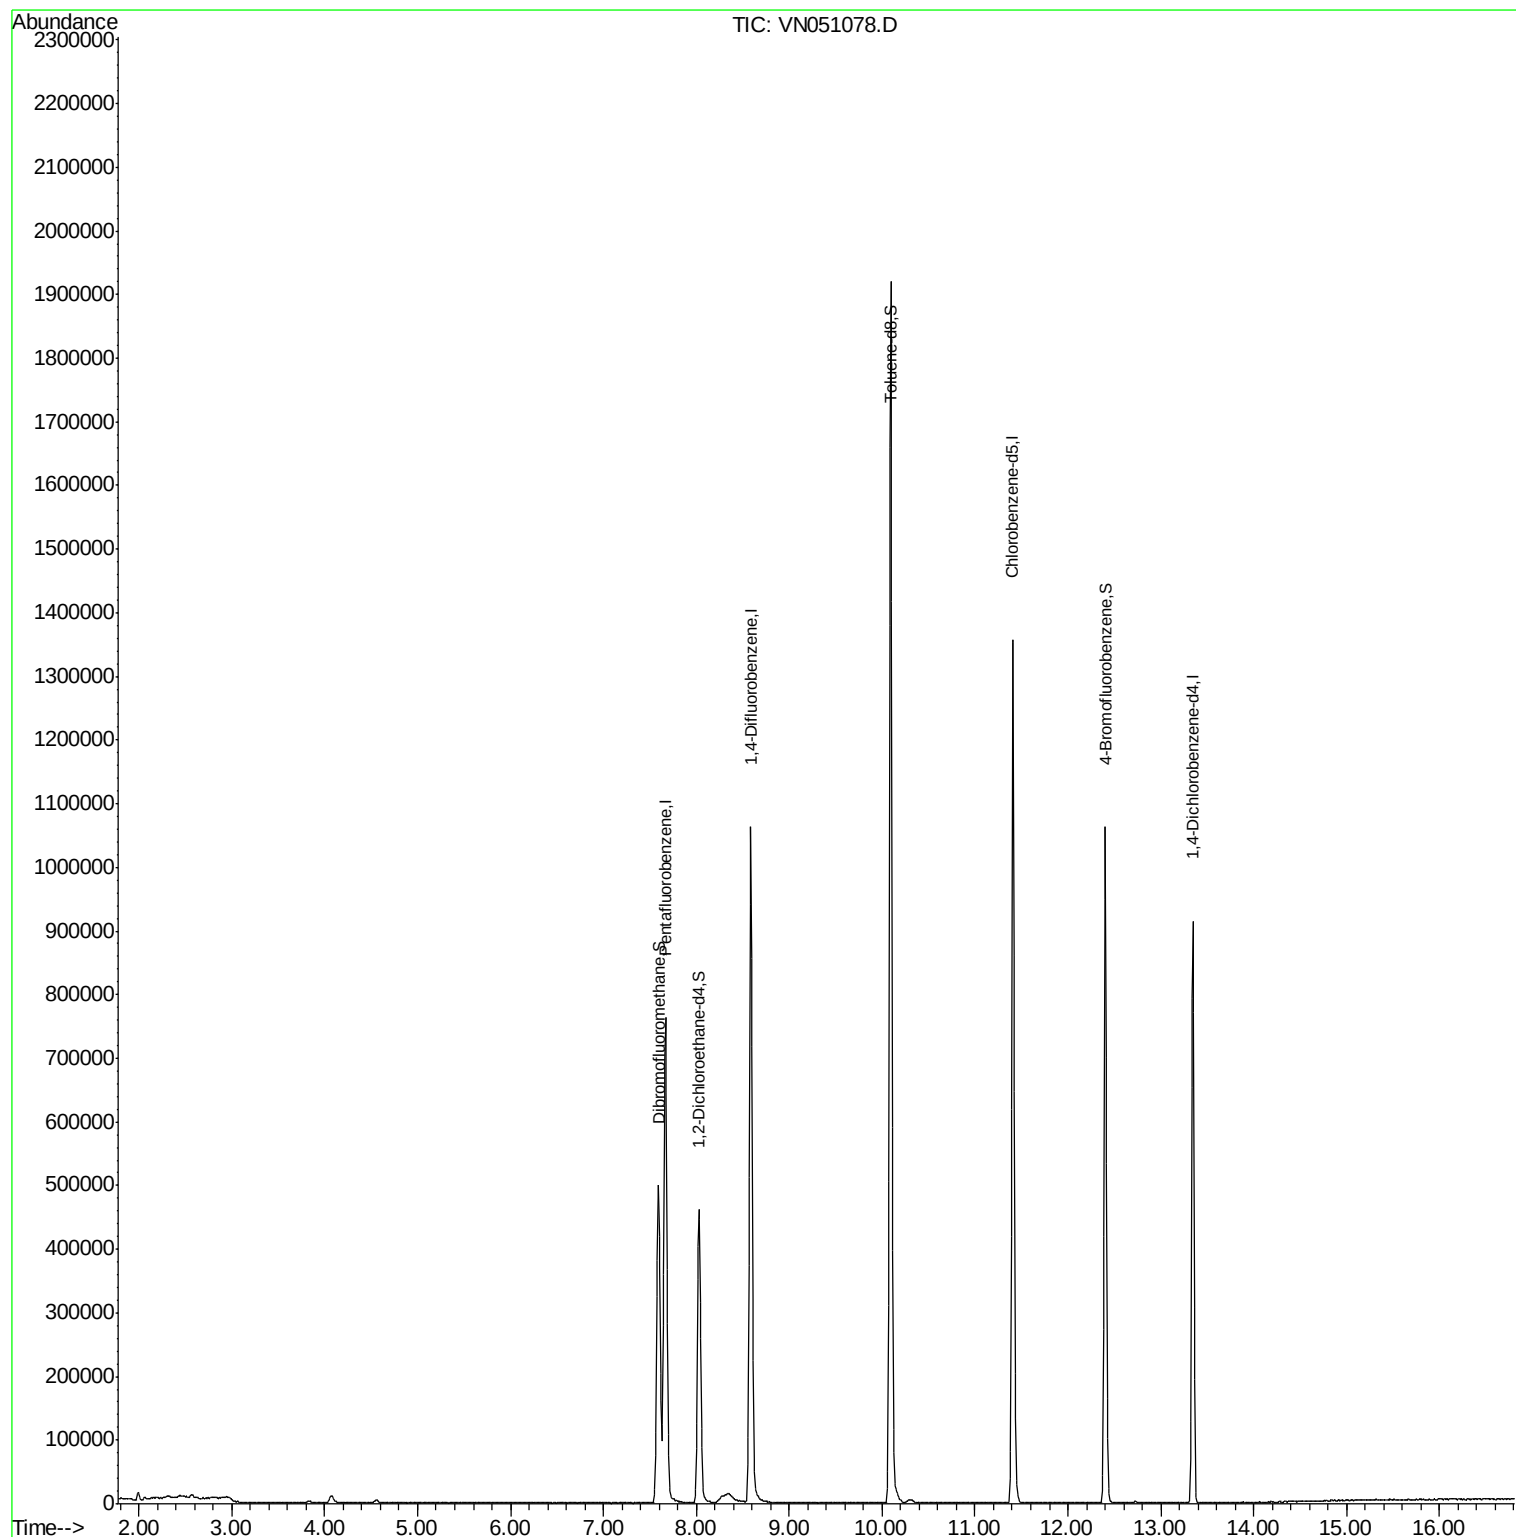

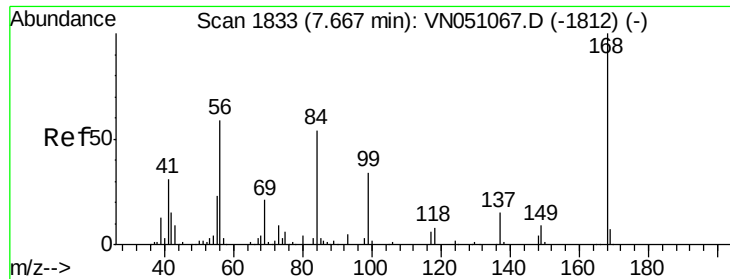

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: VN051078.D

Acq: 10 Sep 2018 15:21

Instrument :

MSVOA_N

ClientSampleId :


STORAGEBLANK-SAMPLEMANAG

Tot Ion:168 Resp: 684083

Ion Ratio Lower Upper

168 100

99 48.1 38.3 57.5

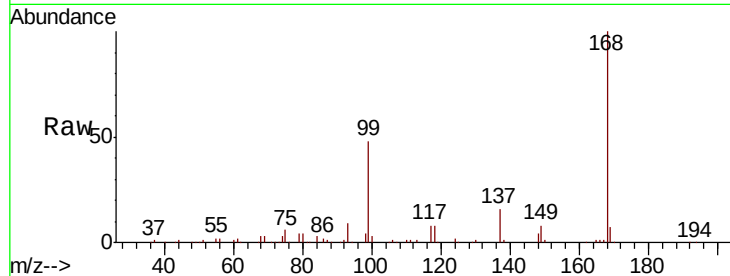

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

7.67



300000

200000

100000

0

Time-->

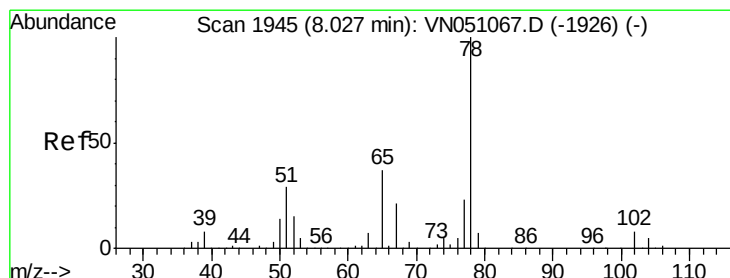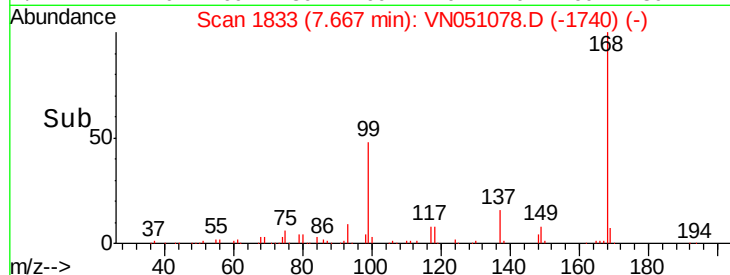

#33

1,2-Dichloroethane-d4

Concen: 52.62 ug/l

RT: 8.03 min Scan# 1945

Delta R.T. -0.00 min

Lab File: VN051078.D


Acq: 10 Sep 2018 15:21

Tgt Ion: 65 Resp: 400564

Ion Ratio Lower Upper

65 100

67 54.9 0.0 112.0

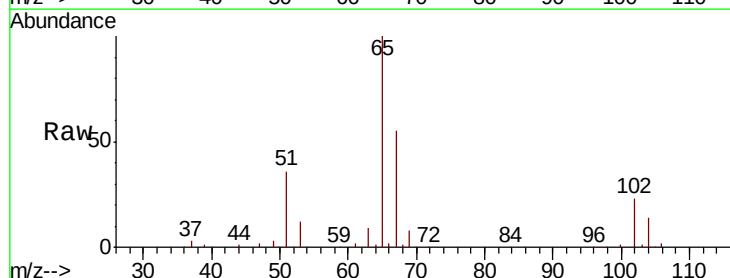

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

8.03


150000


100000

50000

0

Time-->

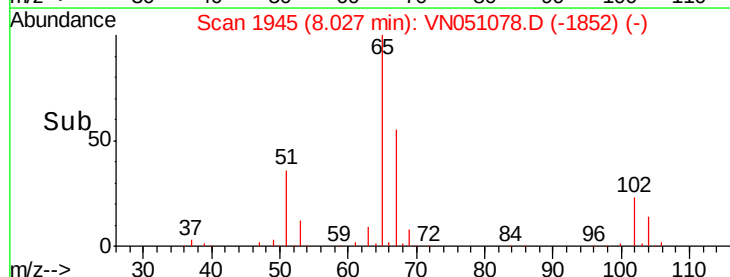


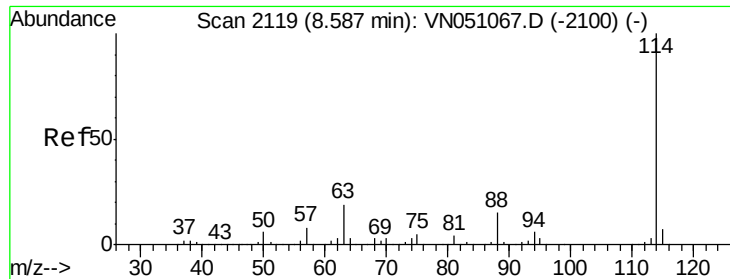




#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. -0.00 min
 Lab File: VN051078.D
 Acq: 10 Sep 2018 15:21

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGEBLANK-SAMPLEMANAG

Tot Ion:114 Resp: 1035369
 Ion Ratio Lower Upper
 114 100
 63 18.8 0.0 37.8
 88 15.4 0.0 30.8

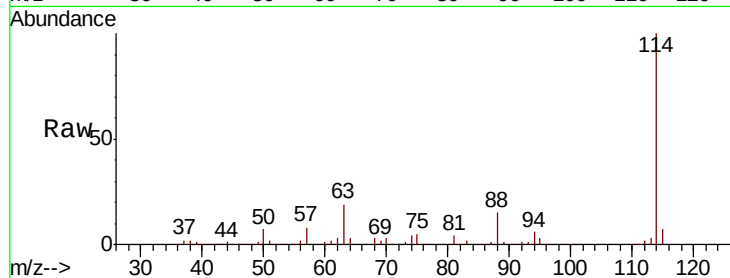


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

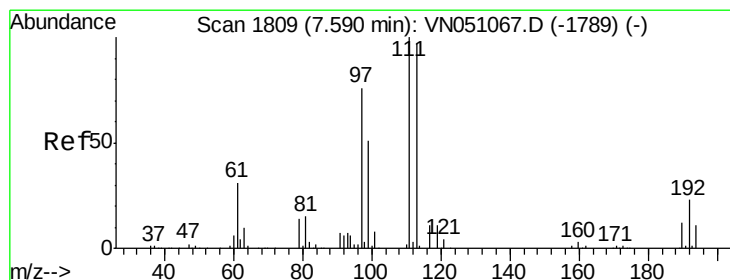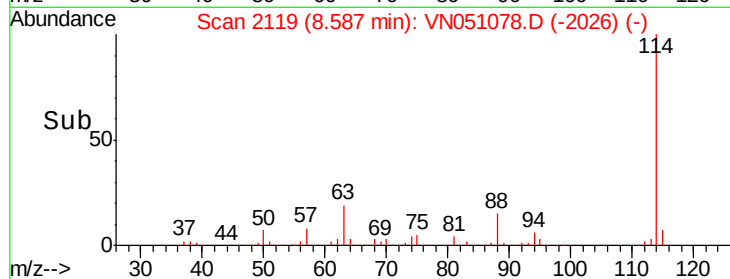
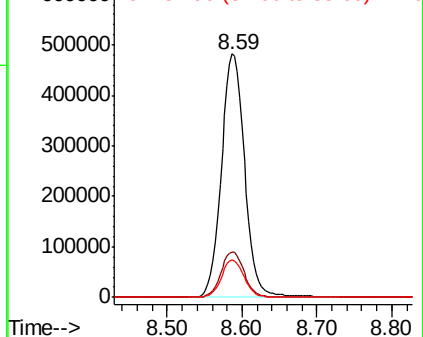



#35
 Dibromofluoromethane
 Concen: 51.08 ug/l
 RT: 7.59 min Scan# 1810
 Delta R.T. 0.00 min
 Lab File: VN051078.D
 Acq: 10 Sep 2018 15:21

Tgt Ion:113 Resp: 397372
 Ion Ratio Lower Upper
 113 100
 111 102.2 83.0 124.6
 192 23.0 18.7 28.1

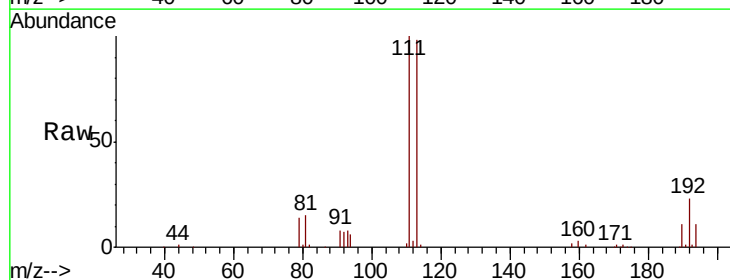

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



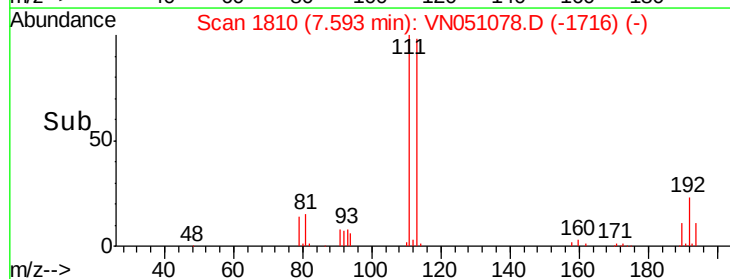
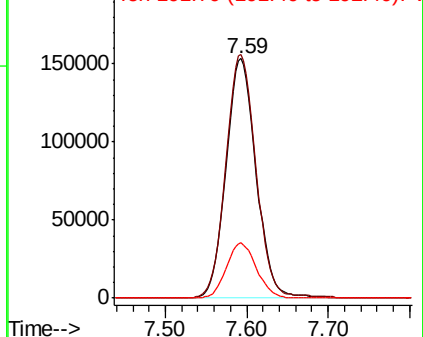


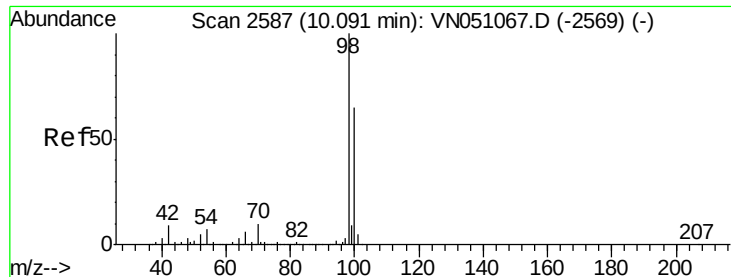

#50
Toluene-d8
Concen: 48.90 ug/l
RT: 10.09 min Scan# 2587
Delta R.T. -0.00 min
Lab File: VN051078.D
Acq: 10 Sep 2018 15:21




Instrument :
MSVOA_N
ClientSampleId :
STORAGEBLANK-SAMPLEMANAG


Tot Ion: 98 Resp: 1443772
Ion Ratio Lower Upper
98 100
100 63.8 52.0 78.0

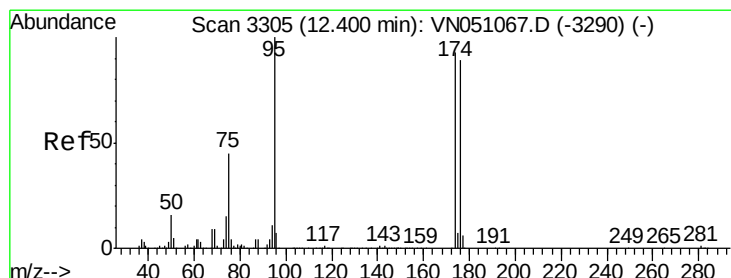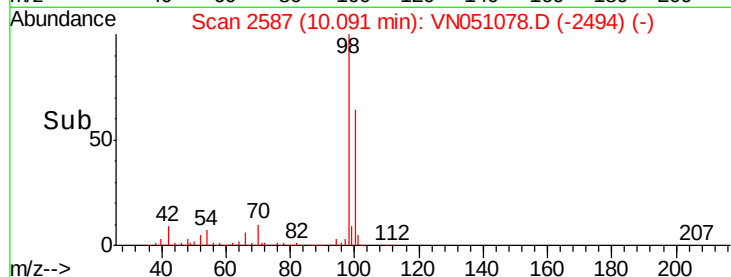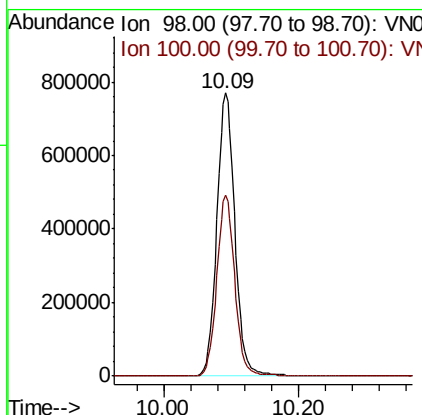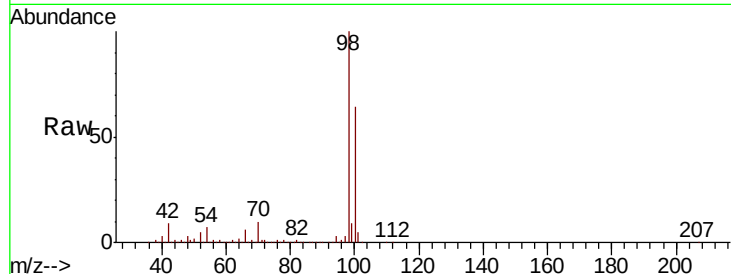

#62
4-Bromofluorobenzene
Concen: 39.18 ug/l
RT: 12.40 min Scan# 3306
Delta R.T. 0.00 min
Lab File: VN051078.D
Acq: 10 Sep 2018 15:21

Tgt Ion: 95 Resp: 382629
Ion Ratio Lower Upper
95 100
174 91.9 0.0 184.8
176 89.2 0.0 178.6


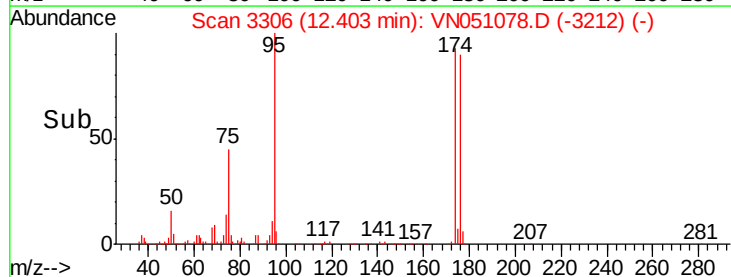
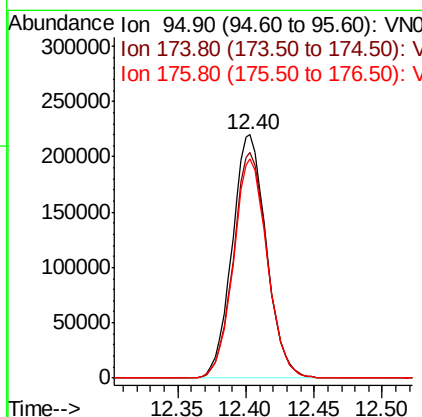
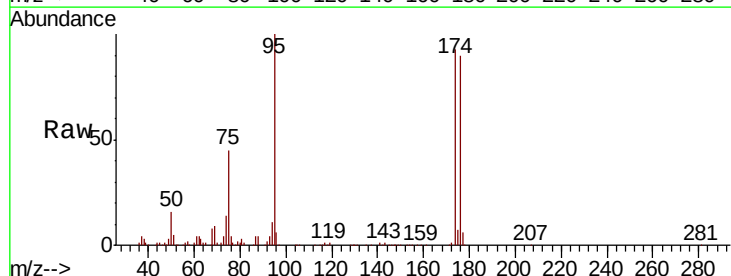


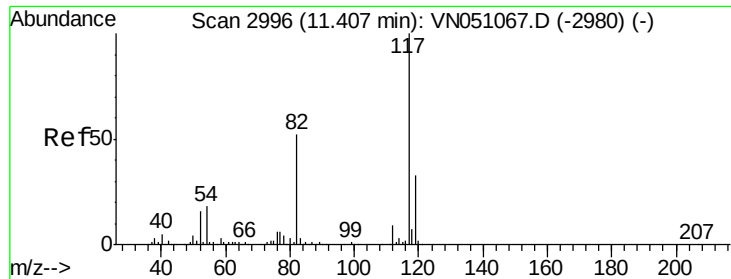

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.41 min Scan# 2997
Delta R.T. 0.00 min
Lab File: VN051078.D
Acq: 10 Sep 2018 15:21

Instrument :
MSVOA_N
ClientSampleId :
STORAGEBLANK-SAMPLEMANAG

Tot Ion:117 Resp: 879277
Ion Ratio Lower Upper
117 100
82 52.4 41.8 62.6
119 32.4 26.2 39.2

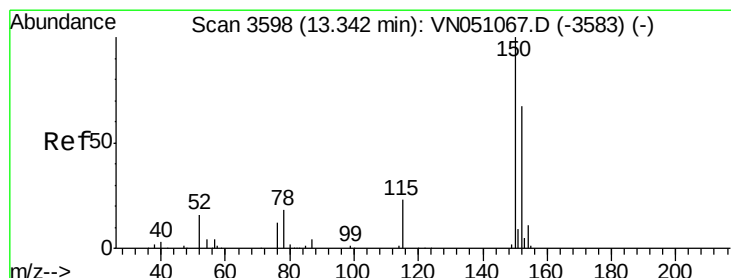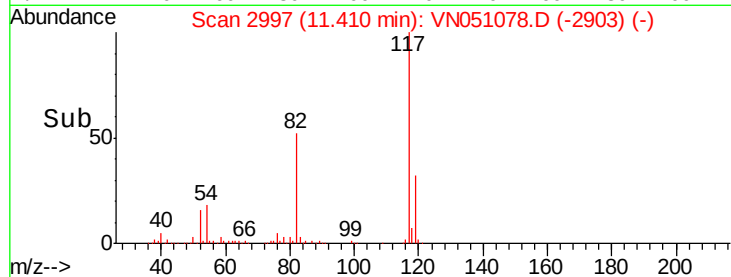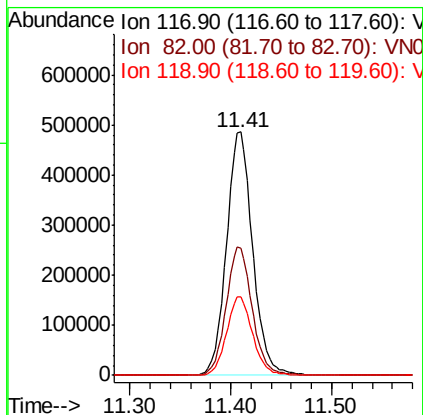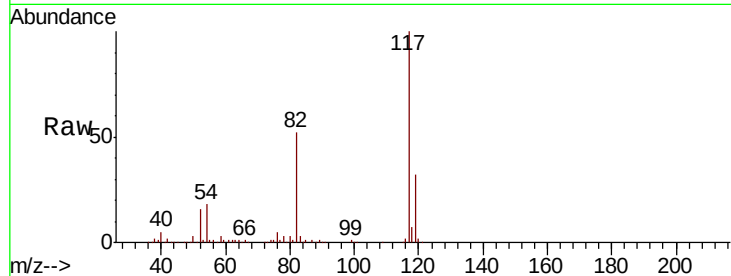

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.35 min Scan# 3599
Delta R.T. 0.00 min
Lab File: VN051078.D
Acq: 10 Sep 2018 15:21

Tgt Ion:152 Resp: 272338
Ion Ratio Lower Upper
152 100
115 56.4 28.2 84.7
150 156.5 0.0 349.0

