


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN091018\
Data File : VN051063.D
Acq On : 10 Sep 2018 7:27
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091018W.M
Title : SW846 8260
Last Update : Tue Sep 11 02:27:09 2018

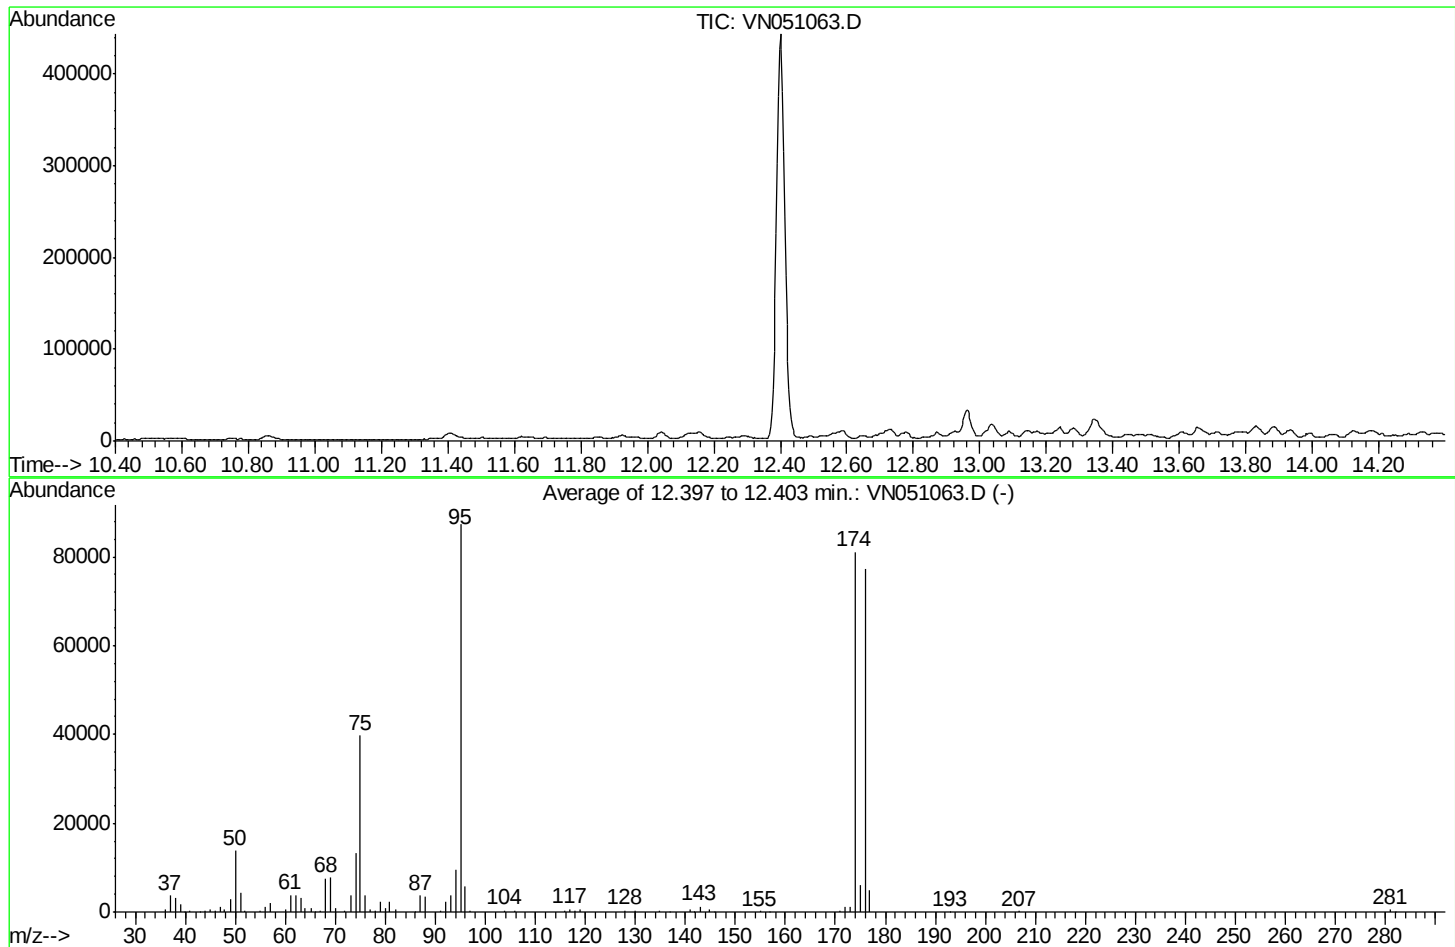

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	13818	PASS
75	95	30	60	45.4	39677	PASS
95	95	100	100	100.0	87309	PASS
96	95	5	9	6.5	5673	PASS
173	174	0.00	2	1.3	1086	PASS
174	95	50	100	92.9	81096	PASS
175	174	5	9	7.3	5947	PASS
176	174	95	101	95.1	77146	PASS
177	176	5	9	6.3	4824	PASS