


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN091018\
 Data File : VN051088.D
 Acq On : 10 Sep 2018 19:51
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091018W.M
 Title : SW846 8260
 Last Update : Tue Sep 11 02:27:09 2018

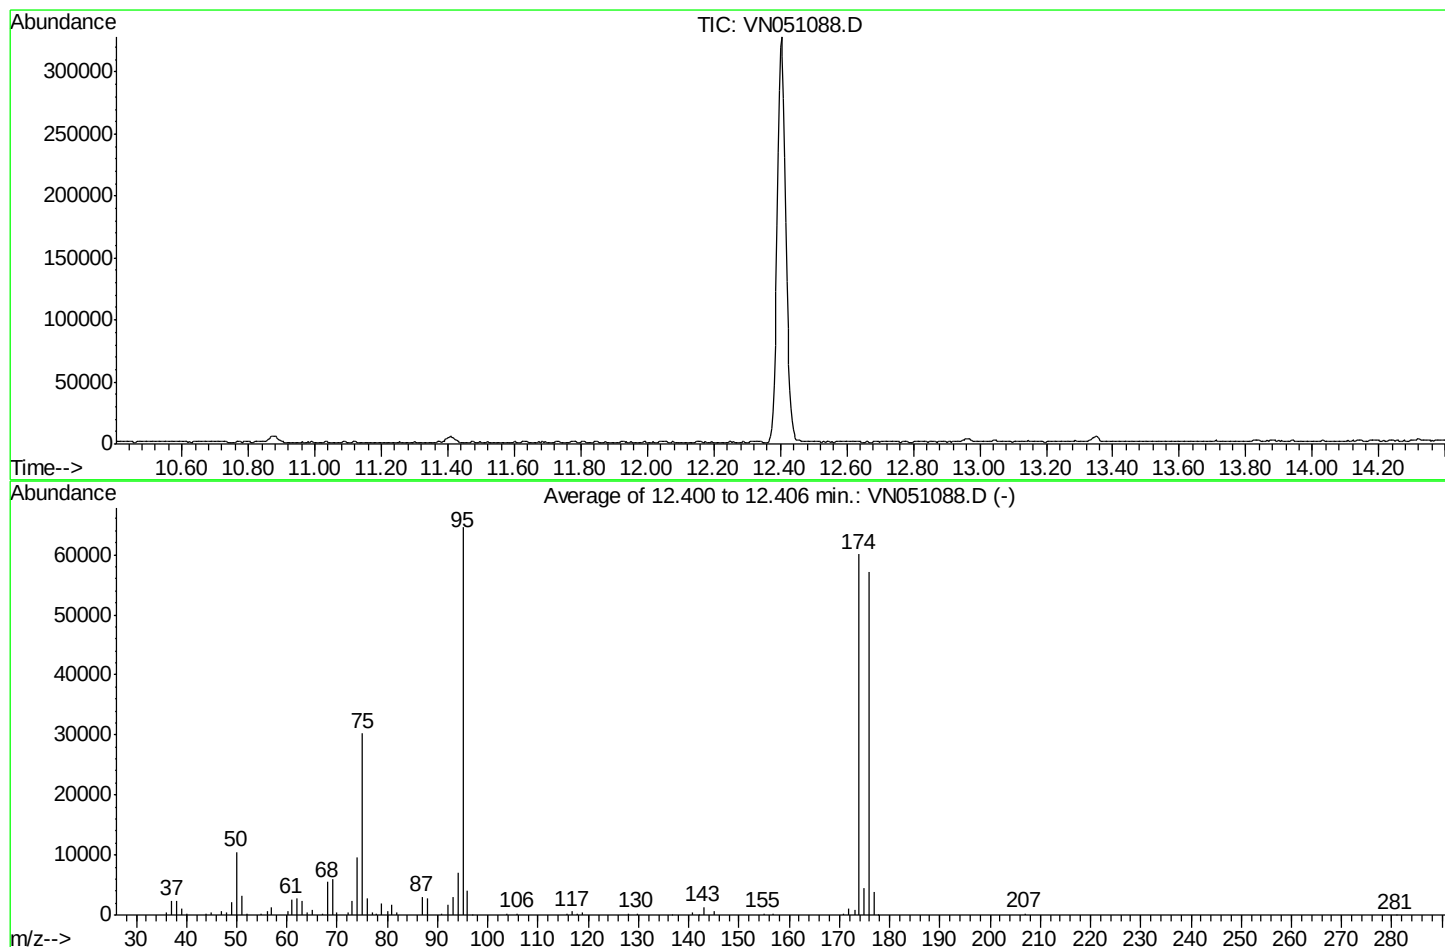

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	10493	PASS
75	95	30	60	46.8	30226	PASS
95	95	100	100	100.0	64578	PASS
96	95	5	9	6.2	4006	PASS
173	174	0.00	2	1.5	908	PASS
174	95	50	100	93.0	60037	PASS
175	174	5	9	7.3	4408	PASS
176	174	95	101	95.3	57213	PASS
177	176	5	9	6.7	3854	PASS