



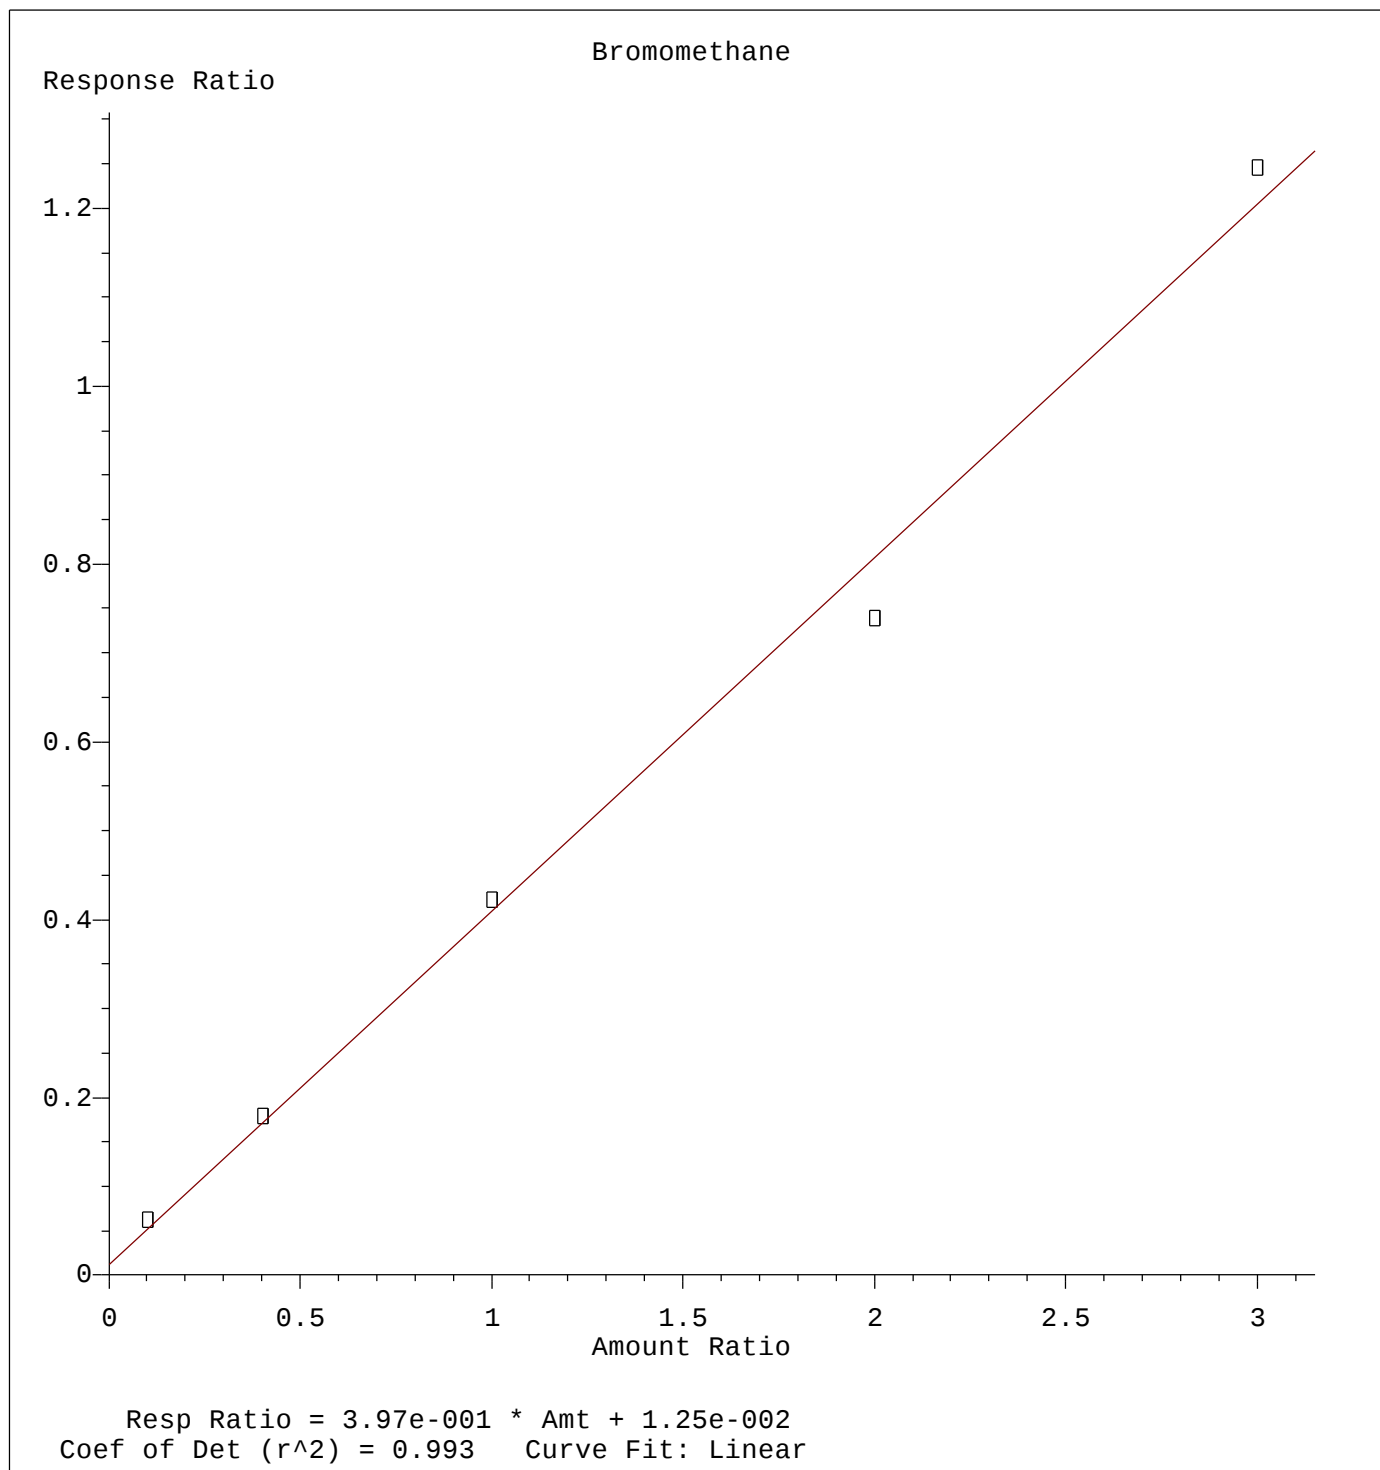

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091019W.M
Calibration Table Last Updated: Fri Sep 13 05:15:45 2019


1,2,3-Trichlorobenzene

Response Ratio

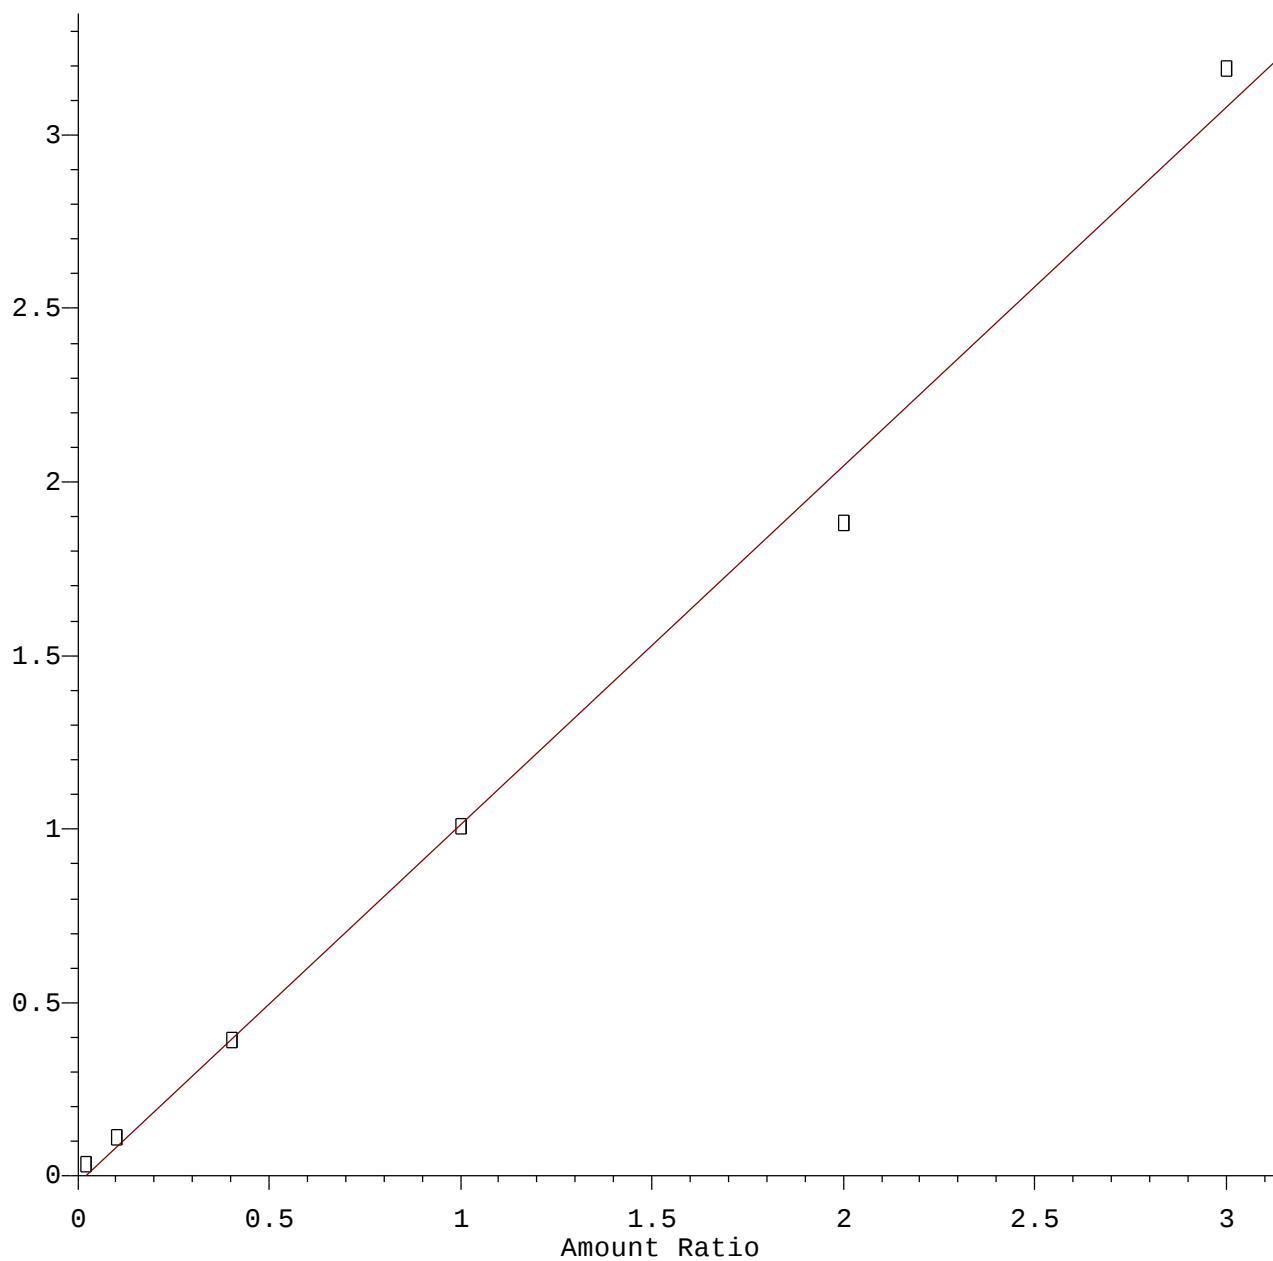


Resp Ratio = 1.03×10^0 * Amt - 2.06×10^{-2}
Coef of Det (r^2) = 0.995 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091019W.M
Calibration Table Last Updated: Fri Sep 13 05:15:45 2019

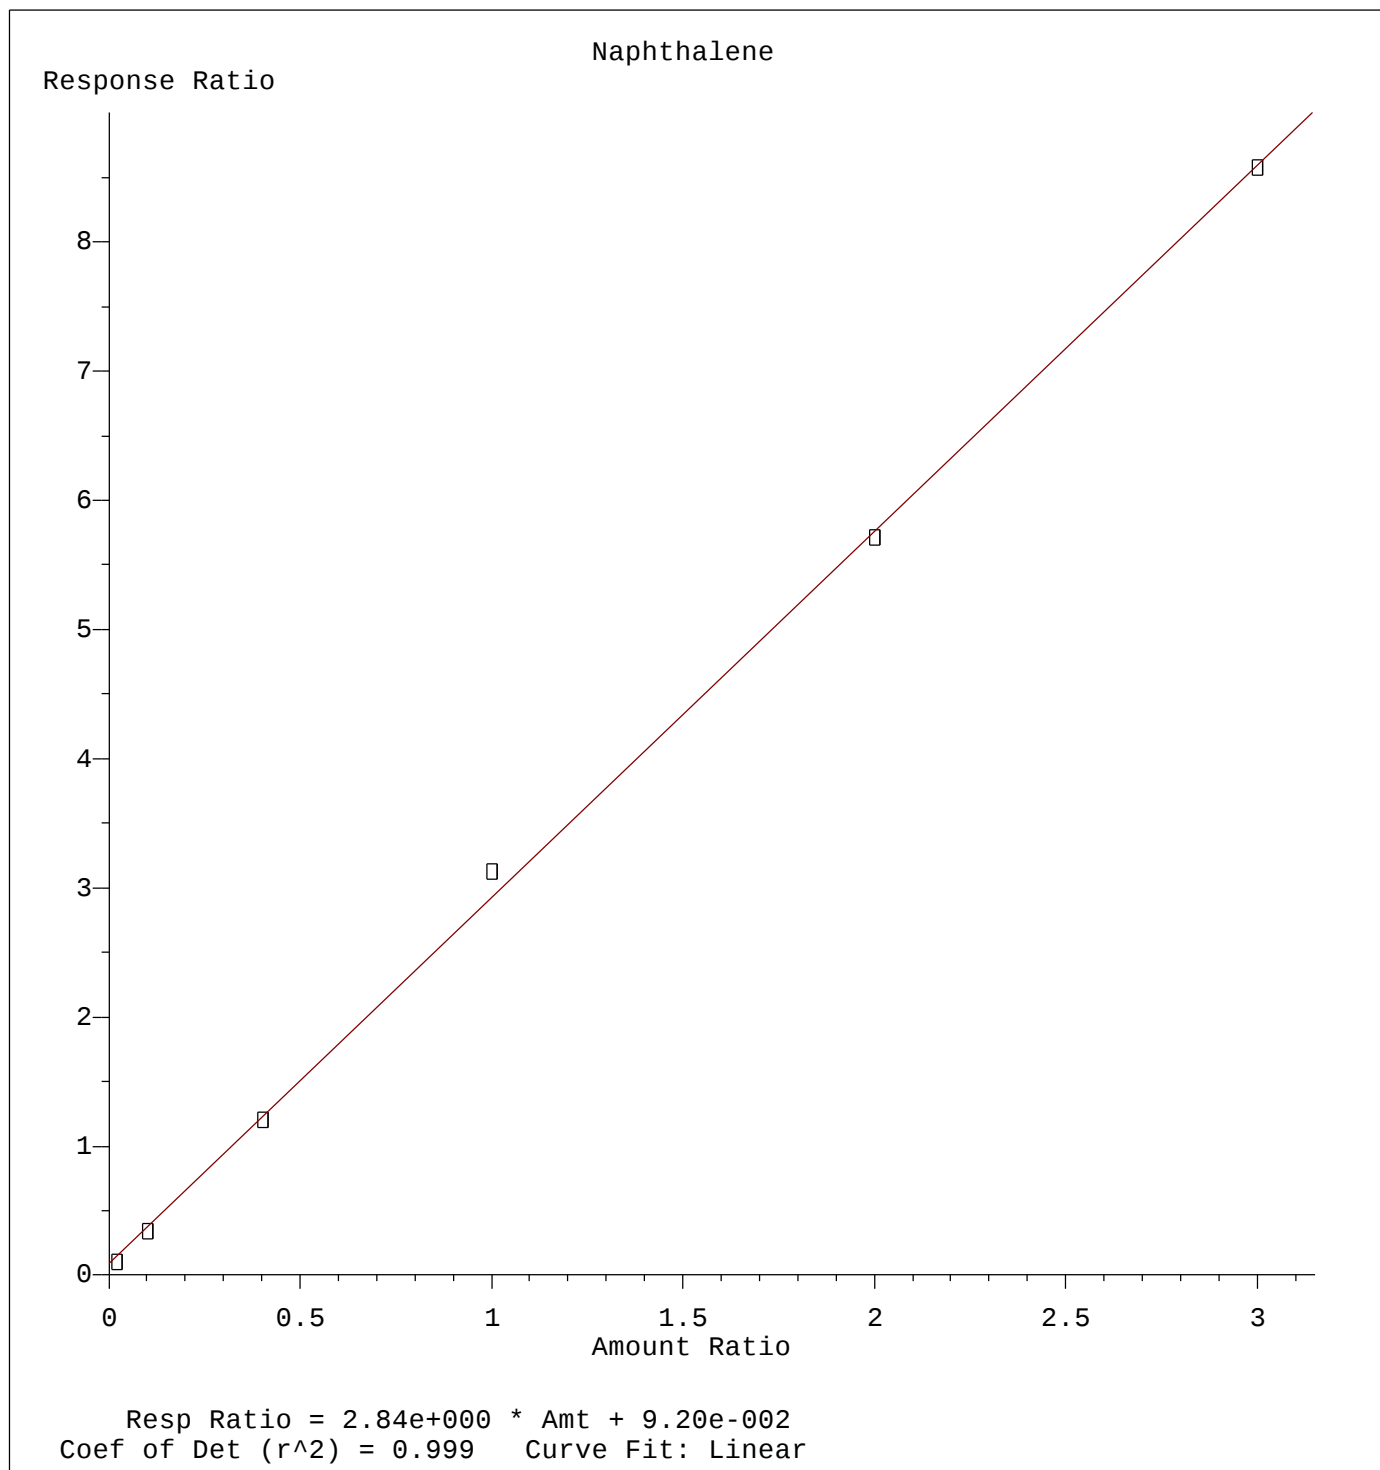


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091019W.M
Calibration Table Last Updated: Fri Sep 13 05:15:45 2019

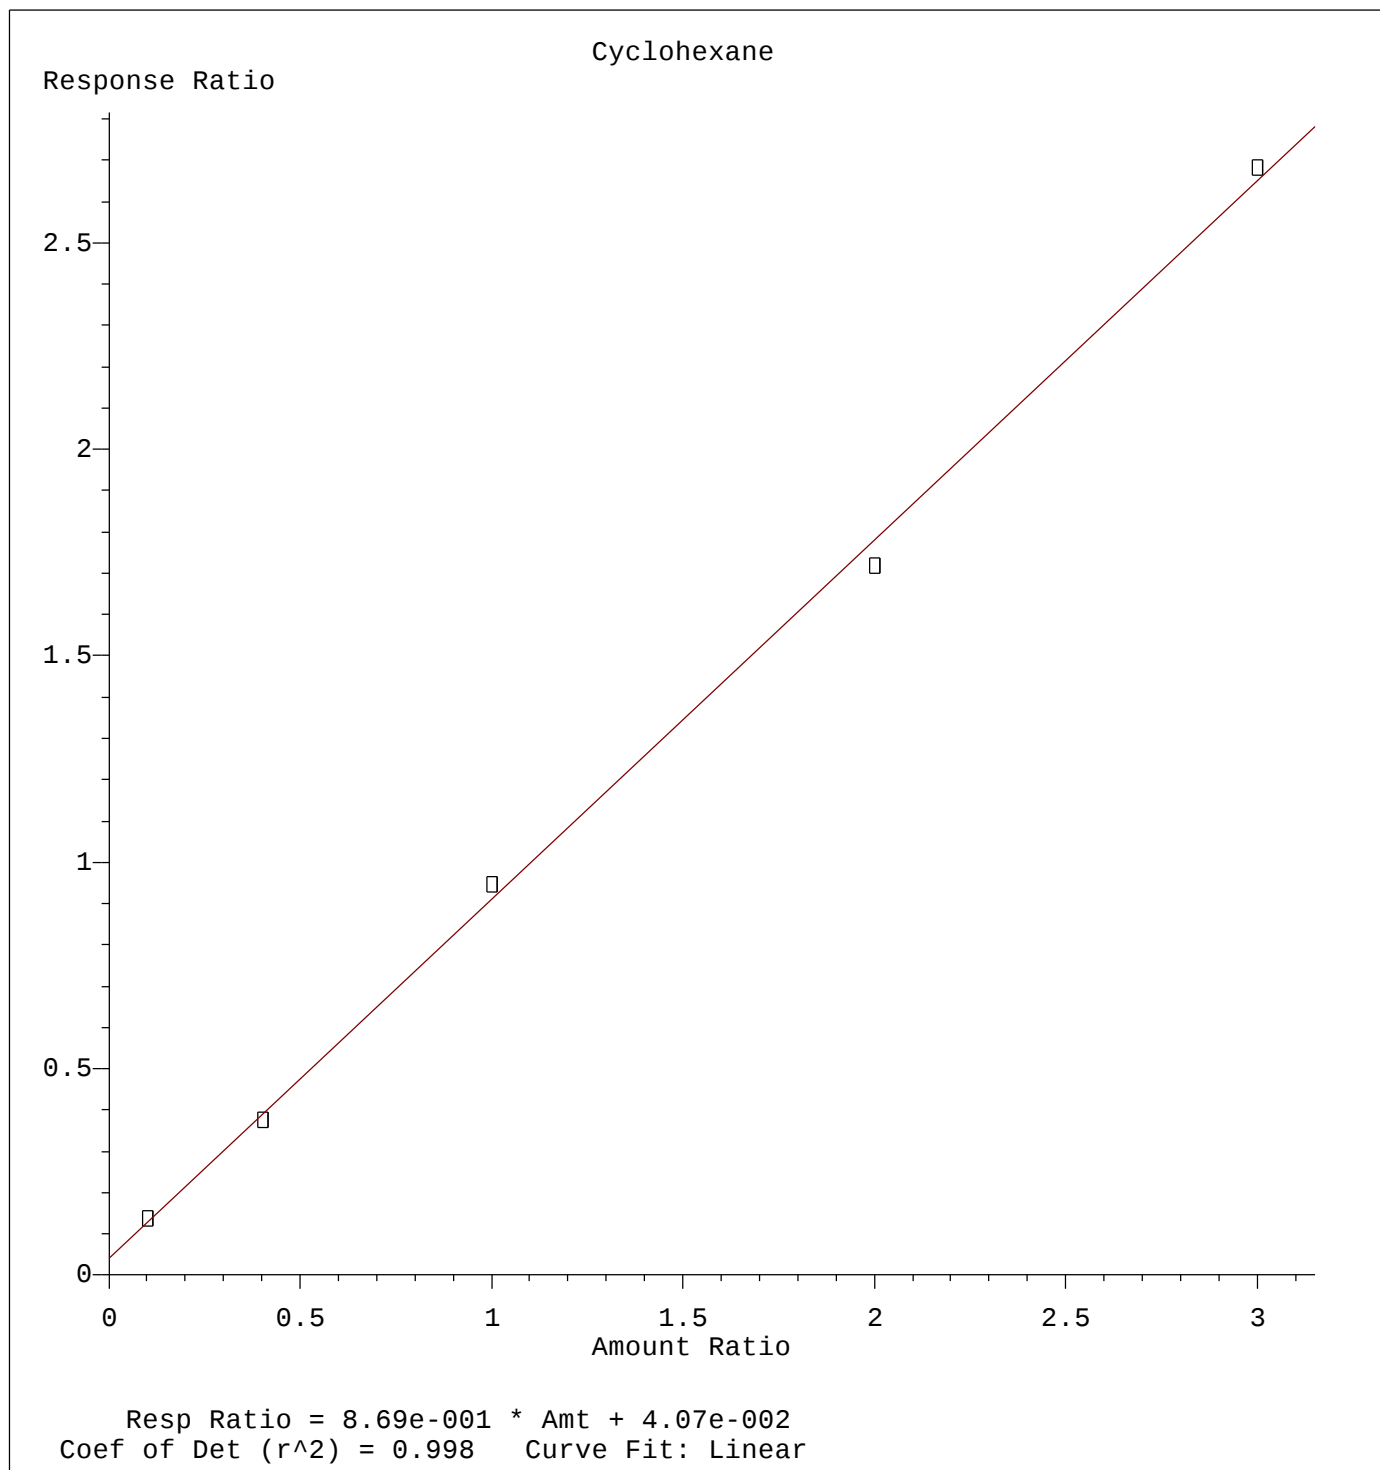

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091019W.M
Calibration Table Last Updated: Fri Sep 13 05:15:45 2019

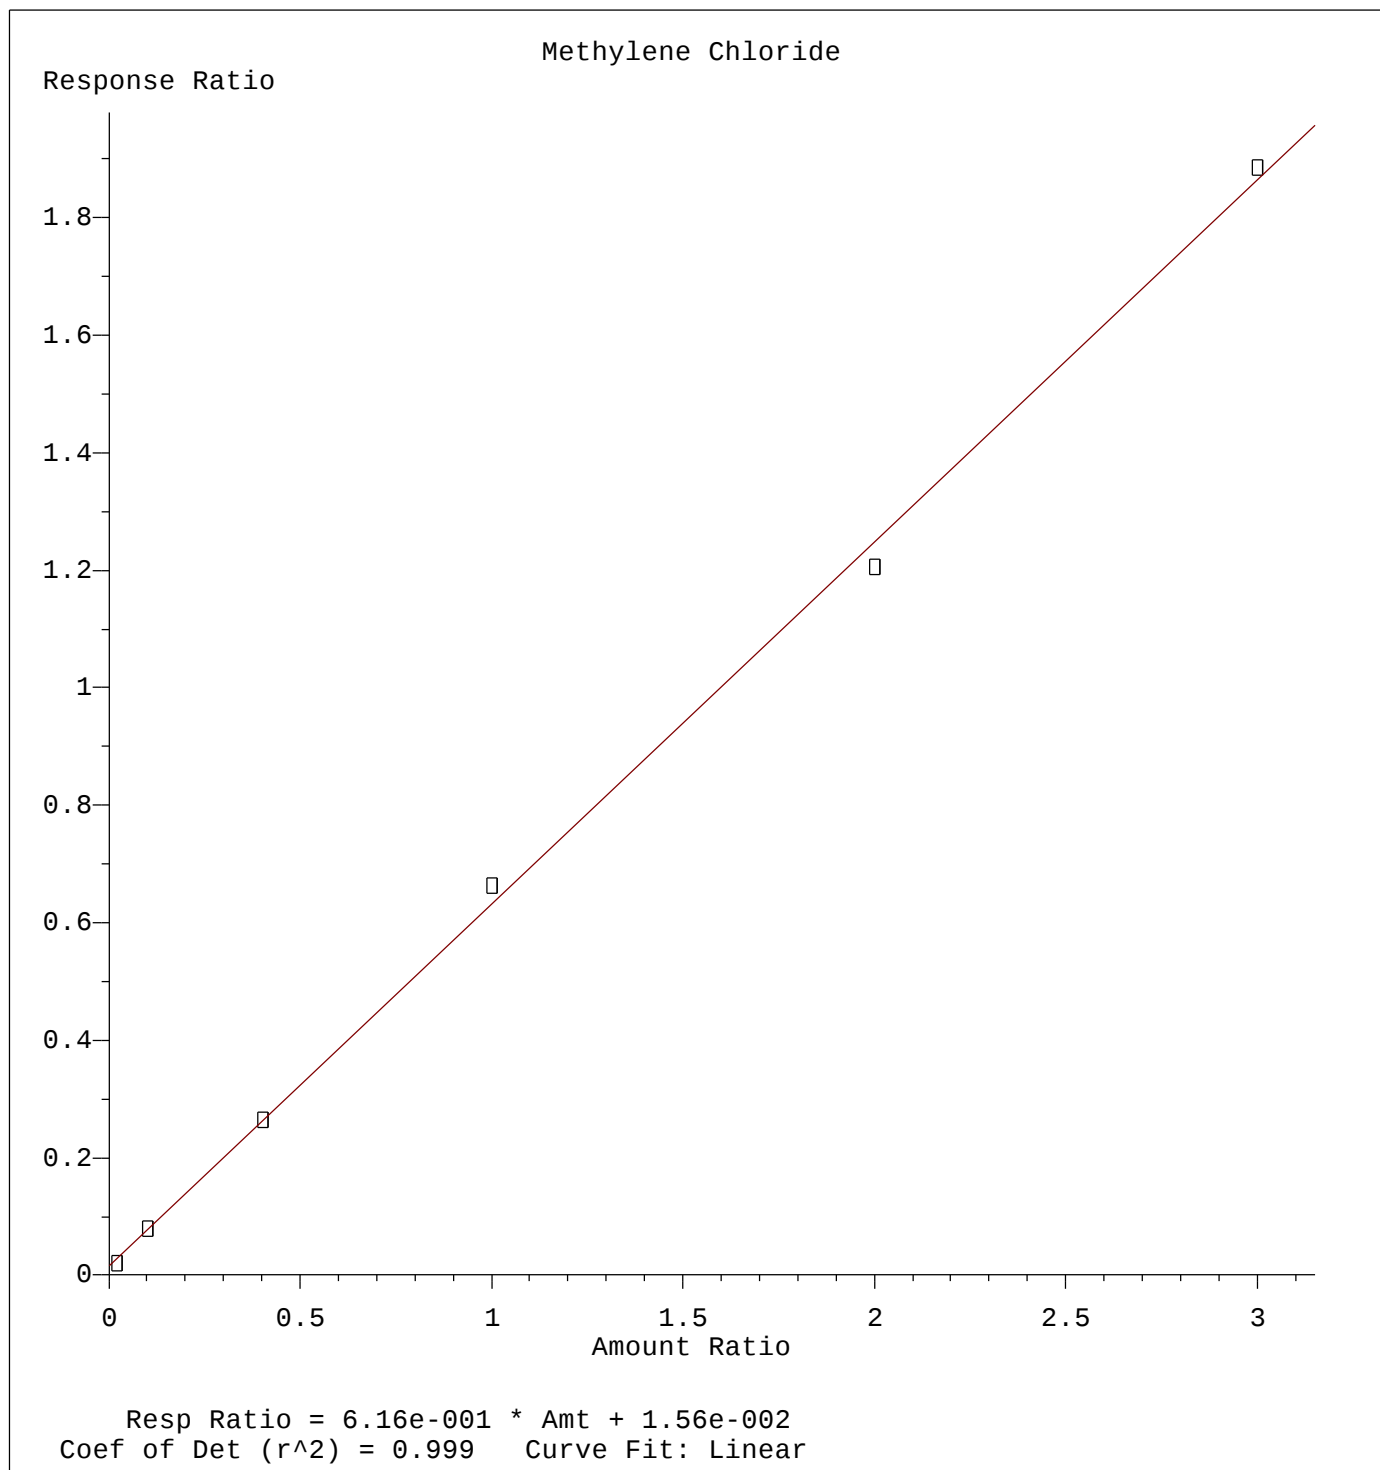

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091019W.M
Calibration Table Last Updated: Fri Sep 13 05:15:45 2019

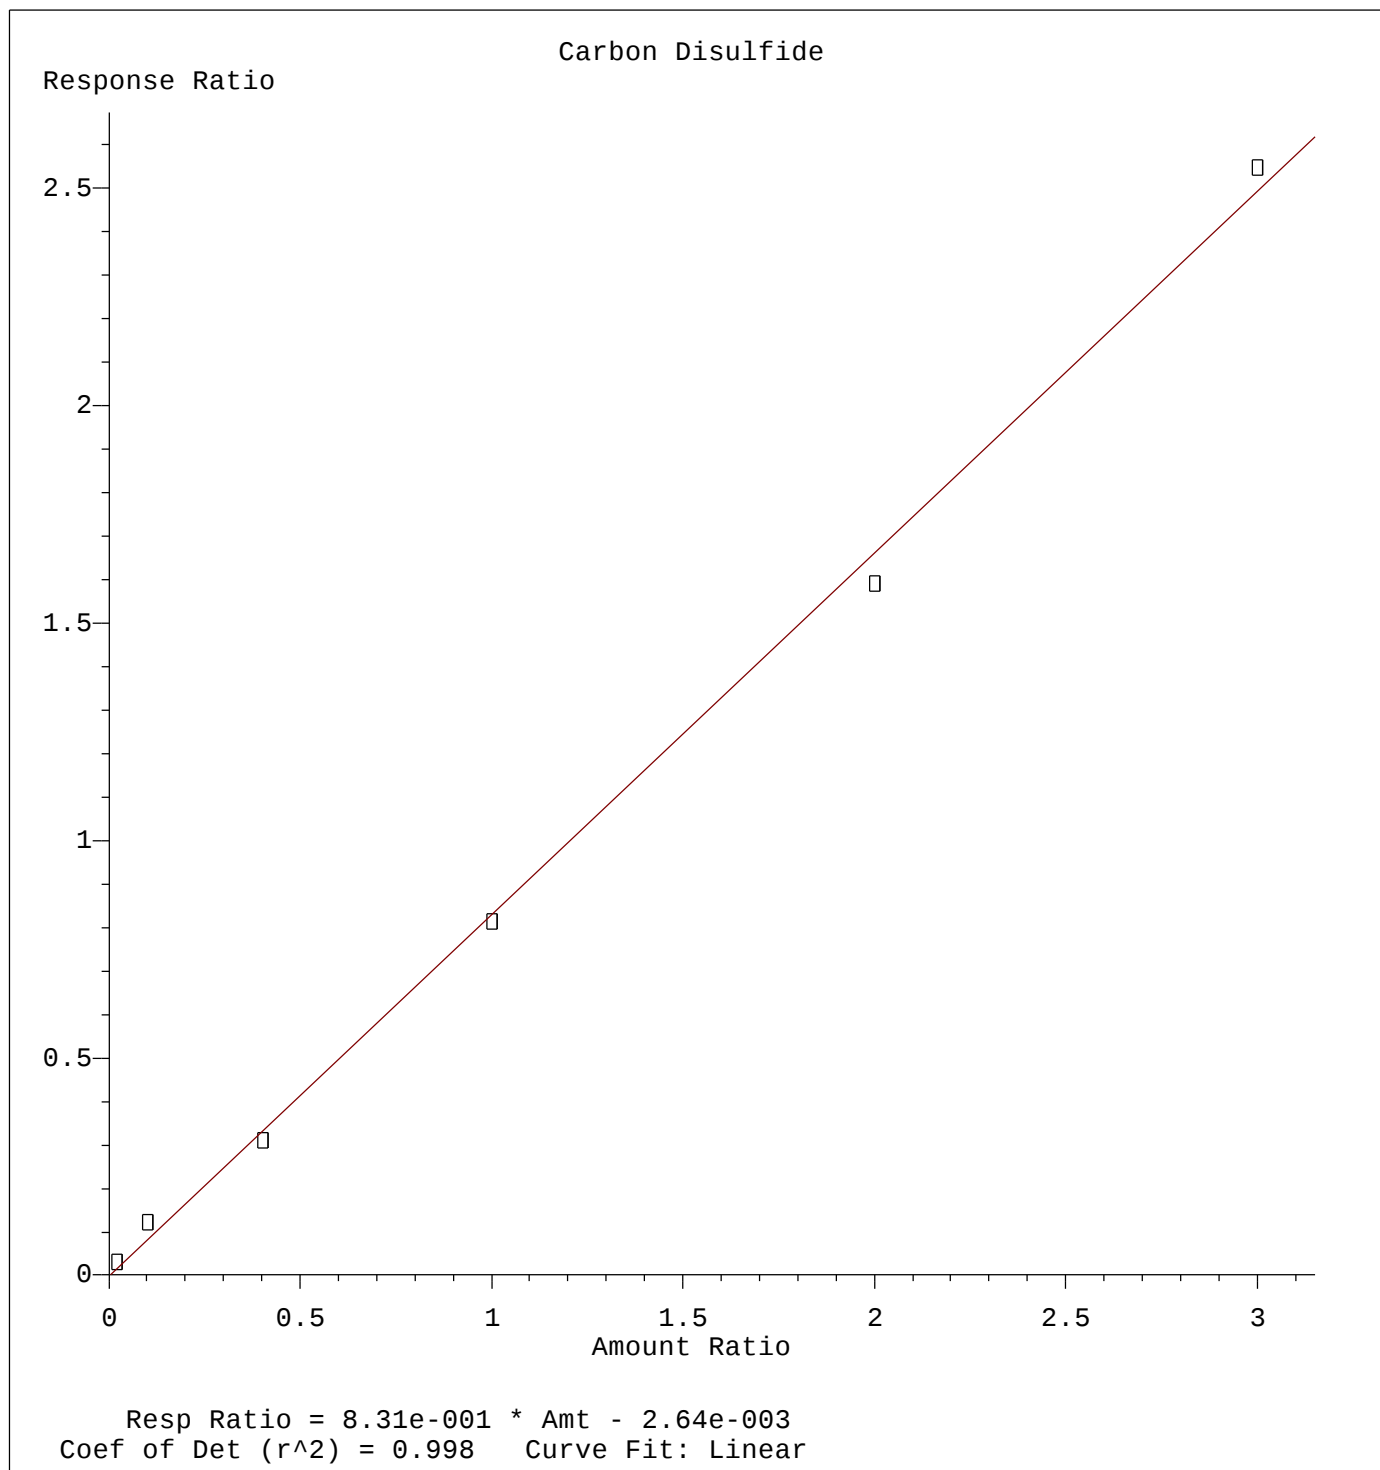

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091019W.M
Calibration Table Last Updated: Fri Sep 13 05:15:45 2019