


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN091019\  
 Data File : VN057828.D  
 Acq On : 10 Sep 2019 2:06  
 Operator : JC/SP  
 Sample : BFB  
 Misc : 5.00mL/MSVOA N/WATER  
 ALS Vial : 33 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N091019W.M  
 Title : SW846 8260  
 Last Update : Tue Sep 10 03:02:13 2019

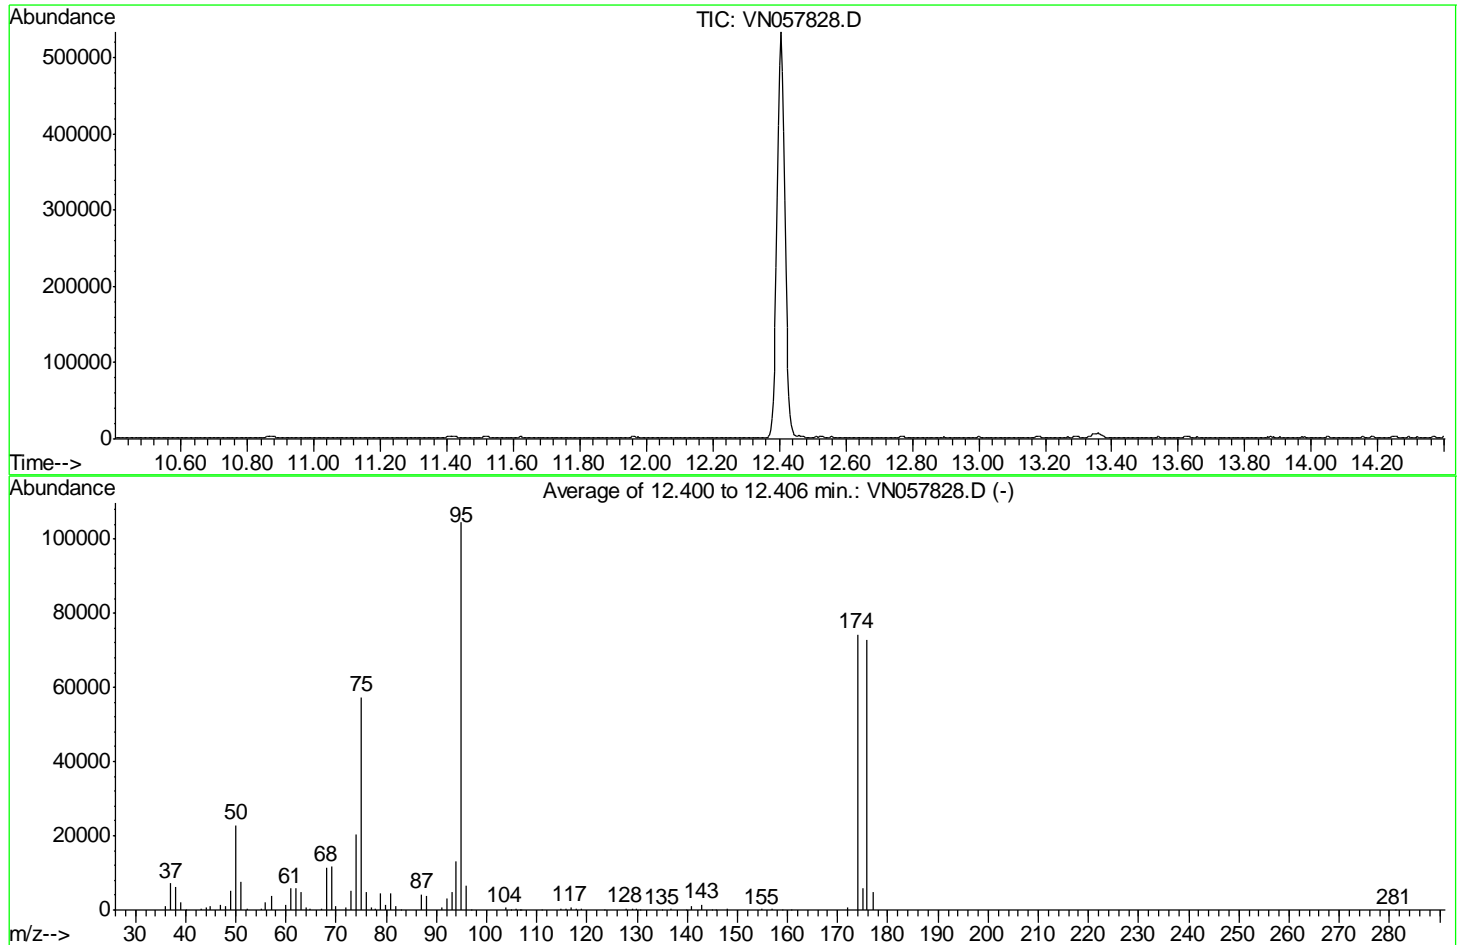

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	22893	PASS
75	95	30	60	54.8	57274	PASS
95	95	100	100	100.0	104480	PASS
96	95	5	9	6.4	6705	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.1	74269	PASS
175	174	5	9	8.1	6010	PASS
176	174	95	101	98.1	72882	PASS
177	176	5	9	6.6	4845	PASS